

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070622\
 Data File : VN073348.D
 Acq On : 06 Jul 2022 16:25
 Operator : JC\MD
 Sample : N3586-01 10X
 Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 31267

Quant Time: Jul 07 04:24:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	329219	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	548327	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	537288	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	298797	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	201911	42.484	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	84.960%		
35) Dibromofluoromethane	7.951	113	169918	46.577	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.160%		
50) Toluene-d8	10.375	98	596339	46.025	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	92.060%		
62) 4-Bromofluorobenzene	12.669	95	276477	55.526	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	111.060%		
Target Compounds					Qvalue	
16) Acetone	4.252	43	3280	1.230	ug/l #	68
18) Methyl Acetate	4.804	43	3312	0.443	ug/l #	48
20) Methylene Chloride	5.016	84	1632	0.348	ug/l #	61
29) Tetrahydrofuran	7.628	42	834	0.287	ug/l #	42
31) Cyclohexane	8.010	56	9435	1.212	ug/l #	54
36) 1,1-Dichloropropene	8.010	75	27292	4.862	ug/l #	51
38) Carbon Tetrachloride	8.016	117	34848	6.003	ug/l #	17
39) Methylcyclohexane	9.404	83	3408	0.488	ug/l #	69
52) Toluene	10.439	92	95736	8.942	ug/l	97
59) 2-Hexanone	11.022	43	1886	0.320	ug/l	76
66) 1,1,1,2-Tetrachloroethane	11.851	131	1174	0.263	ug/l #	1
67) Ethyl Benzene	11.786	91	6537	0.296	ug/l #	61
68) m/p-Xylenes	11.892	106	7973	0.958	ug/l #	63
71) Bromoform	12.357	173	31142	9.522	ug/l #	33
74) N-amyl acetate	12.304	43	9367	0.725	ug/l #	39
75) 1,1,2,2-Tetrachloroethane	12.722	83	2616	0.306	ug/l #	25
76) 1,2,3-Trichloropropane	12.669	75	147956	18.937	ug/l #	1
77) Bromobenzene	12.686	156	95000	15.836	ug/l #	1
78) n-propylbenzene	12.863	91	12697	0.443	ug/l #	49
80) 1,3,5-Trimethylbenzene	12.922	105	24296	1.155	ug/l	73
81) trans-1,4-Dichloro-2-b...	12.669	75	147956	51.935	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.304	105	56286	2.681	ug/l	75
85) sec-Butylbenzene	13.439	105	8769	0.346	ug/l #	56
86) p-Isopropyltoluene	13.551	119	6632	0.324	ug/l #	51
87) 1,3-Dichlorobenzene	13.539	146	3202	0.298	ug/l #	32
88) 1,4-Dichlorobenzene	13.651	146	3993	0.370	ug/l #	26
89) n-Butylbenzene	13.880	91	7289	0.428	ug/l #	1
90) Hexachloroethane	14.310	117	1546	0.406	ug/l	68
92) 1,2-Dibromo-3-Chloropr...	14.568	75	677	0.325	ug/l #	1
95) Naphthalene	15.433	128	48451	2.104	ug/l #	7
96) 1,2,3-Trichlorobenzene	15.615	180	1243	0.211	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070622\
Data File : VN073348.D
Acq On : 06 Jul 2022 16:25
Operator : JC\MD
Sample : N3586-01 10X
Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
31267

Quant Time: Jul 07 04:24:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration



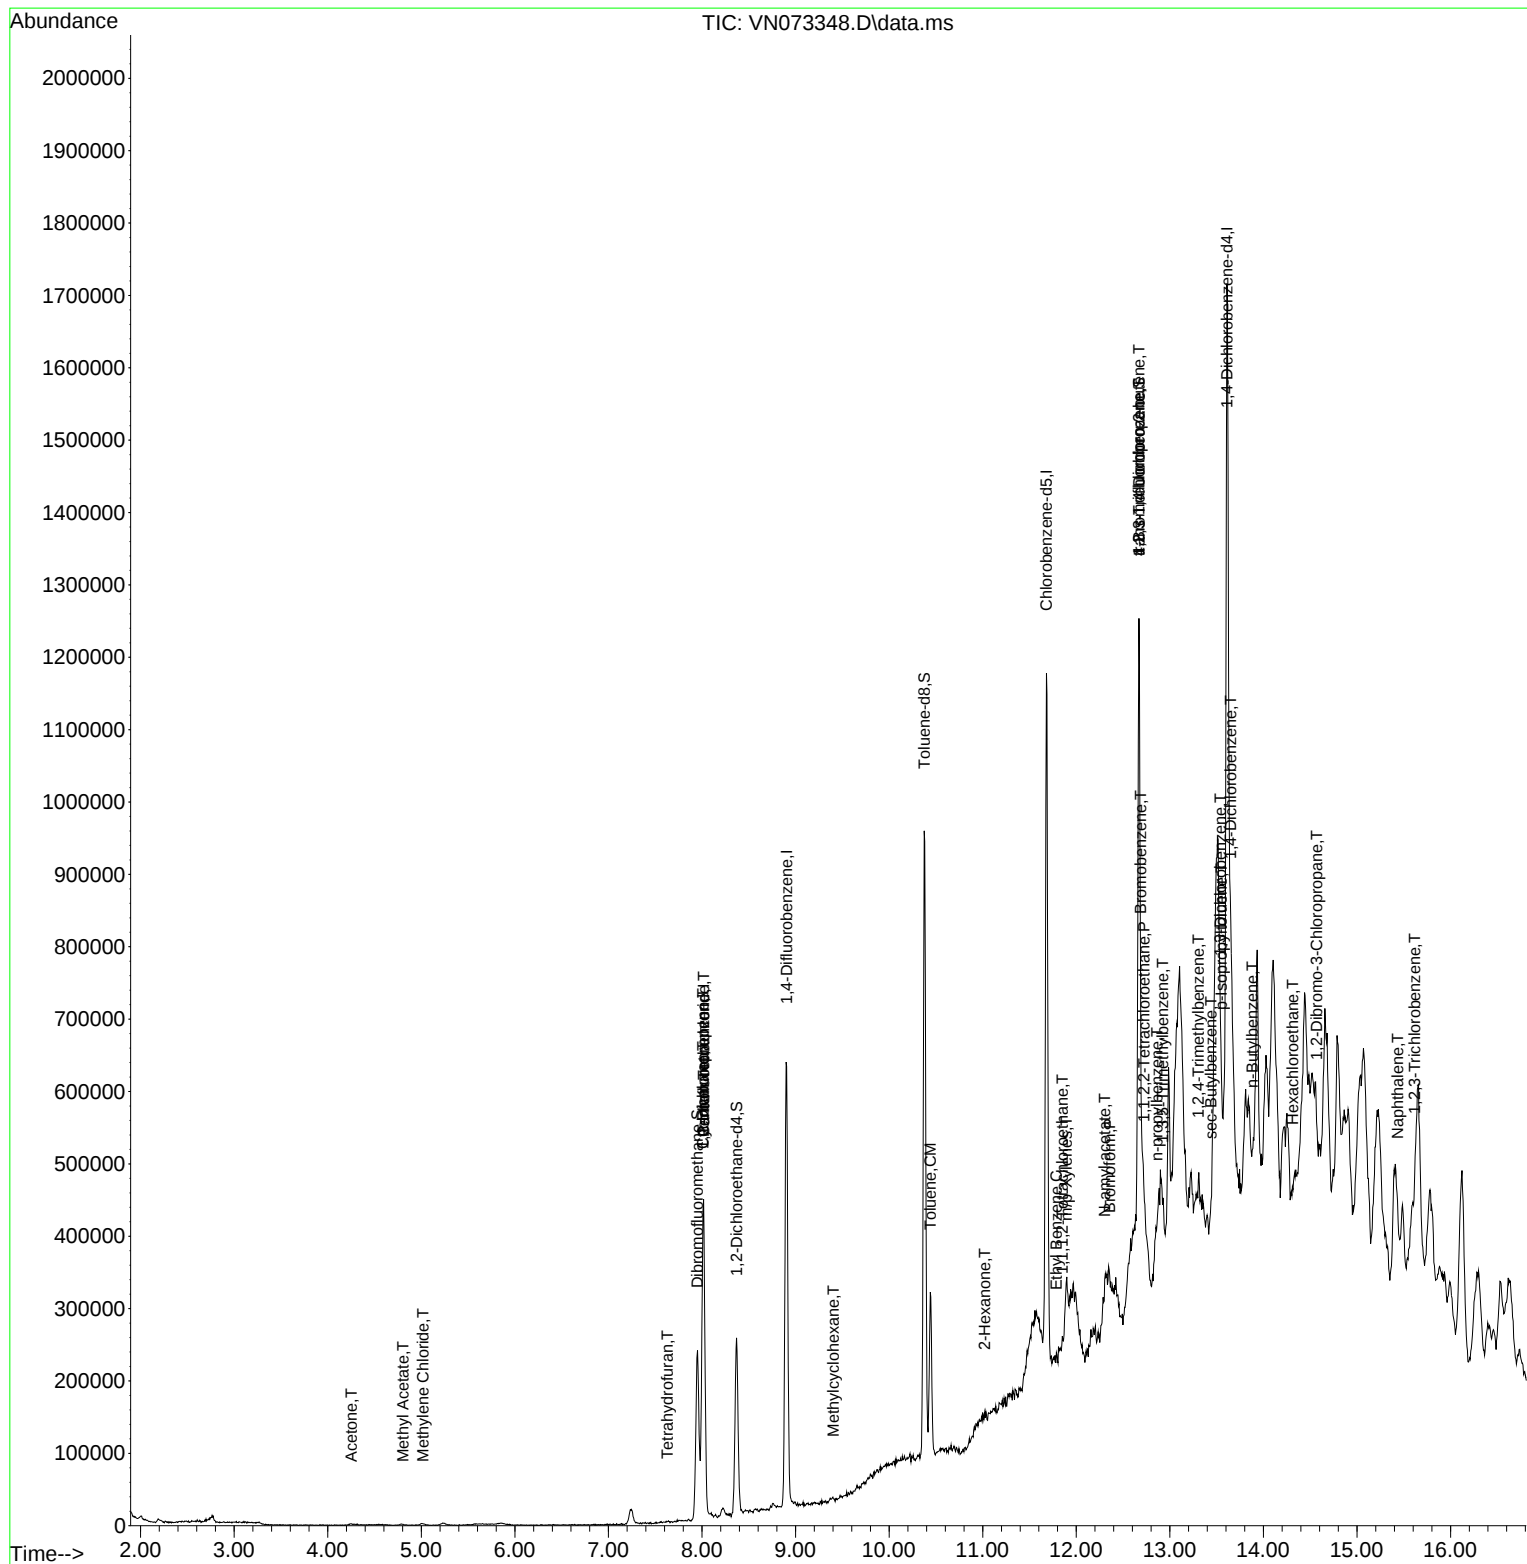


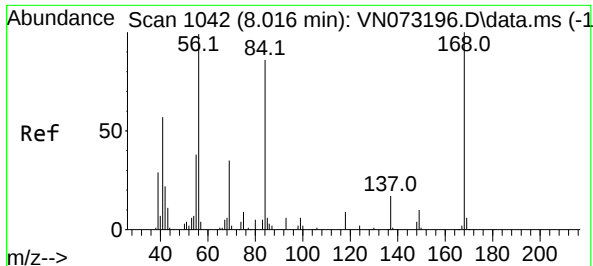

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion:168 Resp: 329219
Ion Ratio Lower Upper
168 100
99 60.1 42.3 63.5

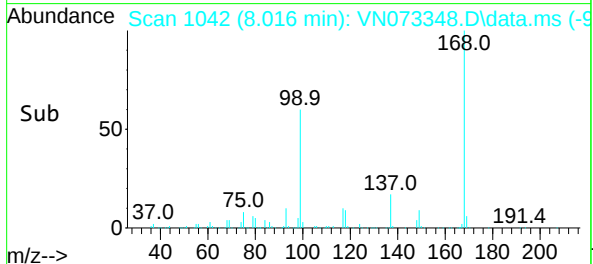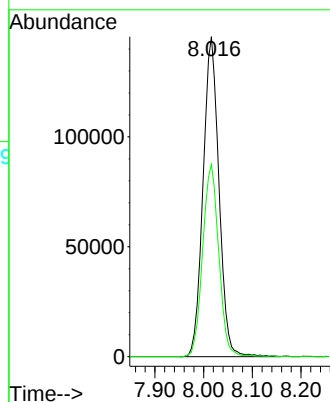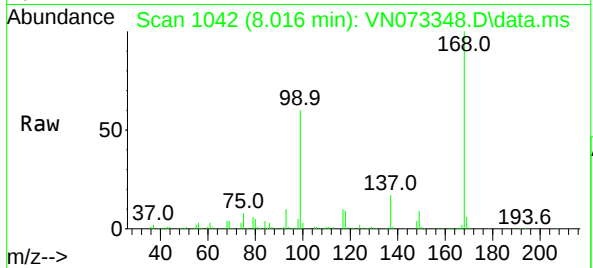

#16
Acetone
Concen: 1.230 ug/l
RT: 4.252 min Scan# 402
Delta R.T. 0.029 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 43 Resp: 3280
Ion Ratio Lower Upper
43 100
58 14.6 26.0 39.0#


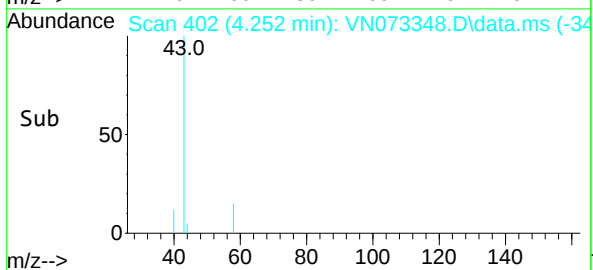
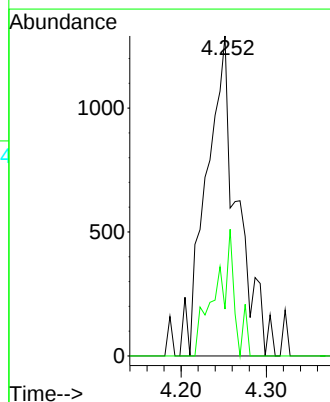
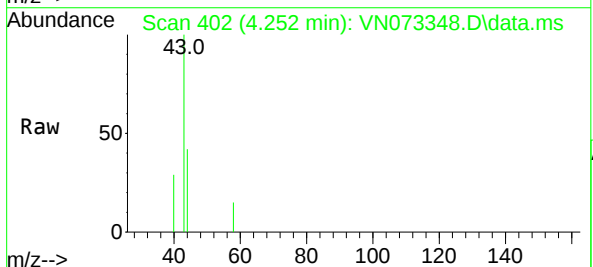


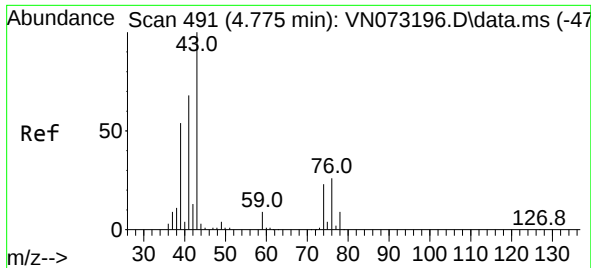

#18
Methyl Acetate
Concen: 0.443 ug/l
RT: 4.804 min Scan# 491
Delta R.T. 0.029 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 43 Resp: 3312
Ion Ratio Lower Upper
43 100
74 0.0 21.6 32.4#

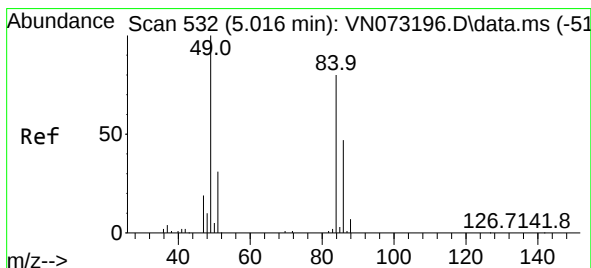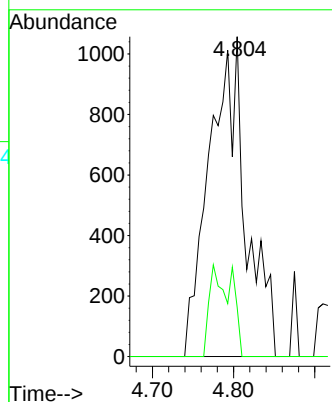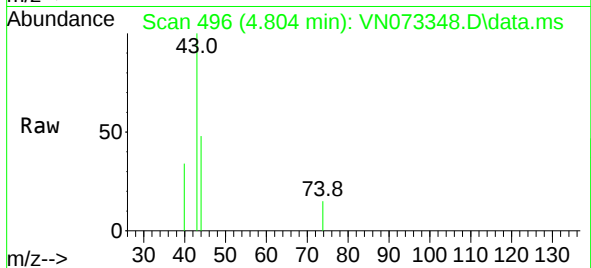

#20
Methylene Chloride
Concen: 0.348 ug/l
RT: 5.016 min Scan# 532
Delta R.T. 0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 84 Resp: 1632
Ion Ratio Lower Upper
84 100
49 50.3 88.3 132.5#
51 40.1 28.2 42.2
86 43.7 50.6 76.0#

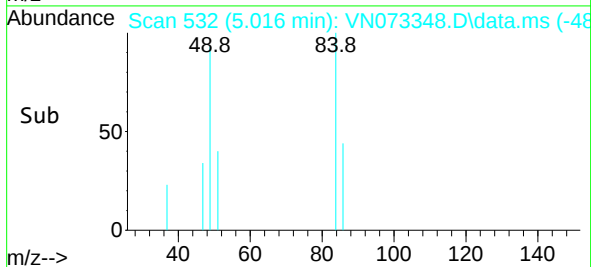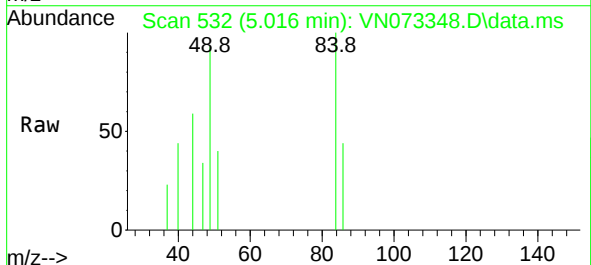



#29

Tetrahydrofuran

Concen: 0.287 ug/l

RT: 7.628 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

31267





Tgt Ion: 42 Resp: 834

Ion Ratio Lower Upper

42 100

72 7.3 39.7 59.5#

71 10.4 36.6 55.0#

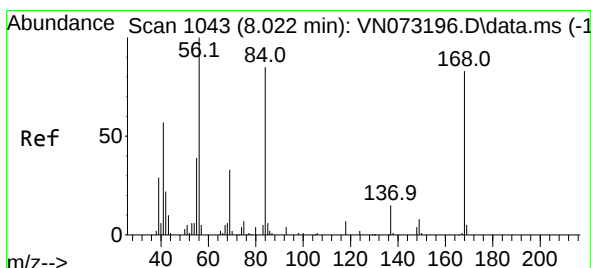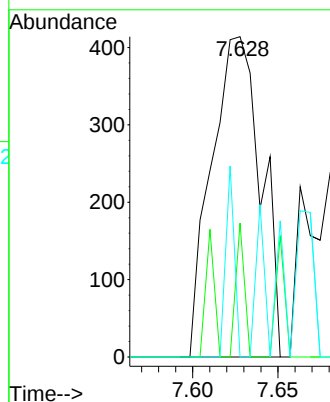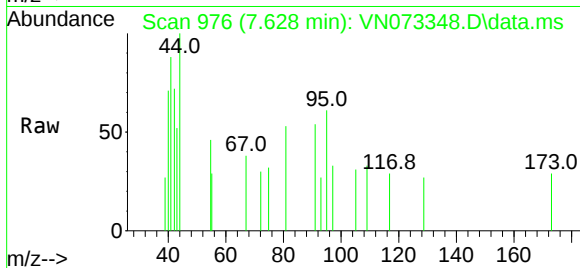

#31

Cyclohexane

Concen: 1.212 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.012 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25




Tgt Ion: 56 Resp: 9435


Ion Ratio Lower Upper

56 100

69 131.9 27.8 41.8#

84 94.8 76.9 115.3

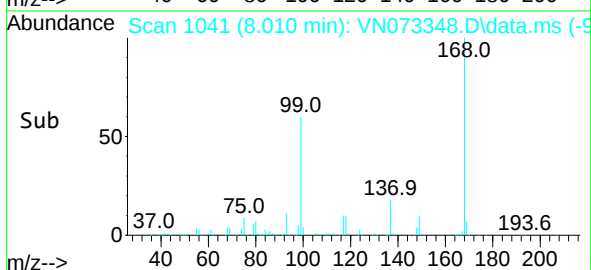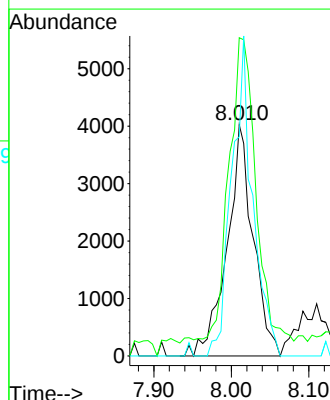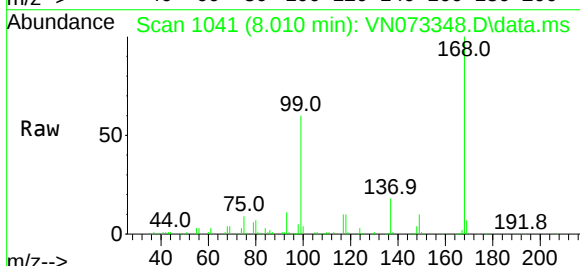

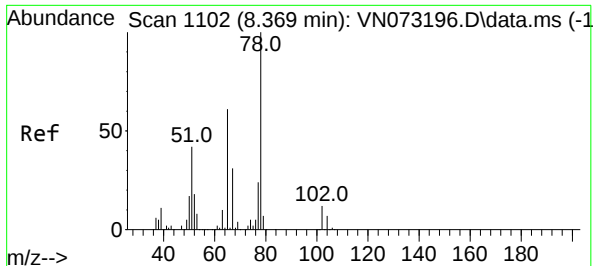

#33

1,2-Dichloroethane-d4

Concen: 42.484 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :





31267

Tgt Ion: 65 Resp: 201911

Ion Ratio Lower Upper

65 100

67 52.0 0.0 104.8

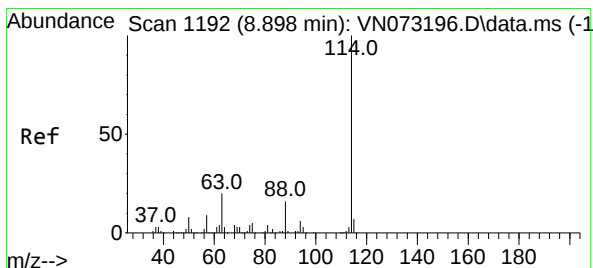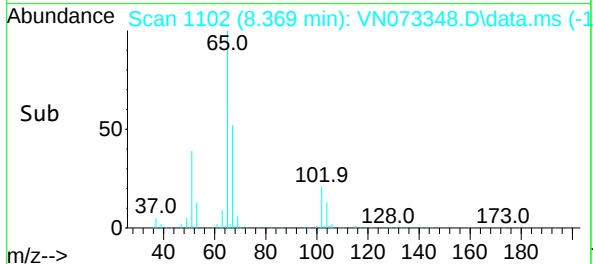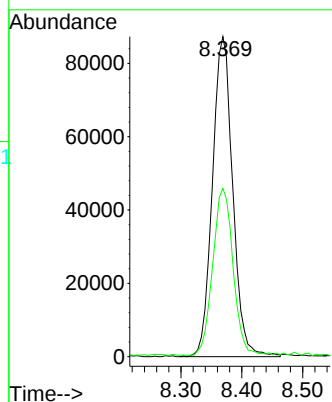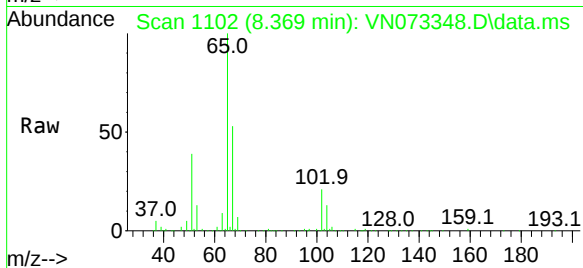

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25




Tgt Ion: 114 Resp: 548327


Ion Ratio Lower Upper

114 100

63 21.0 0.0 40.0

88 16.3 0.0 32.6


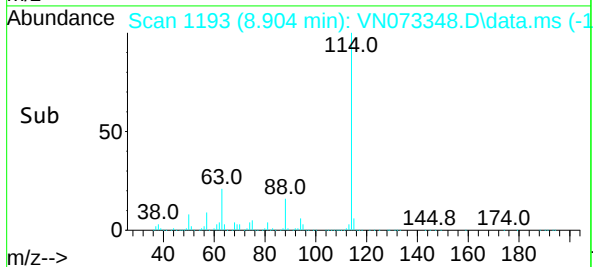

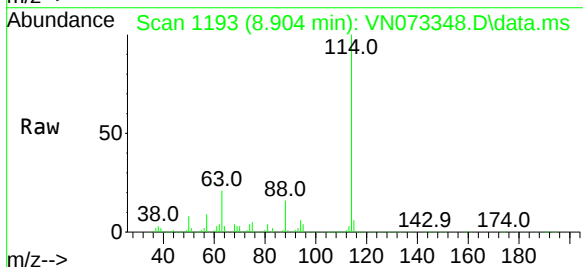


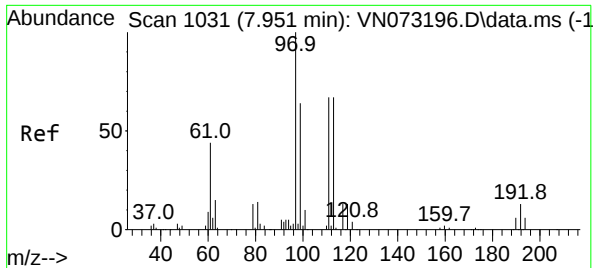

#35
Dibromofluoromethane
Concen: 46.577 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion:113 Resp: 169918
Ion Ratio Lower Upper
113 100
111 103.6 81.4 122.0
192 18.6 17.0 25.6

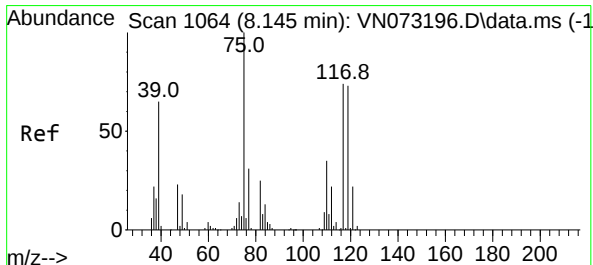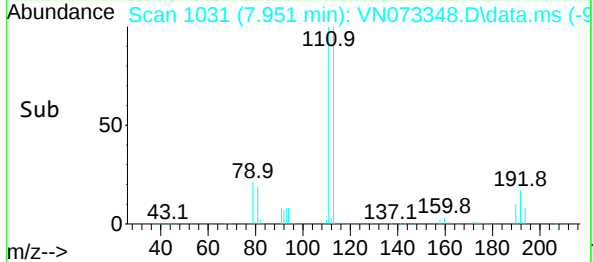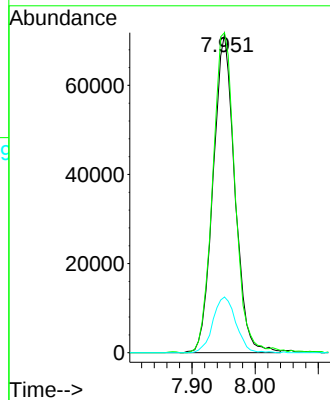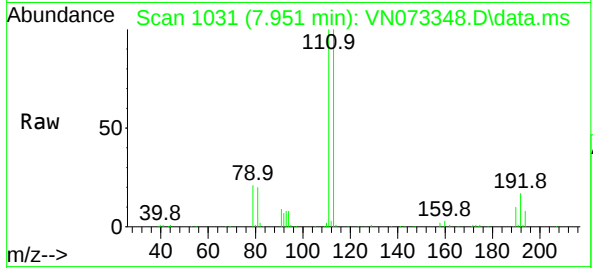

#36
1,1-Dichloropropene
Concen: 4.862 ug/l
RT: 8.010 min Scan# 1041
Delta R.T. -0.135 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 75 Resp: 27292
Ion Ratio Lower Upper
75 100
110 10.2 18.3 54.8#
77 1.9 25.1 37.7#


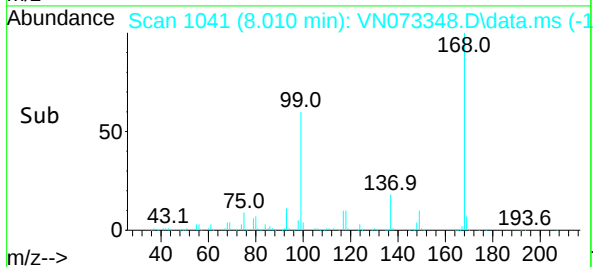
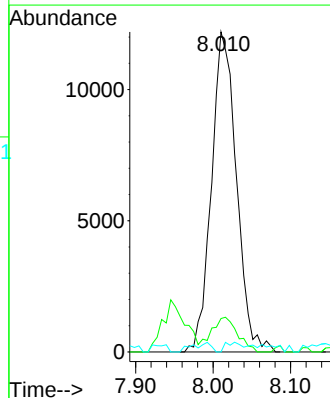
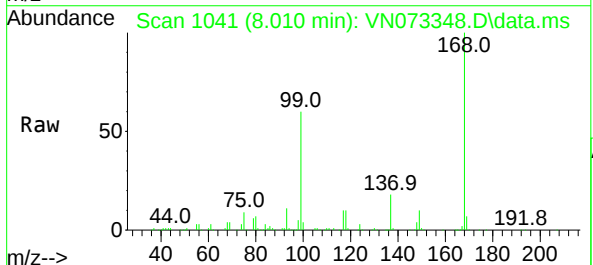


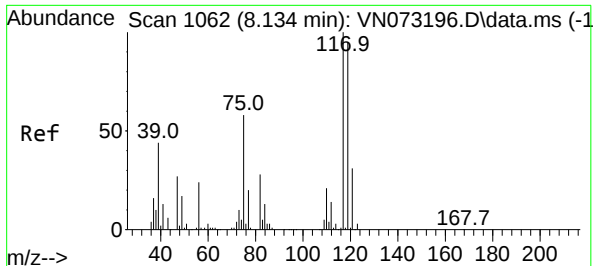

#38
Carbon Tetrachloride
Concen: 6.003 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion:117 Resp: 34848
Ion Ratio Lower Upper
117 100
119 5.0 75.8 113.8#
121 1.7 24.6 37.0#

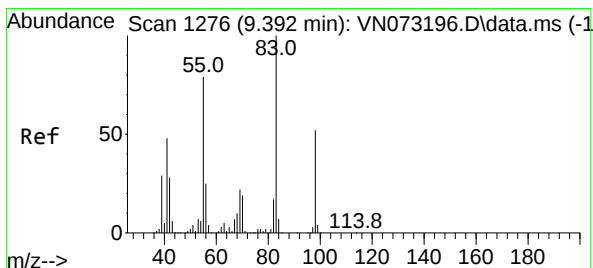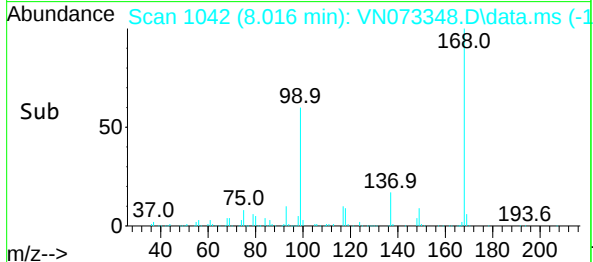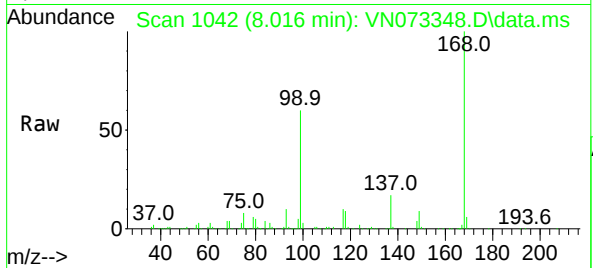

#39
Methylcyclohexane
Concen: 0.488 ug/l
RT: 9.404 min Scan# 1278
Delta R.T. 0.012 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 83 Resp: 3408
Ion Ratio Lower Upper
83 100
55 52.8 57.8 86.8#
98 20.1 39.4 59.2#


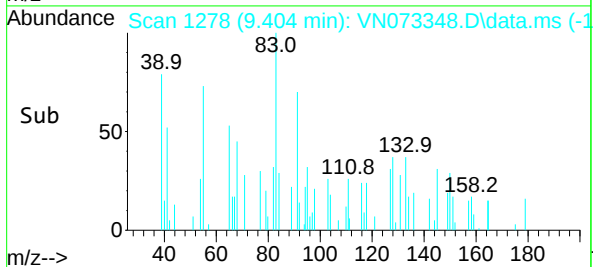

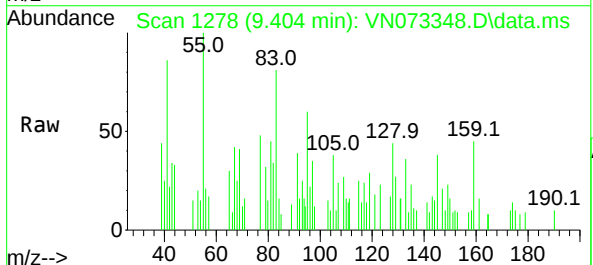




#50
Toluene-d8
Concen: 46.025 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 98 Resp: 596339
Ion Ratio Lower Upper
98 100
100 66.1 52.6 78.8

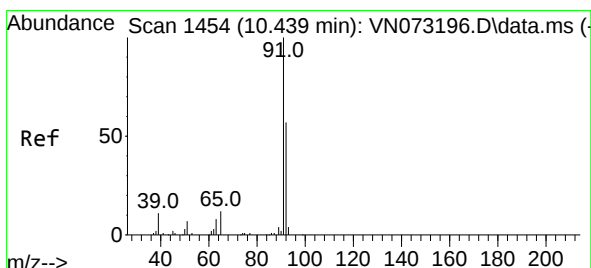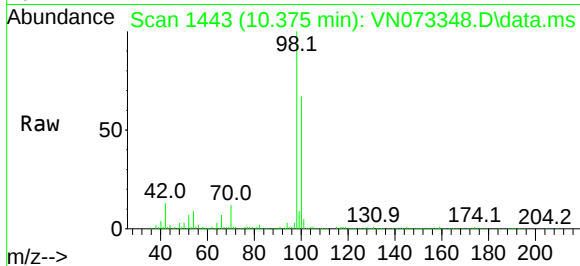

#52
Toluene
Concen: 8.942 ug/l
RT: 10.439 min Scan# 1454
Delta R.T. 0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 92 Resp: 95736
Ion Ratio Lower Upper
92 100
91 169.5 138.6 207.8


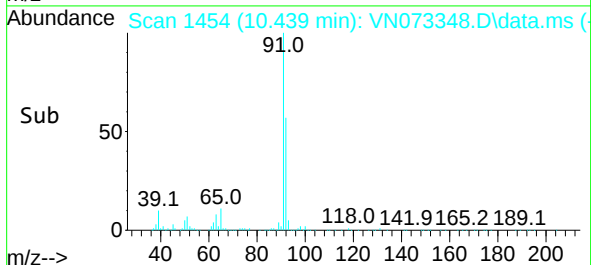

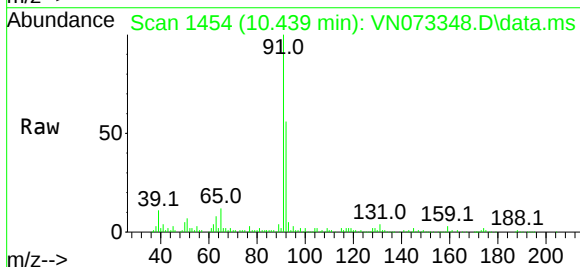




#59
2-Hexanone
Concen: 0.320 ug/l
RT: 11.022 min Scan# 1153
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 43 Resp: 1886
Ion Ratio Lower Upper
43 100
58 41.2 29.7 89.1

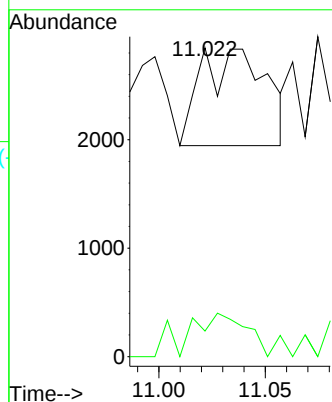

#62
4-Bromofluorobenzene
Concen: 55.526 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 95 Resp: 276477
Ion Ratio Lower Upper
95 100
174 92.5 0.0 167.6
176 73.0 0.0 163.4

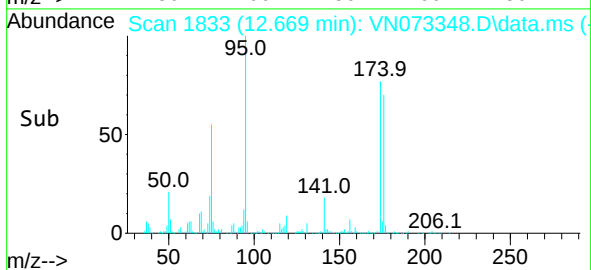

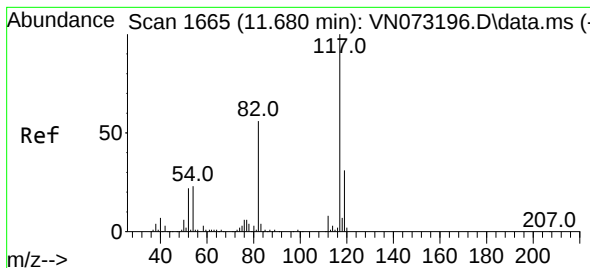

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.680 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

31267





Tgt Ion:117 Resp: 537288

Ion Ratio Lower Upper

117 100

82 56.0 44.2 66.2

119 32.7 25.4 38.0

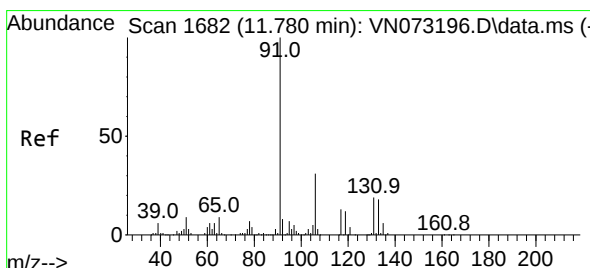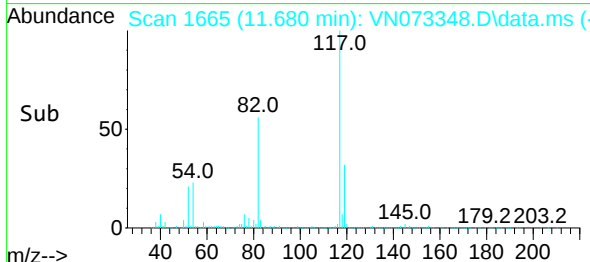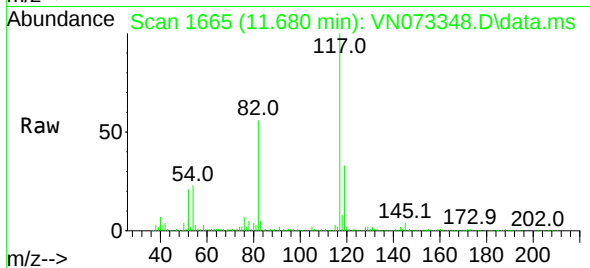

#66

1,1,1,2-Tetrachloroethane

Concen: 0.263 ug/l

RT: 11.851 min Scan# 1694

Delta R.T. 0.071 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25




Tgt Ion:131 Resp: 1174


Ion Ratio Lower Upper

131 100

133 336.5 47.8 143.4#

119 0.0 33.4 100.2#


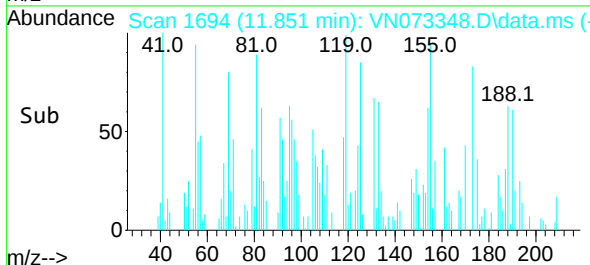

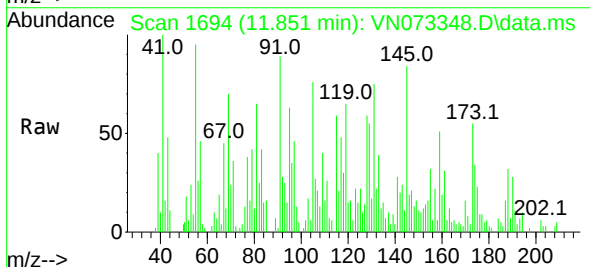


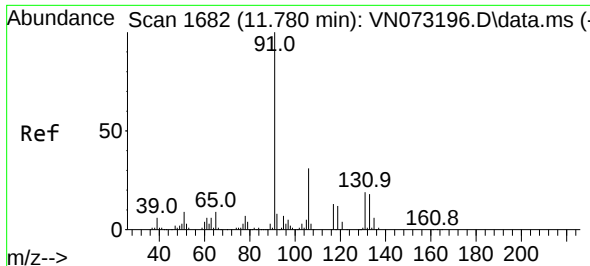

#67
Ethyl Benzene
Concen: 0.296 ug/l
RT: 11.786 min Scan# 11786
Delta R.T. 0.006 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 91 Resp: 6537
Ion Ratio Lower Upper
91 100
106 9.8 24.9 37.3#

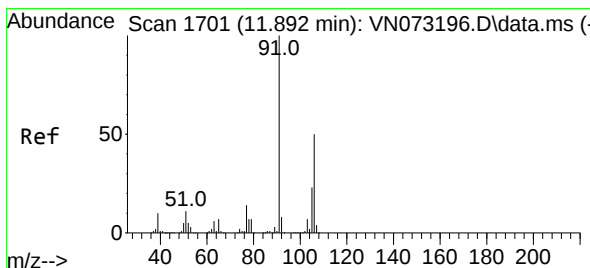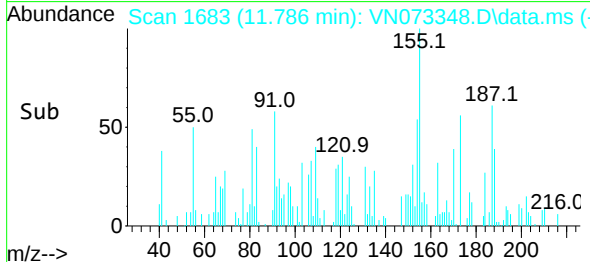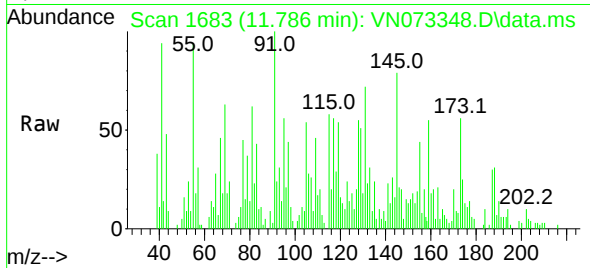

#68
m/p-Xylenes
Concen: 0.958 ug/l
RT: 11.892 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 106 Resp: 7973
Ion Ratio Lower Upper
106 100
91 142.3 158.9 238.3#


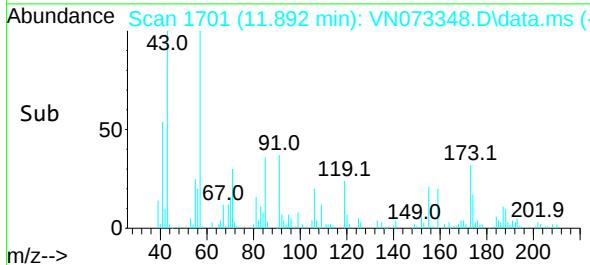

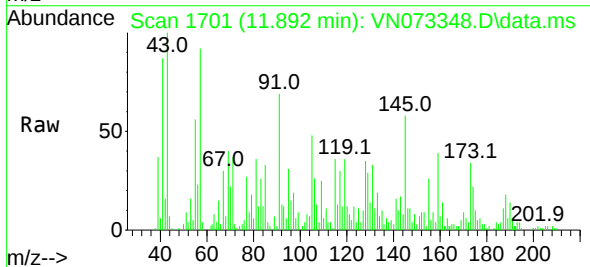




#71
Bromoform
Concen: 9.522 ug/l
RT: 12.357 min Scan# 1780
Delta R.T. -0.041 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion:173 Resp: 31142
Ion Ratio Lower Upper
173 100
175 3.0 24.6 73.6#
254 0.0 0.1 0.1#

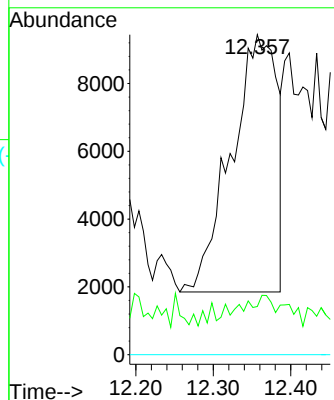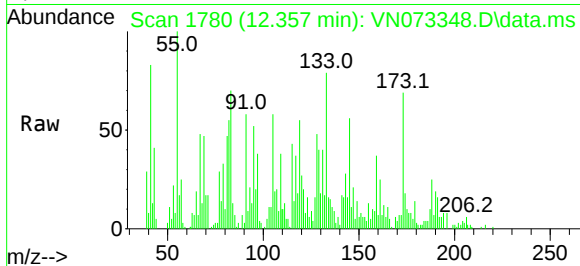

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion:152 Resp: 298797
Ion Ratio Lower Upper
152 100
115 78.9 28.9 86.7
150 137.8 0.0 356.2


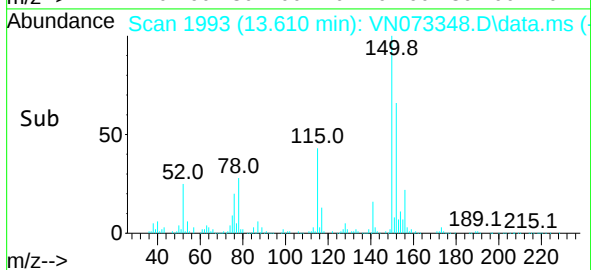
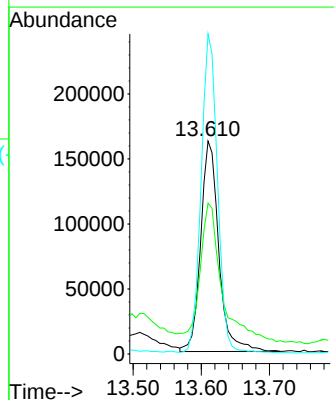
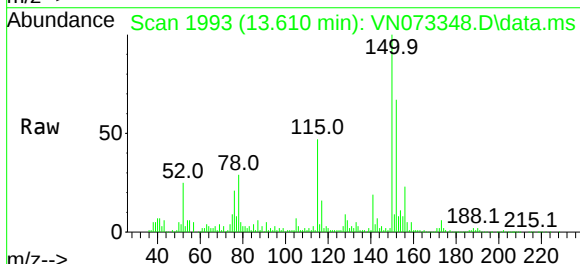


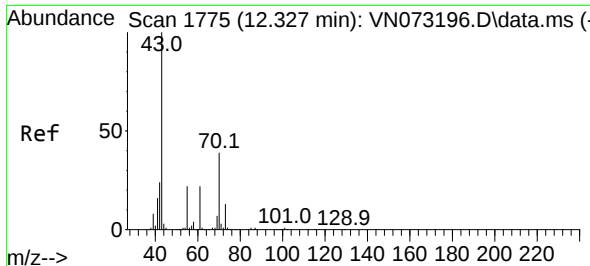

#74
N-amy1 acetate
Concen: 0.725 ug/l
RT: 12.304 min Scan# 1771
Delta R.T. -0.023 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 43 Resp: 9367
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 0.0 21.1 31.7#
61 0.0 21.1 31.7#

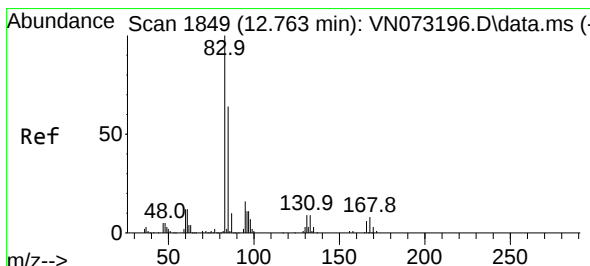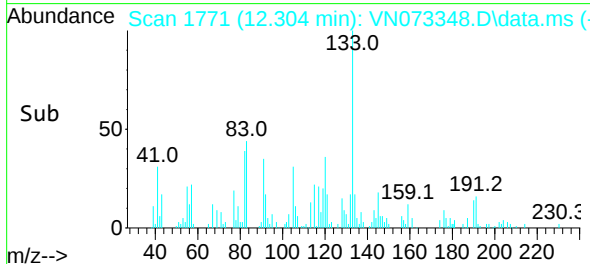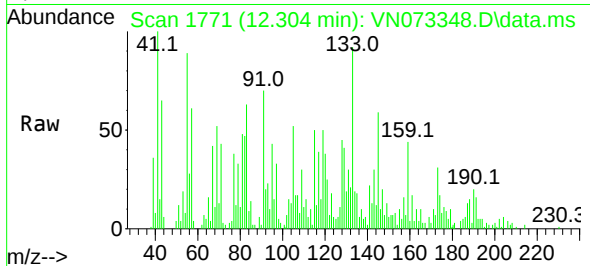

#75
1,1,2,2-Tetrachloroethane
Concen: 0.306 ug/l
RT: 12.722 min Scan# 1842
Delta R.T. -0.041 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 83 Resp: 2616
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.9#
85 0.0 32.3 96.9#


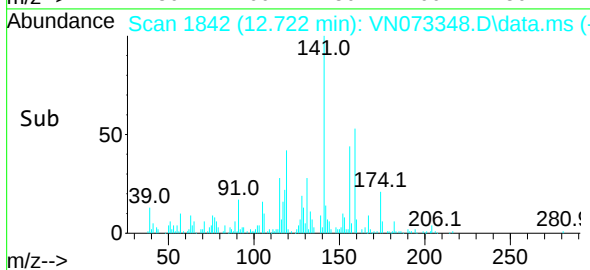

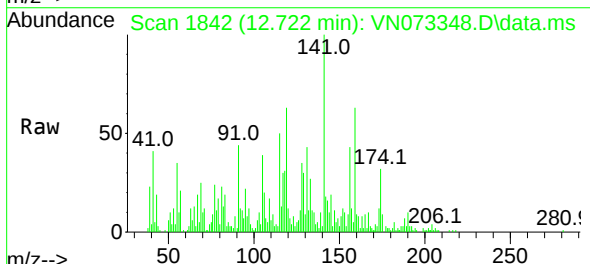




#76
1,2,3-Trichloropropane
Concen: 18.937 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.147 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 75 Resp: 147956
Ion Ratio Lower Upper
75 100
77 10.0 98.5 295.5#

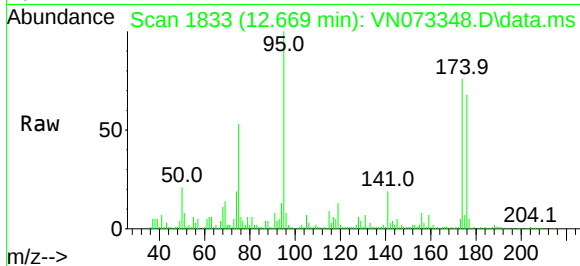

#77
Bromobenzene
Concen: 15.836 ug/l
RT: 12.686 min Scan# 1836
Delta R.T. -0.112 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 156 Resp: 95000
Ion Ratio Lower Upper
156 100
77 15.8 100.5 301.5#
158 0.0 48.9 146.6#


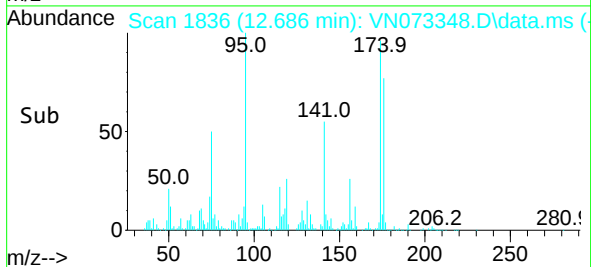

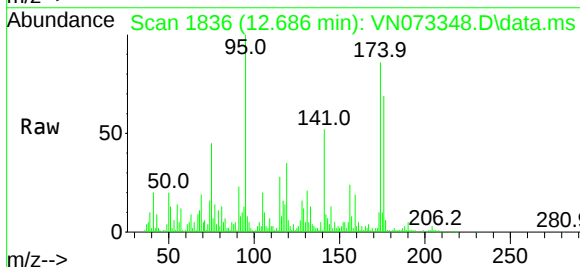




#78
n-propylbenzene
Concen: 0.443 ug/l
RT: 12.863 min Scan# 1866
Delta R.T. 0.006 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 91 Resp: 12697
Ion Ratio Lower Upper
91 100
120 48.5 11.9 35.5#

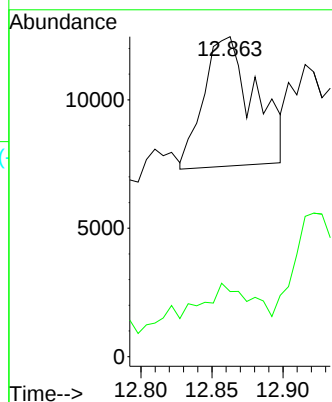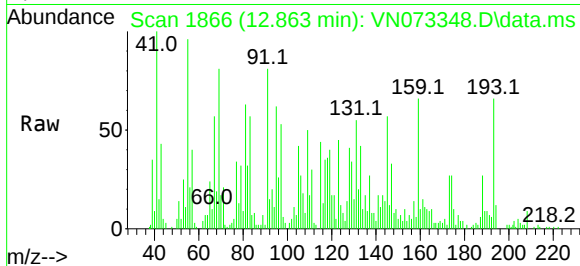

#80
1,3,5-Trimethylbenzene
Concen: 1.155 ug/l
RT: 12.922 min Scan# 1876
Delta R.T. -0.076 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion:105 Resp: 24296
Ion Ratio Lower Upper
105 100
120 31.3 24.9 74.7


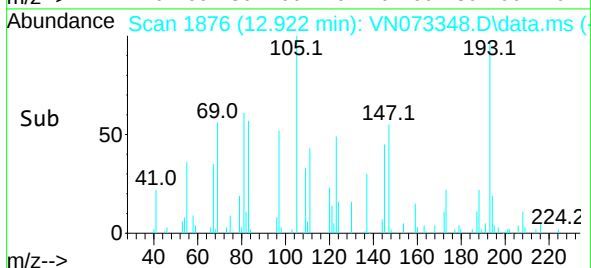

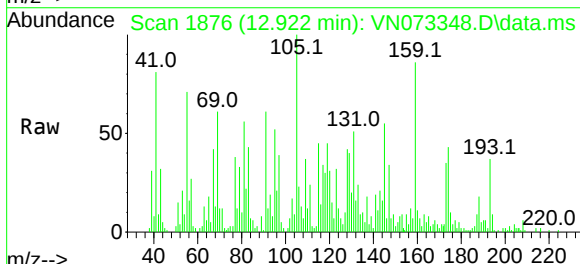


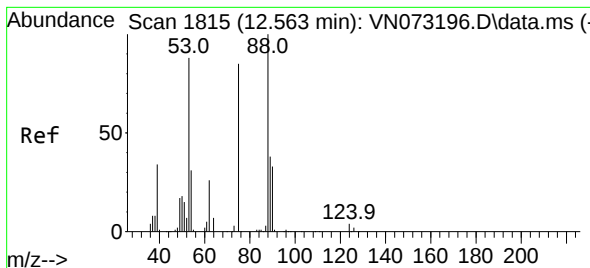

#81
trans-1,4-Dichloro-2-butene
Concen: 51.935 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. 0.106 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 75 Resp: 147956
Ion Ratio Lower Upper
75 100
53 0.5 78.0 117.0#
89 0.0 37.2 55.8#

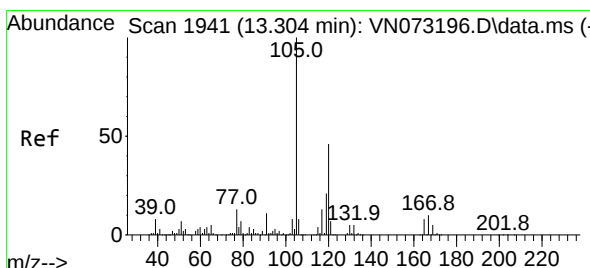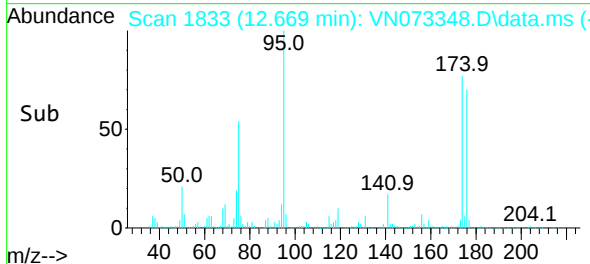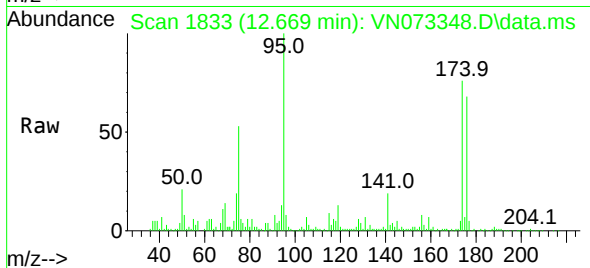

#84
1,2,4-Trimethylbenzene
Concen: 2.681 ug/l
RT: 13.304 min Scan# 1941
Delta R.T. -0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 105 Resp: 56286
Ion Ratio Lower Upper
105 100
120 29.7 23.3 69.8


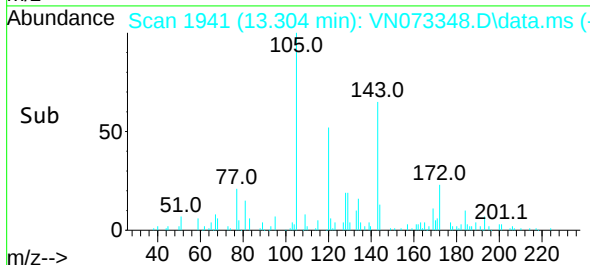

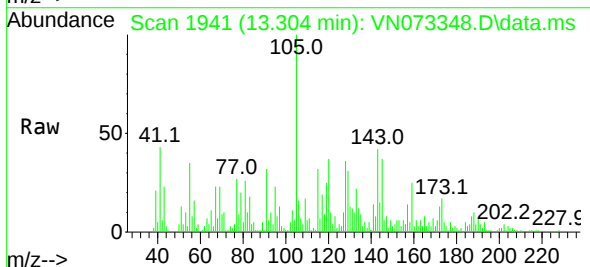


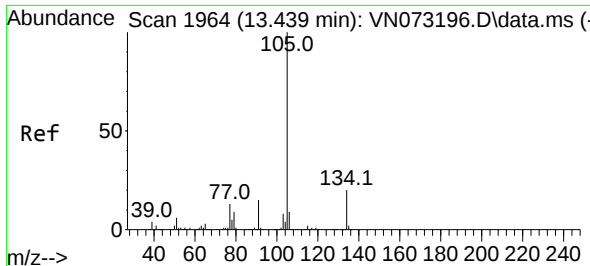

#85
 sec-Butylbenzene
 Concen: 0.346 ug/l
 RT: 13.439 min Scan# 1964
 Delta R.T. 0.000 min
 Lab File: VN073348.D
 Acq: 06 Jul 2022 16:25




Instrument :
 MSVOA_N
 ClientSampleId :
 31267


Tgt Ion:105 Resp: 8769
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

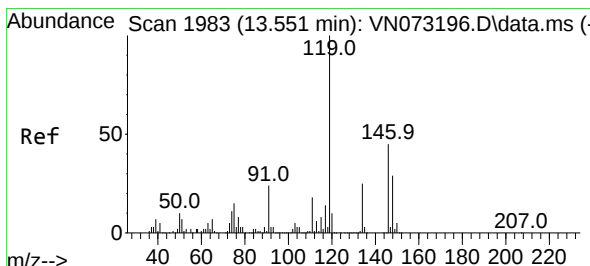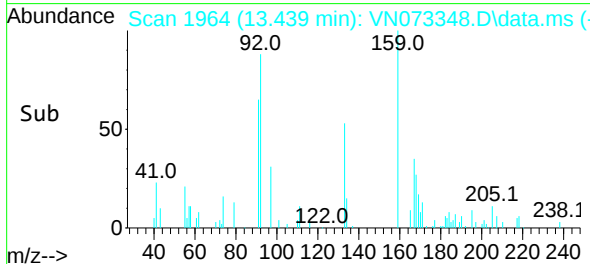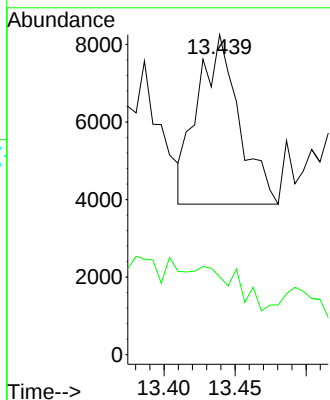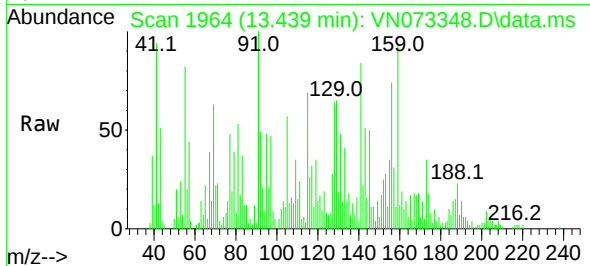

#86
 p-Isopropyltoluene
 Concen: 0.324 ug/l
 RT: 13.551 min Scan# 1983
 Delta R.T. -0.000 min
 Lab File: VN073348.D
 Acq: 06 Jul 2022 16:25

Tgt Ion:119 Resp: 6632
 Ion Ratio Lower Upper
 119 100
 134 0.0 13.3 39.8#
 91 0.0 11.3 33.9#

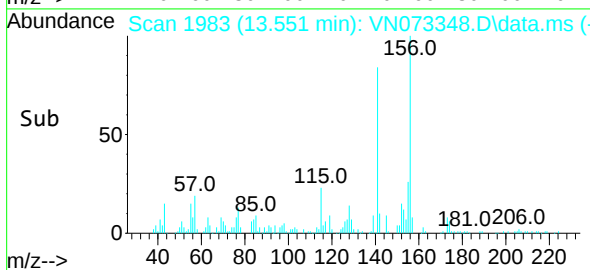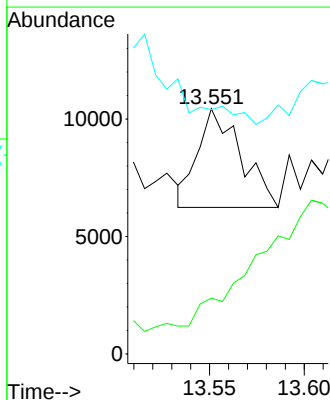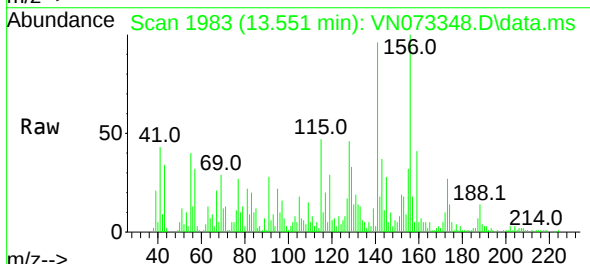



#87

1,3-Dichlorobenzene

Concen: 0.298 ug/l

RT: 13.539 min Scan# 1983

Delta R.T. -0.012 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25

Instrument :

MSVOA_N

ClientSampleId :

31267





Tgt Ion:146 Resp: 3202

Ion Ratio Lower Upper

146 100

111 0.0 20.0 60.0#

148 9.4 32.0 96.0#

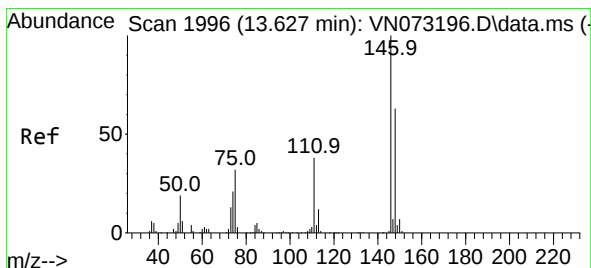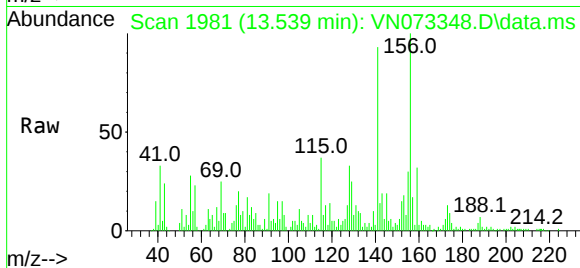

#88

1,4-Dichlorobenzene

Concen: 0.370 ug/l

RT: 13.651 min Scan# 2000

Delta R.T. 0.024 min

Lab File: VN073348.D

Acq: 06 Jul 2022 16:25




Tgt Ion:146 Resp: 3993


Ion Ratio Lower Upper

146 100

111 0.0 19.1 57.1#

148 0.0 31.4 94.3#


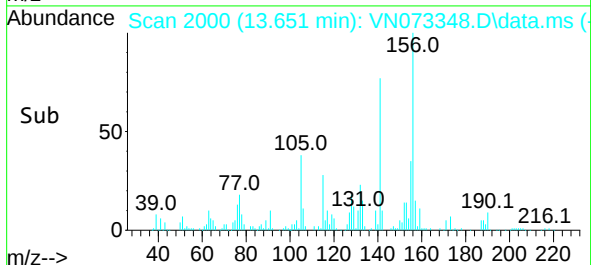
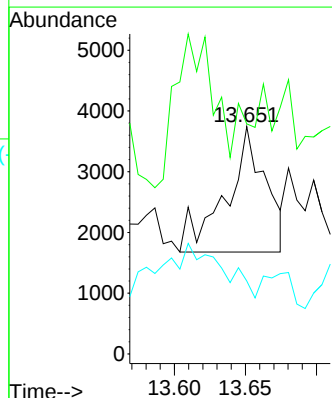
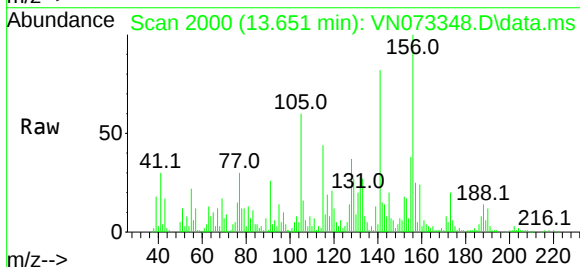




#89
n-Butylbenzene
Concen: 0.428 ug/l
RT: 13.880 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 91 Resp: 7289
Ion Ratio Lower Upper
91 100
92 174.5 26.9 80.7#
134 0.0 13.6 40.8#

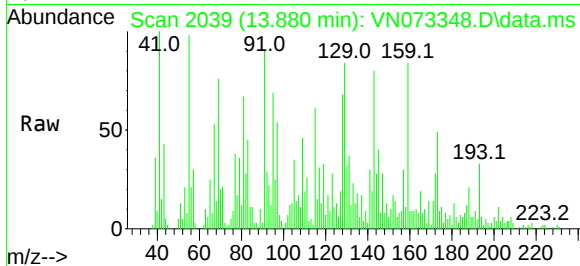

#90
Hexachloroethane
Concen: 0.406 ug/l
RT: 14.310 min Scan# 2112
Delta R.T. 0.165 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 117 Resp: 1546
Ion Ratio Lower Upper
117 100
201 53.0 40.6 122.0


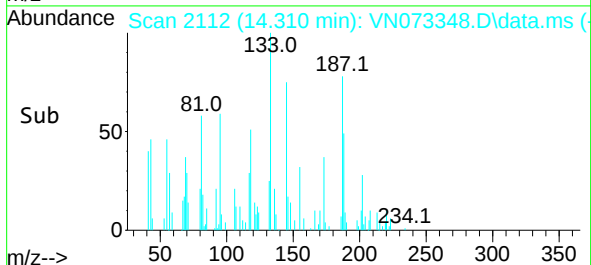

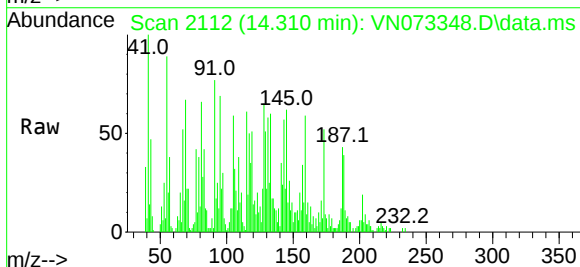


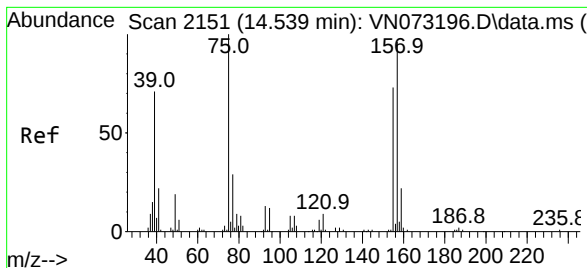

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.325 ug/l
RT: 14.568 min Scan# 2156
Delta R.T. 0.029 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25




Instrument :
MSVOA_N
ClientSampleId :
31267


Tgt Ion: 75 Resp: 677
Ion Ratio Lower Upper
75 100
155 0.0 44.9 134.5#
157 0.0 59.0 176.8#

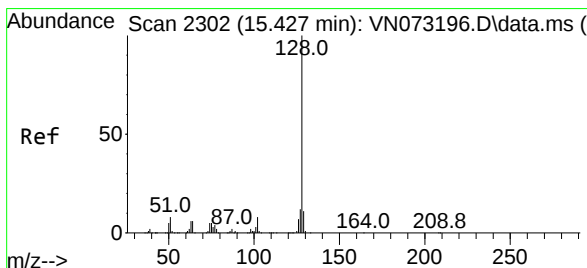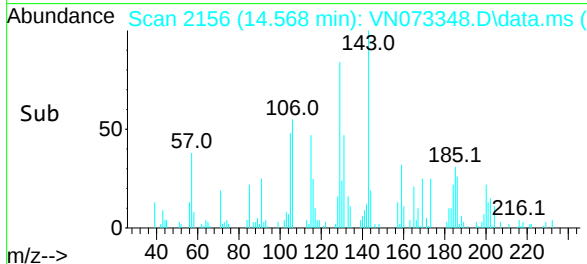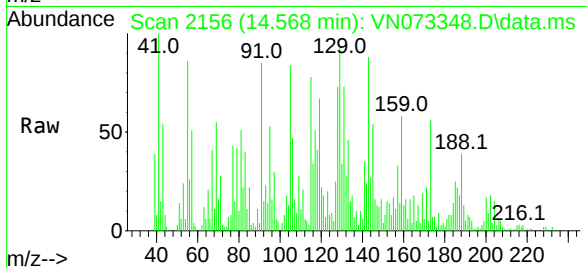

#95
Naphthalene
Concen: 2.104 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. 0.006 min
Lab File: VN073348.D
Acq: 06 Jul 2022 16:25

Tgt Ion: 128 Resp: 48451
Ion Ratio Lower Upper
128 100
127 26.2 10.3 15.5#
129 72.8 8.6 13.0#

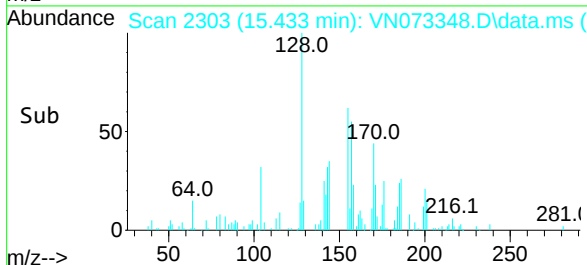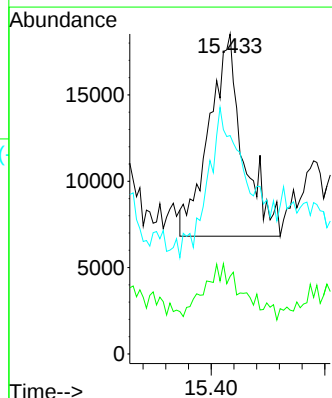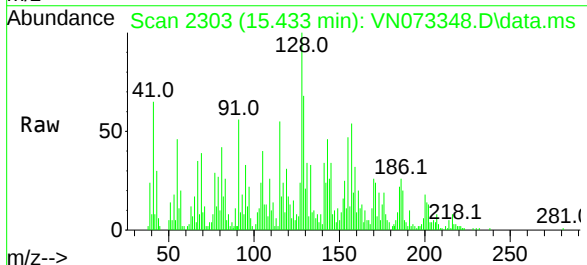

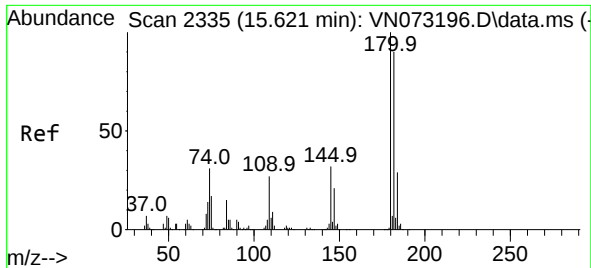

#96
 1,2,3-Trichlorobenzene
 Concen: 0.211 ug/l
 RT: 15.615 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN073348.D
 Acq: 06 Jul 2022 16:25

Instrument :
 MSVOA_N
 ClientSampleId :
 31267

Tgt Ion:180 Resp: 1243
 Ion Ratio Lower Upper
 180 100
 182 210.1 47.8 143.3#
 145 679.6 15.5 46.5#

