


Bromomethane

Response Ratio

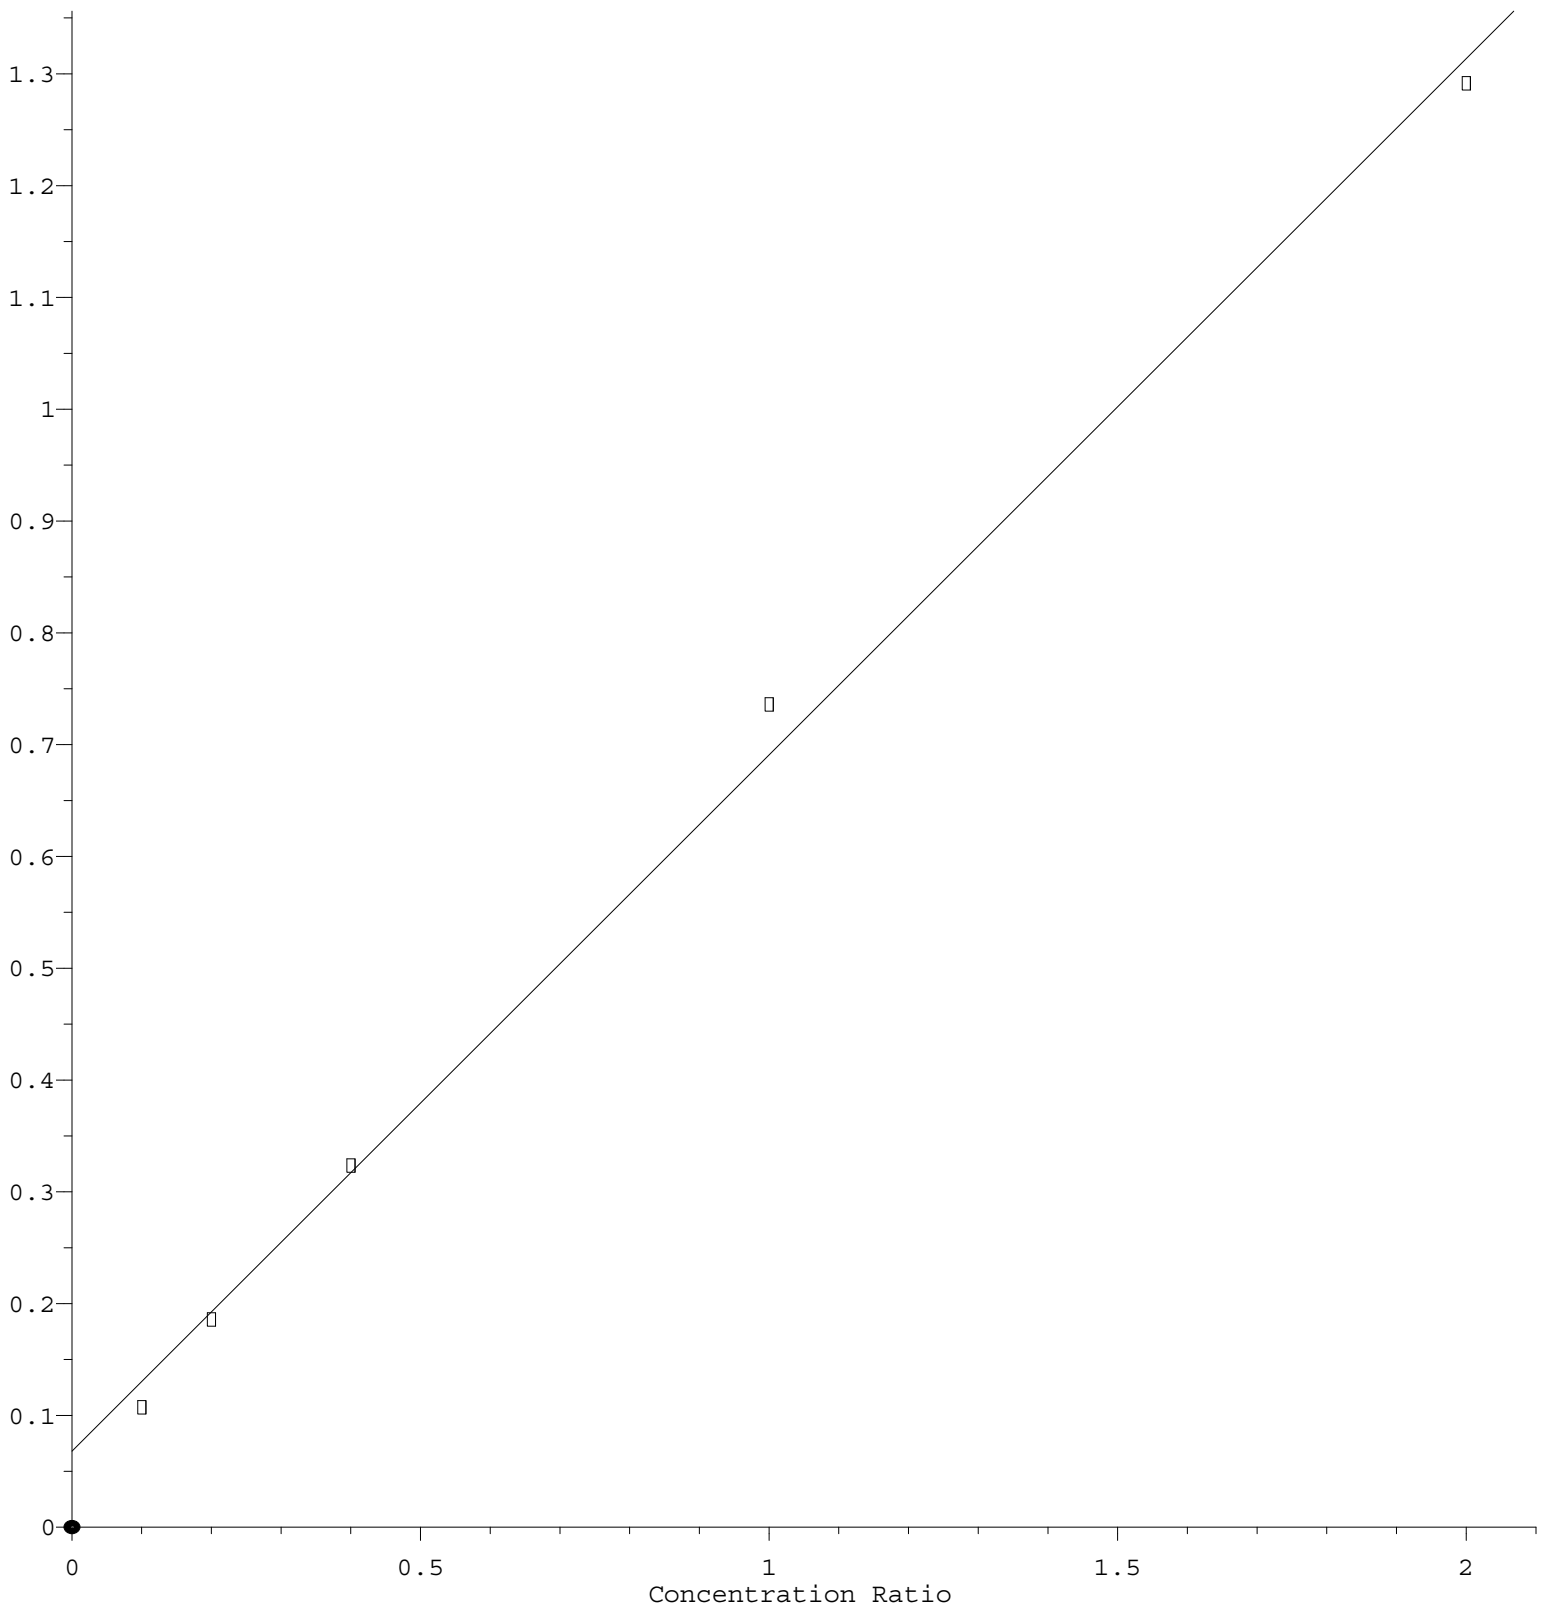

Response = 6.229e-001 * Amt + 6.784e-002


Coef of Det (r^2) = 0.996733 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

1,2,3-Trichlorobenzene

Response Ratio

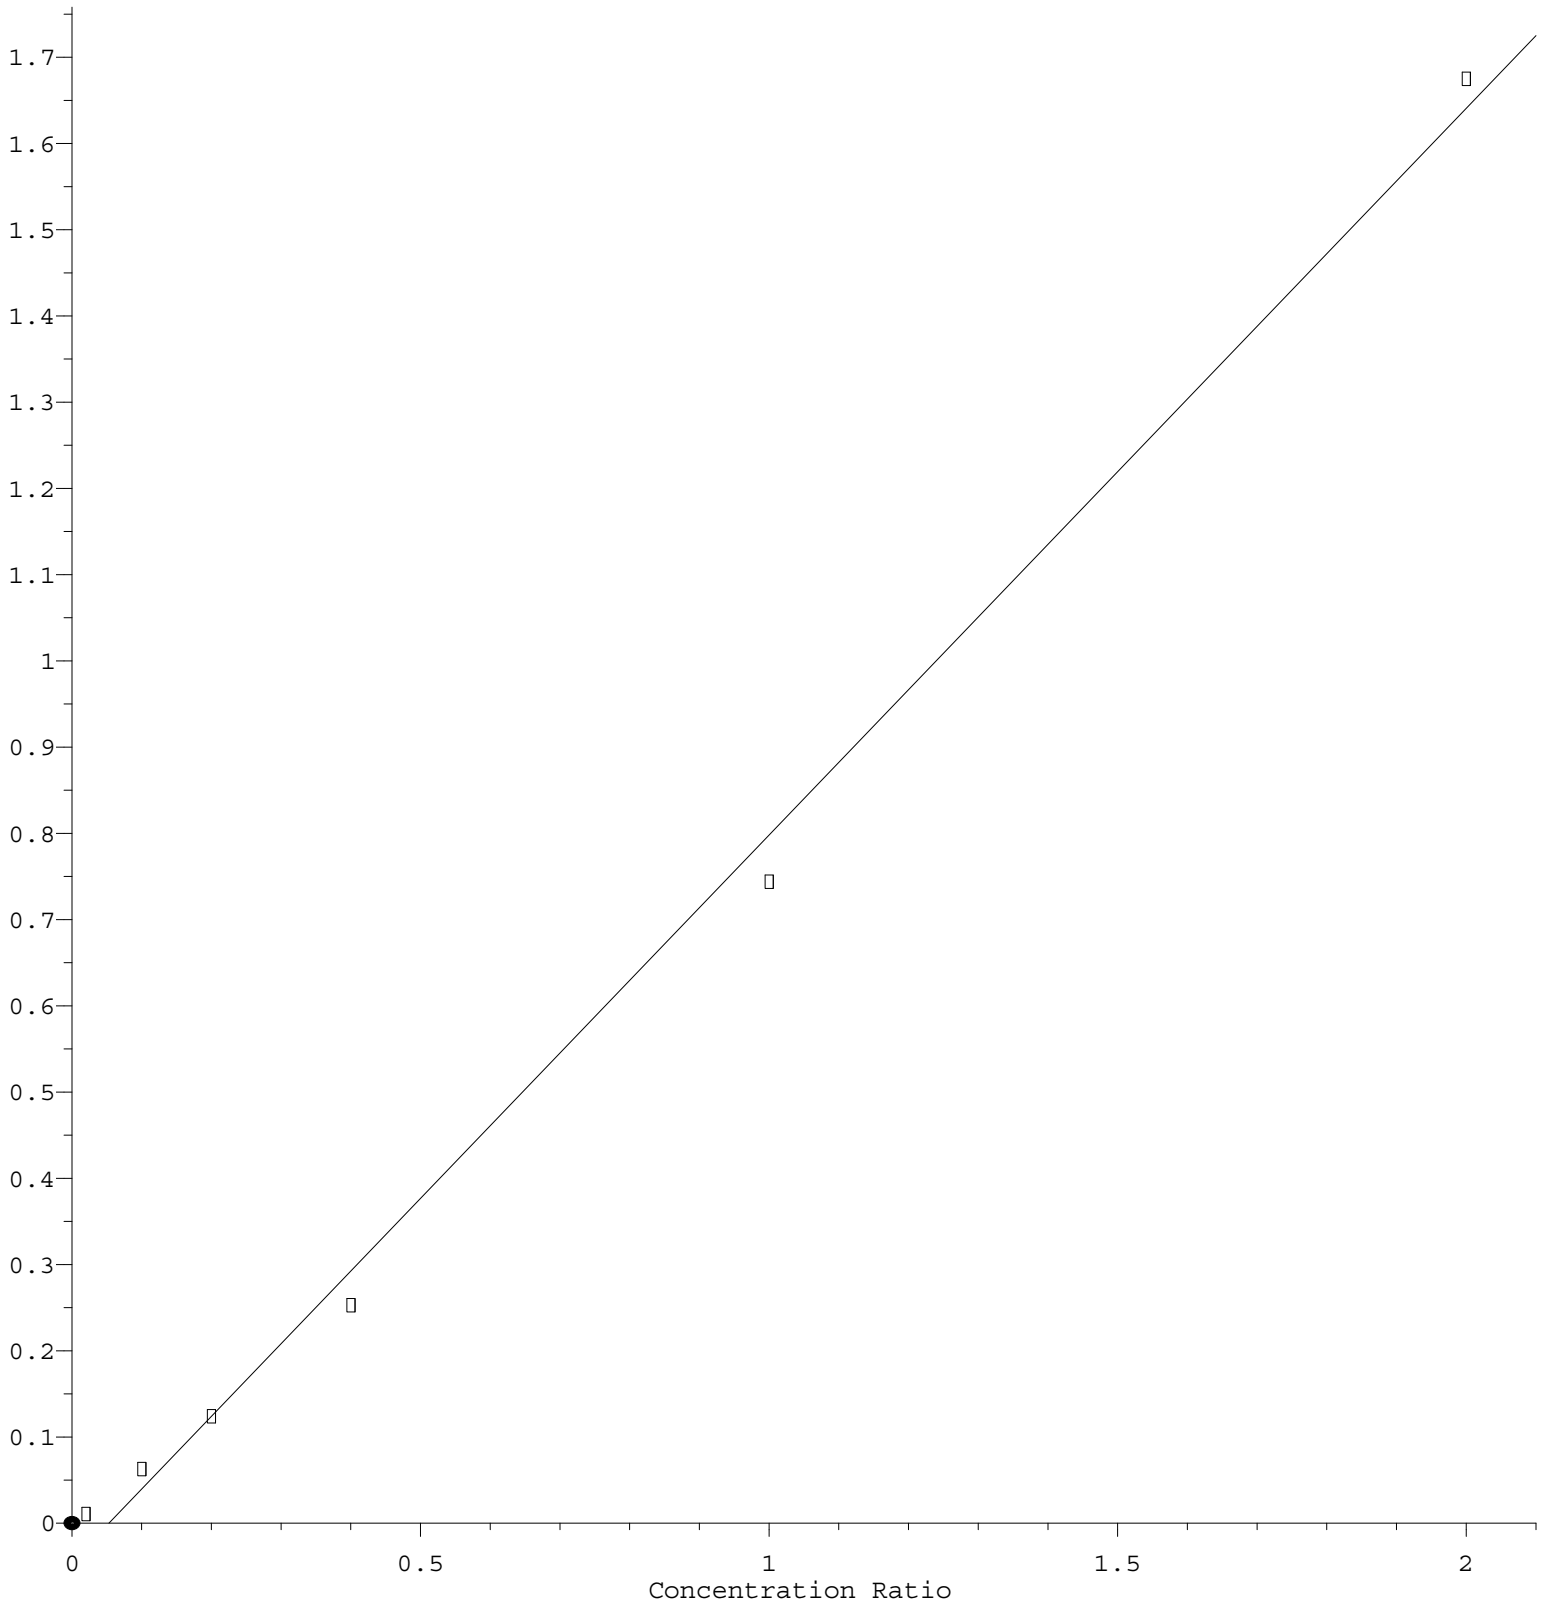

Response = $8.428e-001 * Amt - 4.437e-002$


Coef of Det (r^2) = 0.996293 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Chloroethane


Response Ratio

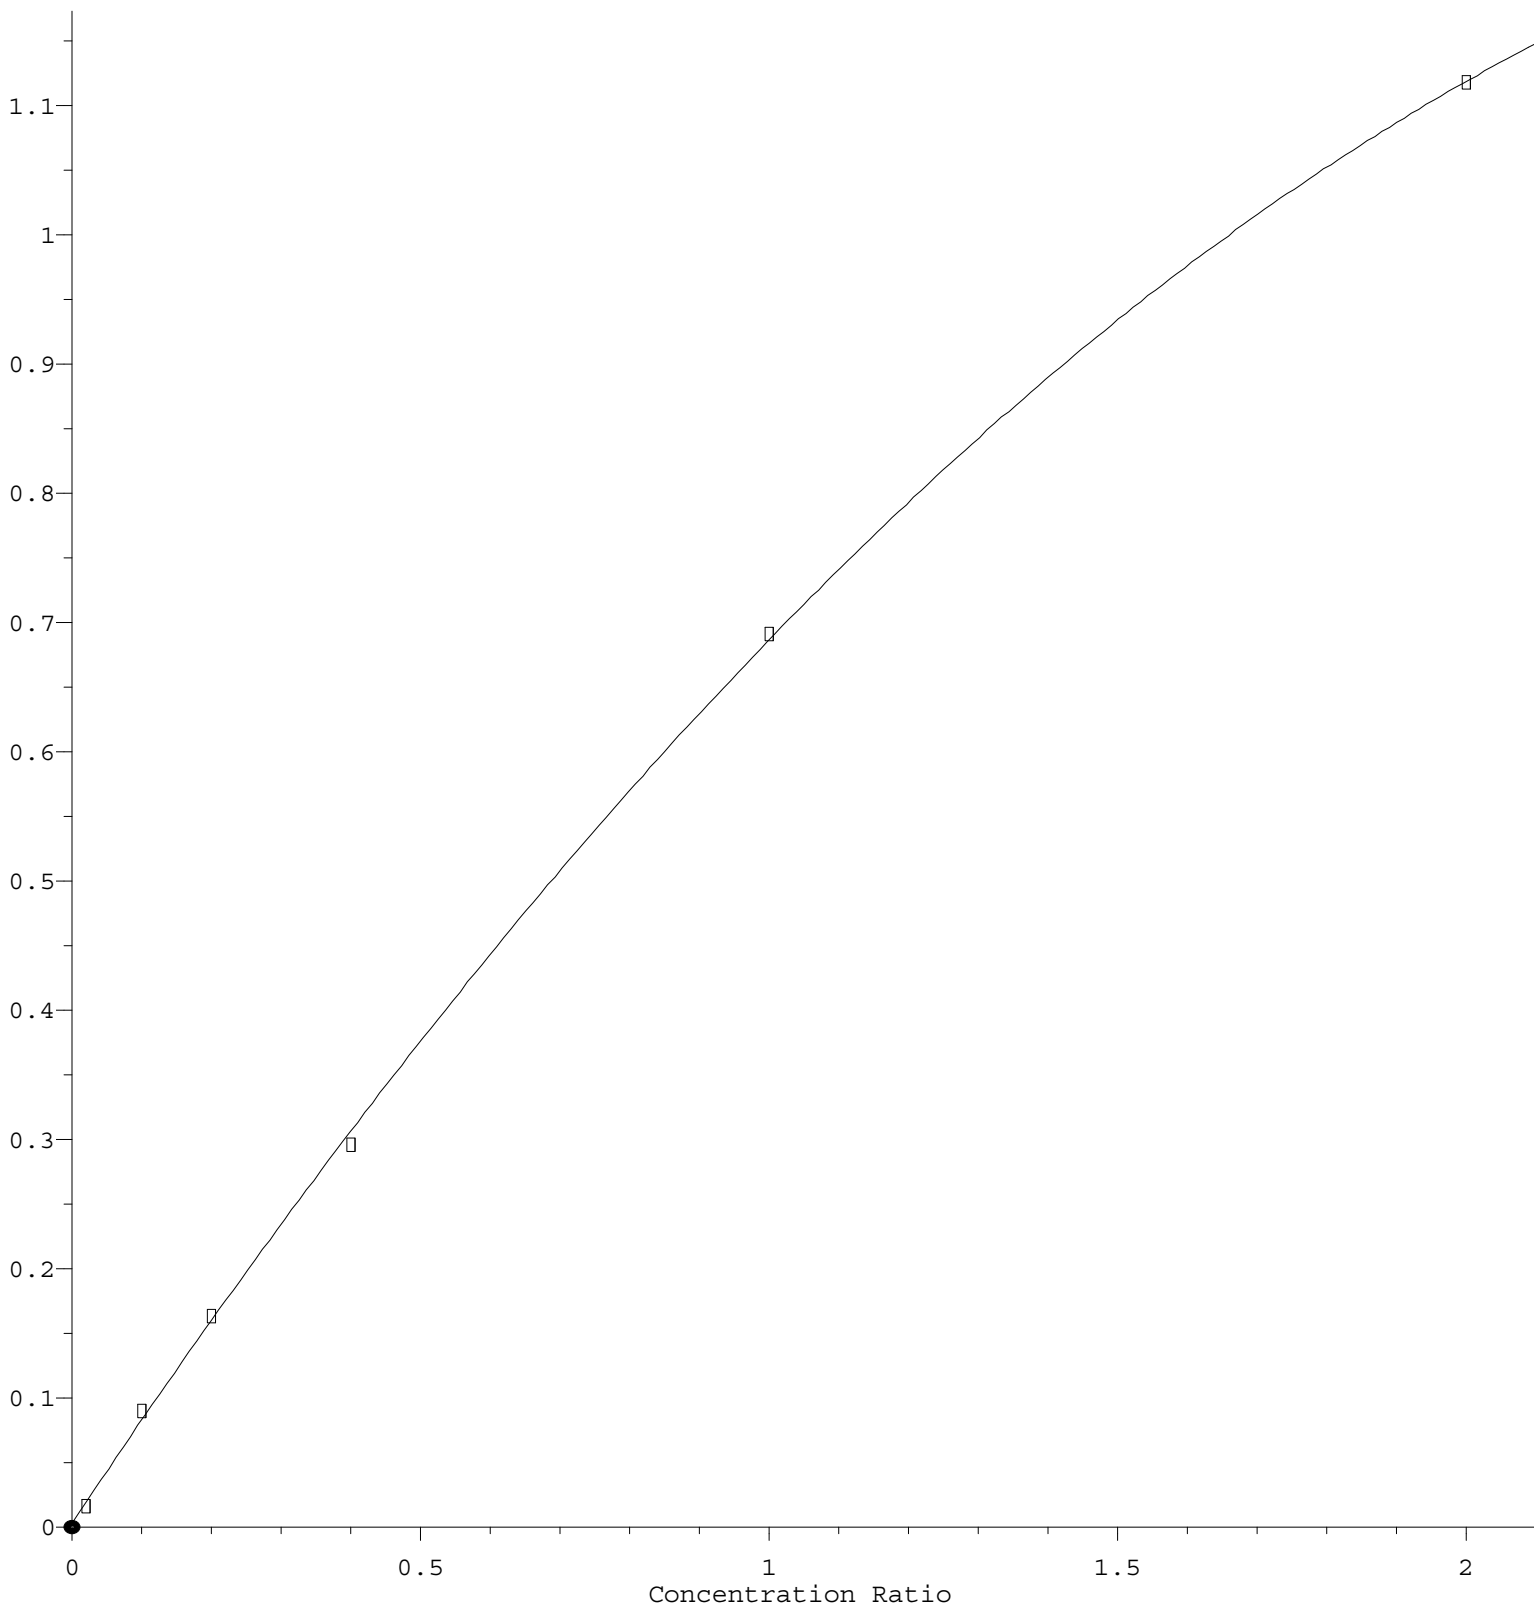

R = -1.256e-001 A*A + 8.088e-001 A + 3.303e-003
Coef of Det (r^2) = 0.999772 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M
Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Trichlorofluoromethane


Response Ratio

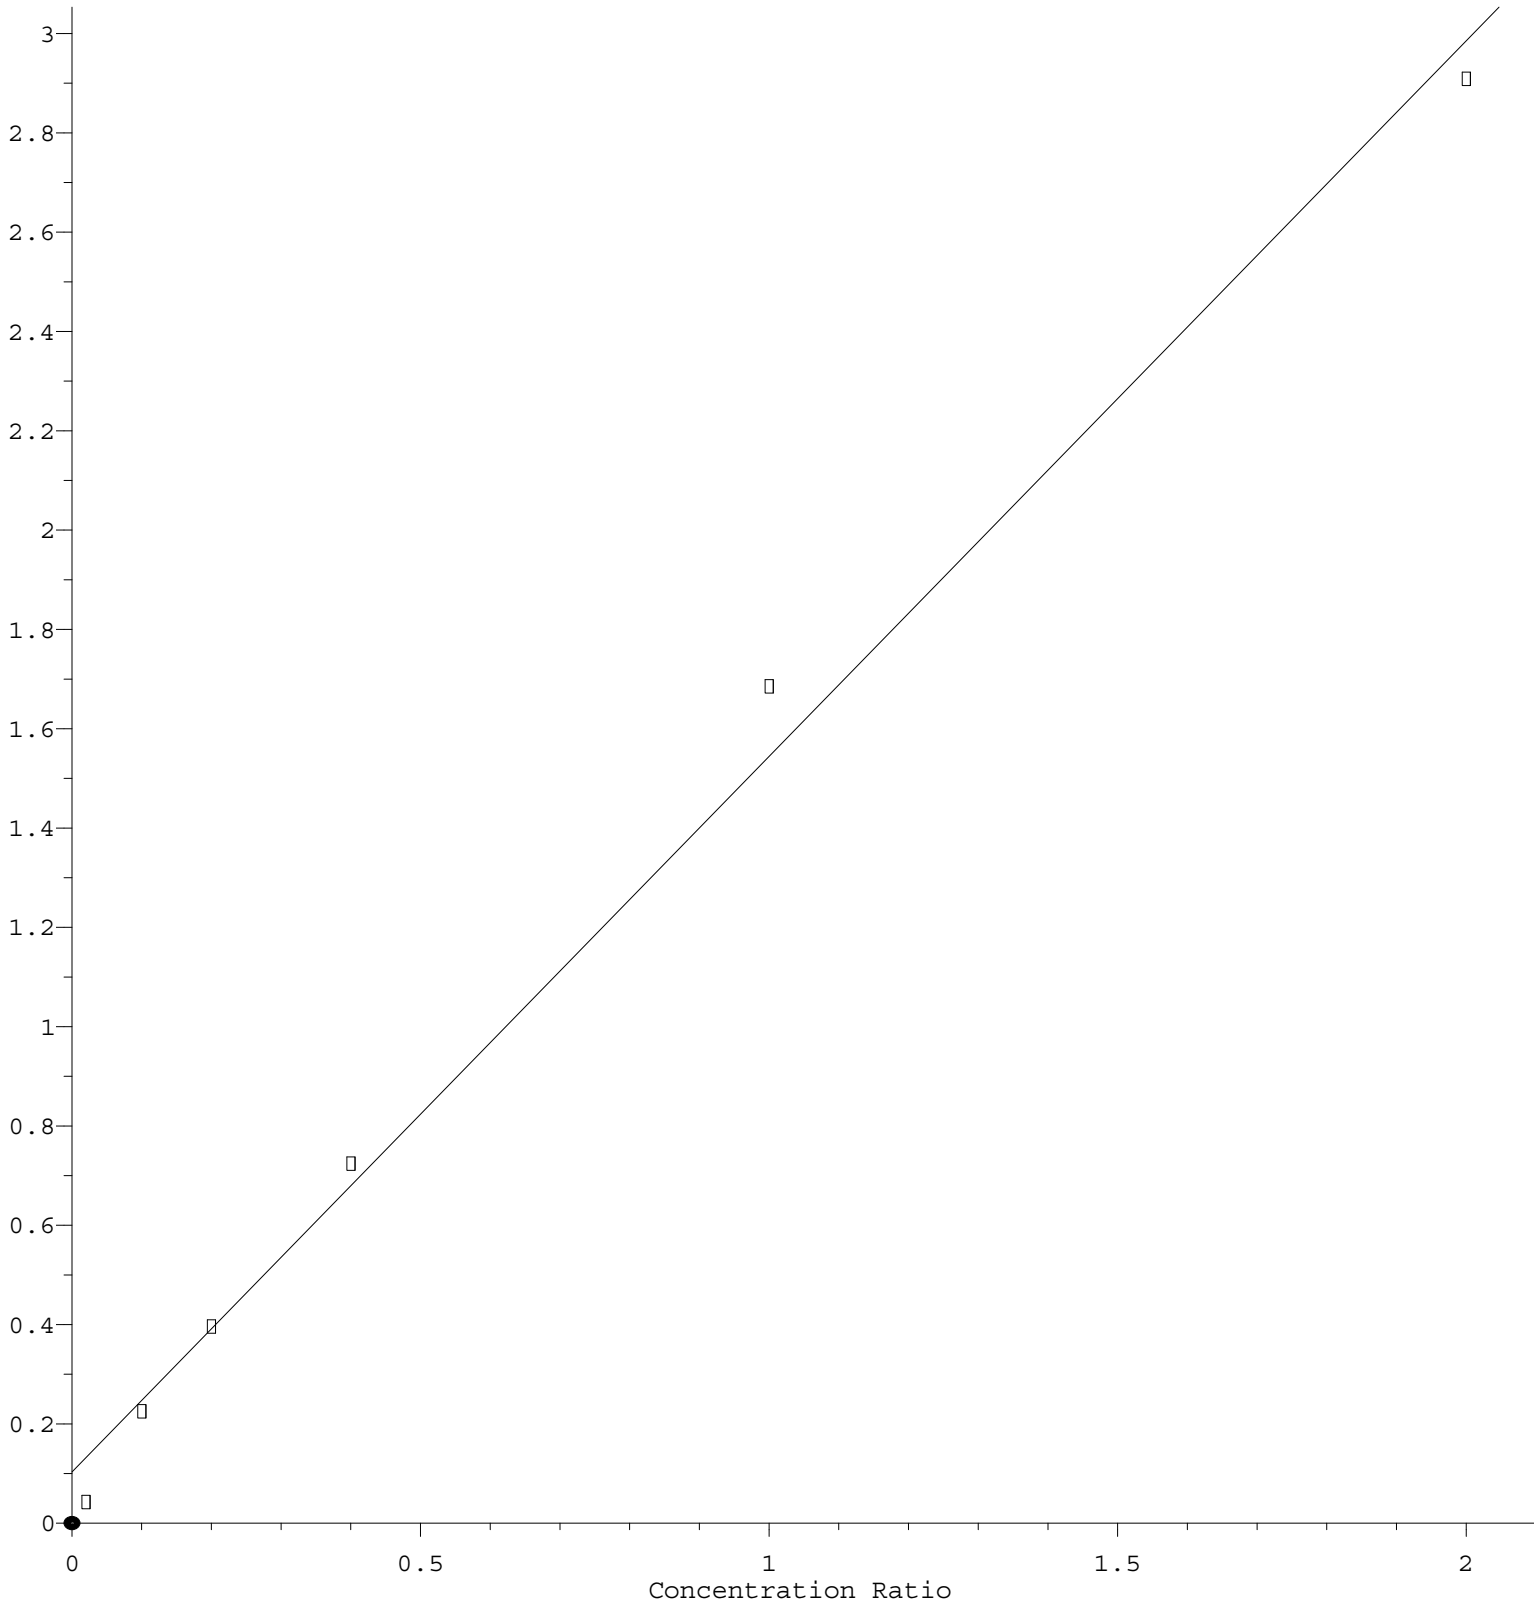

Response = 1.441e+000 * Amt + 1.032e-001
Coef of Det (r^2) = 0.994028 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M
Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Acrolein

Response Ratio

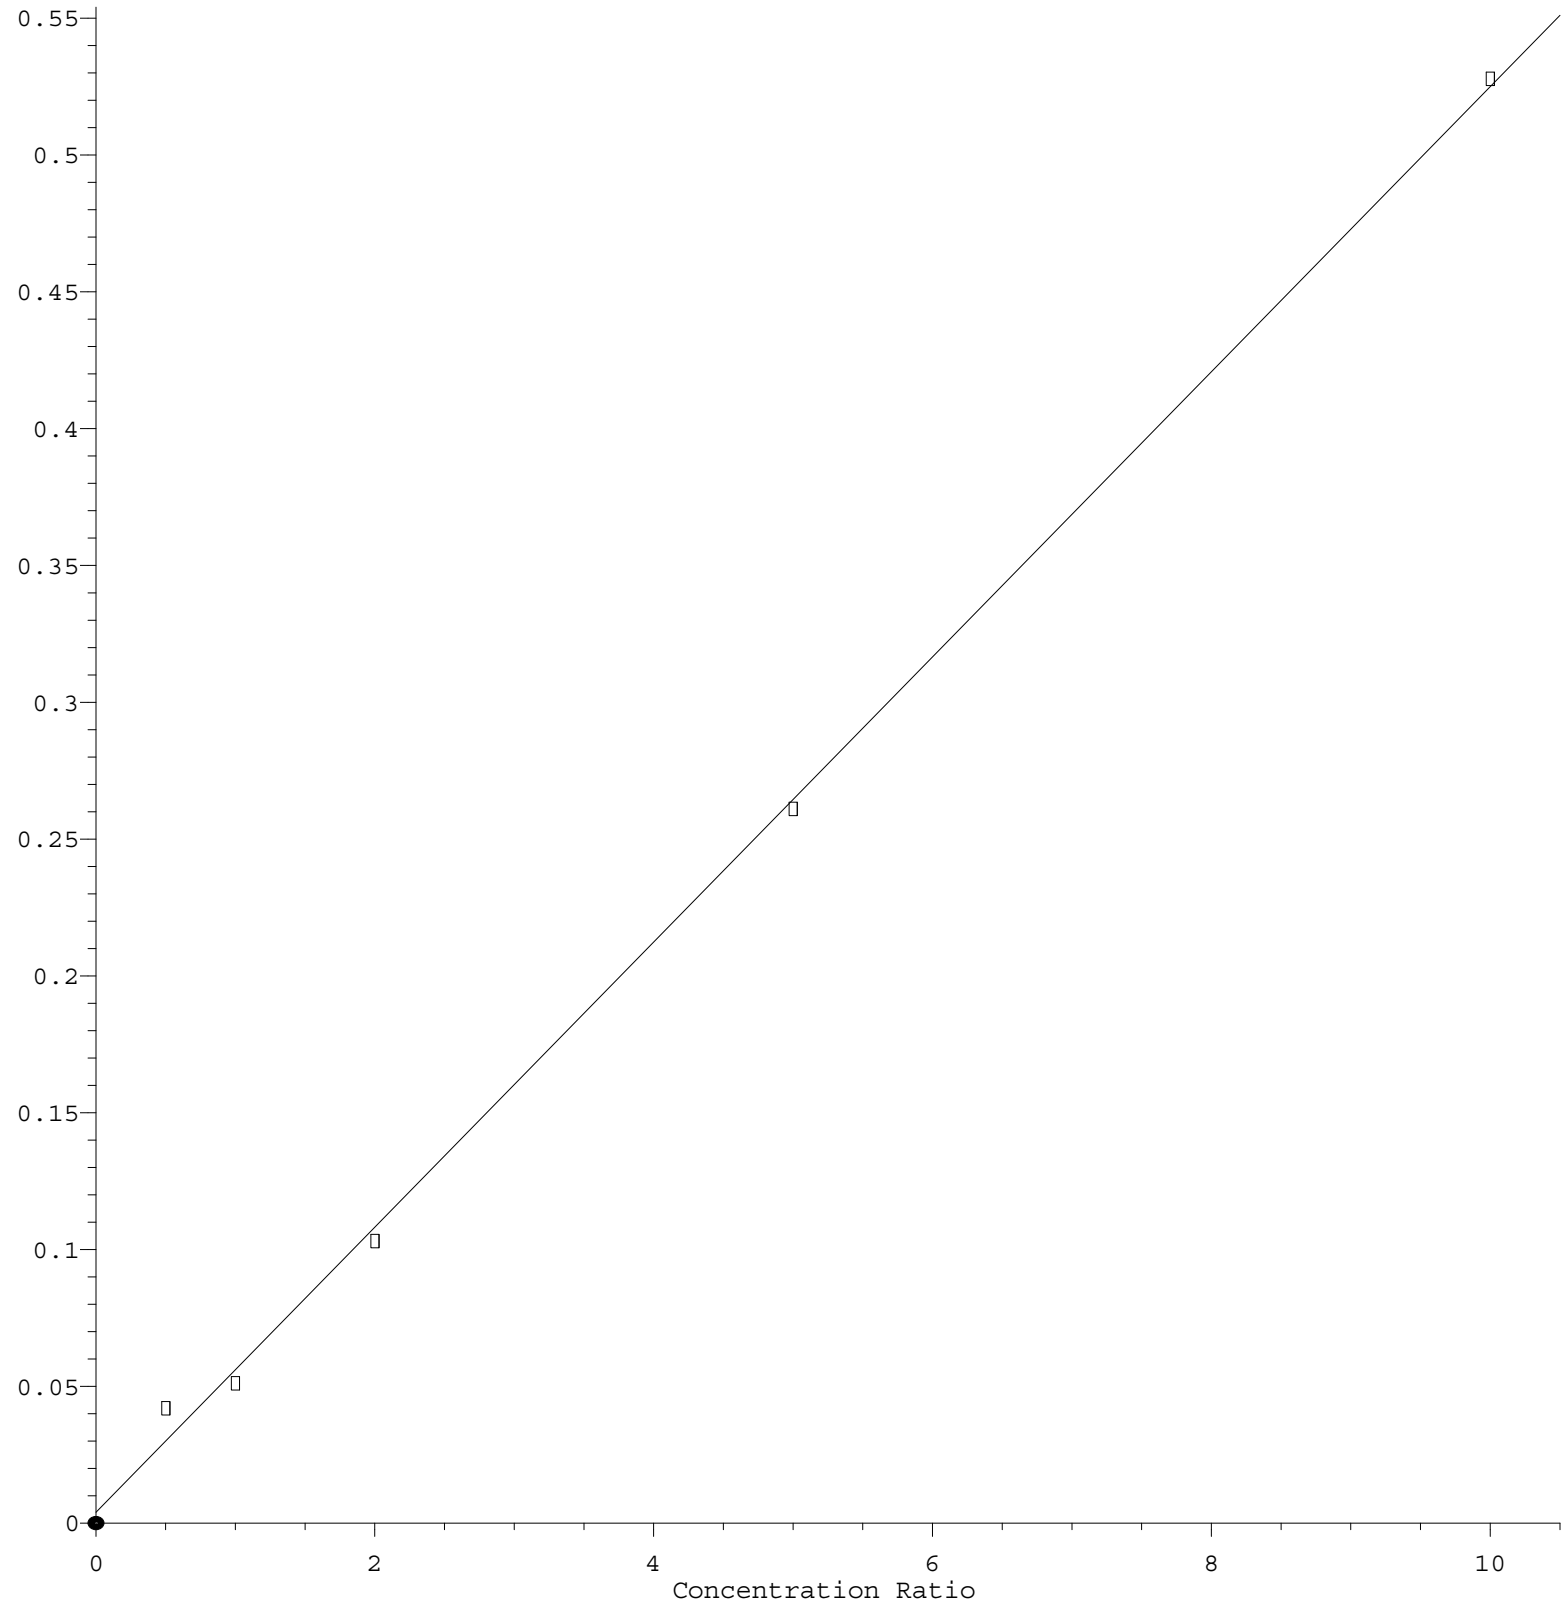

Response = 5.206e-002 * Amt + 4.397e-003


Coef of Det (r^2) = 0.998731 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Methylene Chloride

Response Ratio

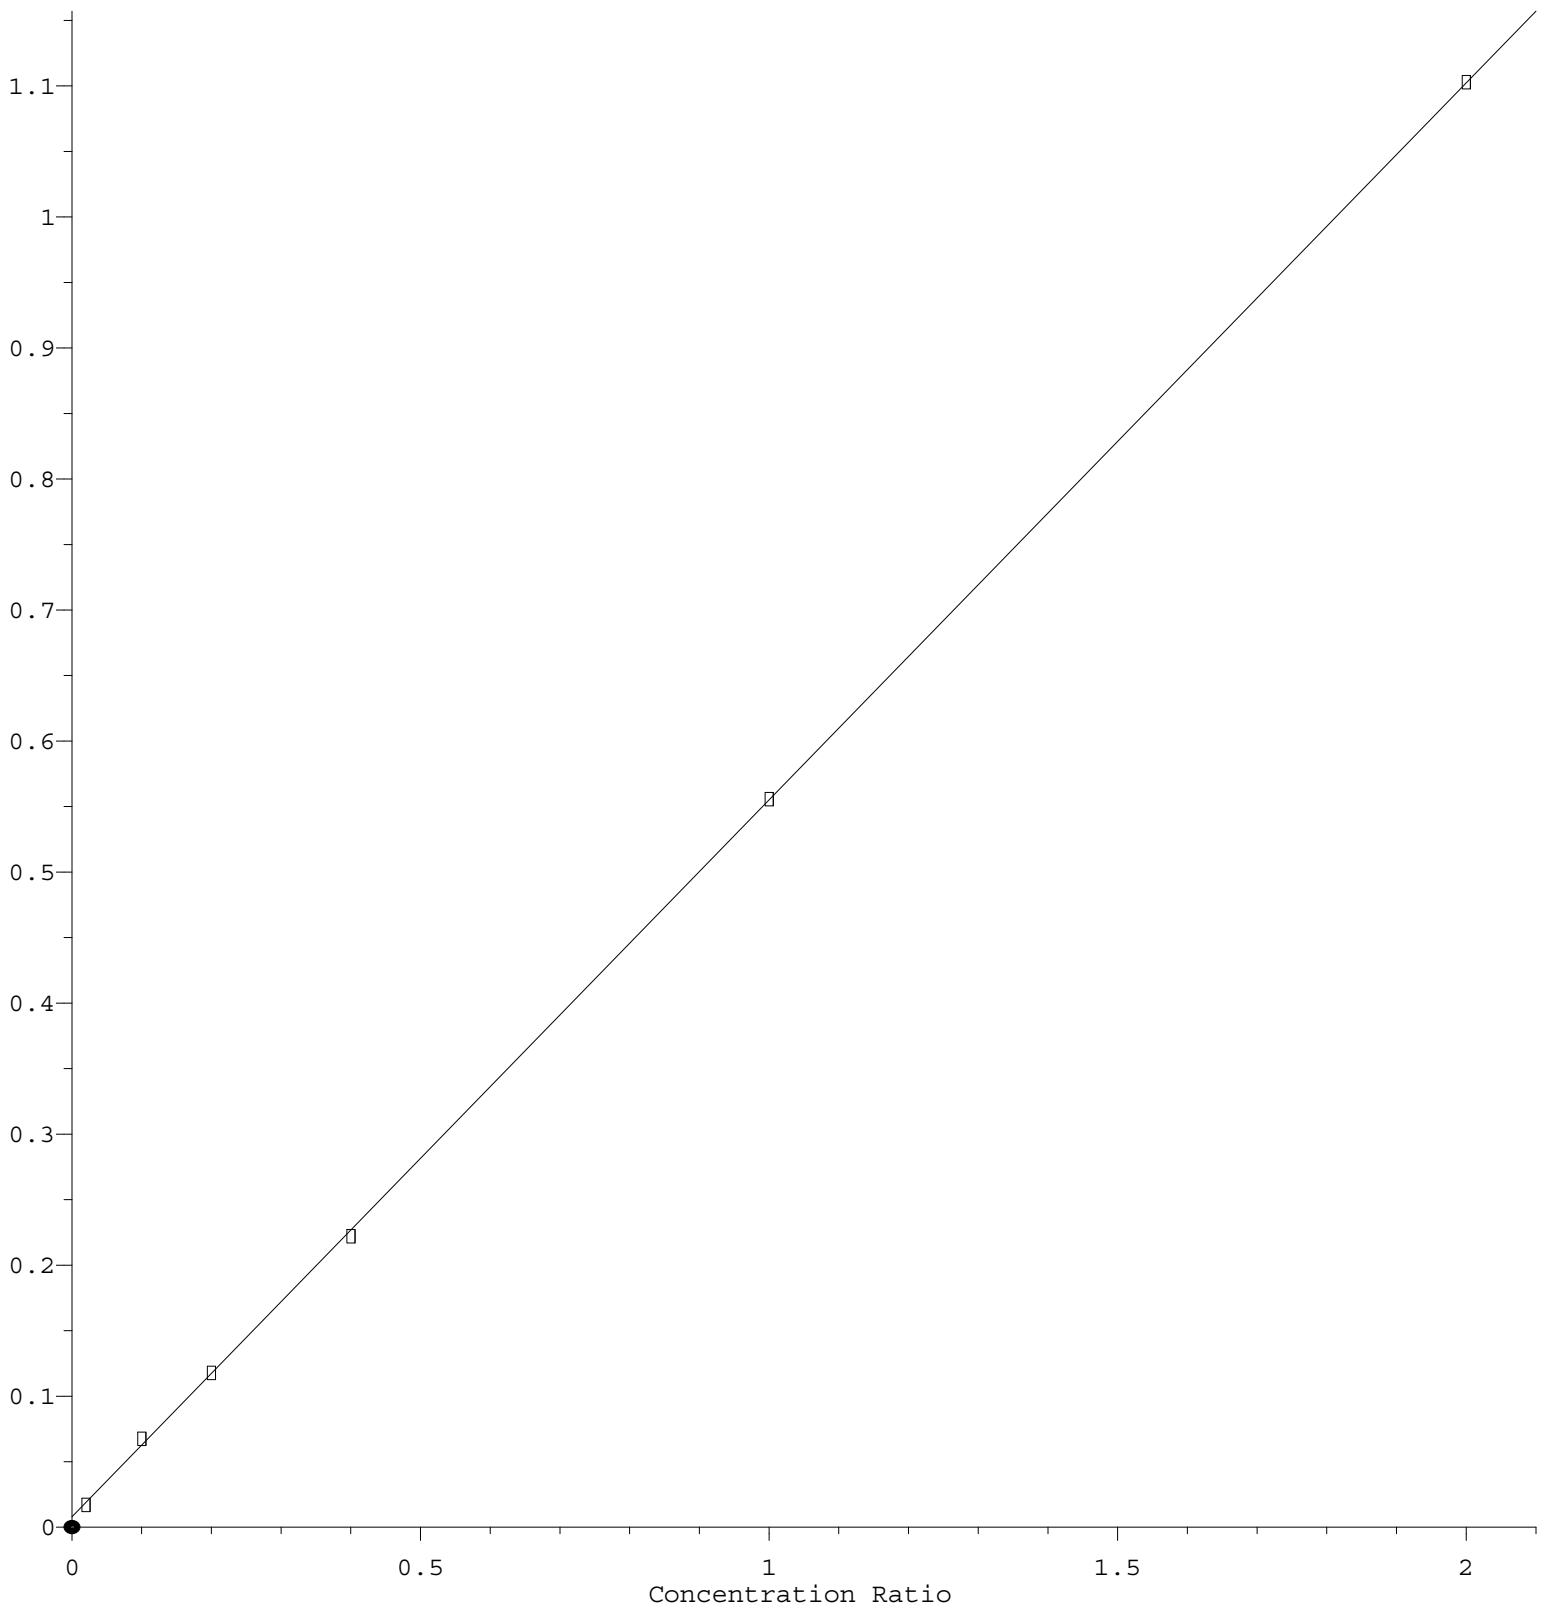

$$\text{Response} = 5.473\text{e-}001 * \text{Amt} + 7.726\text{e-}003$$


Coef of Det (r²) = 0.999943 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

1,4-Dioxane

Response Ratio

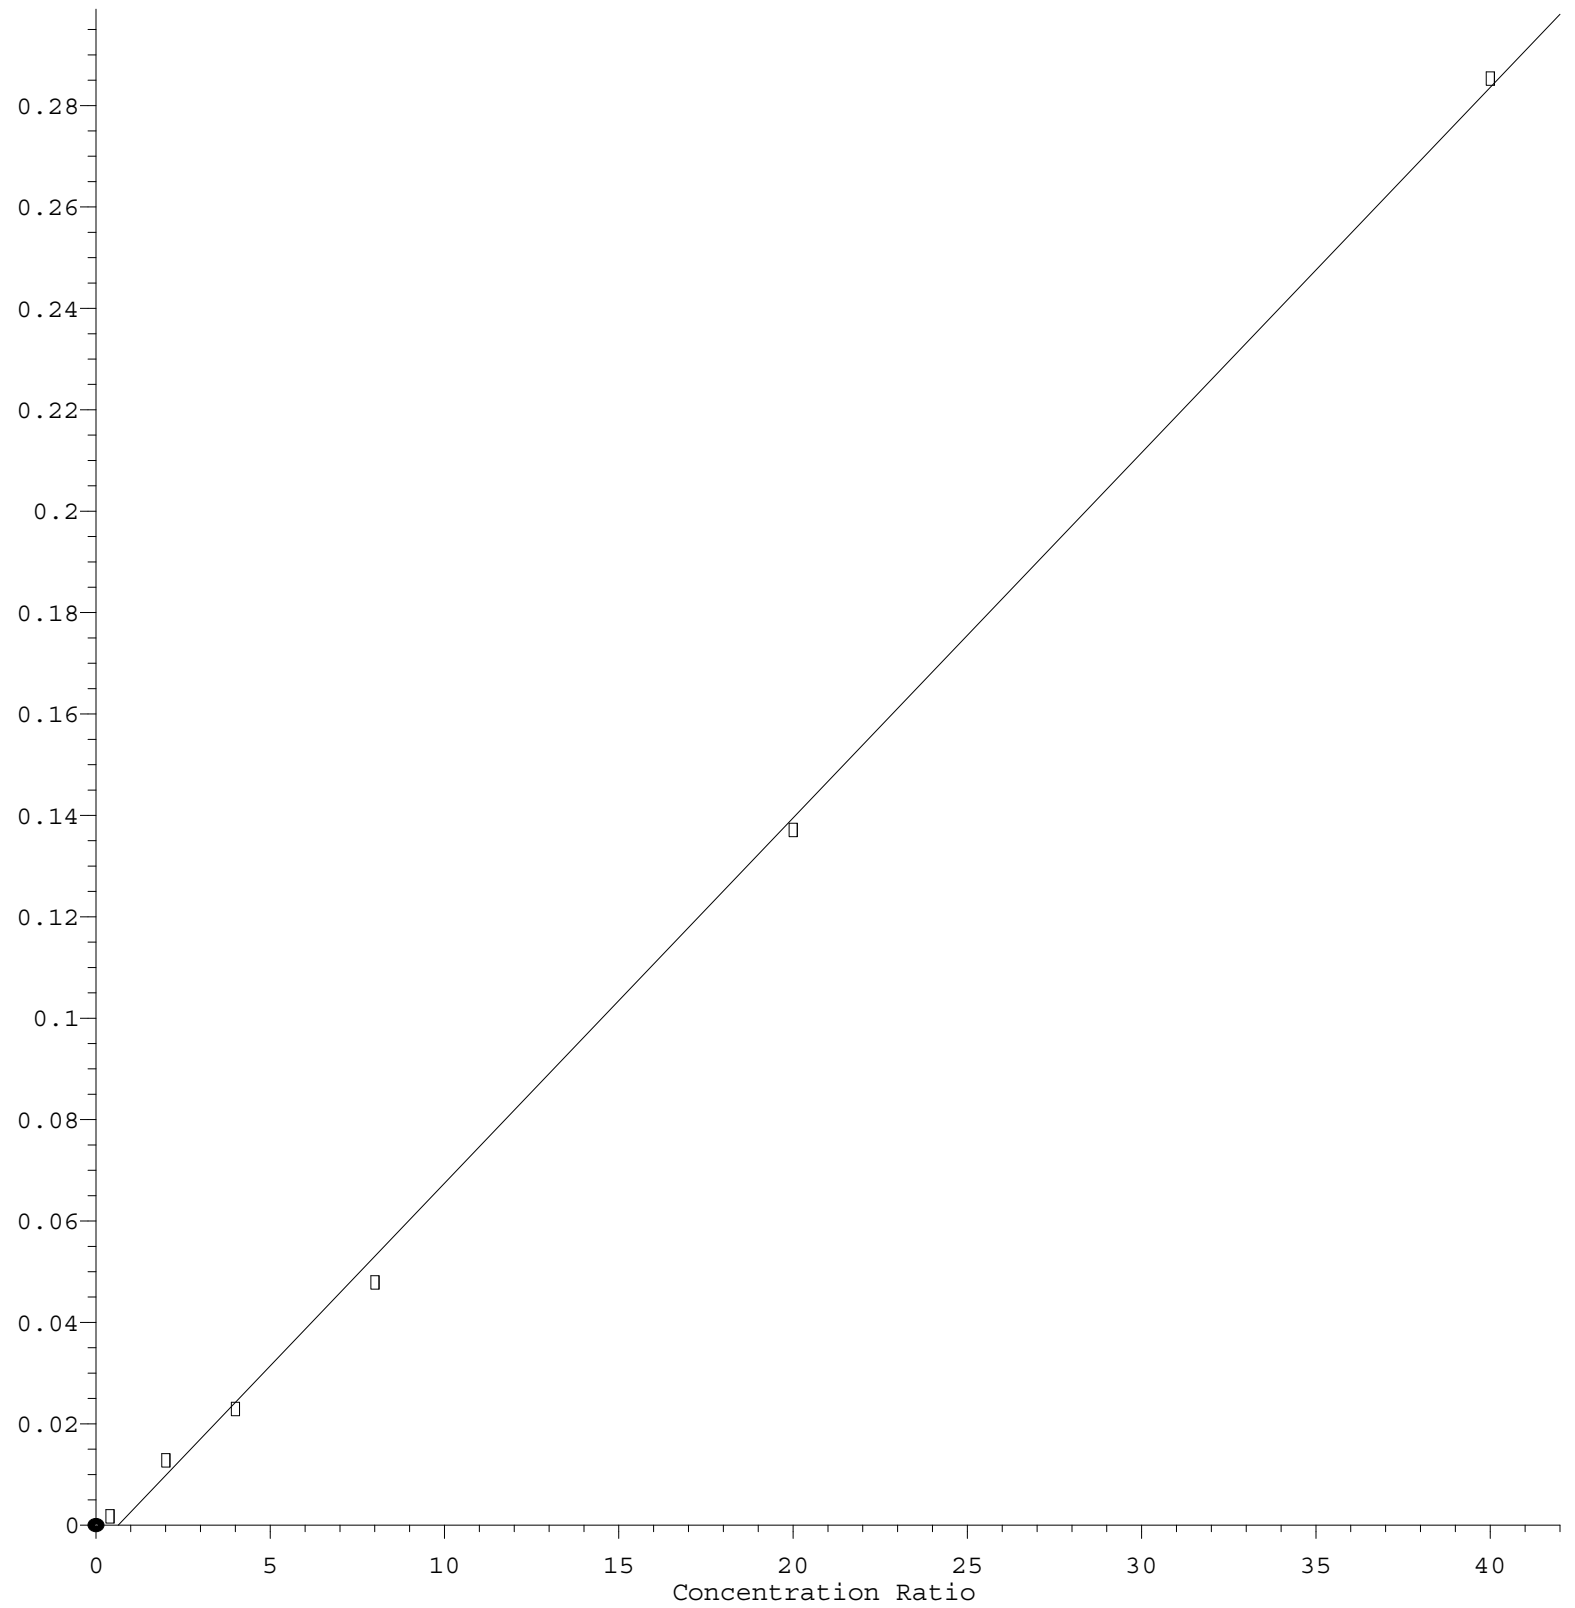

Response = $7.197e-003 * Amt - 4.625e-003$


Coef of Det (r^2) = 0.999042 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

t-1,3-Dichloropropene

Response Ratio

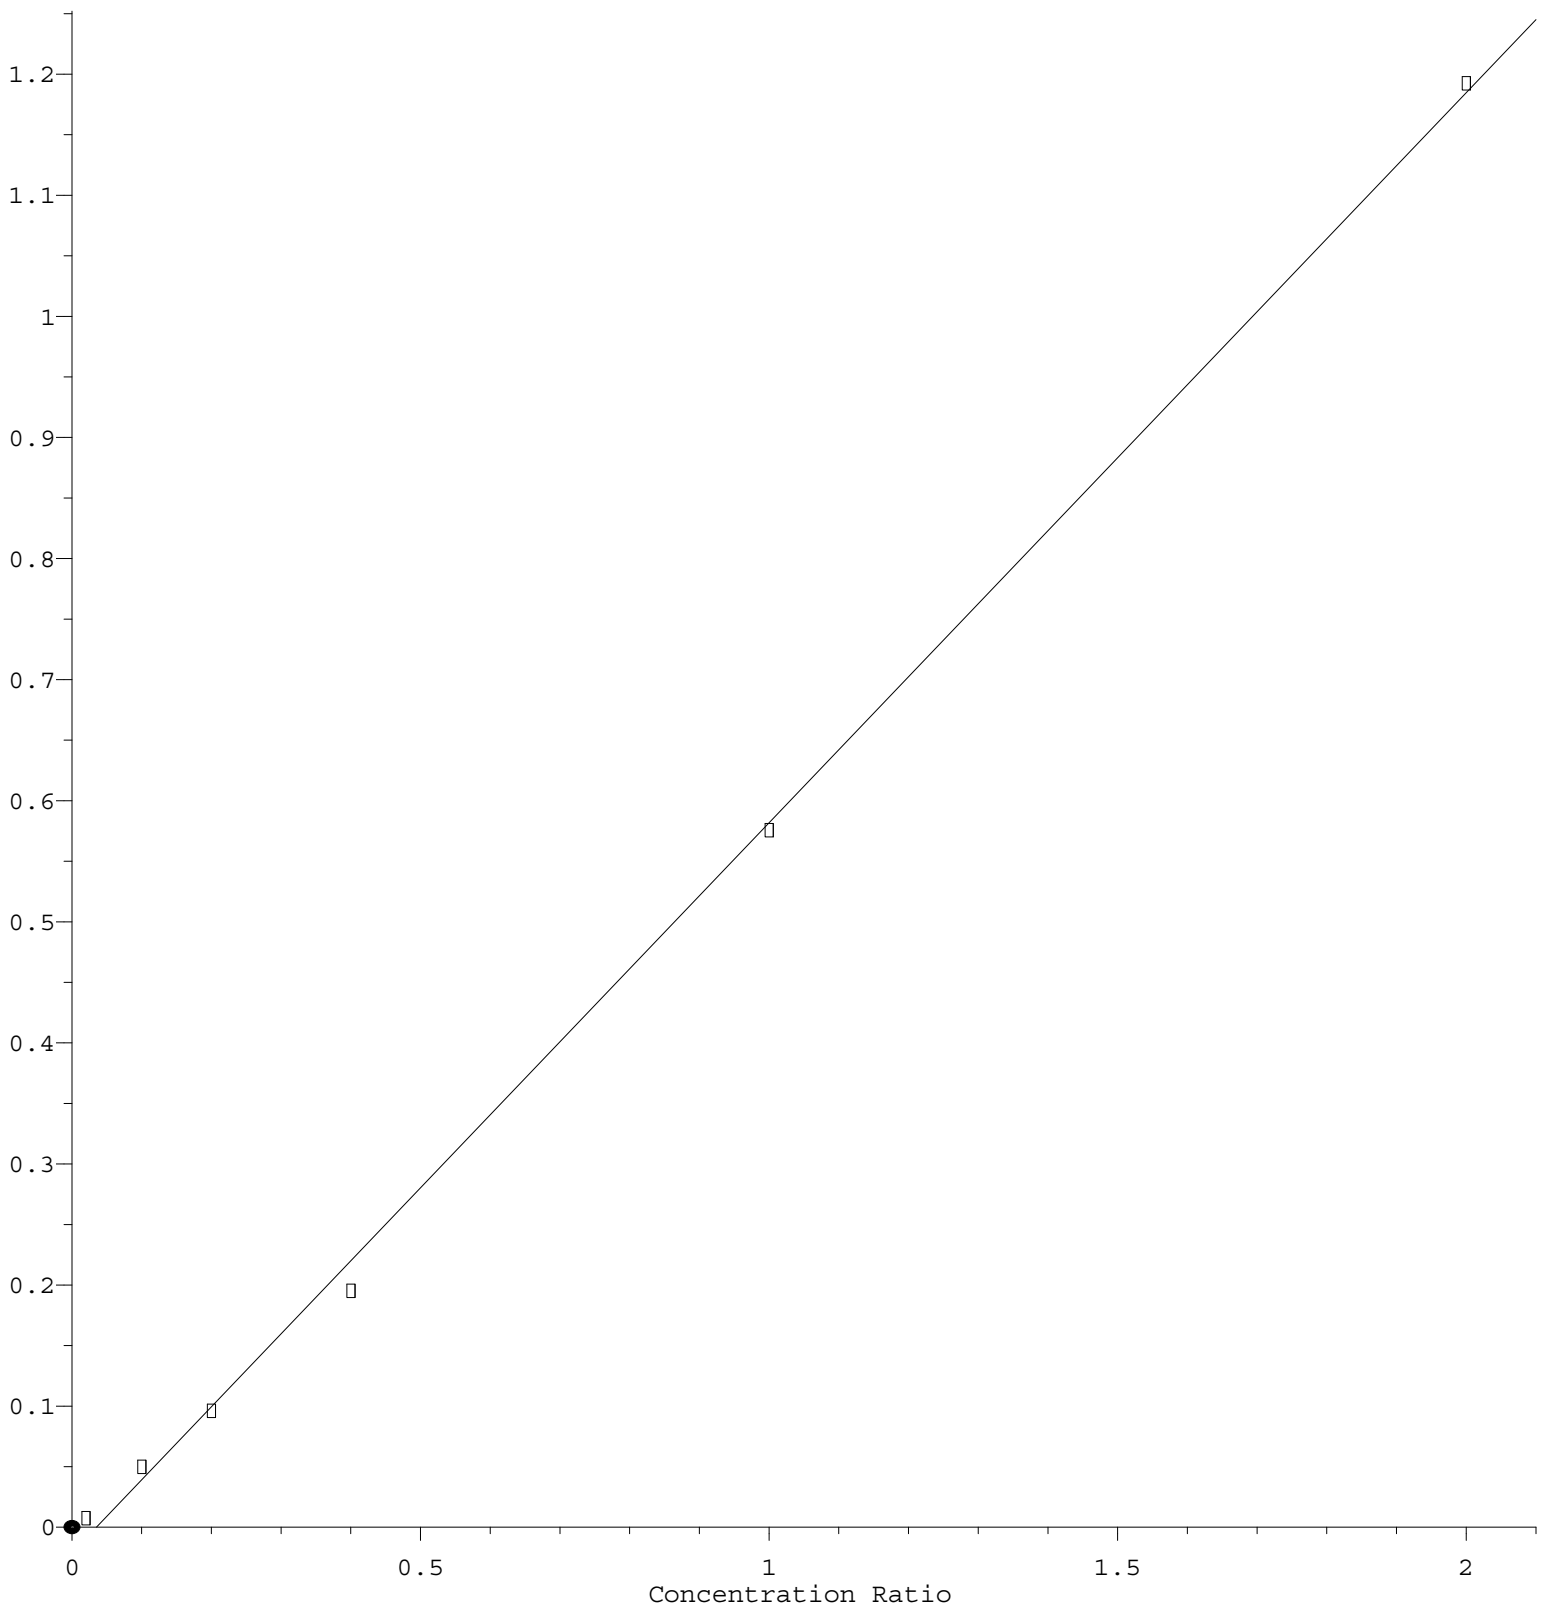

Response = 6.029e-001 * Amt - 2.103e-002


Coef of Det (r^2) = 0.998947 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

2-Chloroethyl Vinyl ether

Response Ratio

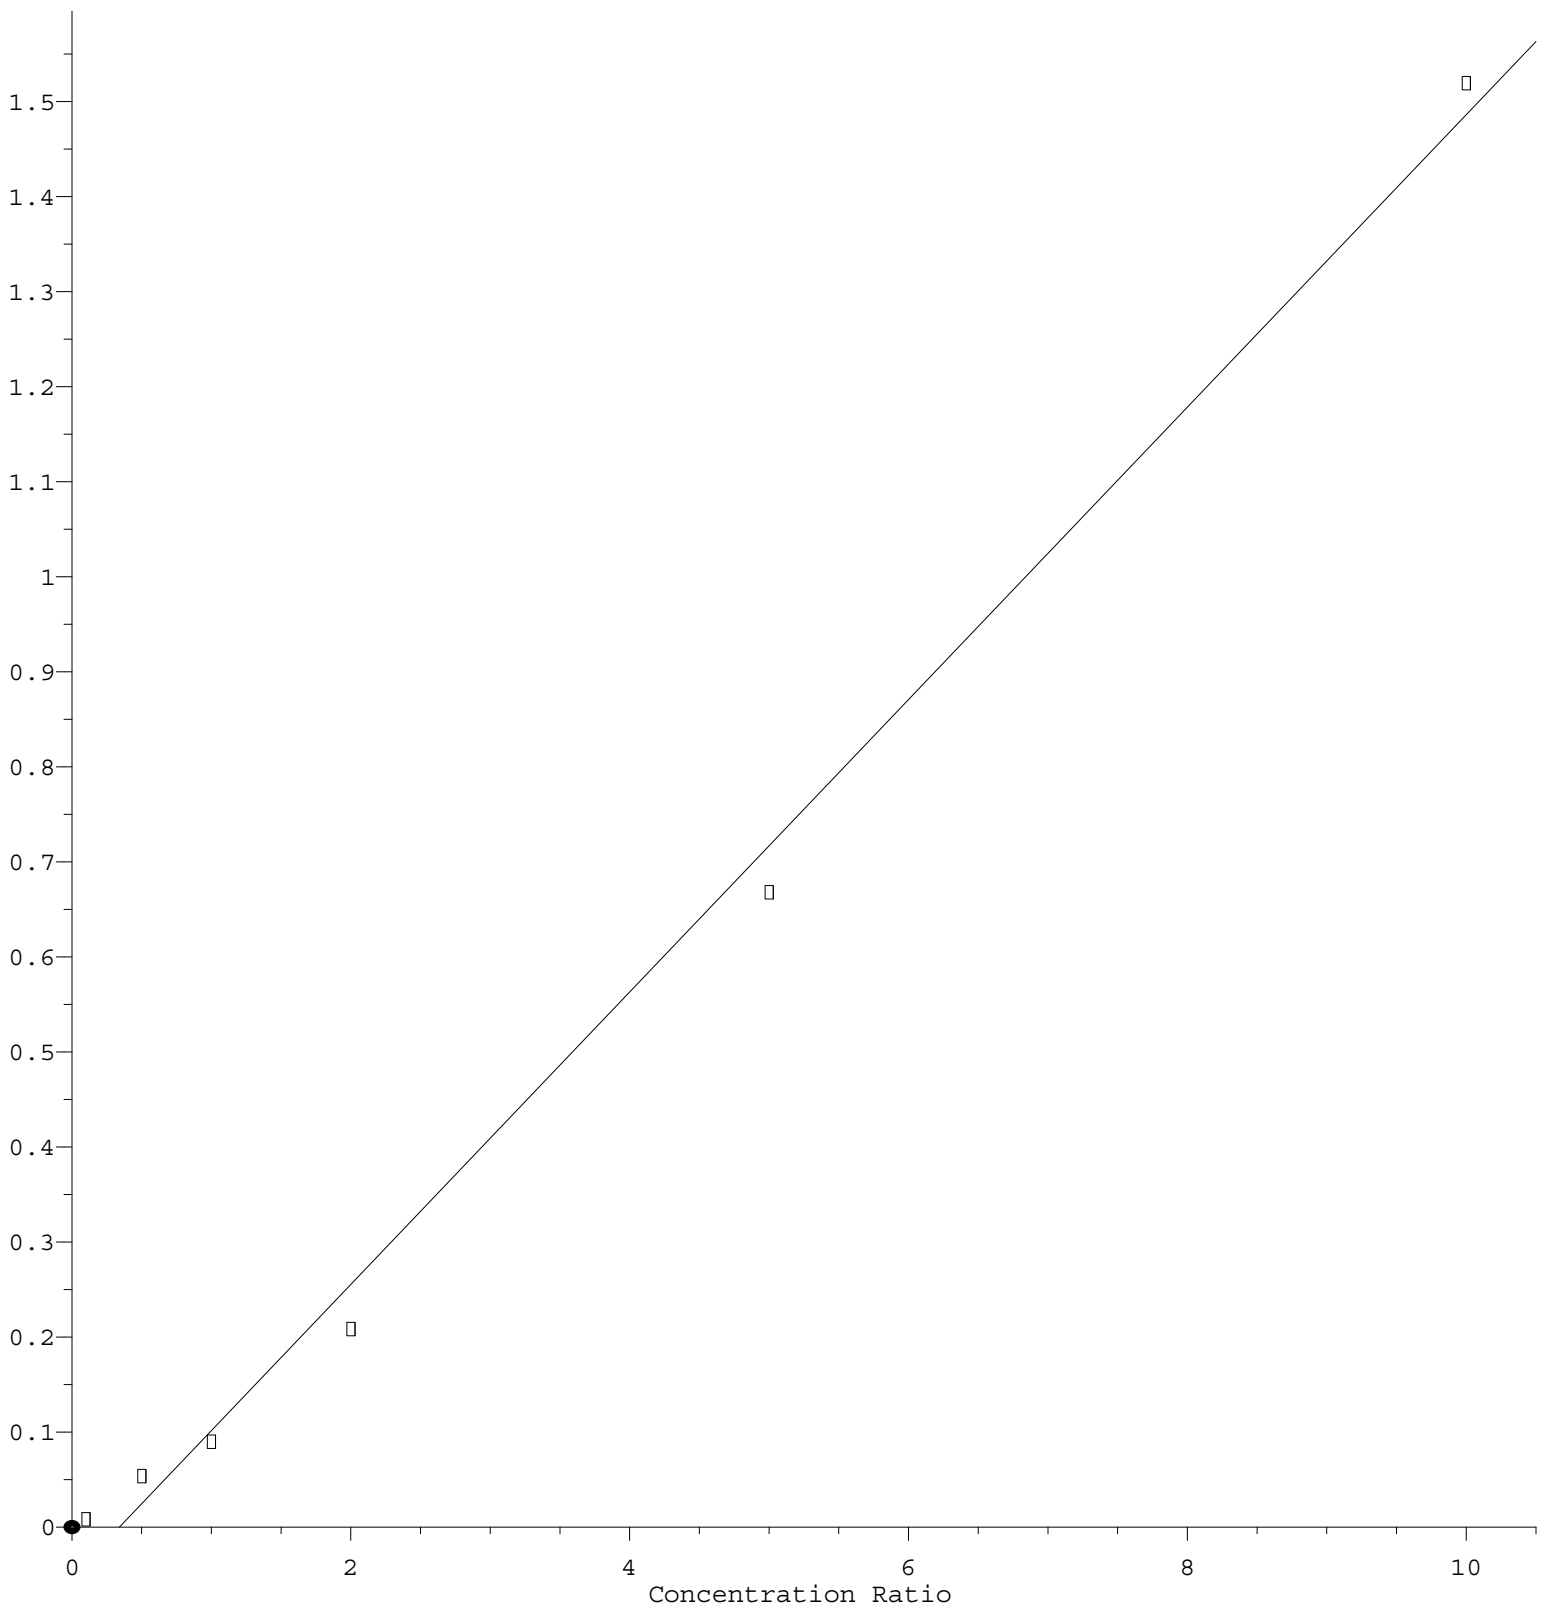

Response = 1.539e-001 * Amt - 5.235e-002


Coef of Det (r^2) = 0.994951 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Dibromochloromethane

Response Ratio

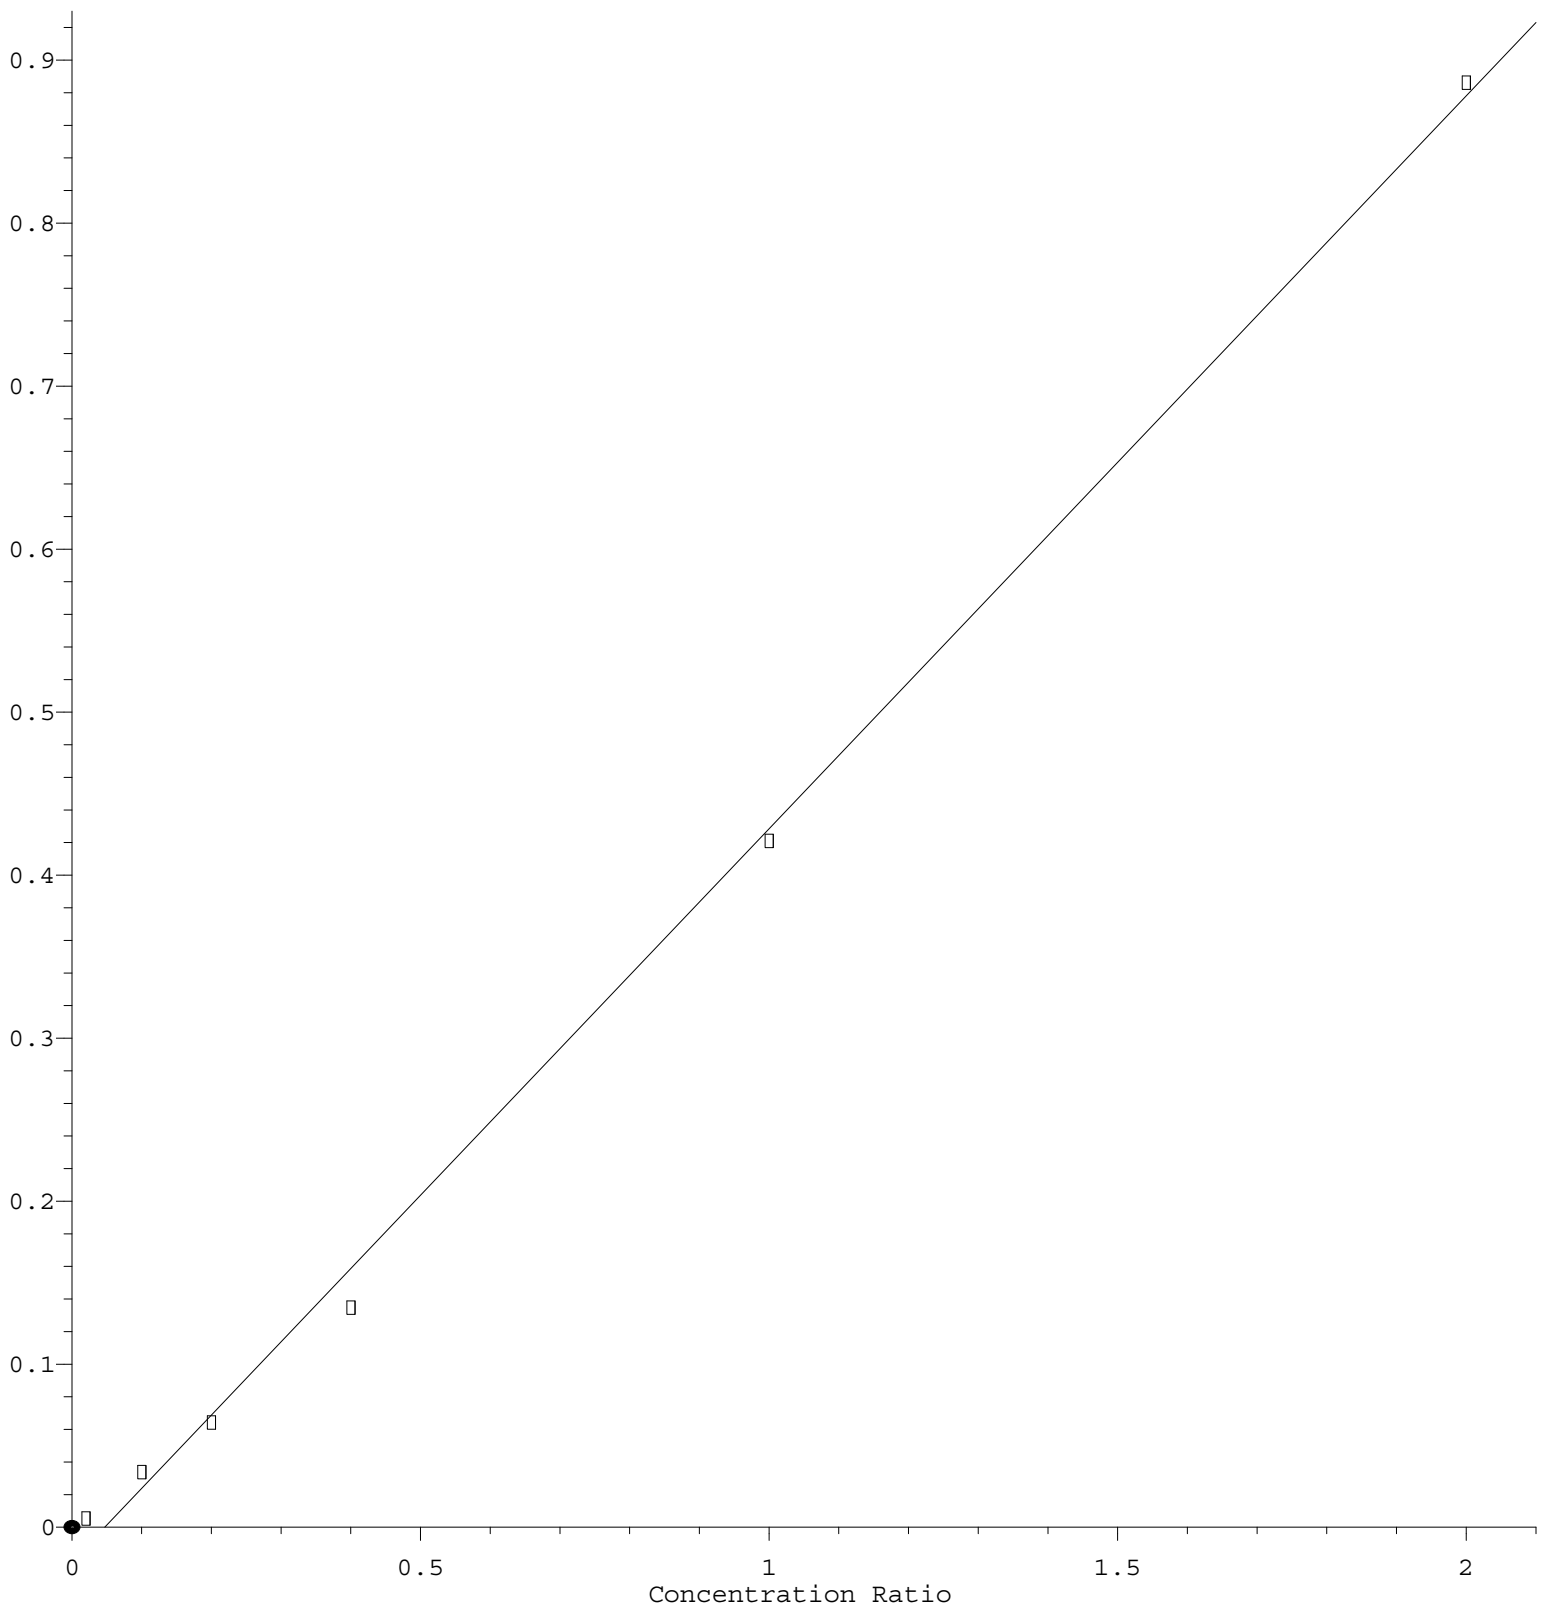

Response = 4.495e-001 * Amt - 2.119e-002


Coef of Det (r^2) = 0.998090 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Bromoform

Response Ratio

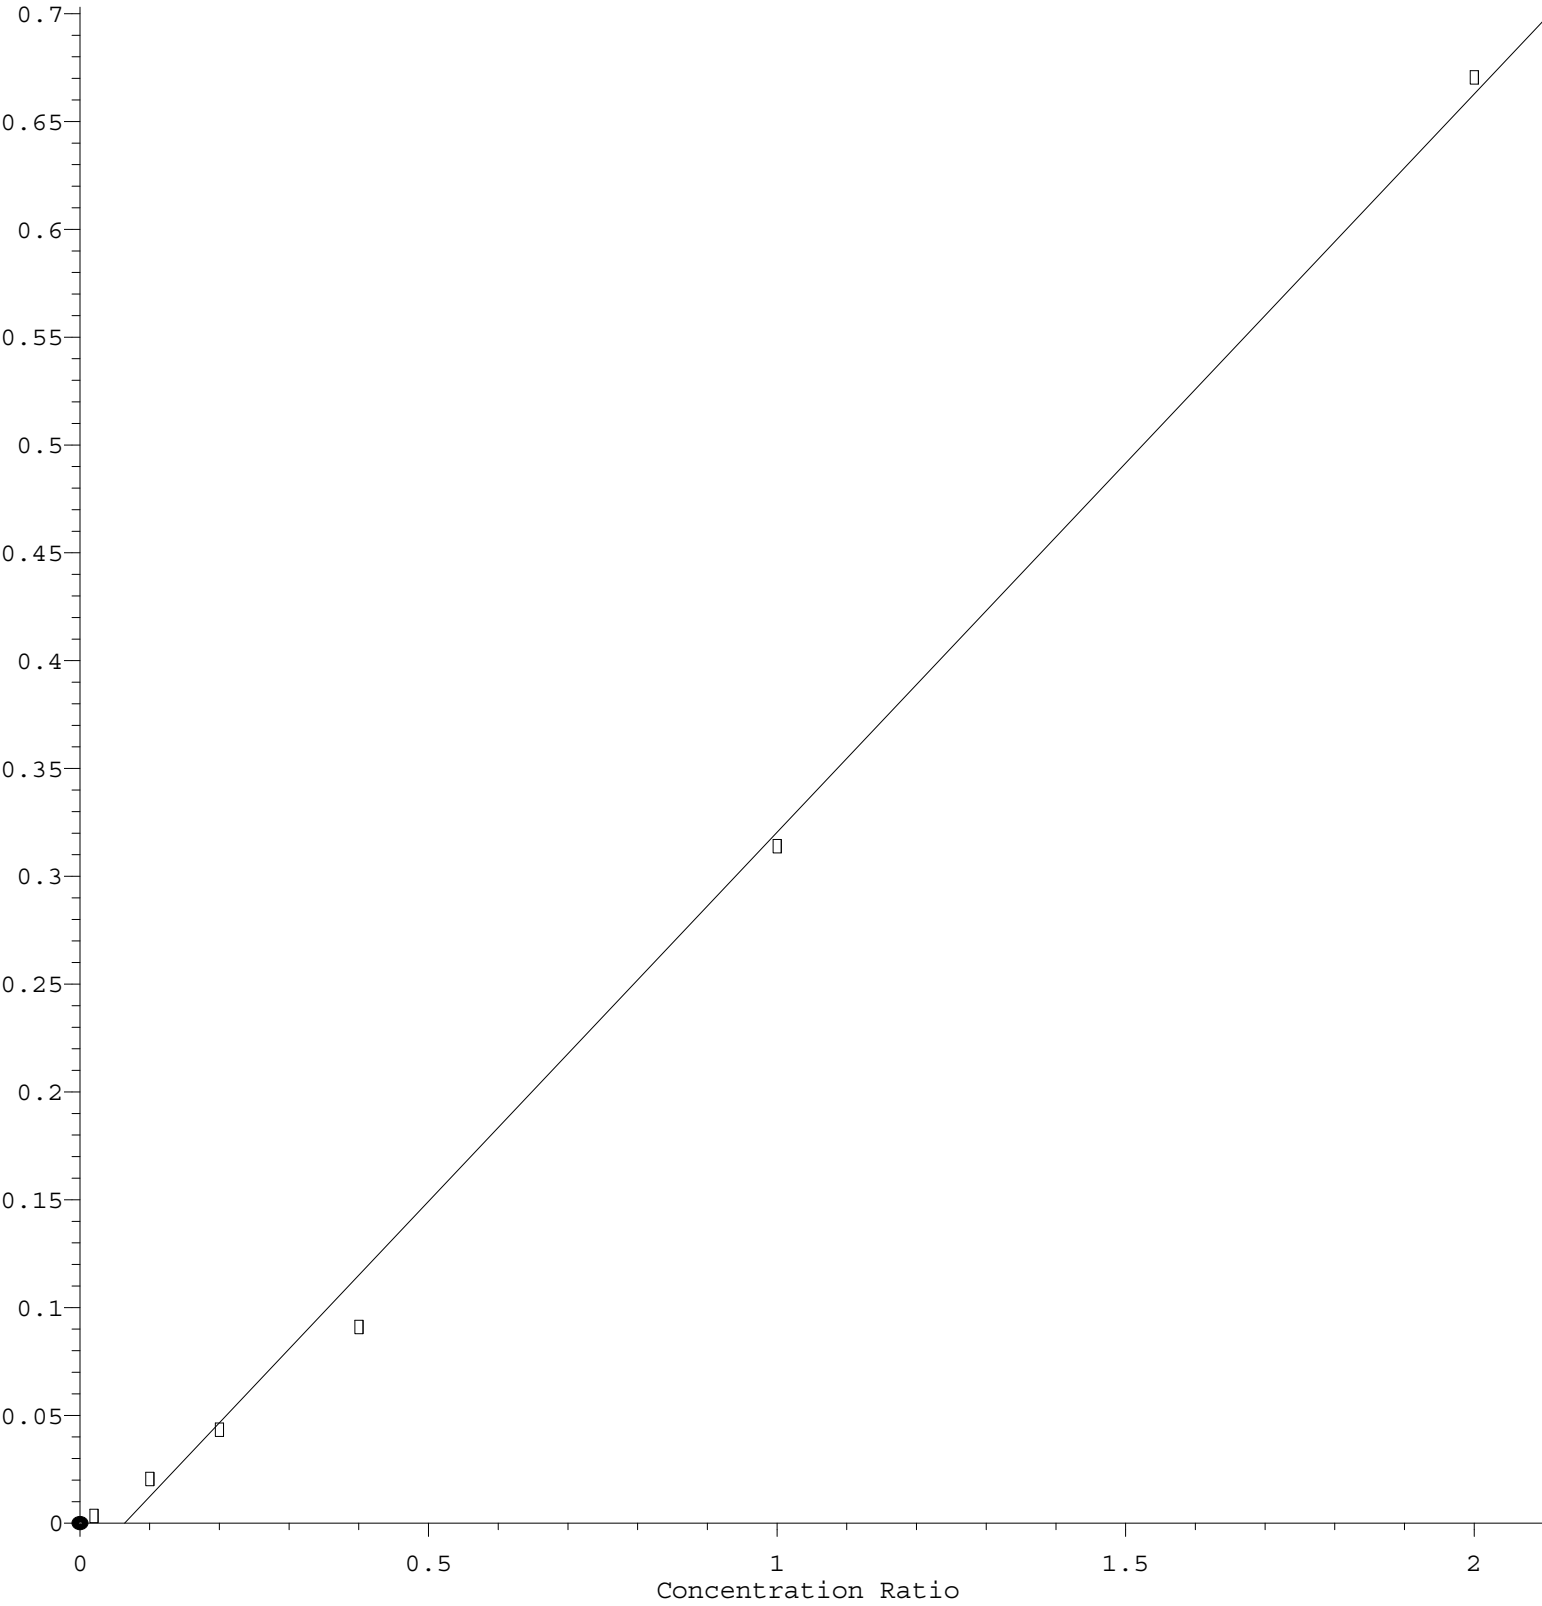

Response = 3.421e-001 * Amt - 2.173e-002


Coef of Det (r^2) = 0.996792 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

1,2,4-Trichlorobenzene

Response Ratio

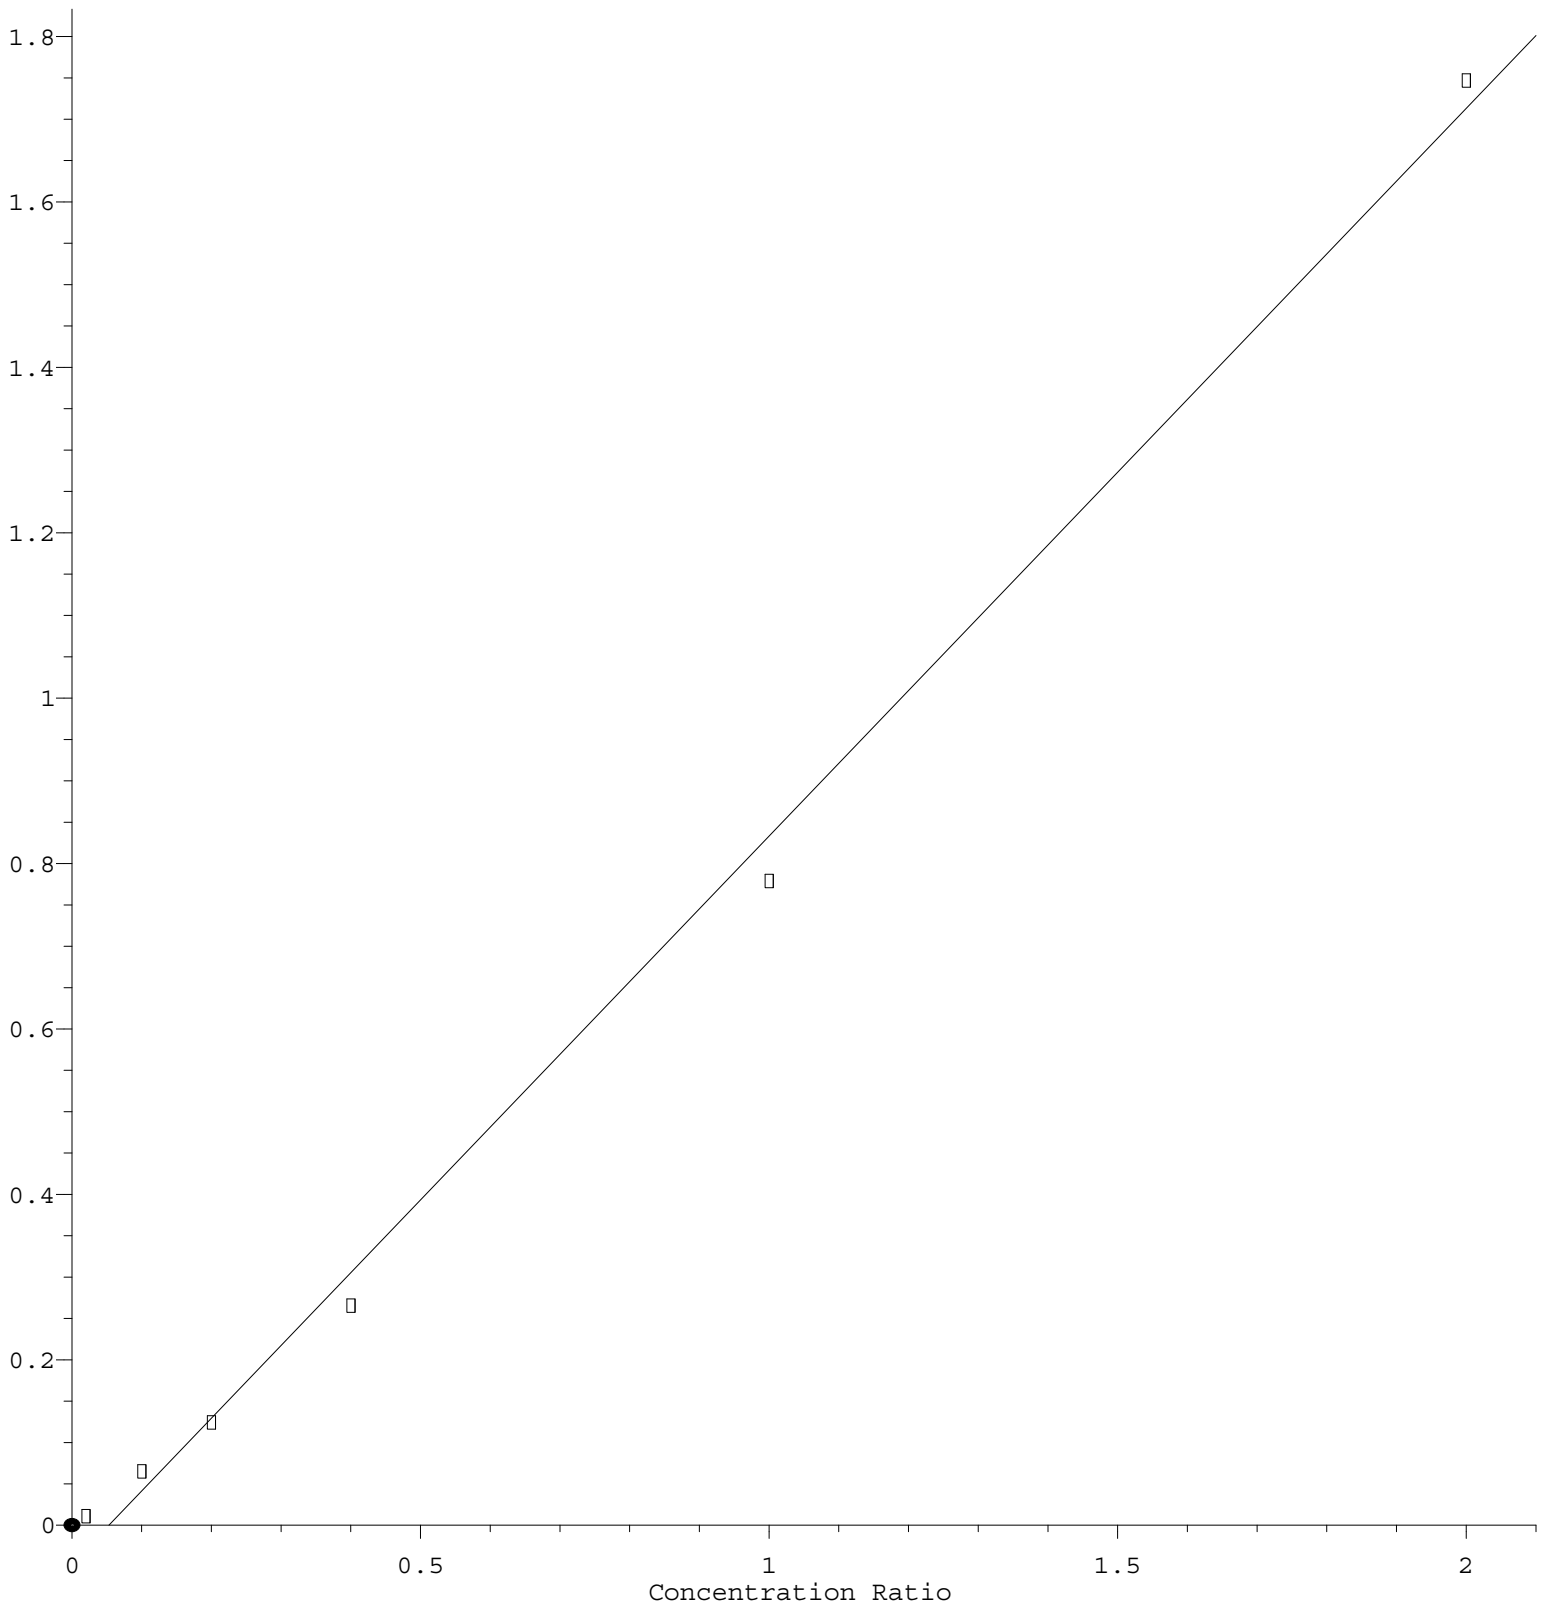

Response = 8.800e-001 * Amt - 4.707e-002


Coef of Det (r^2) = 0.996529 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021

Naphthalene

Response Ratio

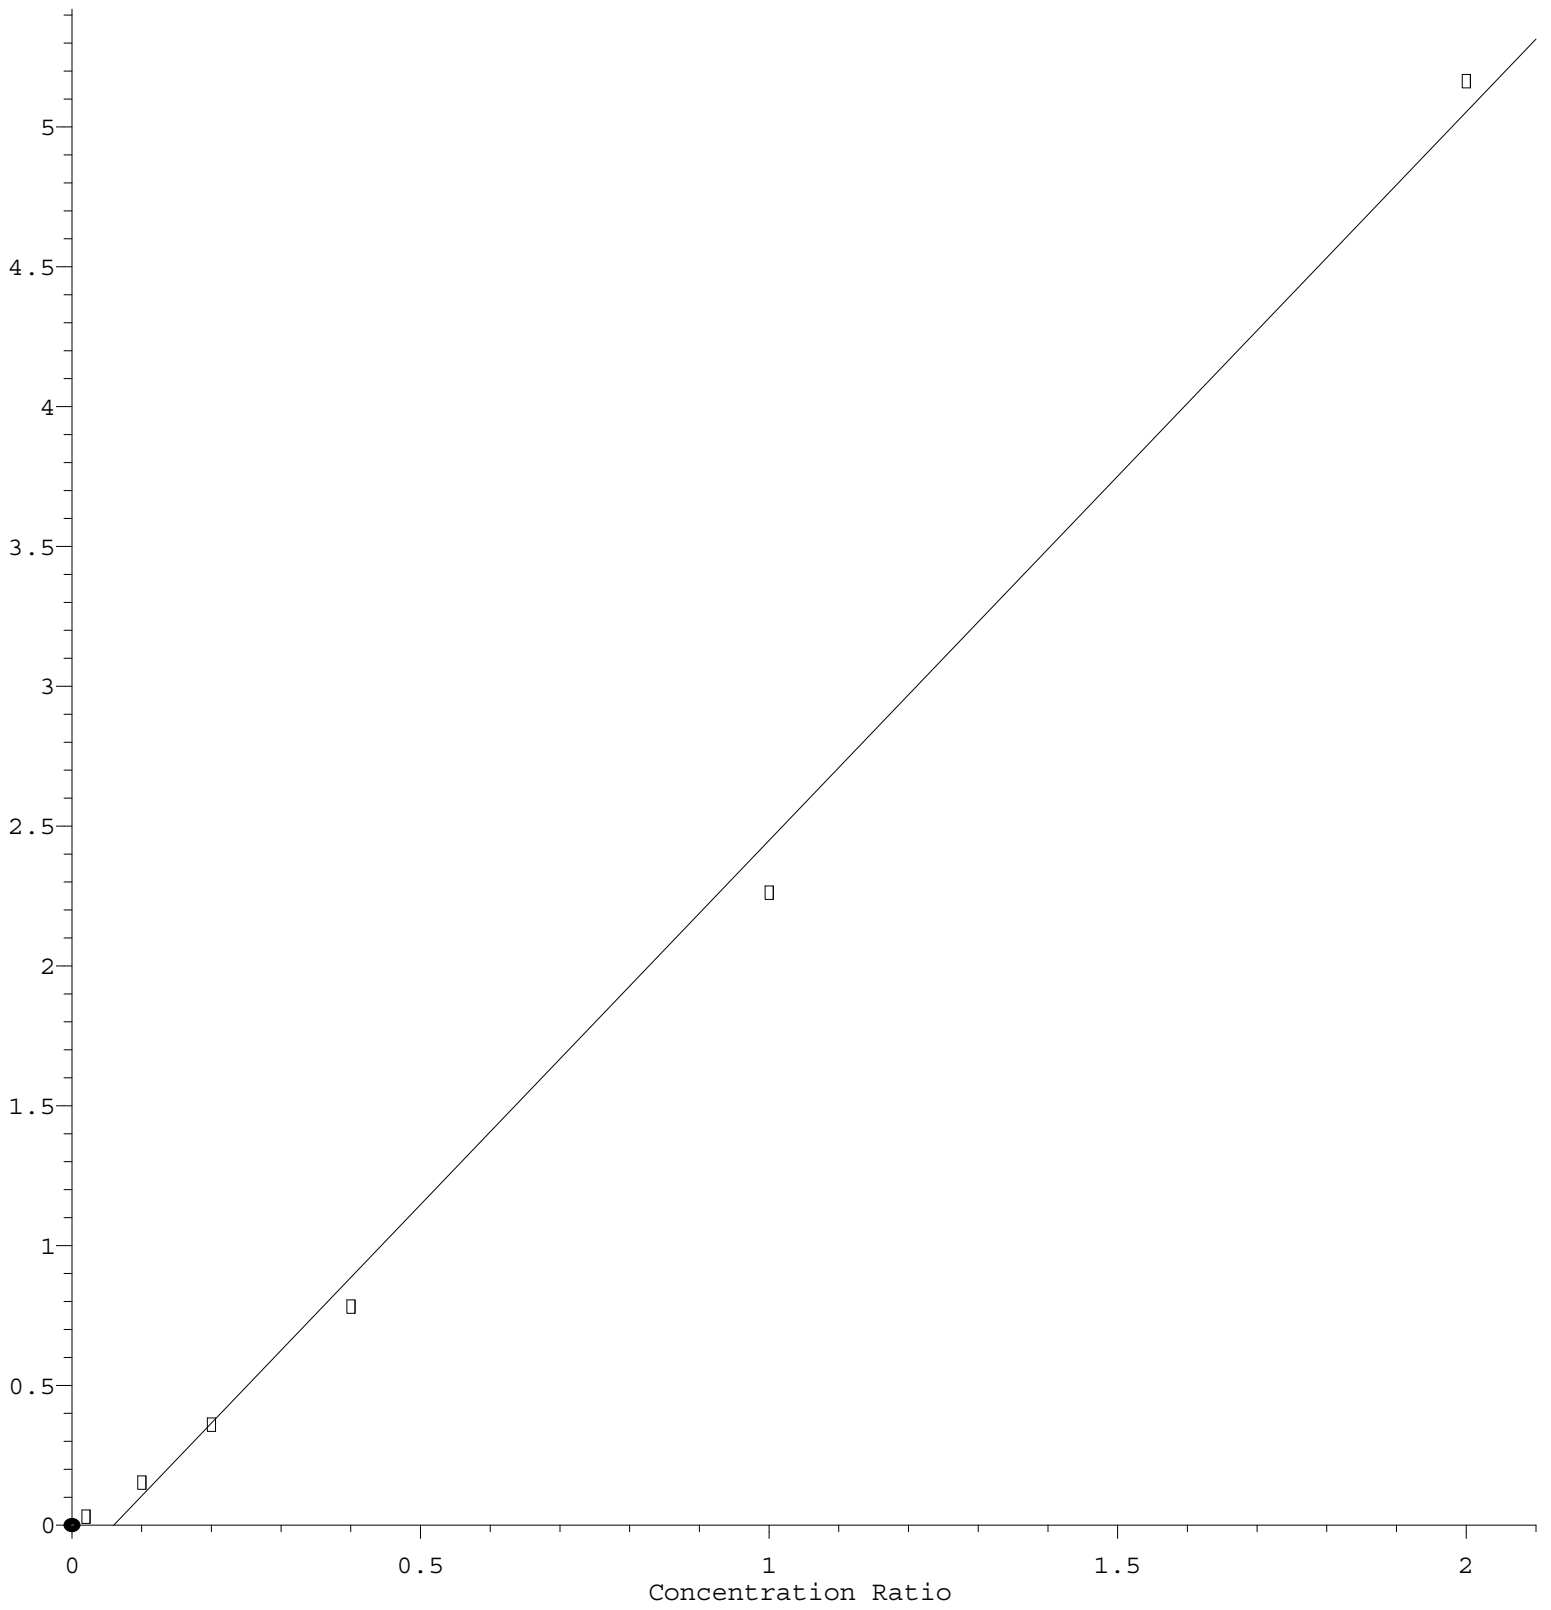

Response = 2.605e+000 * Amt - 1.569e-001

Coef of Det (r^2) = 0.996040 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N070721W.M

Calibration Table Last Updated: Wed Jul 07 16:18:53 2021