


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070721\
Data File : VN067630.D
Acq On : 7 Jul 2021 11:46
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Title : SW846 8260
Last Update : Wed Jul 07 16:18:53 2021

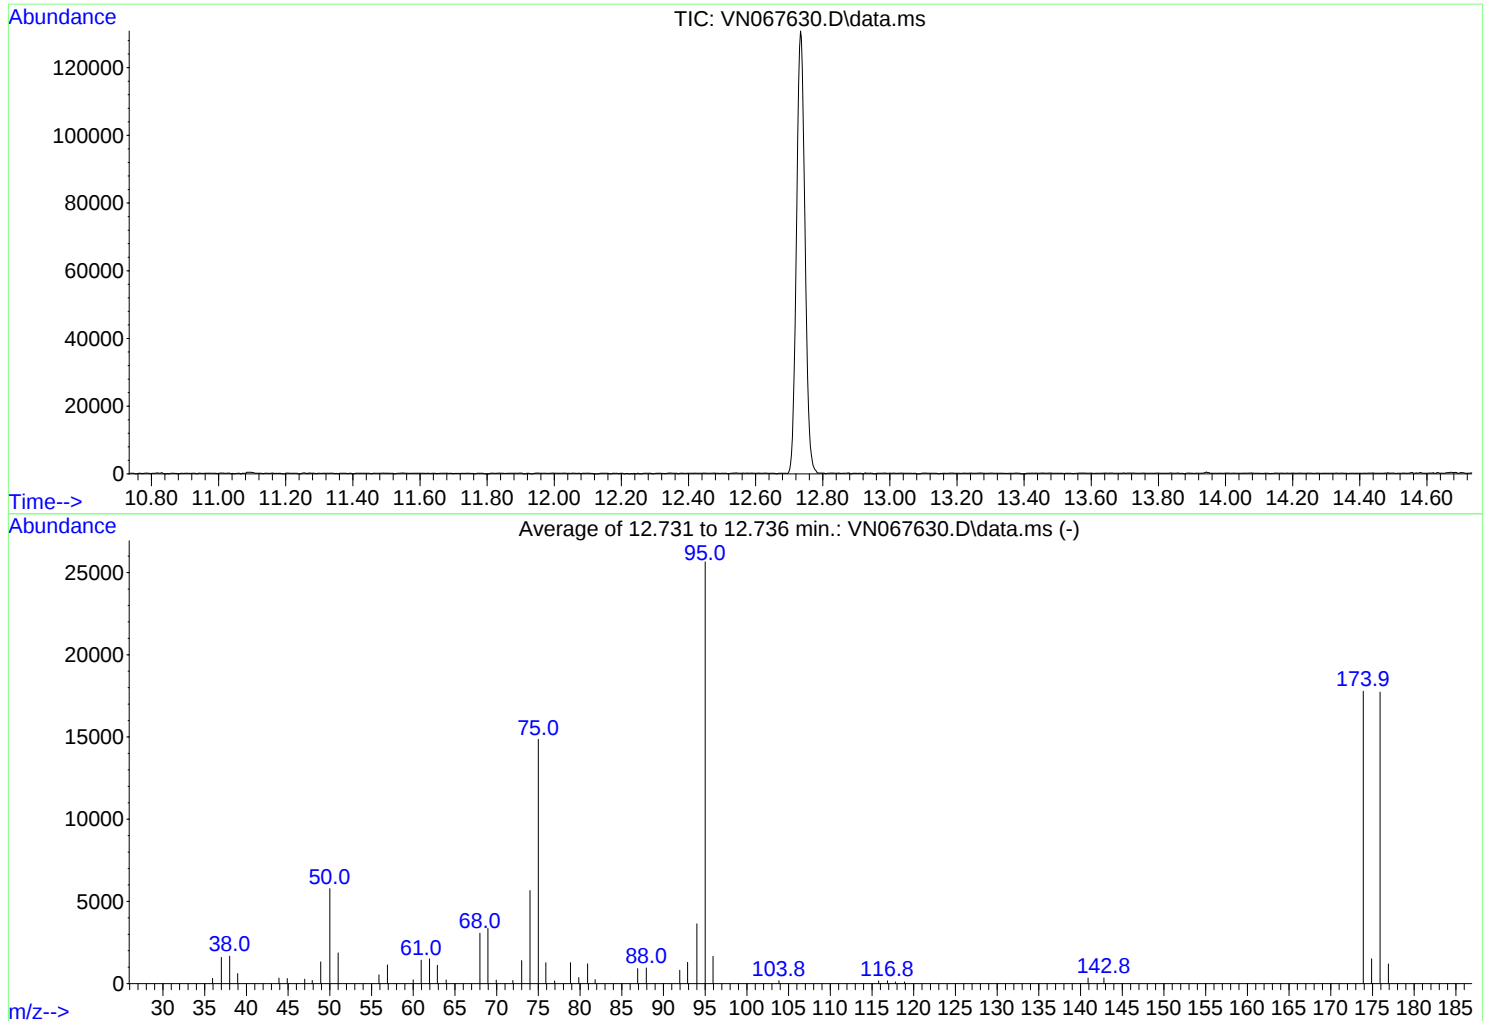

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3990

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	5781	PASS
75	95	30	60	57.9	14855	PASS
95	95	100	100	100.0	25651	PASS
96	95	5	9	6.5	1668	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.4	17792	PASS
175	174	5	9	8.5	1507	PASS
176	174	95	101	99.7	17733	PASS
177	176	5	9	6.8	1202	PASS