

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070722\
 Data File : VN073360.D
 Acq On : 07 Jul 2022 09:42
 Operator : JC\MD
 Sample : VN0707MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0707MBL01

Quant Time: Jul 07 15:02:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	295824	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.898	114	488897	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	438916	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	202164	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	184008	43.088	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.180%
35) Dibromofluoromethane	7.945	113	156686	48.171	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.340%
50) Toluene-d8	10.375	98	514163	44.507	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.020%
62) 4-Bromofluorobenzene	12.669	95	215564	48.555	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070722\
Data File : VN073360.D
Acq On : 07 Jul 2022 09:42
Operator : JC\MD
Sample : VN0707MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0707MBL01

Quant Time: Jul 07 15:02:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




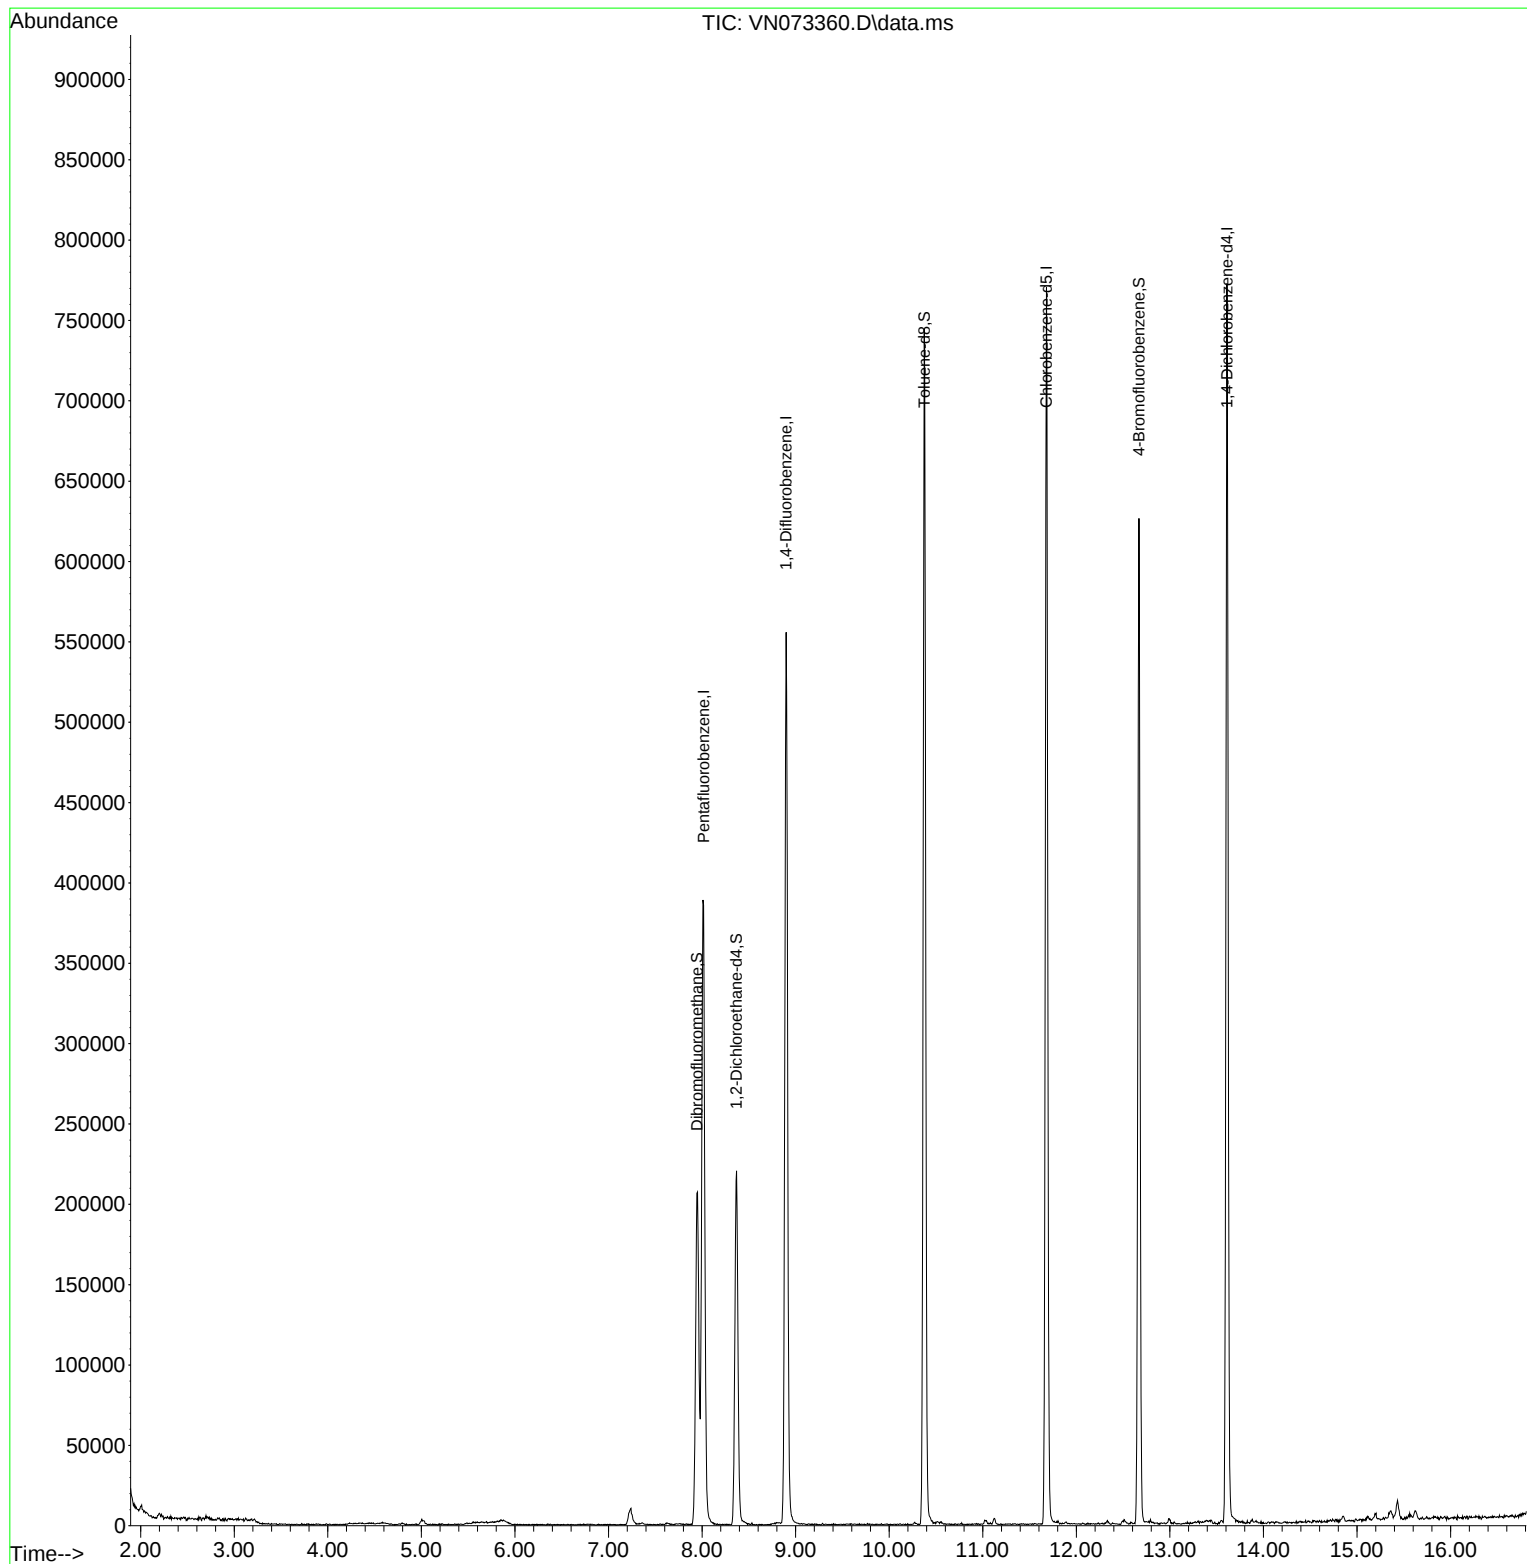


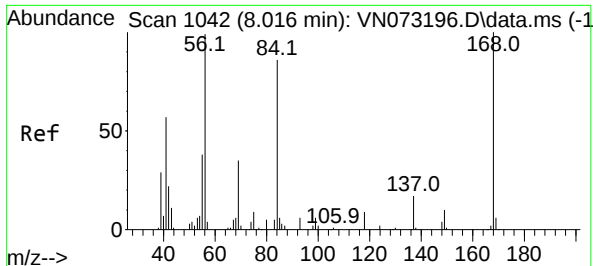

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42




Instrument :
MSVOA_N
ClientSampleId :
VN0707MBL01

Tgt Ion:168 Resp: 295824
Ion Ratio Lower Upper
168 100
99 57.6 42.3 63.5

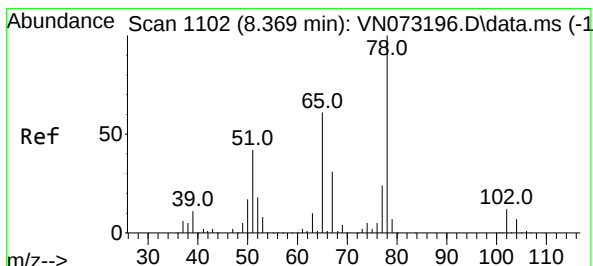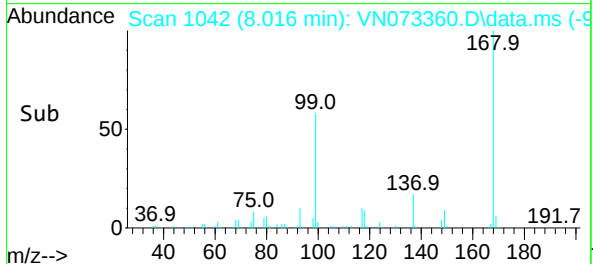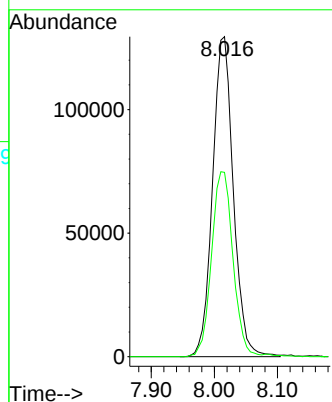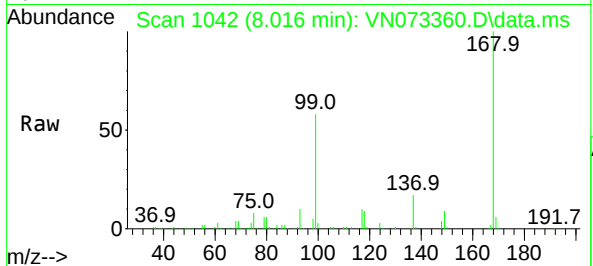

#33
1,2-Dichloroethane-d4
Concen: 43.088 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42

Tgt Ion: 65 Resp: 184008
Ion Ratio Lower Upper
65 100
67 53.0 0.0 104.8

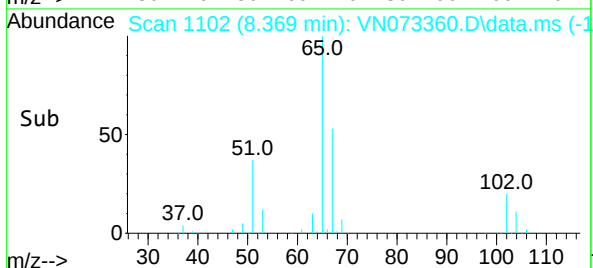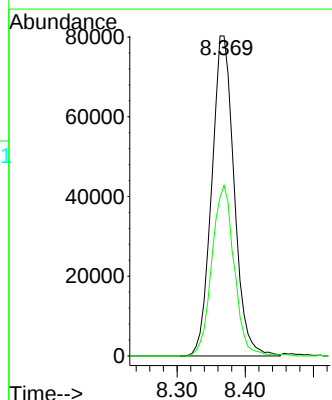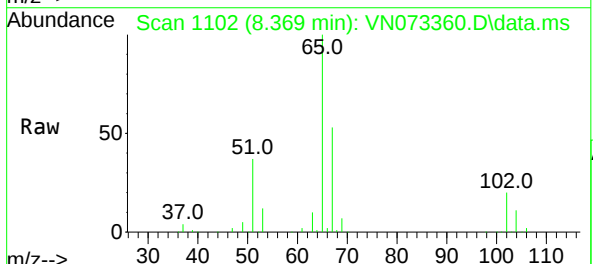



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.898 min Scan# 1192

Delta R.T. 0.000 min

Lab File: VN073360.D

Acq: 07 Jul 2022 09:42

Instrument :

MSVOA_N

ClientSampleId :

VN0707MBL01




Tgt Ion:114 Resp: 488897

Ion Ratio Lower Upper

114 100

63 21.3 0.0 40.0

88 15.5 0.0 32.6

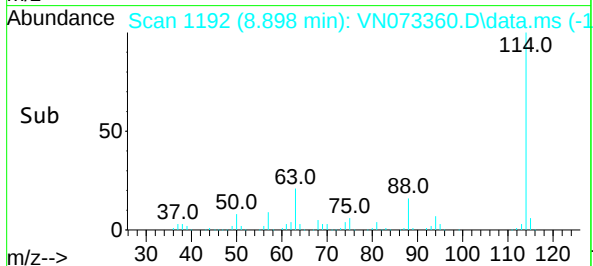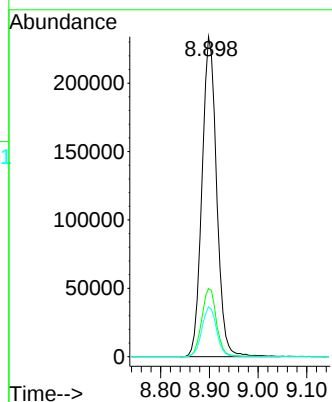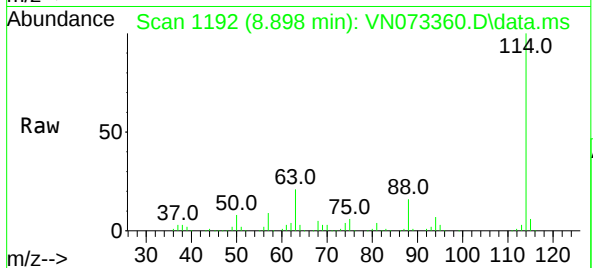

#35

Dibromofluoromethane

Concen: 48.171 ug/l

RT: 7.945 min Scan# 1030

Delta R.T. -0.006 min

Lab File: VN073360.D

Acq: 07 Jul 2022 09:42




Tgt Ion:113 Resp: 156686


Ion Ratio Lower Upper

113 100

111 103.7 81.4 122.0

192 18.6 17.0 25.6

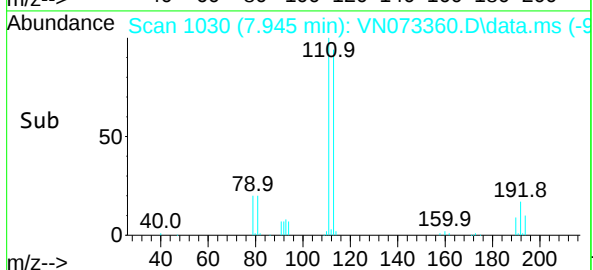
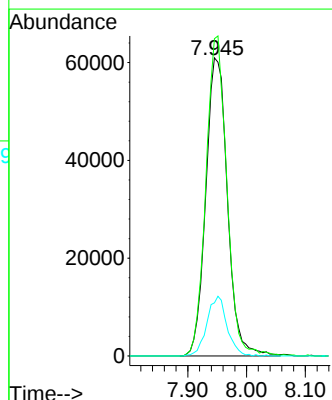
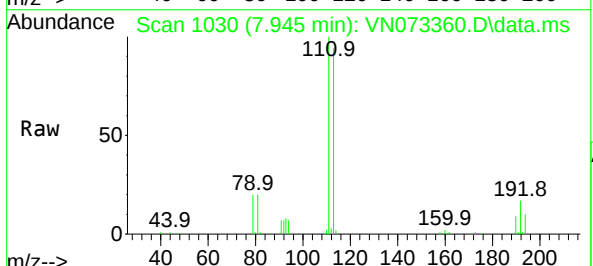


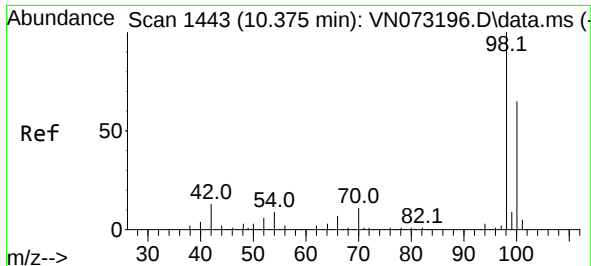

#50
Toluene-d8
Concen: 44.507 ug/l
RT: 10.375 min Scan# 1443
Delta R.T. -0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42




Instrument :
MSVOA_N
ClientSampleId :
VN0707MBL01


Tgt Ion: 98 Resp: 514163
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

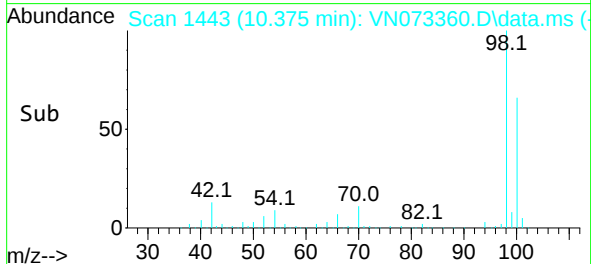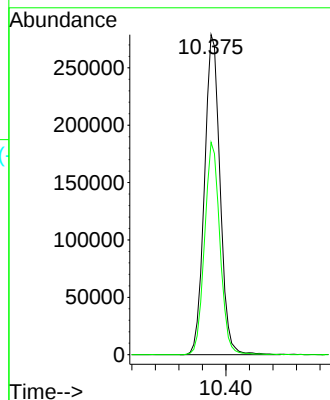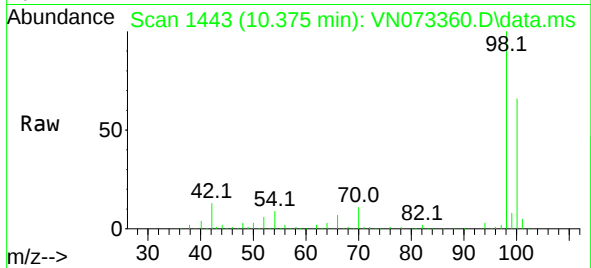

#62
4-Bromofluorobenzene
Concen: 48.555 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42

Tgt Ion: 95 Resp: 215564
Ion Ratio Lower Upper
95 100
174 74.2 0.0 167.6
176 72.1 0.0 163.4


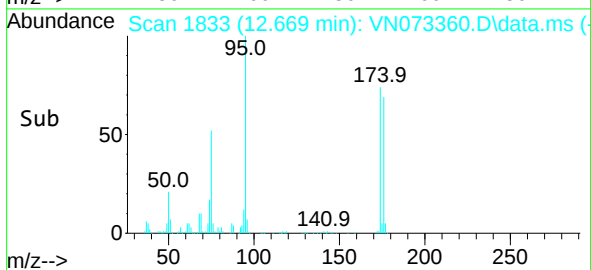
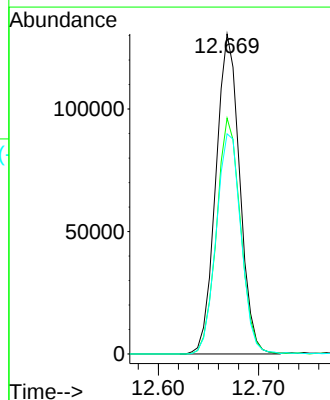
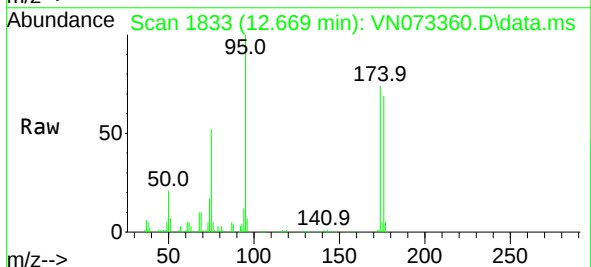


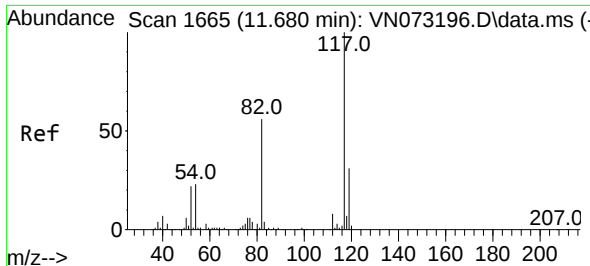

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 1165
Delta R.T. 0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42

Instrument :
MSVOA_N
ClientSampleId :
VN0707MBL01

Tgt Ion:117 Resp: 438916
Ion Ratio Lower Upper
117 100
82 55.9 44.2 66.2
119 32.3 25.4 38.0

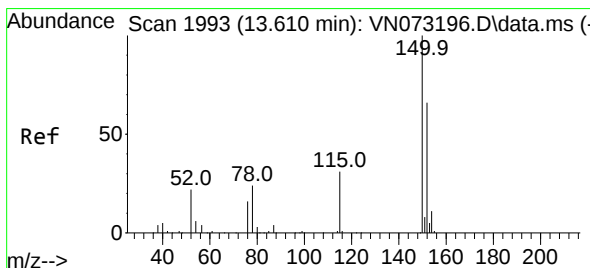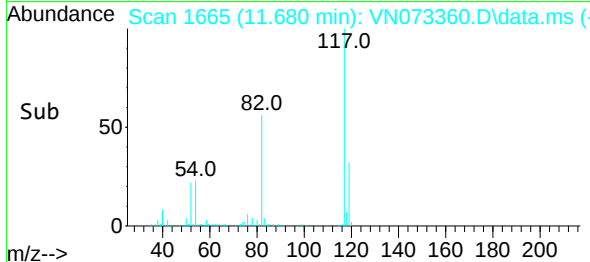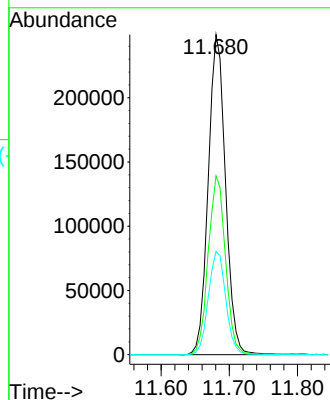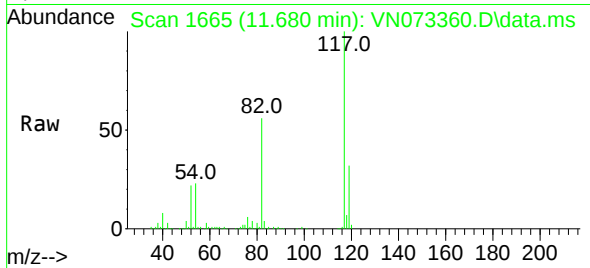

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073360.D
Acq: 07 Jul 2022 09:42

Tgt Ion:152 Resp: 202164
Ion Ratio Lower Upper
152 100
115 59.7 28.9 86.7
150 156.7 0.0 356.2

