


1,2,4-Trichlorobenzene

Response Ratio

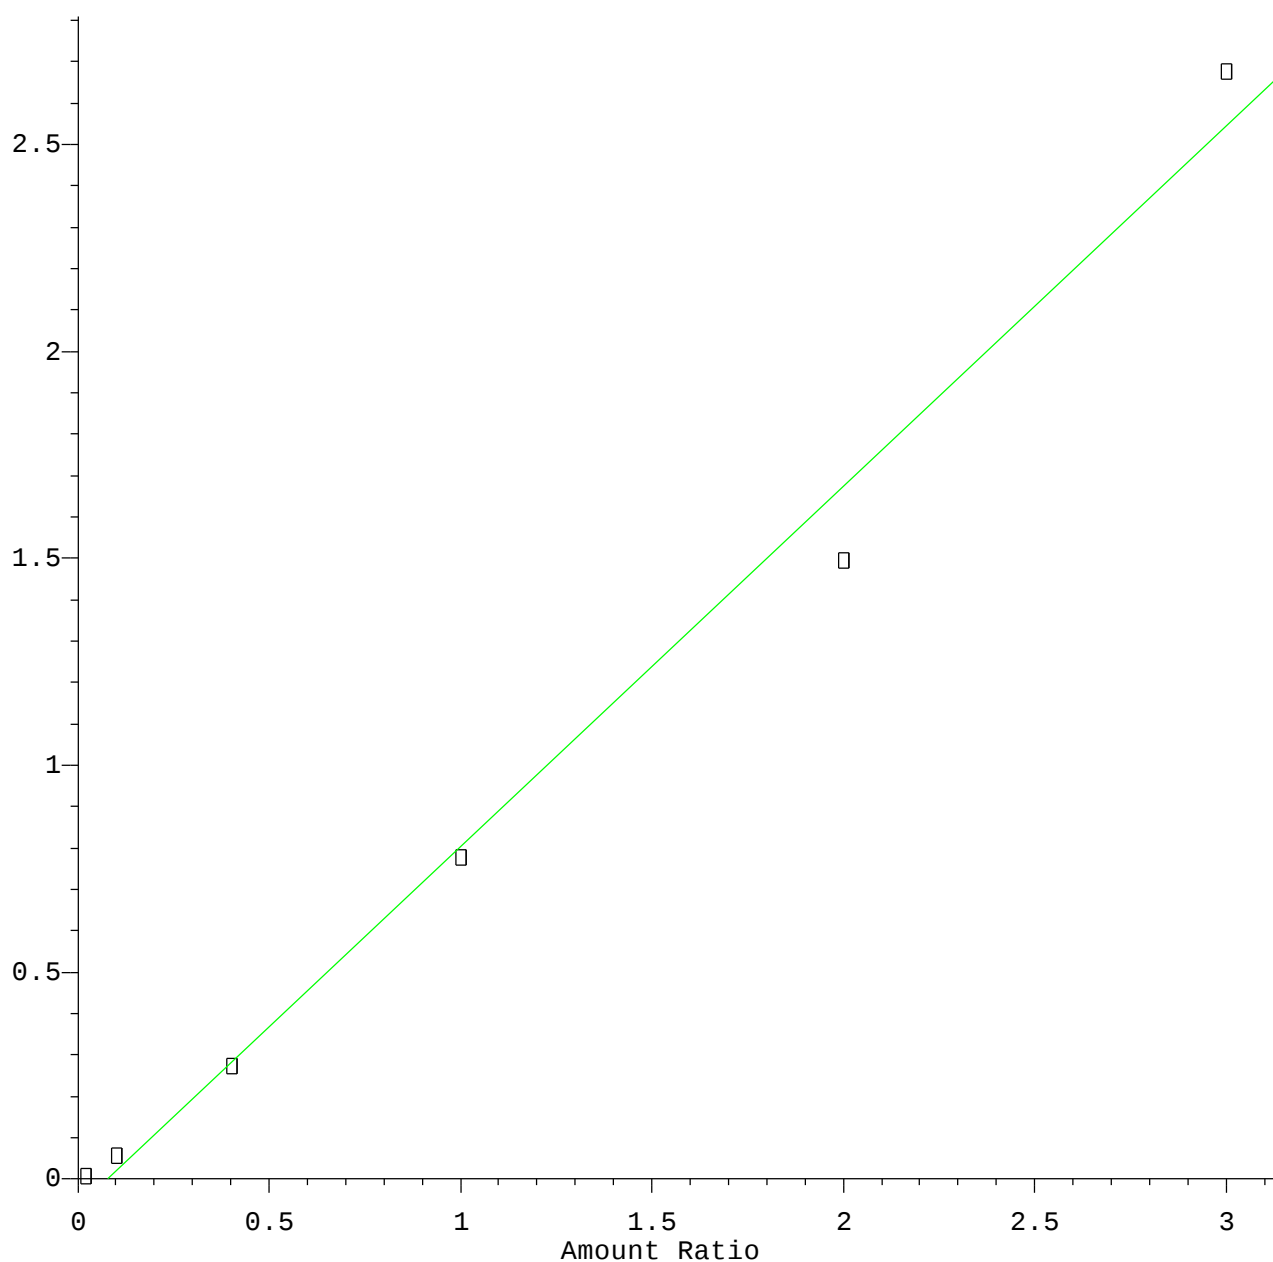


Resp Ratio = $8.71e-001 * \text{Amt} - 6.65e-002$
Coef of Det (r^2) = 0.990 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Calibration Table Last Updated: Wed Jul 08 12:39:14 2020

Ethyl methacrylate

Response Ratio

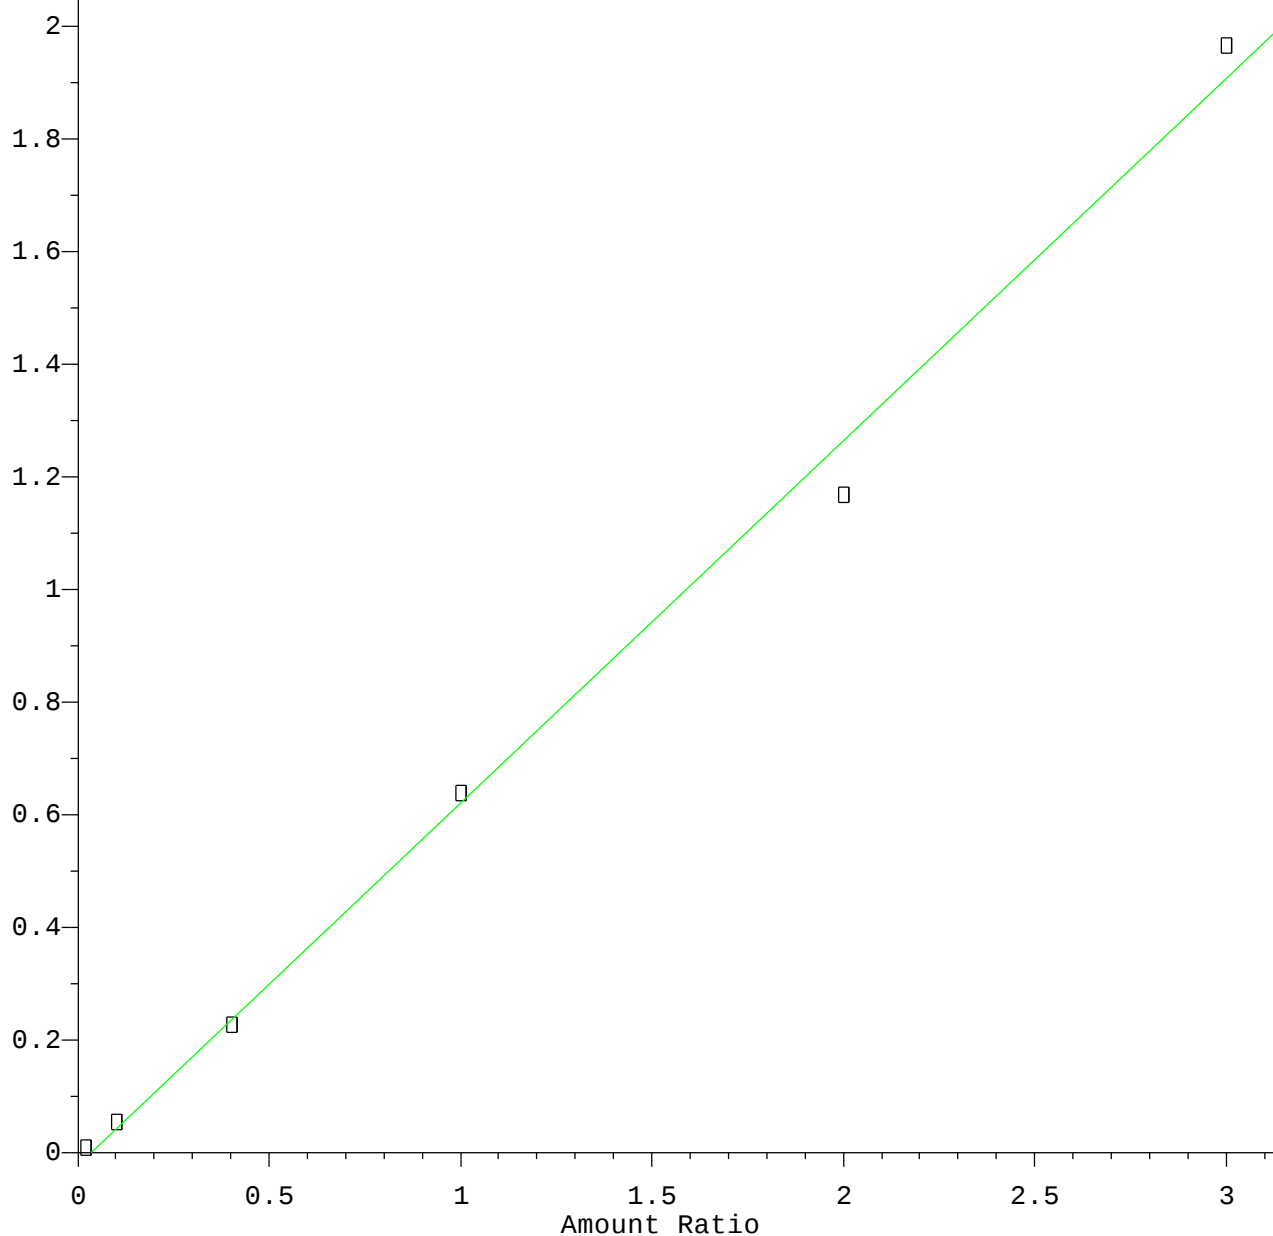


Resp Ratio = $6.43 \times 10^{-1} \times \text{Amt} - 2.20 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Calibration Table Last Updated: Wed Jul 08 12:39:14 2020

Naphthalene

Response Ratio

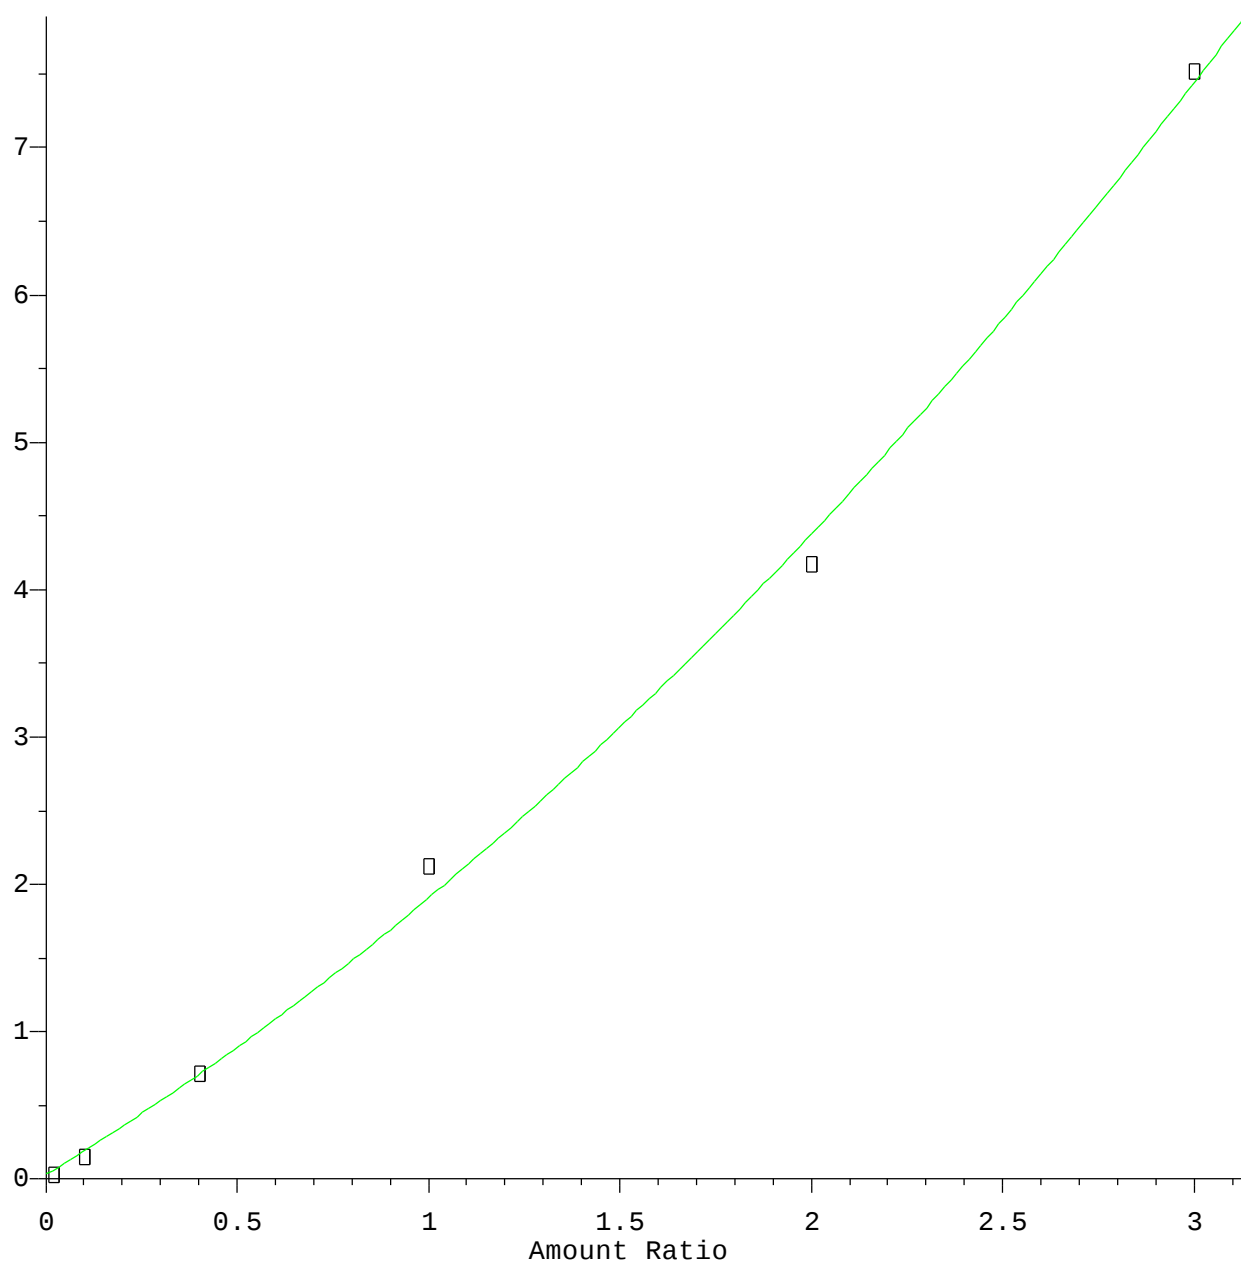


$R = 2.97e-001 A^2 + 1.58e+000 A + 3.09e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Calibration Table Last Updated: Wed Jul 08 12:39:14 2020

Naphthalene

Response Ratio

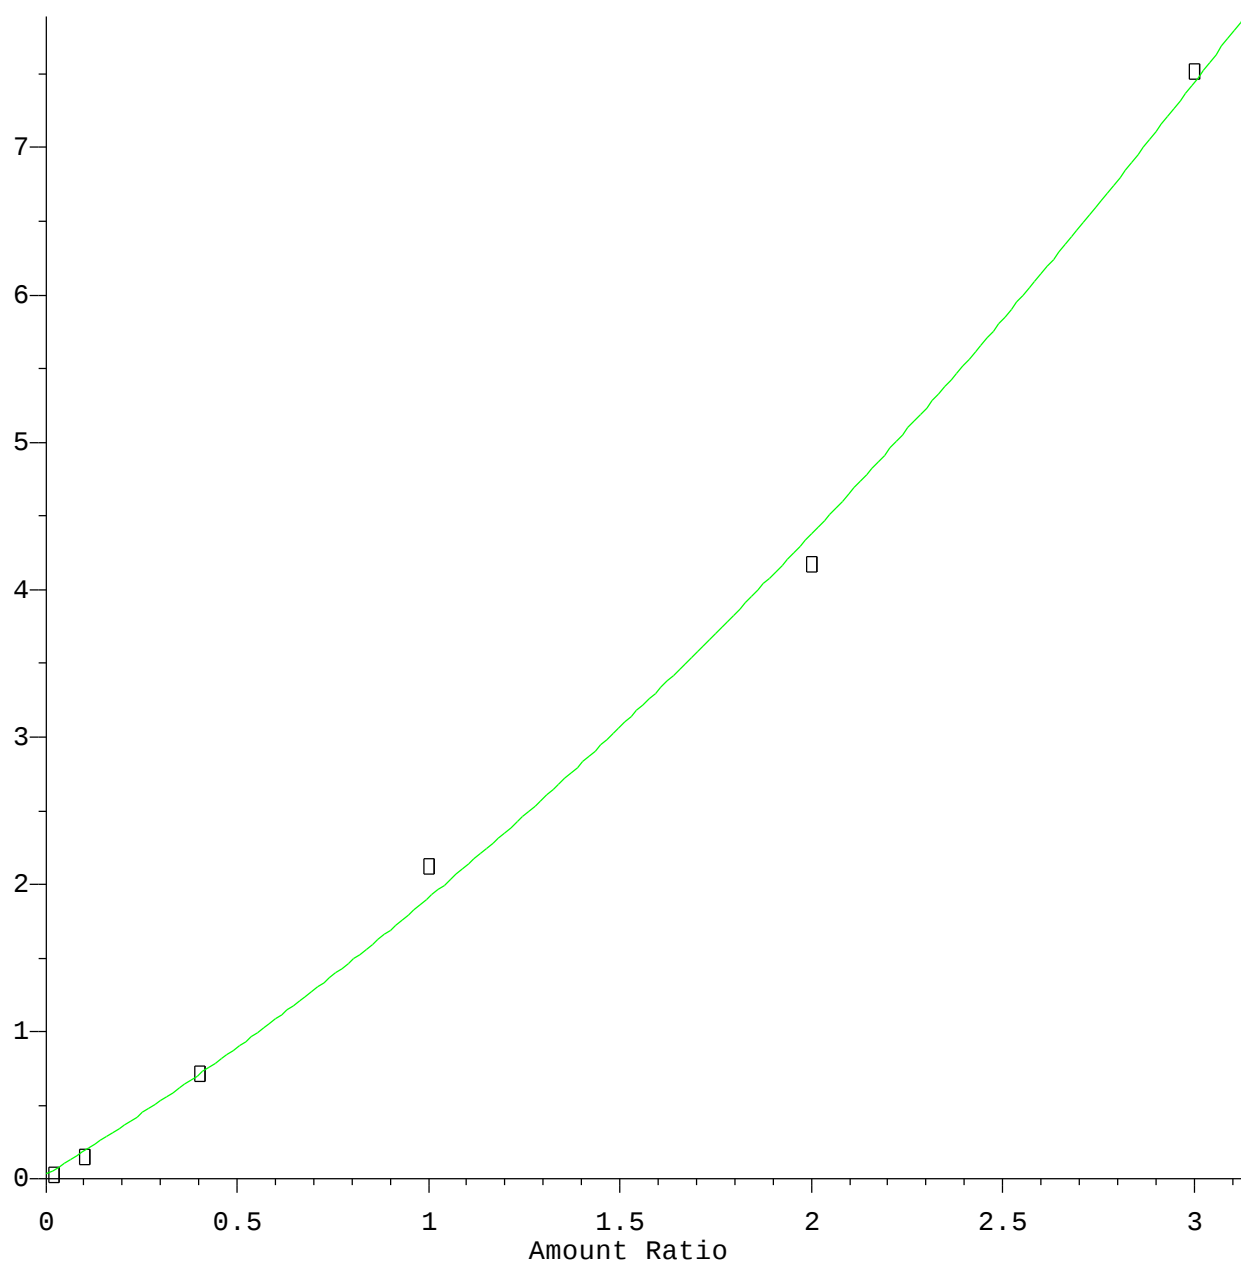


$R = 2.97e-001 A^2 + 1.58e+000 A + 3.09e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Calibration Table Last Updated: Wed Jul 08 12:39:14 2020

1,2,3-Trichlorobenzene

Response Ratio

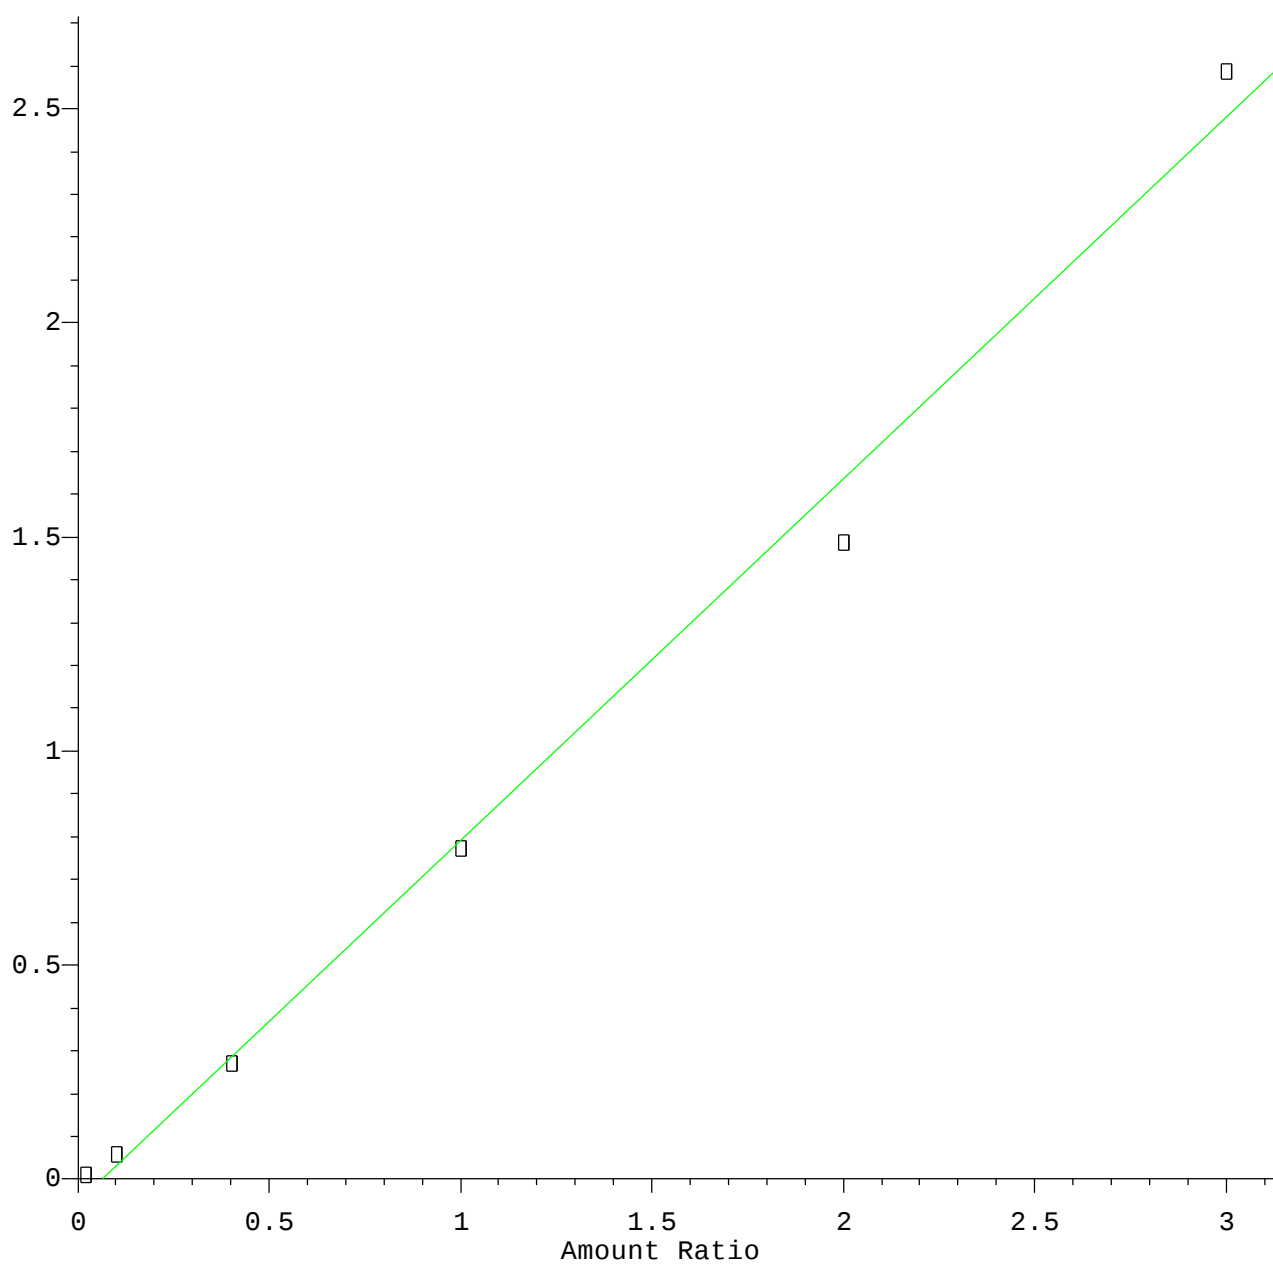

Resp Ratio = $8.44 \times 10^{-1} \times \text{Amt} - 5.44 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Calibration Table Last Updated: Wed Jul 08 12:39:14 2020