


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070820\
Data File : VN062420.D
Acq On : 8 Jul 2020 21:03
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Title : SW846 8260
Last Update : Thu Jul 09 02:12:34 2020

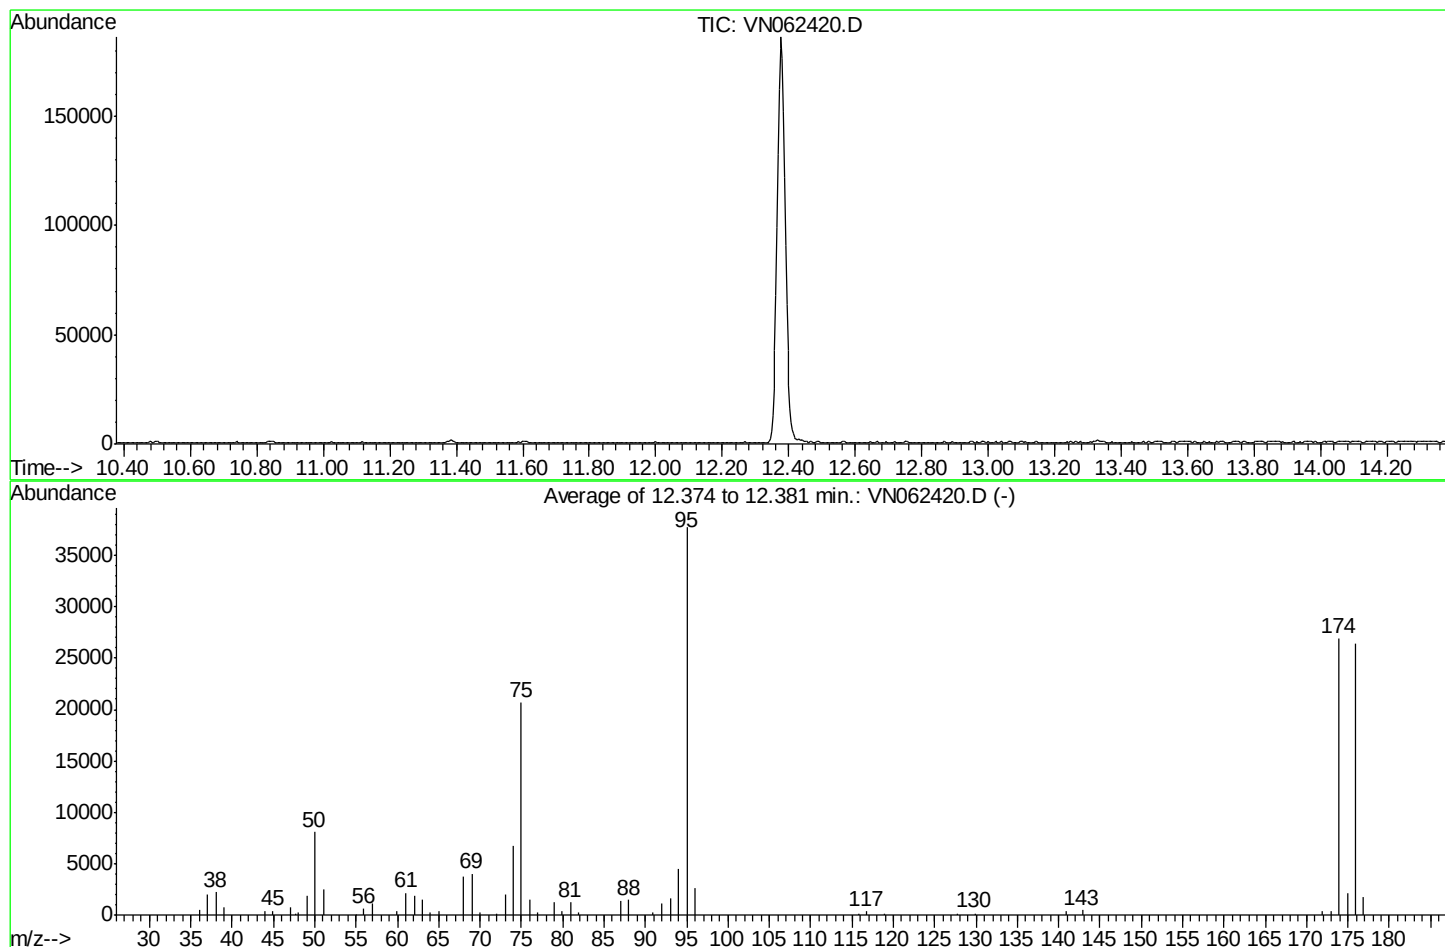

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	8074	PASS
75	95	30	60	54.7	20656	PASS
95	95	100	100	100.0	37733	PASS
96	95	5	9	6.9	2589	PASS
173	174	0.00	2	1.5	391	PASS
174	95	50	100	71.2	26864	PASS
175	174	5	9	7.8	2104	PASS
176	174	95	101	98.3	26418	PASS
177	176	5	9	6.7	1776	PASS