

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070821\
 Data File : VN067669.D
 Acq On : 8 Jul 2021 17:32
 Operator : JC/MD
 Sample : PB137565ZHE#03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 09 03:55:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	340960	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	651969	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	698407	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	256406	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	275746	53.512	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 107.020%			
35) Dibromofluoromethane	8.024	113	195270	49.573	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 99.140%			
50) Toluene-d8	10.446	98	872860	52.940	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 105.880%			
62) 4-Bromofluorobenzene	12.734	95	305984	52.535	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 105.060%			
Target Compounds			Qvalue			
5) Bromomethane	2.829	94	25	Below Cal	#	4
6) Chloroethane	2.998	64	95	Below Cal	#	44
11) Tert butyl alcohol	5.393	59	282	0.381	ug/l #	71
13) Acrolein	4.039	56	303	Below Cal		85
16) Acetone	4.299	43	35901	22.142	ug/l	96
18) Methyl Acetate	4.873	43	4071	0.894	ug/l #	74
20) Methylene Chloride	5.093	84	30681	7.514	ug/l	91
25) 2-Butanone	7.351	43	10840	4.026	ug/l	96
29) Tetrahydrofuran	7.708	42	2380	1.344	ug/l	93
31) Cyclohexane	8.091	56	9598	1.328	ug/l #	33
36) 1,1-Dichloropropene	8.088	75	32529	5.371	ug/l #	52
37) Ethyl Acetate	7.351	43	10840	1.847	ug/l #	69
38) Carbon Tetrachloride	8.088	117	37952	6.353	ug/l #	17
41) Methacrylonitrile	7.694	41	739	0.245	ug/l #	45
43) Isopropyl Acetate	8.566	43	49373	4.783	ug/l #	90
45) 1,2-Dichloropropane	9.633	63	3160	0.688	ug/l #	44
48) Methyl methacrylate	9.550	41	10852	2.377	ug/l #	12
49) 1,4-Dioxane	9.620	88	152	33.753	ug/l #	20
51) 4-Methyl-2-Pentanone	10.336	43	8003	1.262	ug/l #	68
53) t-1,3-Dichloropropene	10.448	75	51	1.751	ug/l #	1
54) cis-1,3-Dichloropropene	10.247	75	77686	10.972	ug/l #	63
57) 1,3-Dichloropropane	11.095	76	47328	6.065	ug/l #	43
59) 2-Hexanone	11.095	43	715338	161.610	ug/l #	54
60) Dibromochloromethane	11.492	129	492	2.441	ug/l #	11
71) Bromoform	12.731	173	680	3.318	ug/l #	1
76) 1,2,3-Trichloropropane	12.734	75	173087	33.055	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	173087	106.574	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.265	180	205	2.720	ug/l #	52
95) Naphthalene	15.509	128	2161	3.174	ug/l #	72
96) 1,2,3-Trichlorobenzene	15.705	180	256	2.692	ug/l #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070821\
Data File : VN067669.D
Acq On : 8 Jul 2021 17:32
Operator : JC/MD
Sample : PB137565ZHE#03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 09 03:55:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

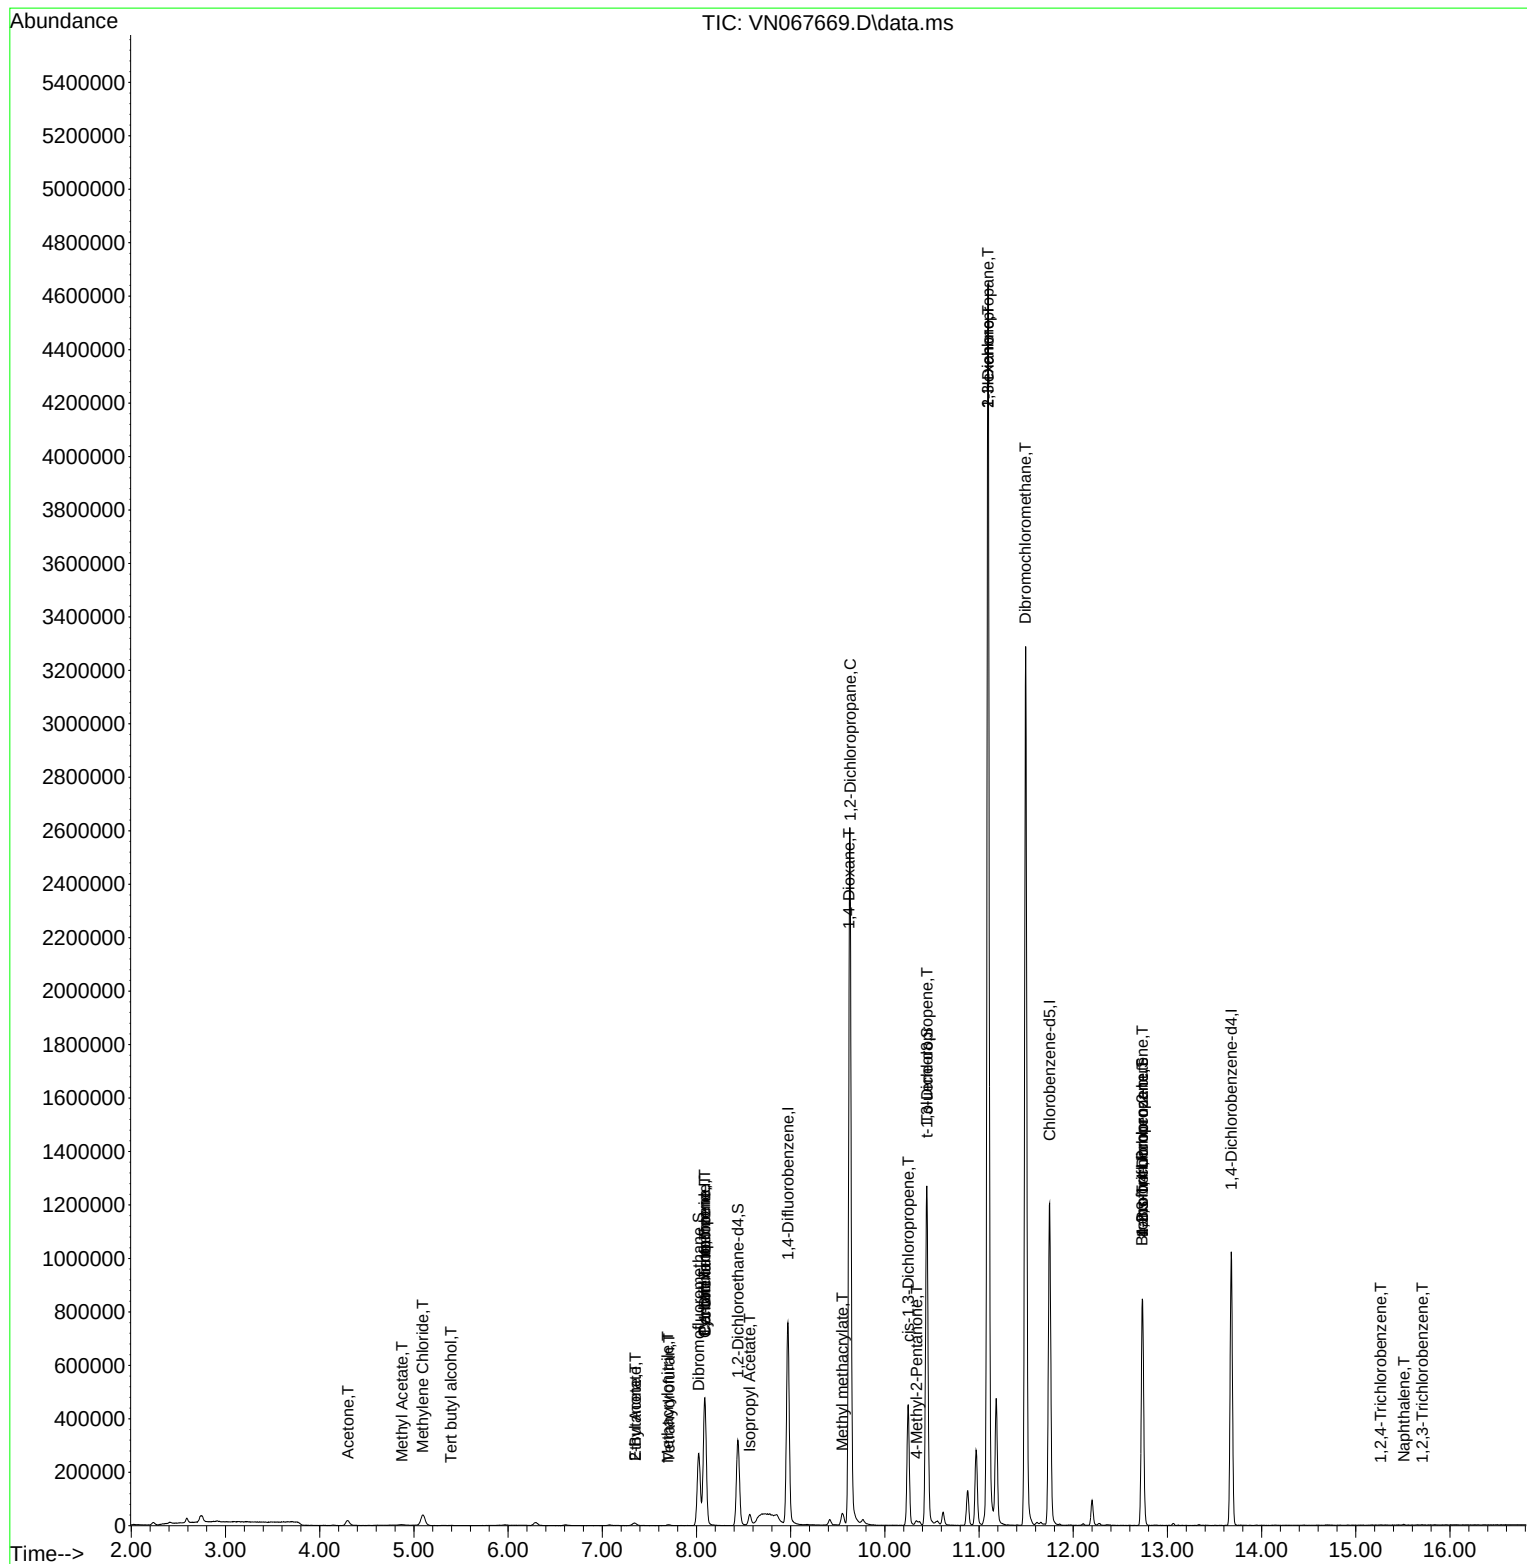

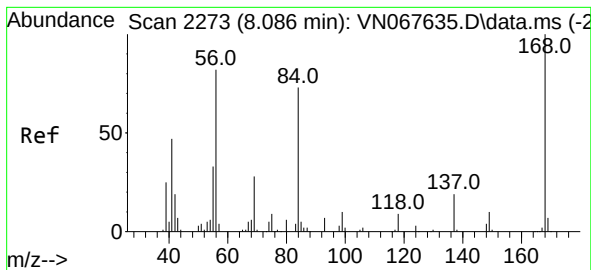

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067669.D





Acq: 8 Jul 2021 17:32

Tgt Ion:168 Resp: 340960

Ion Ratio Lower Upper

168 100

99 64.7 62.9 94.3

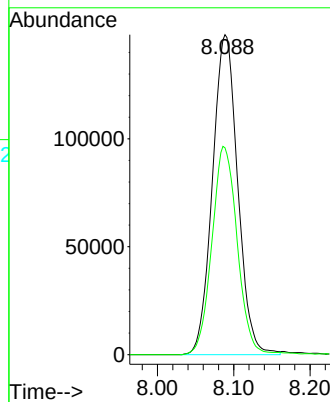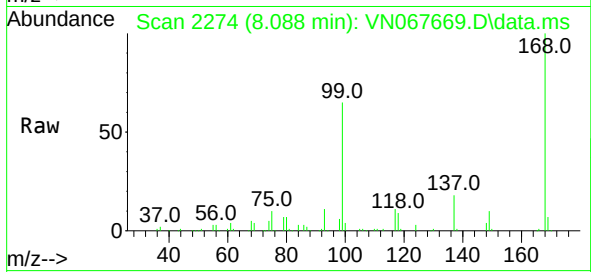

#5

Bromomethane

Concen: Below Cal

RT: 2.829 min Scan# 313

Delta R.T. -0.003 min

Lab File: VN067669.D




Acq: 8 Jul 2021 17:32


Tgt Ion: 94 Resp: 25

Ion Ratio Lower Upper

94 100


96 0.0 73.7 110.5#

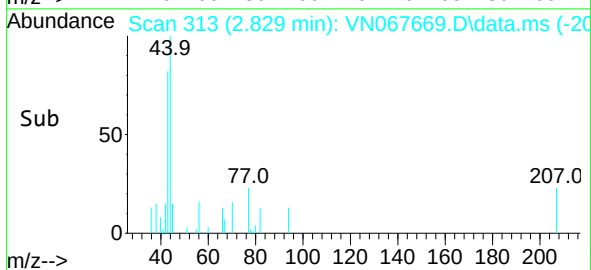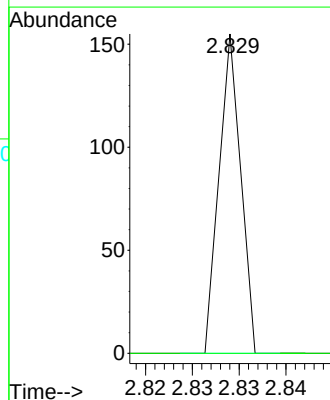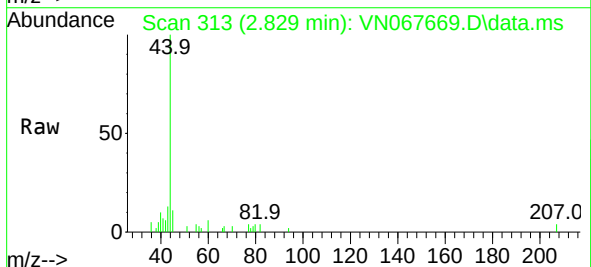






#6
Chloroethane
Concen: Below Cal
RT: 2.998 min Scan# 376
Delta R.T. -0.008 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 64 Resp: 95
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#



#11
Tert butyl alcohol
Concen: 0.381 ug/l
RT: 5.393 min Scan# 1269
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 59 Resp: 282
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


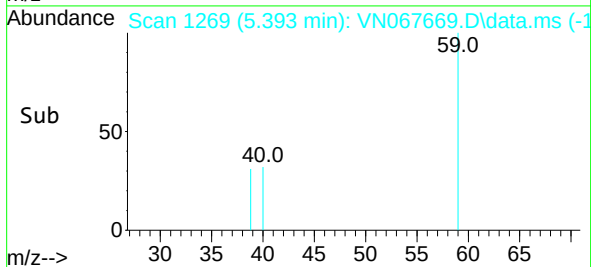

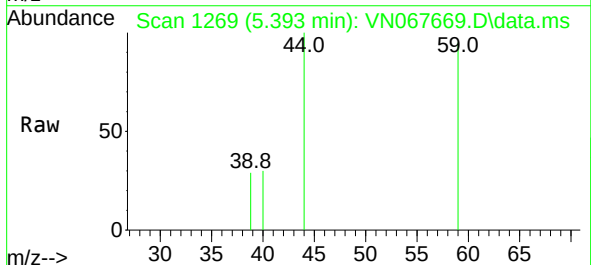




#13
Acrolein
Concen: Below Cal
RT: 4.039 min Scan# 764
Delta R.T. -0.000 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 303
Ion Ratio Lower Upper
56 100
55 59.4 57.4 86.0



#16
Acetone
Concen: 22.142 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.011 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 43 Resp: 35901
Ion Ratio Lower Upper
43 100
58 28.6 21.2 31.8



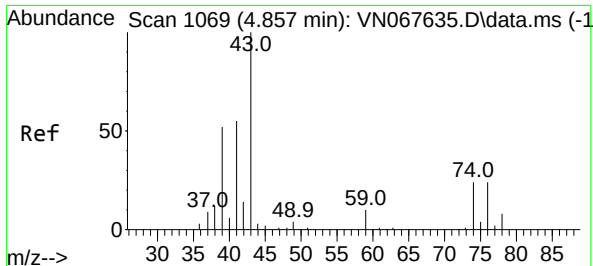

#18

Methyl Acetate

Concen: 0.894 ug/l

RT: 4.873 min Scan# 1075

Delta R.T. 0.016 min

Lab File: VN067669.D





Acq: 8 Jul 2021 17:32

Tgt Ion: 43 Resp: 4071

Ion Ratio Lower Upper

43 100

74 9.2 17.4 26.0#

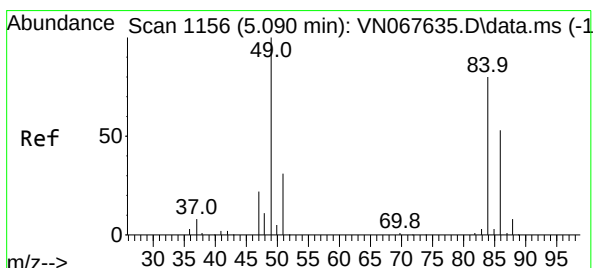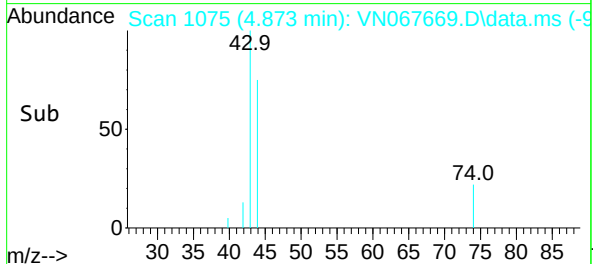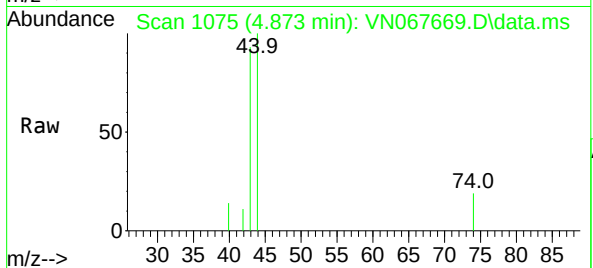

#20

Methylene Chloride

Concen: 7.514 ug/l

RT: 5.093 min Scan# 1157

Delta R.T. 0.003 min

Lab File: VN067669.D

Acq: 8 Jul 2021 17:32

Tgt Ion: 84 Resp: 30681




Ion Ratio Lower Upper


84 100

49 121.9 110.9 166.3

51 40.0 32.6 49.0

86 61.4 51.6 77.4


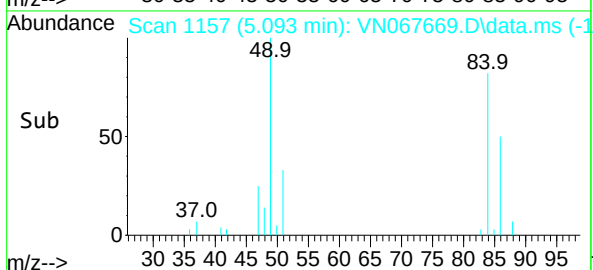

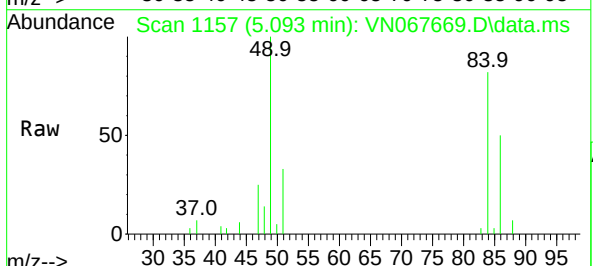


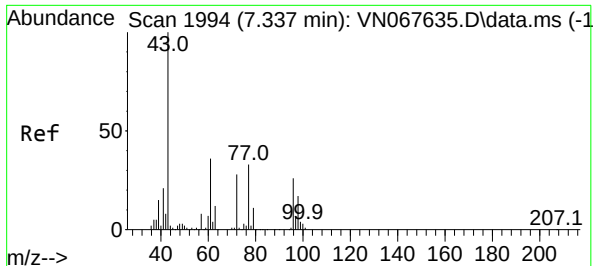

#25
2-Butanone
Concen: 4.026 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.014 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 10840
Ion Ratio Lower Upper
43 100
72 26.7 19.7 29.5

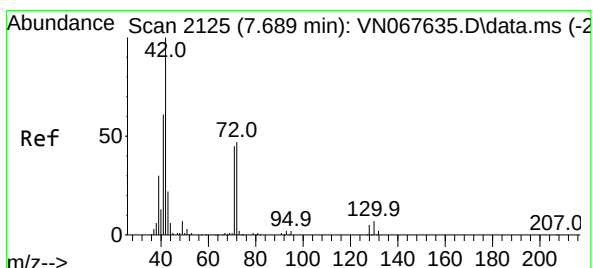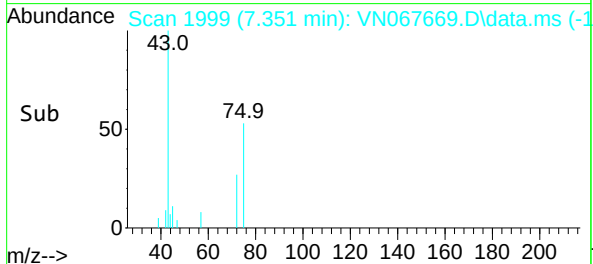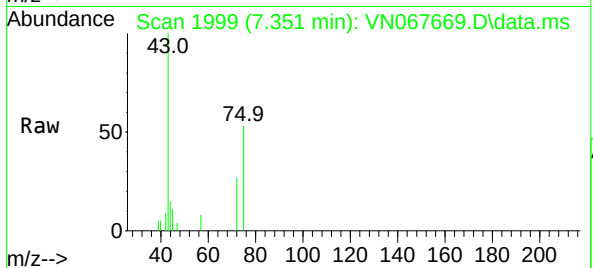

#29
Tetrahydrofuran
Concen: 1.344 ug/l
RT: 7.708 min Scan# 2132
Delta R.T. 0.019 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 42 Resp: 2380
Ion Ratio Lower Upper
42 100
72 34.2 32.8 49.2
71 37.3 31.2 46.8


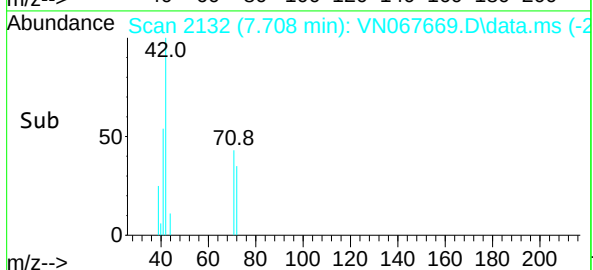

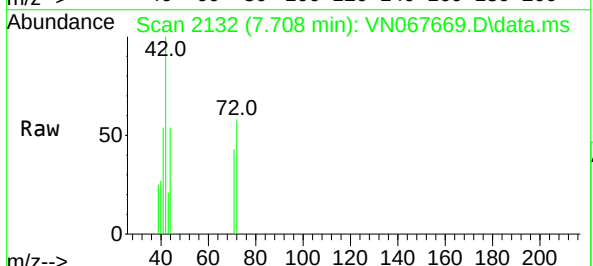




#31
Cyclohexane
Concen: 1.328 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 9598
Ion Ratio Lower Upper
56 100
69 130.9 27.3 40.9#
84 102.9 64.9 97.3#

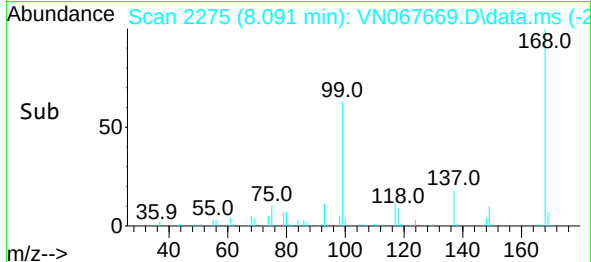

#33
1,2-Dichloroethane-d4
Concen: 53.512 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 65 Resp: 275746
Ion Ratio Lower Upper
65 100
67 50.6 0.0 98.6


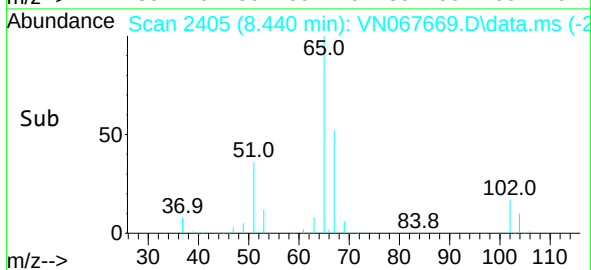






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 651969
Ion Ratio Lower Upper
114 100
63 22.2 0.0 49.0
88 15.1 0.0 36.6

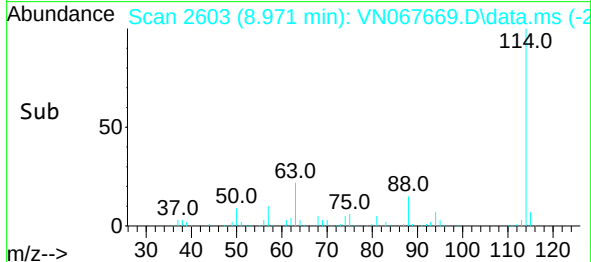

#35
Dibromofluoromethane
Concen: 49.573 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32


Tgt Ion:113 Resp: 195270
Ion Ratio Lower Upper
113 100
111 103.3 83.8 125.8
192 16.2 13.4 20.0

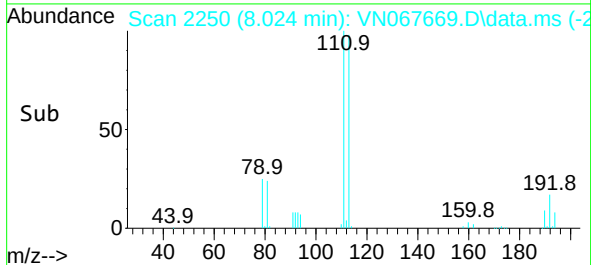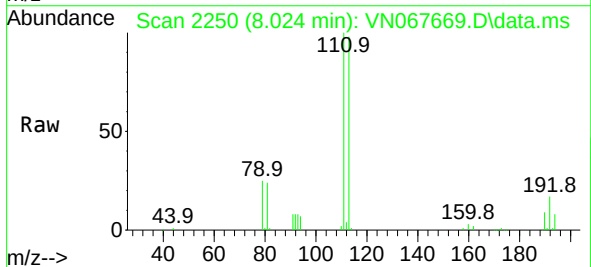






#36
1,1-Dichloropropene
Concen: 5.371 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 32529
Ion Ratio Lower Upper
75 100
110 9.4 15.7 47.0#
77 0.0 24.6 37.0#



#37
Ethyl Acetate
Concen: 1.847 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.067 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32


Tgt Ion: 43 Resp: 10840
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.1 12.1#

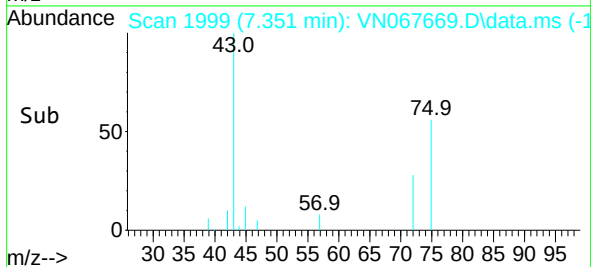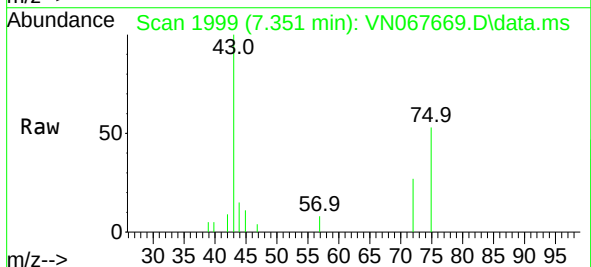



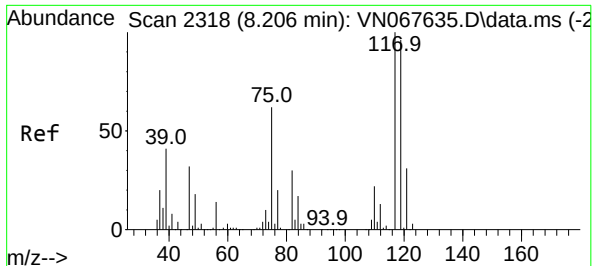


#38
Carbon Tetrachloride
Concen: 6.353 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32


Instrument :
MSVOA_N
ClientSampleId :

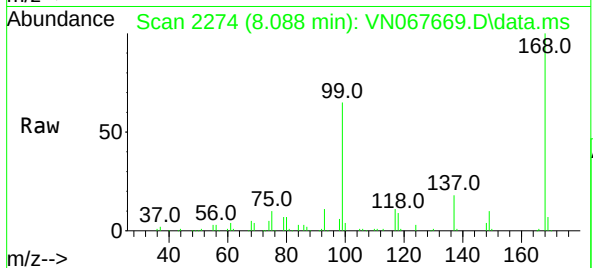



Tgt Ion:117 Resp: 37952
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.2#
121 0.0 23.5 35.3#

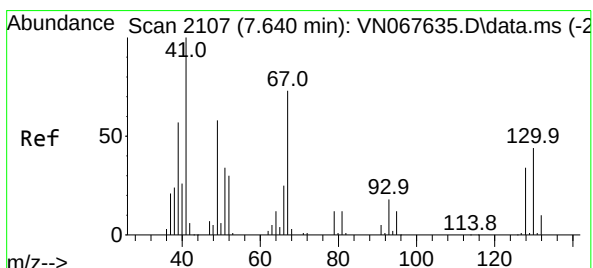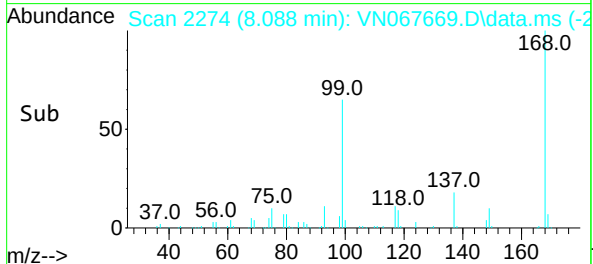


#41
Methacrylonitrile
Concen: 0.245 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.054 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

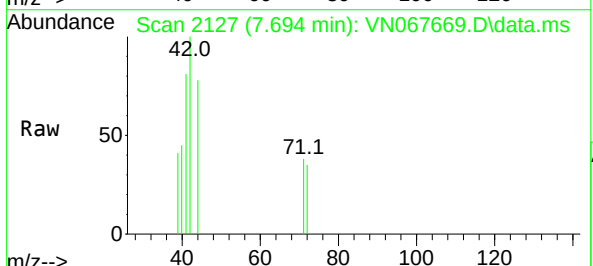


Tgt Ion: 41 Resp: 739
Ion Ratio Lower Upper
41 100
39 71.7 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#

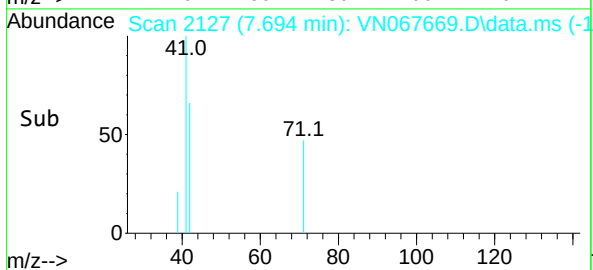






#43
Isopropyl Acetate
Concen: 4.783 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 43 Resp: 49373
Ion Ratio Lower Upper
43 100
61 17.1 19.0 28.4#
87 11.1 9.5 14.3




#45
1,2-Dichloropropane
Concen: 0.688 ug/l
RT: 9.633 min Scan# 2850
Delta R.T. 0.142 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

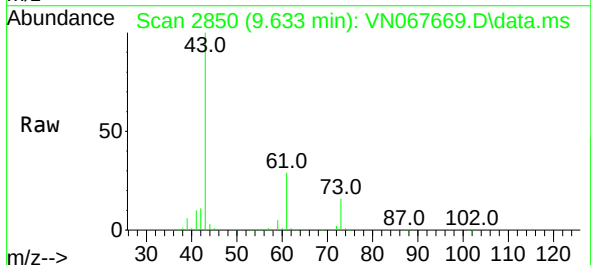

Tgt Ion: 63 Resp: 3160
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

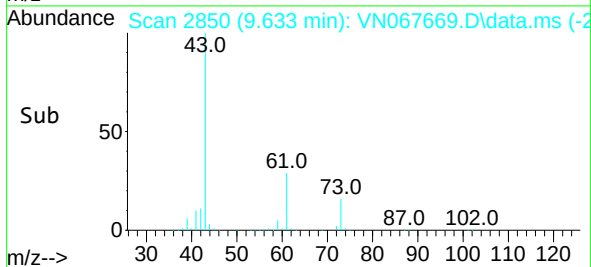



#48

Methyl methacrylate

Concen: 2.377 ug/l

RT: 9.550 min Scan# 2819

Delta R.T. -0.013 min

Lab File: VN067669.D

Acq: 8 Jul 2021 17:32





Tgt Ion: 41 Resp: 10852

Ion Ratio Lower Upper

41 100

69 0.0 64.6 96.8#

39 0.0 53.3 79.9#



#49

1,4-Dioxane

Concen: 33.753 ug/l

RT: 9.620 min Scan# 2845

Delta R.T. 0.049 min

Lab File: VN067669.D

Acq: 8 Jul 2021 17:32




Tgt Ion: 88 Resp: 152


Ion Ratio Lower Upper

88 100

43 0.0 28.8 43.2#

58 0.0 60.4 90.6#


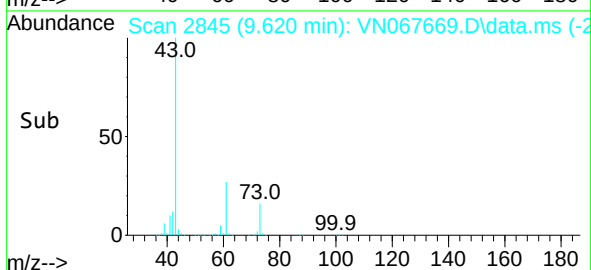




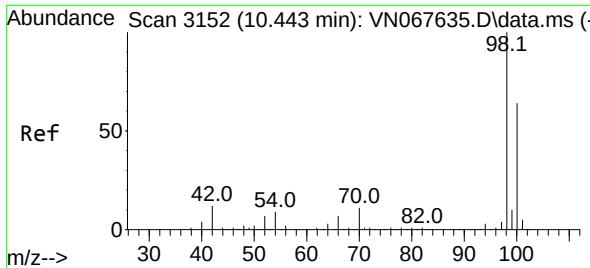

#50
Toluene-d8
Concen: 52.940 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 872860
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

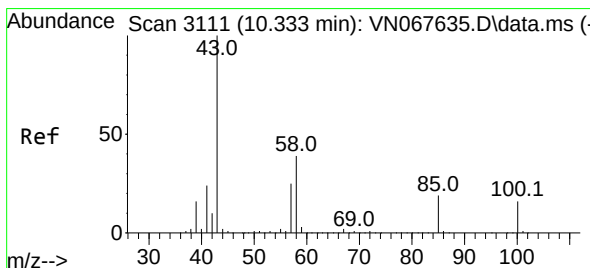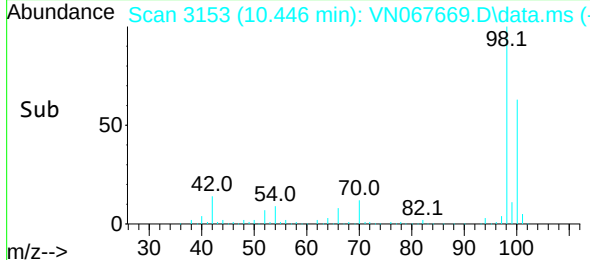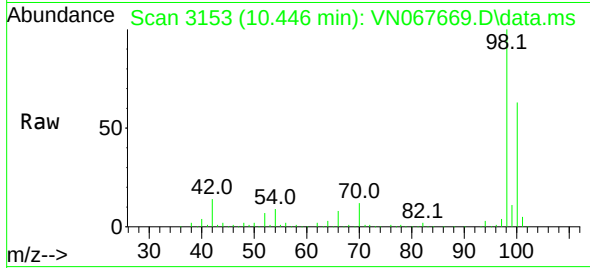

#51
4-Methyl-2-Pentanone
Concen: 1.262 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 43 Resp: 8003
Ion Ratio Lower Upper
43 100
58 54.7 28.6 43.0#


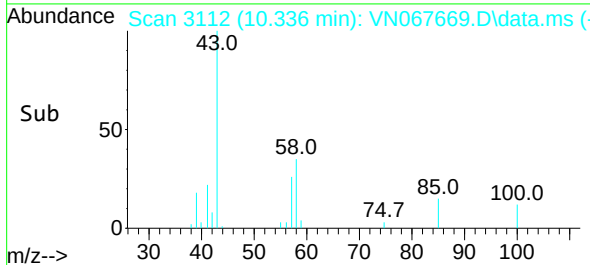

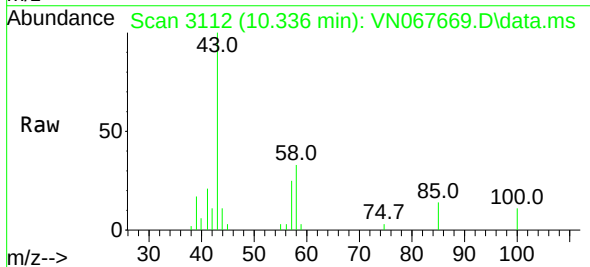




#53
t-1,3-Dichloropropene
Concen: 1.751 ug/l
RT: 10.448 min Scan# 3154
Delta R.T. -0.274 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 51
Ion Ratio Lower Upper
75 100
77 181.0 25.1 37.7#

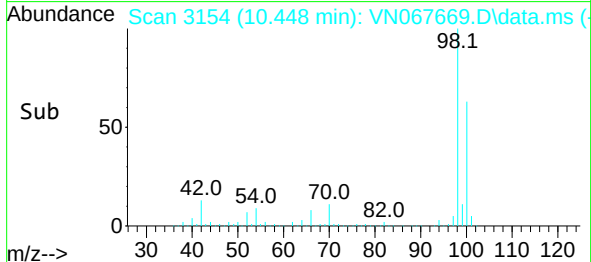

#54
cis-1,3-Dichloropropene
Concen: 10.972 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 75 Resp: 77686
Ion Ratio Lower Upper
75 100
77 0.8 24.6 37.0#
39 41.4 50.7 76.1#


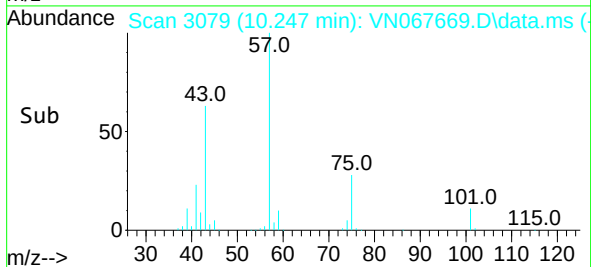

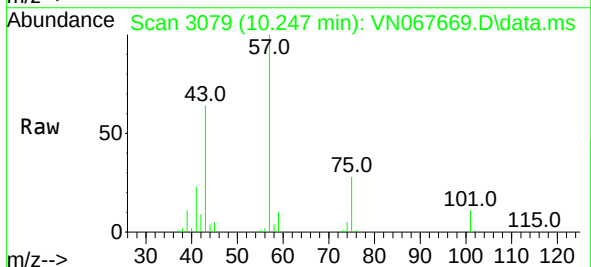




#57
1,3-Dichloropropane
Concen: 6.065 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 47328
Ion Ratio Lower Upper
76 100
78 0.1 25.7 38.5#

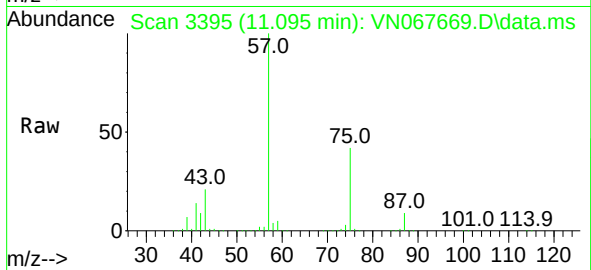

#59
2-Hexanone
Concen: 161.610 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 43 Resp: 715338
Ion Ratio Lower Upper
43 100
58 18.0 24.7 74.1#


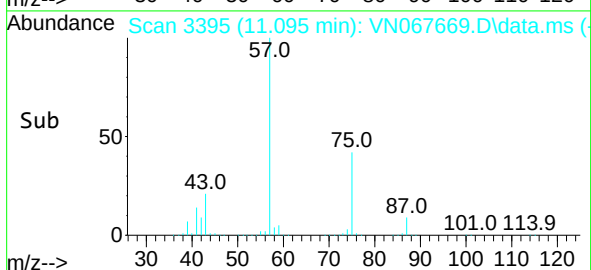

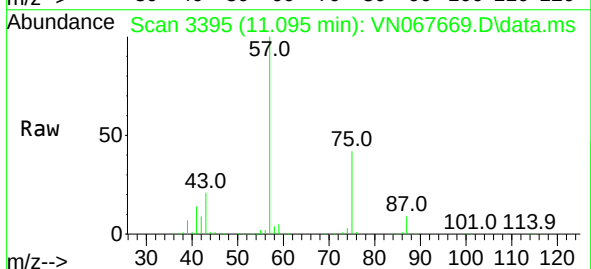




#60
Dibromochloromethane
Concen: 2.441 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.250 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 492
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

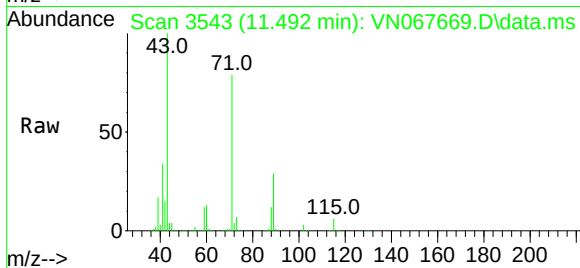

#62
4-Bromofluorobenzene
Concen: 52.535 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion: 95 Resp: 305984
Ion Ratio Lower Upper
95 100
174 71.1 0.0 122.0
176 67.8 0.0 117.6


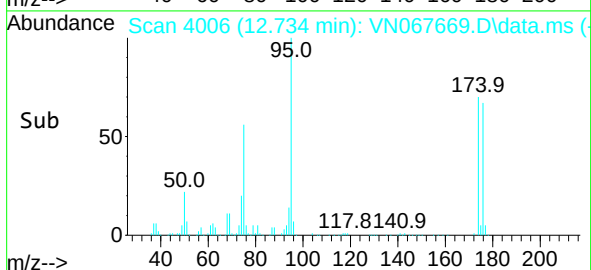

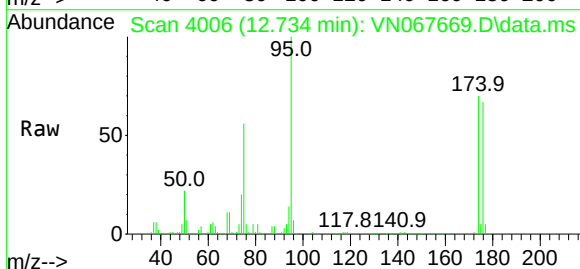


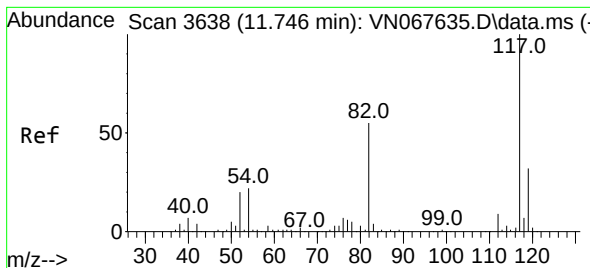

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 698407
Ion Ratio Lower Upper
117 100
82 57.0 53.1 79.7
119 32.0 25.5 38.3

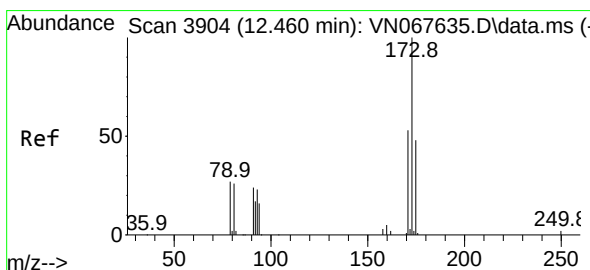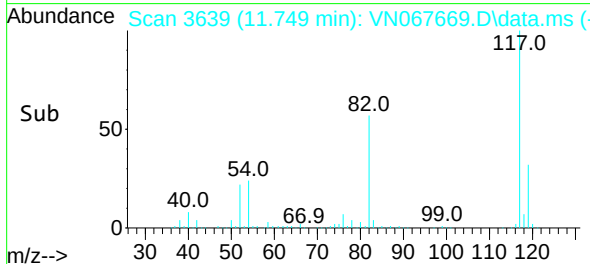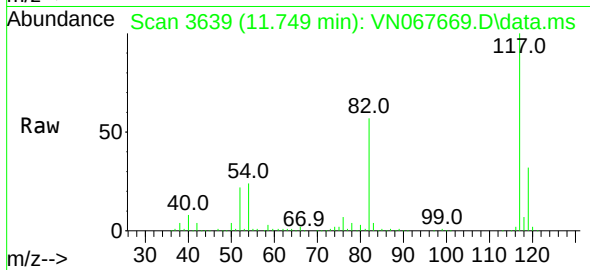

#71
Bromoform
Concen: 3.318 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.271 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion:173 Resp: 680
Ion Ratio Lower Upper
173 100
175 2213.4 23.9 71.8#
254 0.0 0.0 0.0


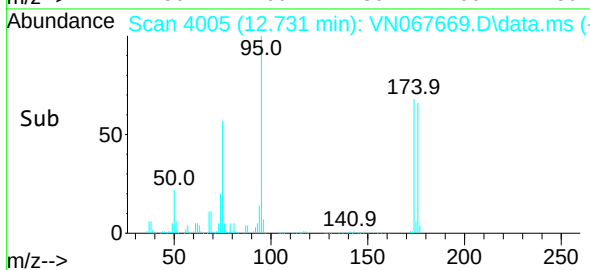

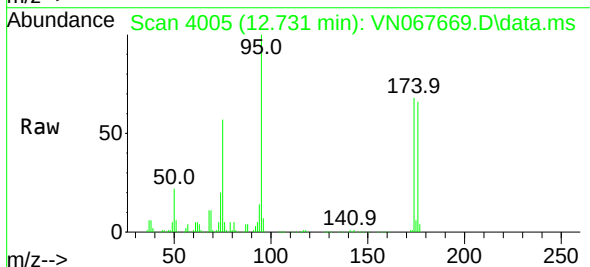


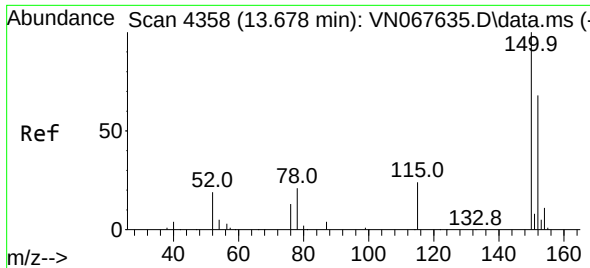

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. 0.000 min
 Lab File: VN067669.D
 Acq: 8 Jul 2021 17:32




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 256406
 Ion Ratio Lower Upper
 152 100
 115 63.2 36.1 108.5
 150 159.2 0.0 351.8

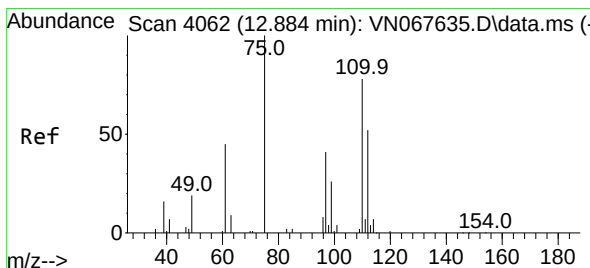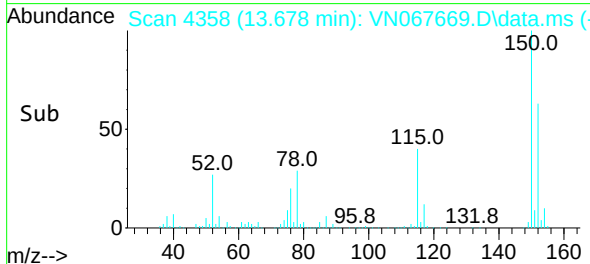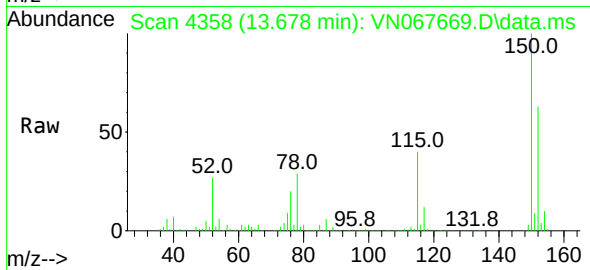

#76
 1,2,3-Trichloropropane
 Concen: 33.055 ug/l
 RT: 12.734 min Scan# 4006
 Delta R.T. -0.150 min
 Lab File: VN067669.D
 Acq: 8 Jul 2021 17:32

Tgt Ion: 75 Resp: 173087
 Ion Ratio Lower Upper
 75 100
 77 0.9 0.0 0.0#


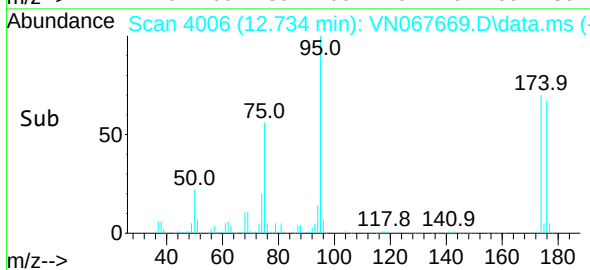

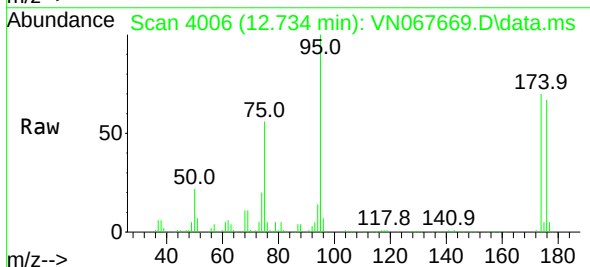




#81
trans-1,4-Dichloro-2-butene
Concen: 106.574 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 173087
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

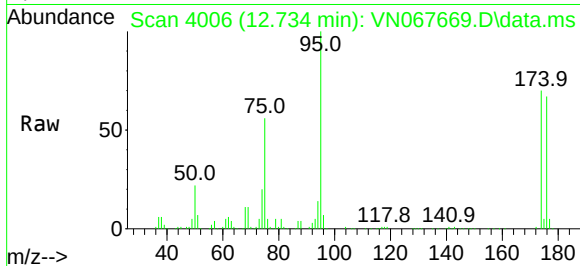

#93
1,2,4-Trichlorobenzene
Concen: 2.720 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion:180 Resp: 205
Ion Ratio Lower Upper
180 100
182 137.1 47.5 142.5
145 0.0 17.2 51.6#


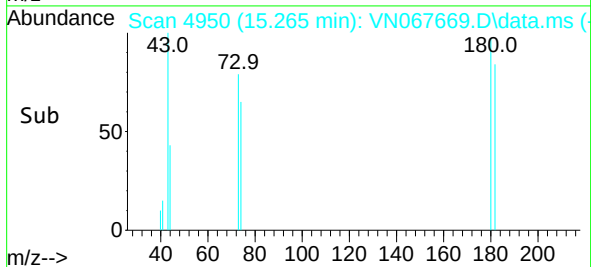

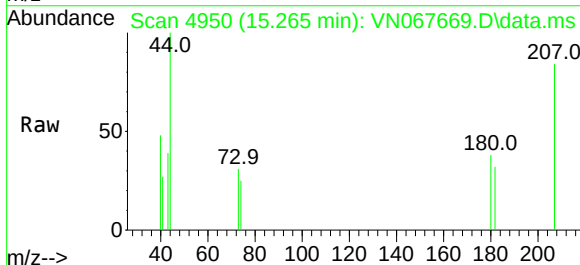




#95
Naphthalene
Concen: 3.174 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128 Resp: 2161
Ion Ratio Lower Upper
128 100
127 2.5 10.6 15.8#
129 0.0 8.6 12.8#

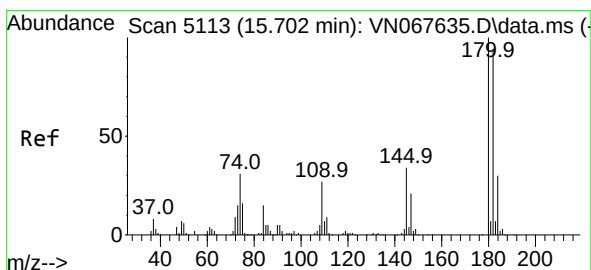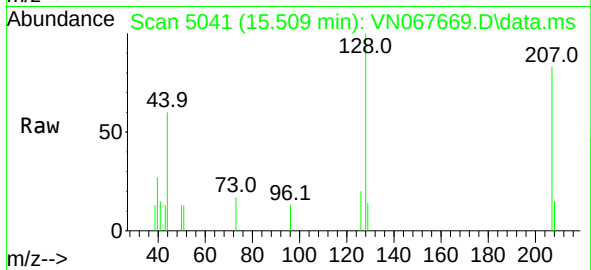

#96
1,2,3-Trichlorobenzene
Concen: 2.692 ug/l
RT: 15.705 min Scan# 5114
Delta R.T. 0.003 min
Lab File: VN067669.D
Acq: 8 Jul 2021 17:32

Tgt Ion:180 Resp: 256
Ion Ratio Lower Upper
180 100
182 84.4 47.8 143.3
145 0.0 18.2 54.6#

