

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN070822\  
Data File : VN073405.D  
Acq On : 08 Jul 2022 20:11  
Operator : JC\MD  
Sample : N3642-05  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M

Title : SW846 8260

Signal : TIC: VN073405.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 7.951       | 1021          | 1031        | 1036         | rBV      | 204401         | 489541        | 36.12%          | 6.077%        |
| 2         | 8.016       | 1036          | 1042        | 1055         | rVB      | 376249         | 860490        | 63.48%          | 10.682%       |
| 3         | 8.369       | 1088          | 1102        | 1115         | rBV      | 216880         | 507095        | 37.41%          | 6.295%        |
| 4         | 8.904       | 1184          | 1193        | 1209         | rBV      | 549300         | 1115322       | 82.28%          | 13.846%       |
| 5         | 10.380      | 1435          | 1444        | 1458         | rBV      | 729320         | 1335622       | 98.54%          | 16.580%       |
| 6         | 11.680      | 1656          | 1665        | 1679         | rBV      | 745234         | 1355452       | 100.00%         | 16.827%       |
| 7         | 12.669      | 1826          | 1833        | 1843         | rBV      | 623621         | 1059523       | 78.17%          | 13.153%       |
| 8         | 13.610      | 1986          | 1993        | 2003         | rBV      | 777822         | 1332383       | 98.30%          | 16.540%       |




Sum of corrected areas: 8055428

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN070822\  
Data File : VN073405.D  
Acq On : 08 Jul 2022 20:11  
Operator : JC\MD  
Sample : N3642-05  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

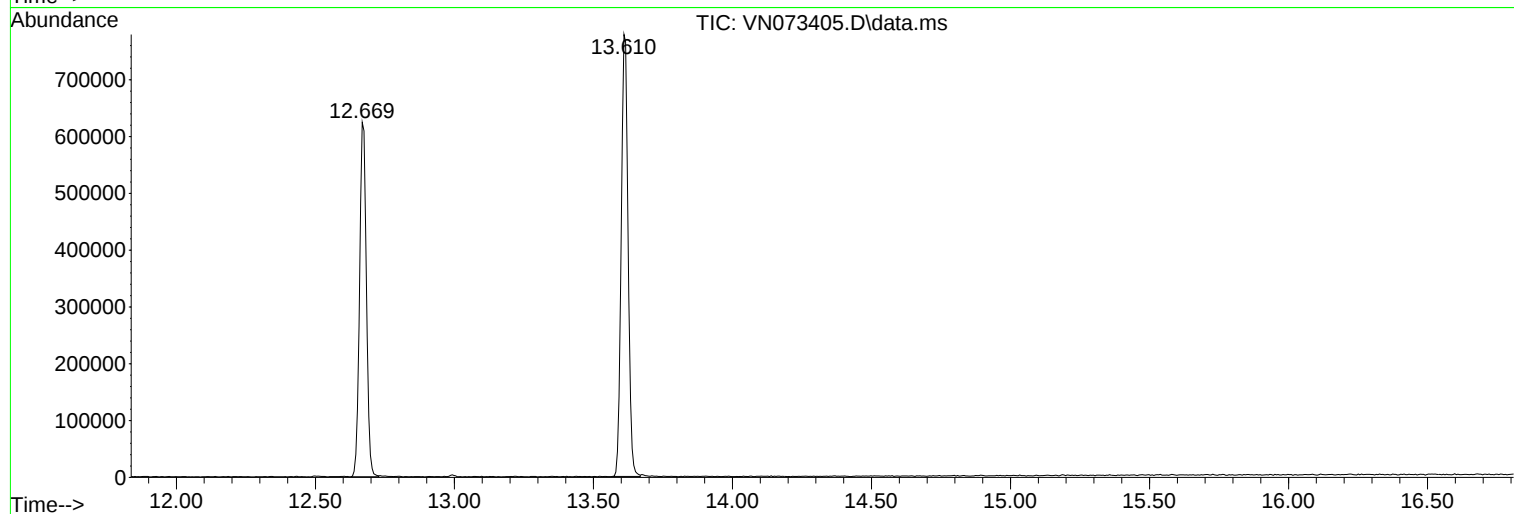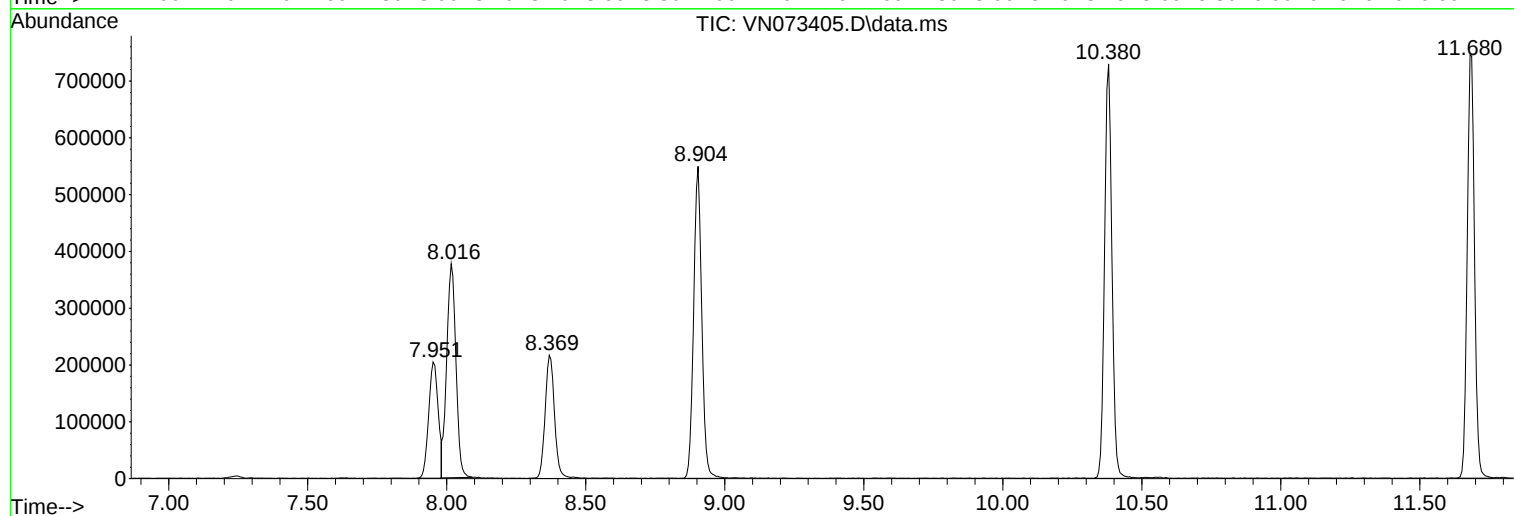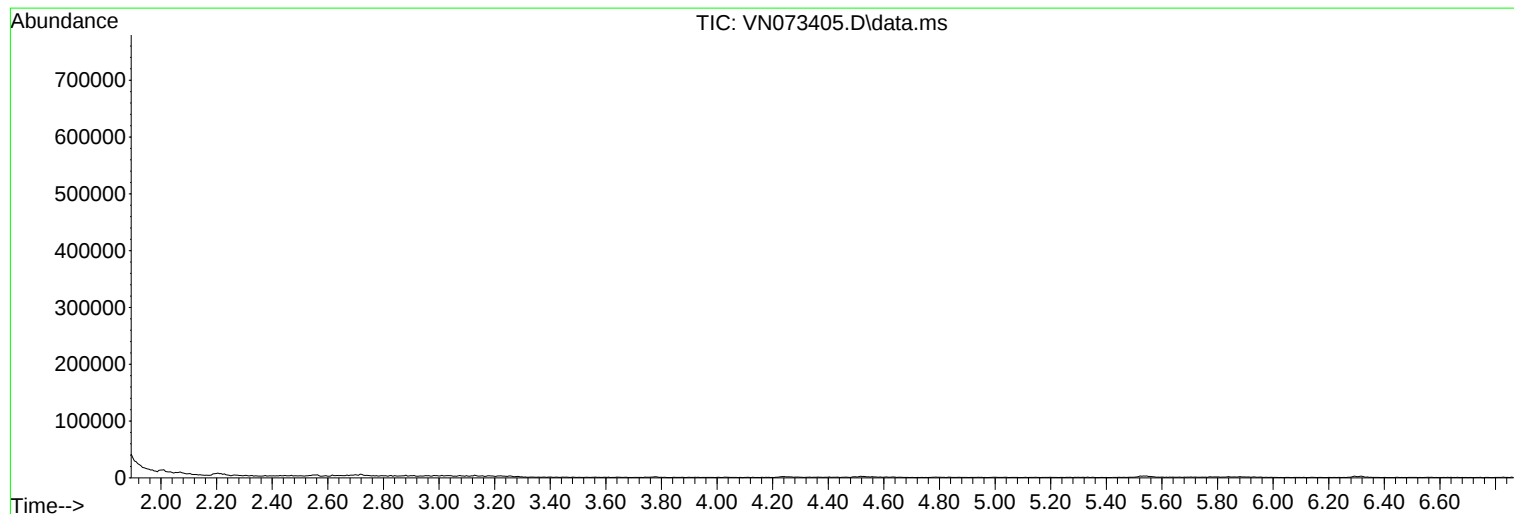

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN070822\  
Data File : VN073405.D  
Acq On : 08 Jul 2022 20:11  
Operator : JC\MD  
Sample : N3642-05  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN070822\  
Data File : VN073405.D  
Acq On : 08 Jul 2022 20:11  
Operator : JC\MD  
Sample : N3642-05  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|