
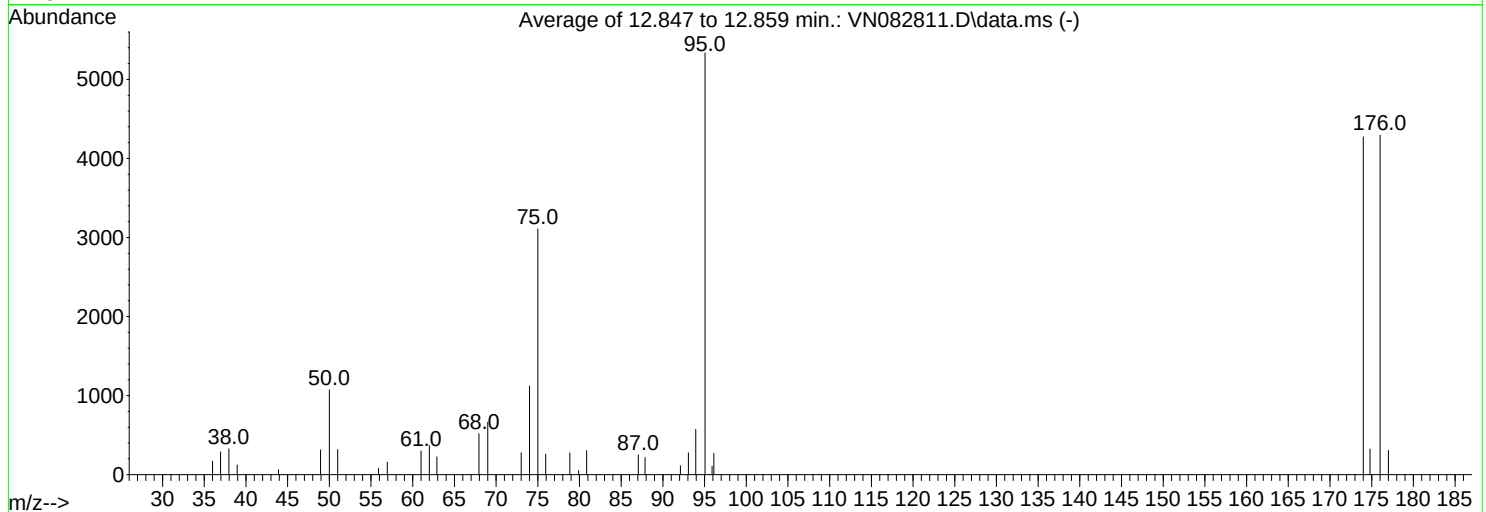


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070824\
Data File : VN082811.D
Acq On : 08 Jul 2024 09:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

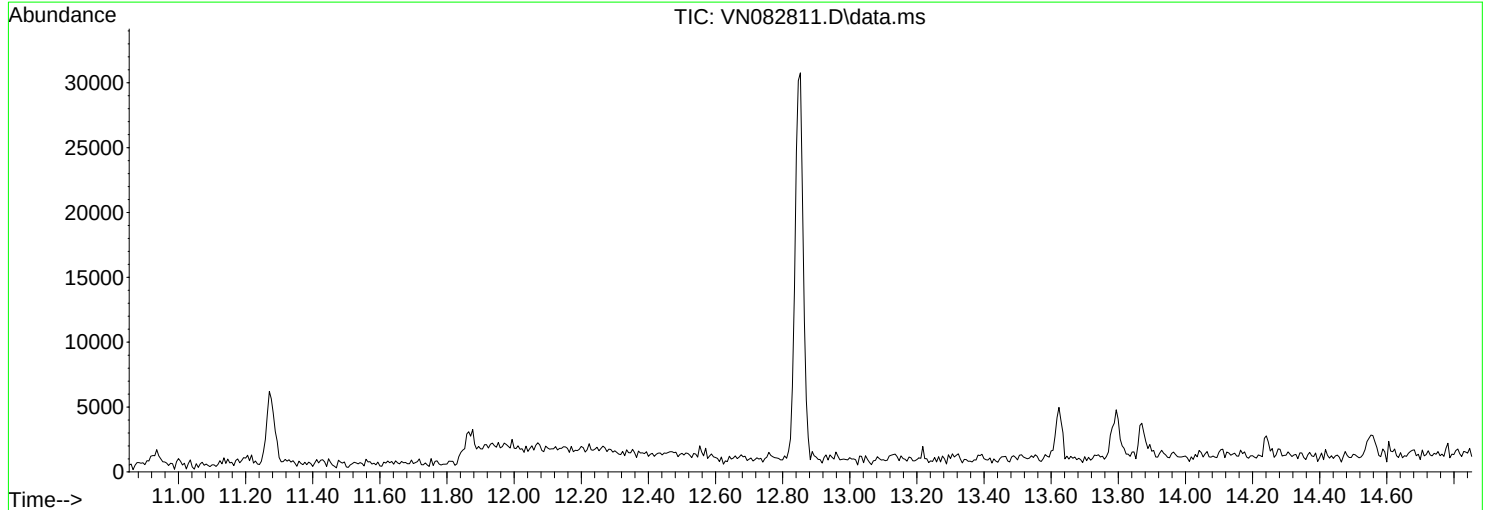

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	1073	PASS
75	95	30	60	58.3	3109	PASS
95	95	100	100	100.0	5336	PASS
96	95	5	9	5.1	270	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.1	4274	PASS
175	174	5	9	7.6	323	PASS
176	174	95	101	100.5	4295	PASS
177	176	5	9	7.2	308	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	172	62.00	368	87.05	251	177.00	301
36.95	289	62.90	225	87.85	216		
37.95	325	67.95	517	92.10	113		
38.95	122	69.00	663	93.05	275		
43.90	60	73.00	278	93.95	572		
48.95	314	74.00	1121	95.05	5336		
50.00	1073	75.00	3109	95.90	105		
51.00	318	75.95	260	96.10	270		
55.90	78	78.85	275	174.00	4274		
56.95	159	79.90	51	174.80	323		
61.00	300	80.85	304	176.00	4295		

Instrument :

MSVOA_N

ClientSampleId :

BFB