

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070825\
 Data File : VN087301.D
 Acq On : 08 Jul 2025 15:57
 Operator : JC\MD
 Sample : Q2480-06 1000X
 Misc : 6.16g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 GPX6

Quant Time: Jul 09 01:34:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:15:00 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	215311	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	426299	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	422033	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	194412	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	156850	58.044	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	116.080%
35) Dibromofluoromethane	8.171	113	135569	49.666	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.340%
50) Toluene-d8	10.565	98	549365	51.634	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.260%
62) 4-Bromofluorobenzene	12.847	95	180309	47.630	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	95.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070825\
Data File : VN087301.D
Acq On : 08 Jul 2025 15:57
Operator : JC\MD
Sample : Q2480-06 1000X
Misc : 6.16g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
GPX6

Quant Time: Jul 09 01:34:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:15:00 2025
Response via : Initial Calibration




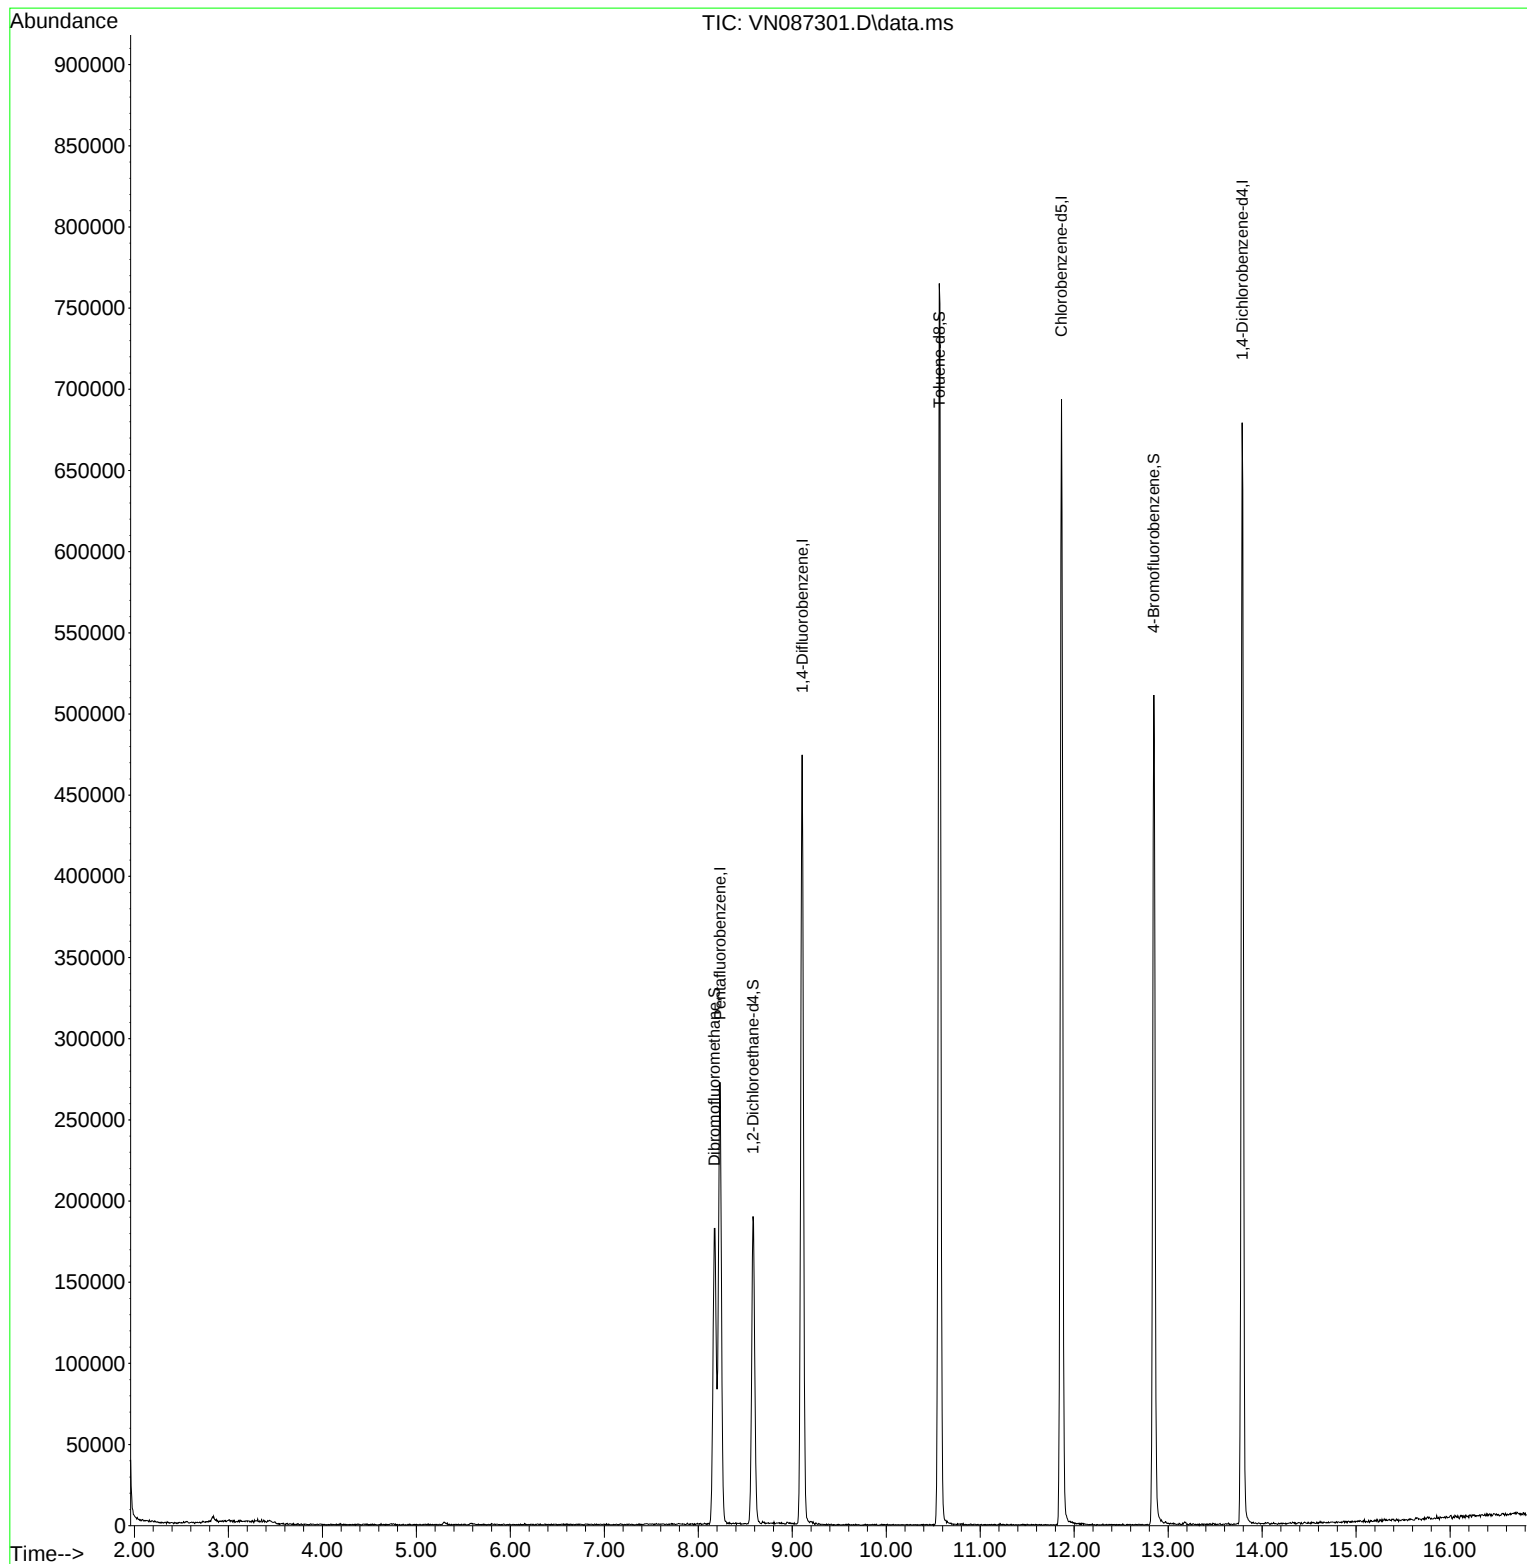


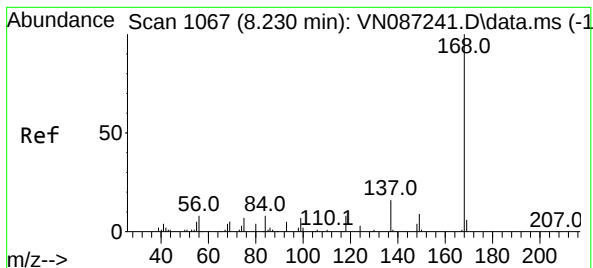

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.001 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57




Instrument :
MSVOA_N
ClientSampleId :
GPX6


Tgt Ion:168 Resp: 215311
Ion Ratio Lower Upper
168 100
99 55.6 42.6 64.0

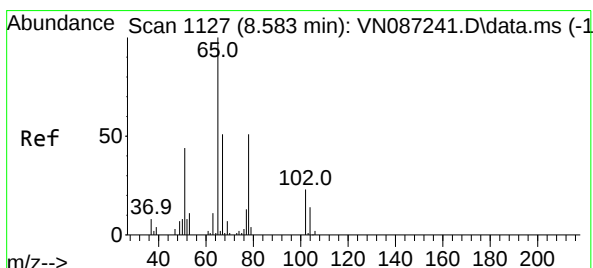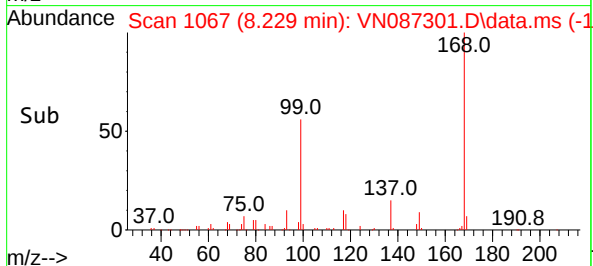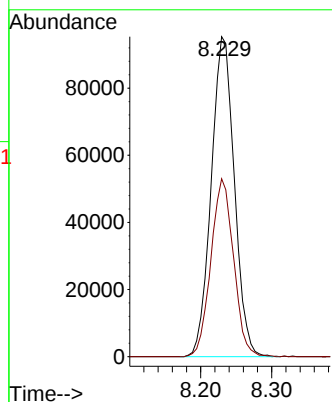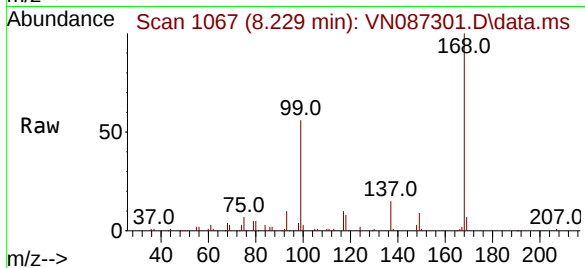

#33
1,2-Dichloroethane-d4
Concen: 58.044 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57

Tgt Ion: 65 Resp: 156850
Ion Ratio Lower Upper
65 100
67 50.5 0.0 102.6


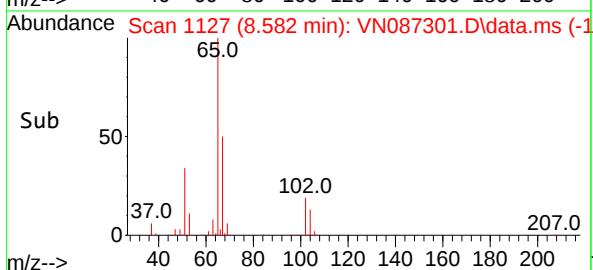
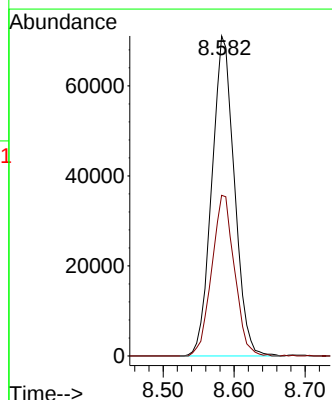
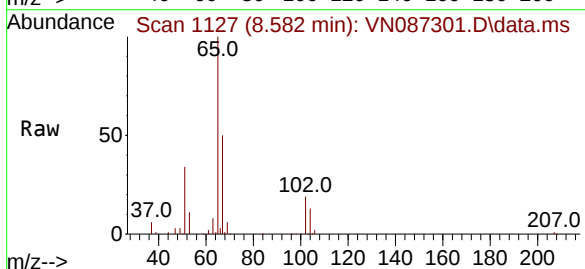


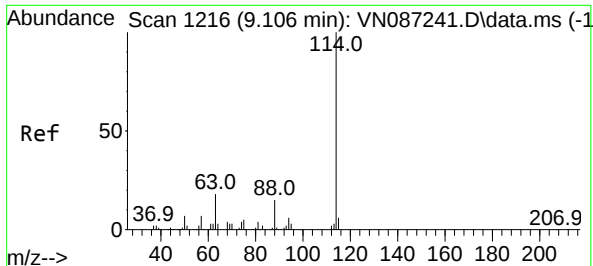

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57




Instrument :
MSVOA_N
ClientSampleId :
GPX6


Tgt Ion:114 Resp: 426299
Ion Ratio Lower Upper
114 100
63 18.4 0.0 36.6
88 14.5 0.0 29.6

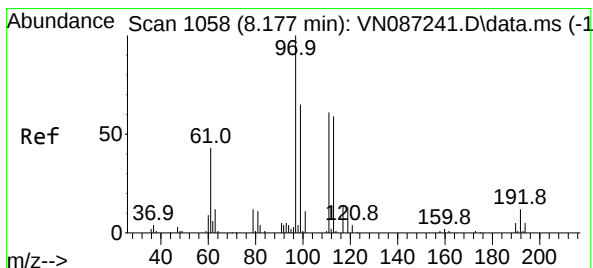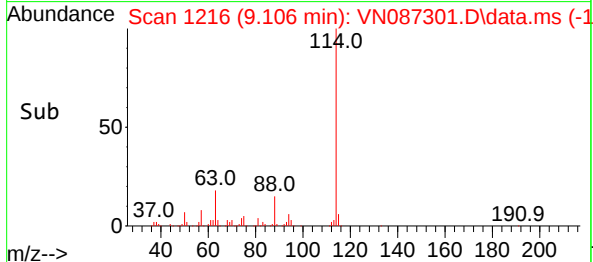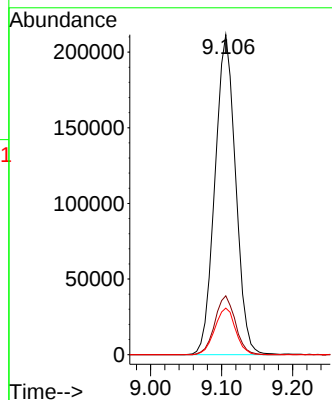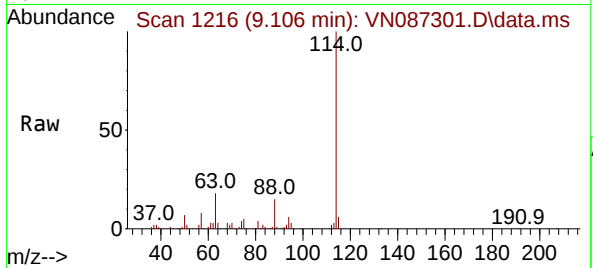

#35
Dibromofluoromethane
Concen: 49.666 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57

Tgt Ion:113 Resp: 135569
Ion Ratio Lower Upper
113 100
111 103.6 81.4 122.2
192 19.3 15.1 22.7


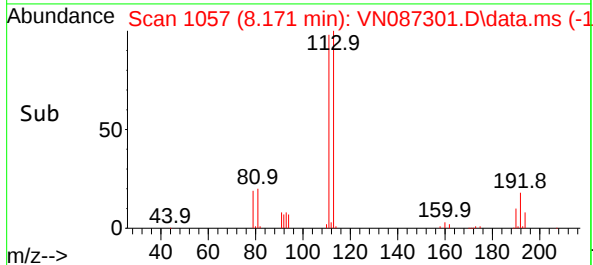
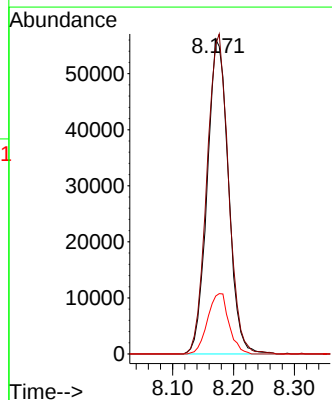
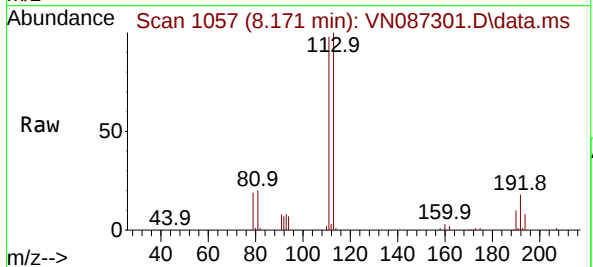


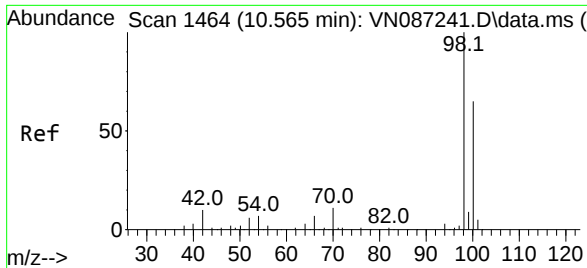

#50
Toluene-d8
Concen: 51.634 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57




Instrument :
MSVOA_N
ClientSampleId :
GPX6


Tgt Ion: 98 Resp: 549365
Ion Ratio Lower Upper
98 100
100 63.7 52.1 78.1

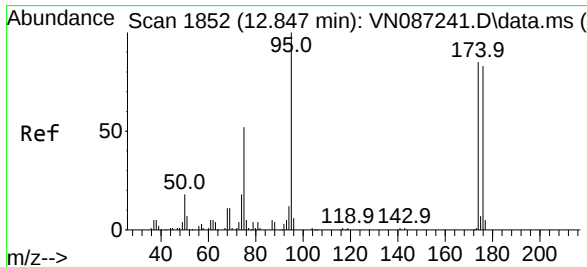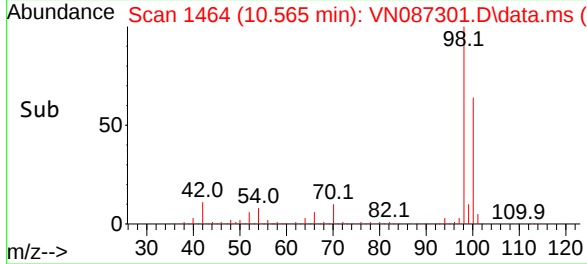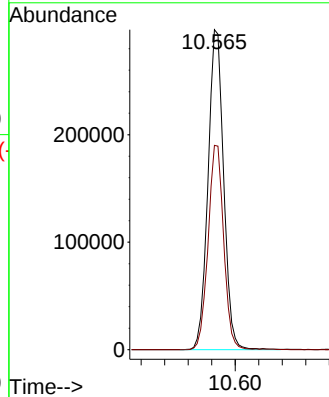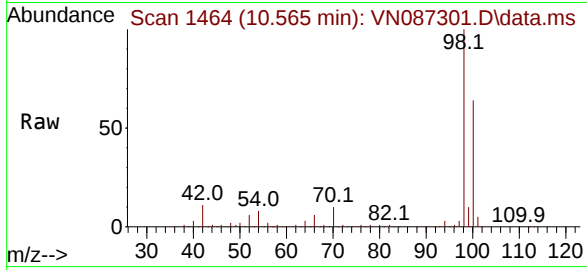

#62
4-Bromofluorobenzene
Concen: 47.630 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57

Tgt Ion: 95 Resp: 180309
Ion Ratio Lower Upper
95 100
174 84.9 0.0 169.6
176 80.7 0.0 161.6


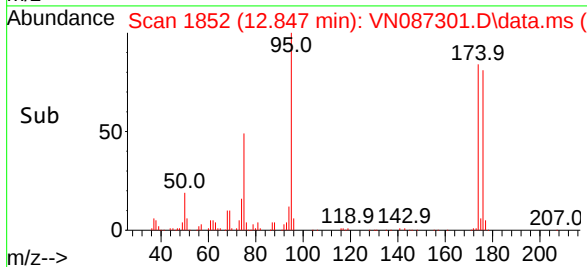
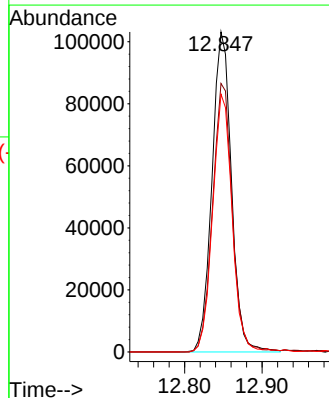
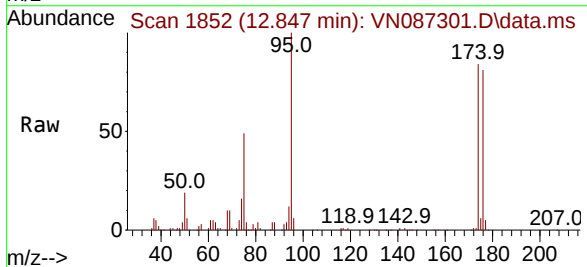


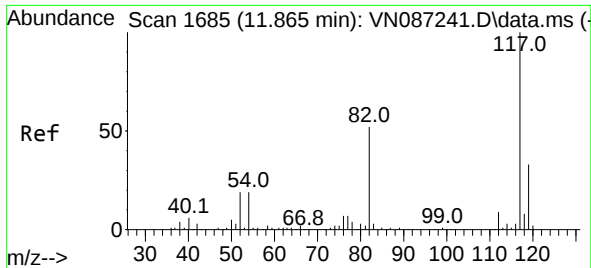

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57

Instrument :
MSVOA_N
ClientSampleId :
GPX6

Tgt Ion:117 Resp: 422033
Ion Ratio Lower Upper
117 100
82 51.8 41.9 62.9
119 31.7 26.2 39.4

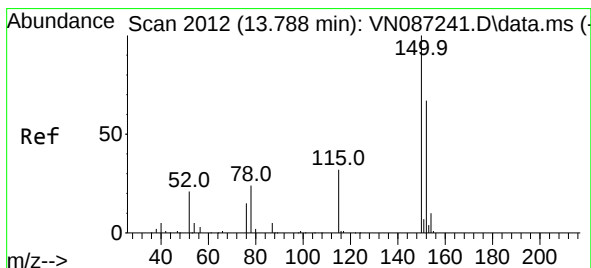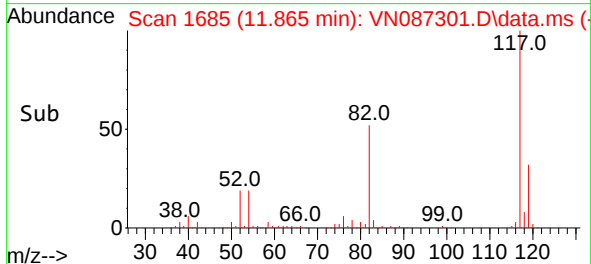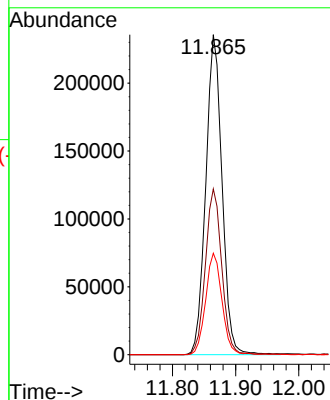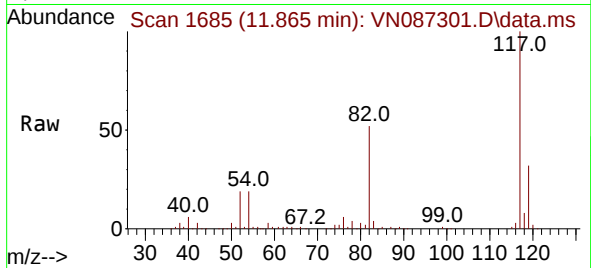

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN087301.D
Acq: 08 Jul 2025 15:57

Tgt Ion:152 Resp: 194412
Ion Ratio Lower Upper
152 100
115 57.7 28.3 84.9
150 157.8 0.0 344.6

