

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070825\
 Data File : VN087304.D
 Acq On : 08 Jul 2025 17:00
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jul 09 01:34:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:15:00 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	300024	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	593922	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	359599	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	255360	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	251591	66.815	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	133.640%#
35) Dibromofluoromethane	8.171	113	202843	53.339	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.680%
50) Toluene-d8	10.571	98	724491	48.876	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.760%
62) 4-Bromofluorobenzene	12.847	95	220885	41.881	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	83.760%
Target Compounds						
20) Methylene Chloride	5.294	84	11239	3.524	ug/l	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070825\
Data File : VN087304.D
Acq On : 08 Jul 2025 17:00
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jul 09 01:34:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:15:00 2025
Response via : Initial Calibration




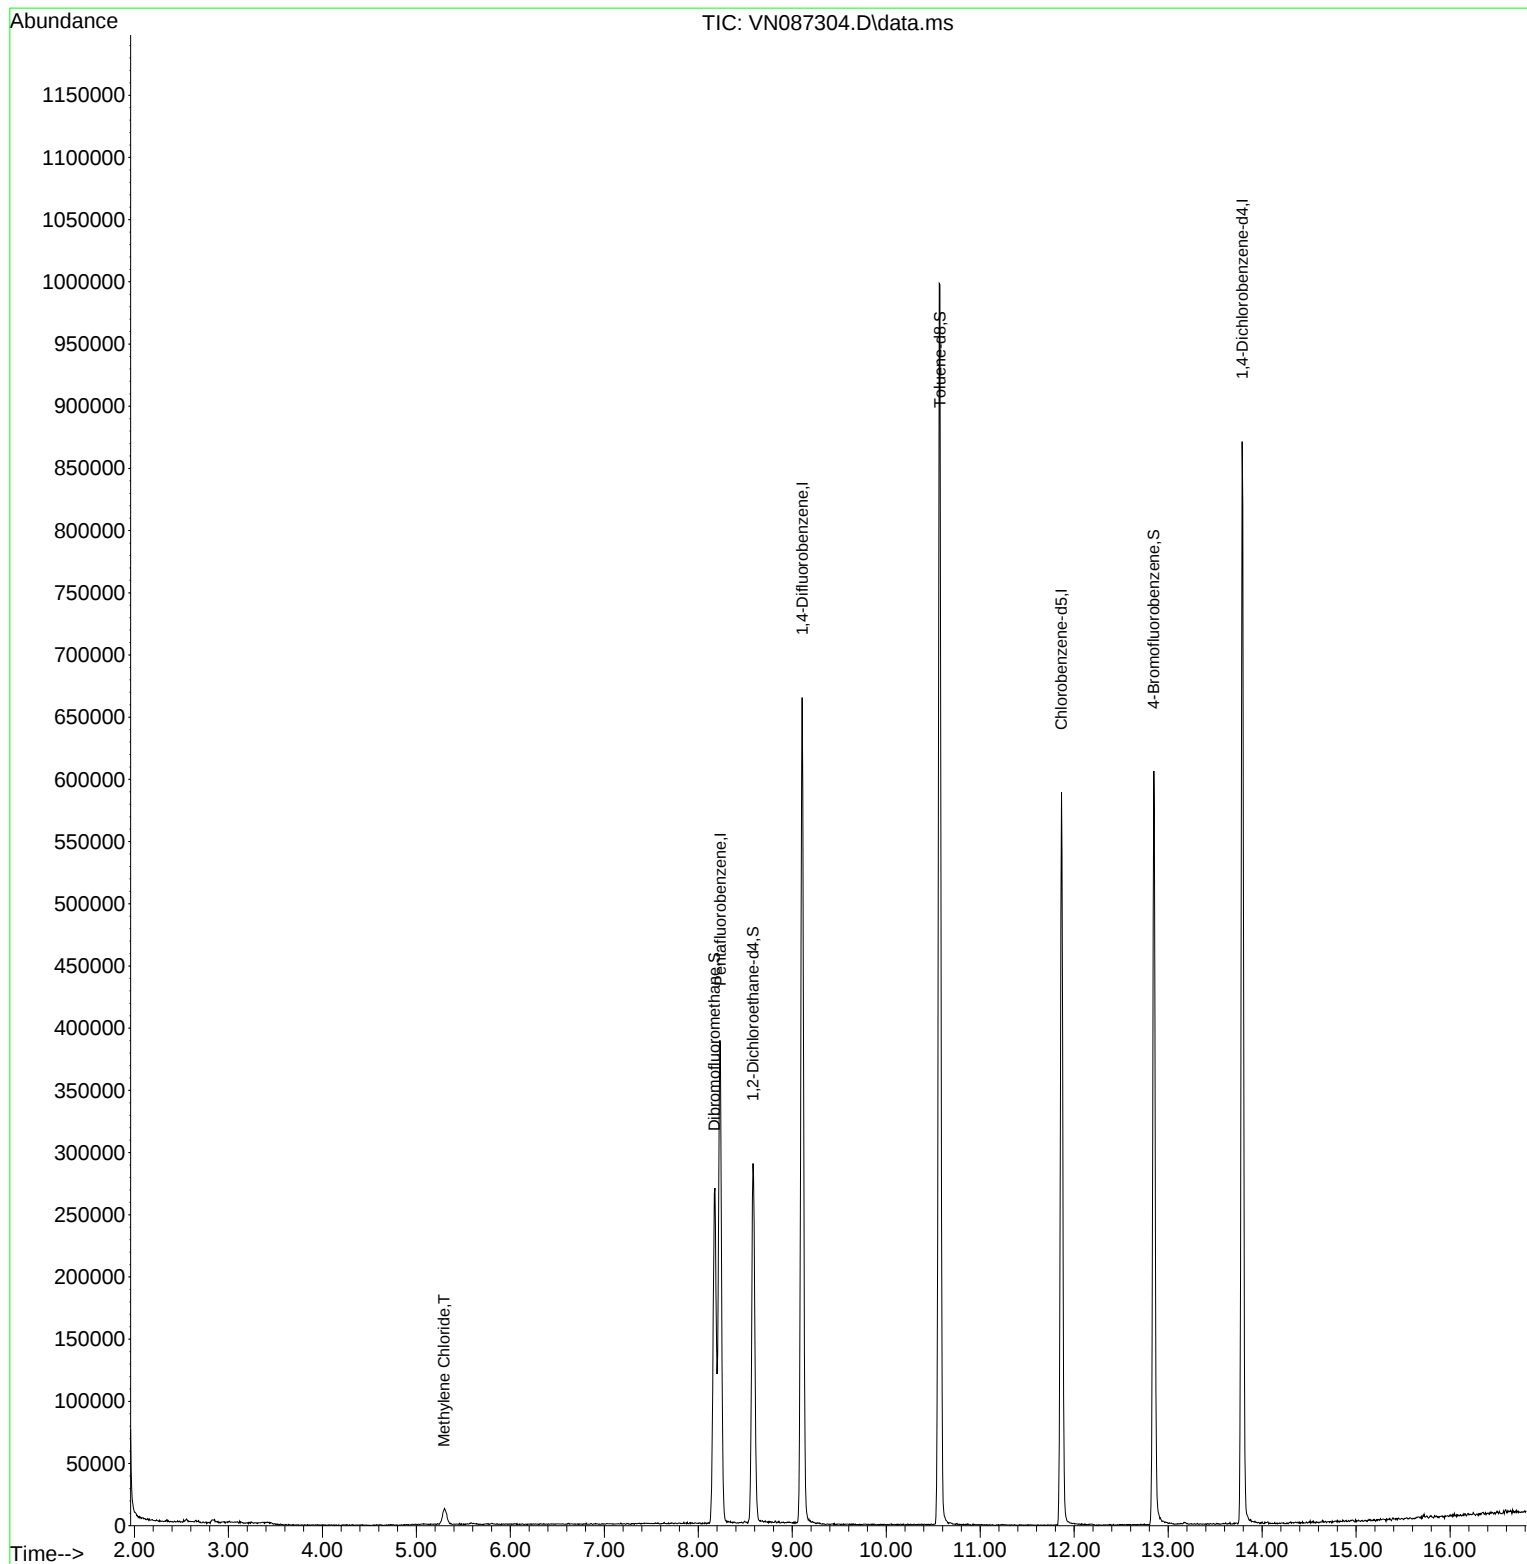


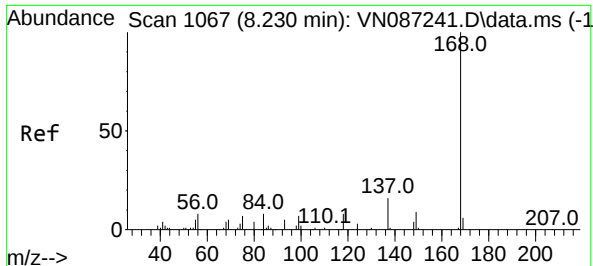

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1067
Delta R.T. 0.005 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 300024
Ion Ratio Lower Upper
168 100
99 56.2 42.6 64.0

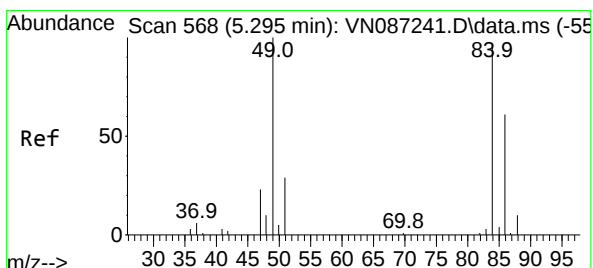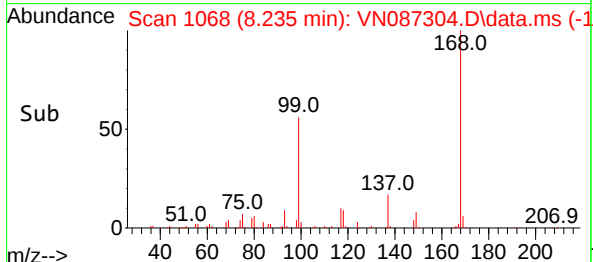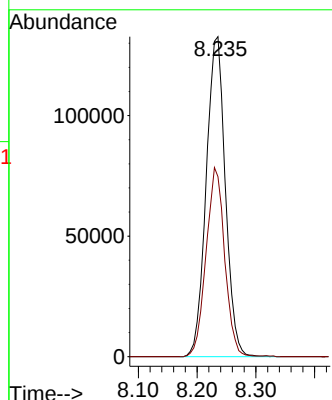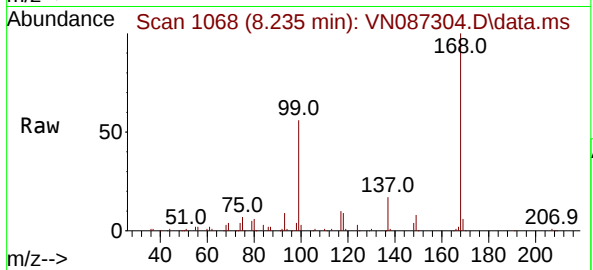

#20
Methylene Chloride
Concen: 3.524 ug/l
RT: 5.294 min Scan# 568
Delta R.T. -0.000 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00

Tgt Ion: 84 Resp: 11239
Ion Ratio Lower Upper
84 100
49 90.8 82.1 123.1
51 28.7 23.5 35.3
86 54.9 49.7 74.5

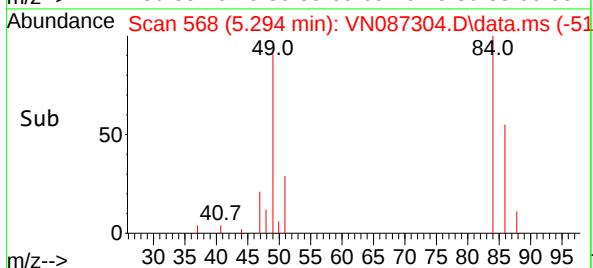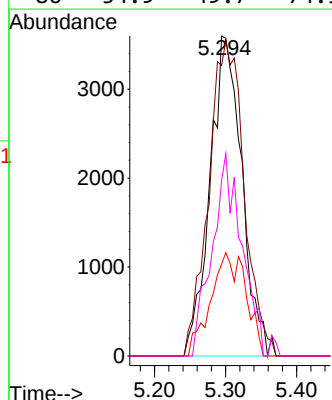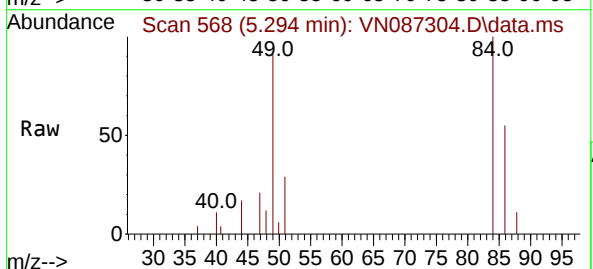

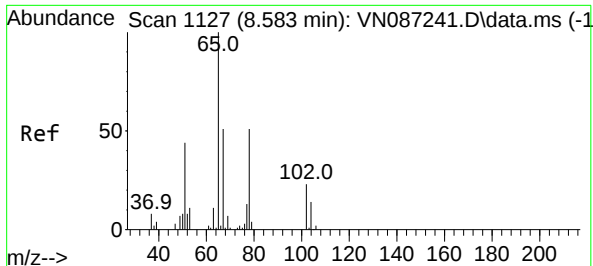

#33

1,2-Dichloroethane-d4

Concen: 66.815 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VN087304.D

Acq: 08 Jul 2025 17:00

Instrument :

MSVOA_N

ClientSampleId :





IBLK

Tgt Ion: 65 Resp: 251591

Ion Ratio Lower Upper

65 100

67 51.8 0.0 102.6

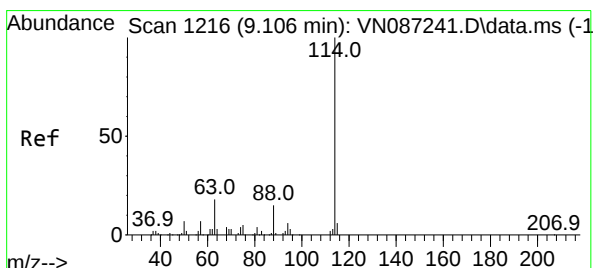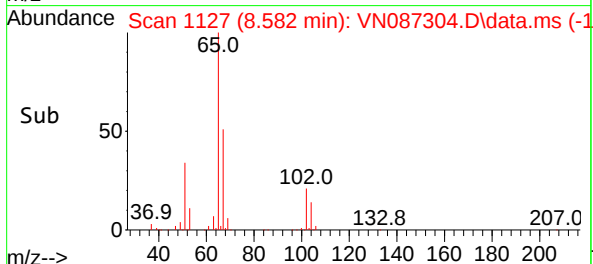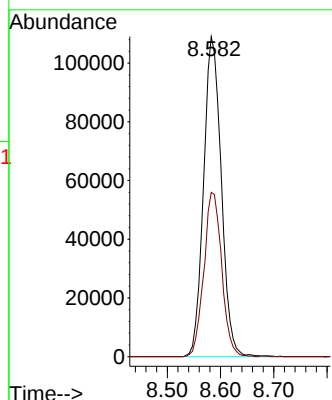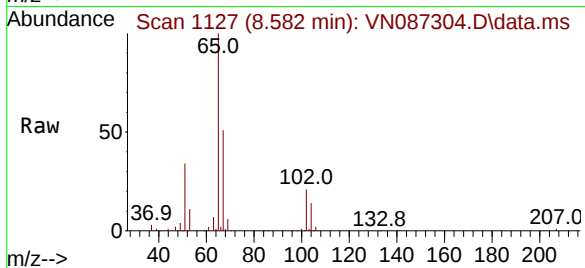

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN087304.D

Acq: 08 Jul 2025 17:00




Tgt Ion: 114 Resp: 593922


Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.6

88 15.1 0.0 29.6


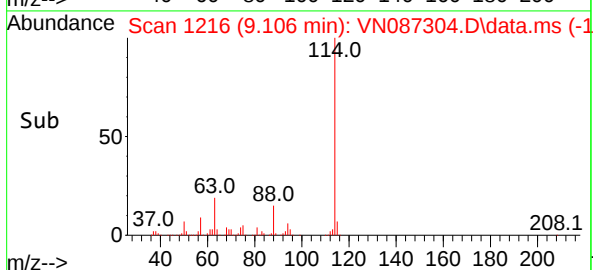
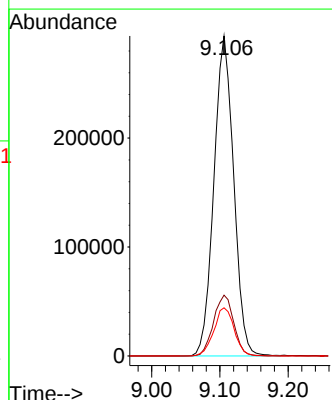
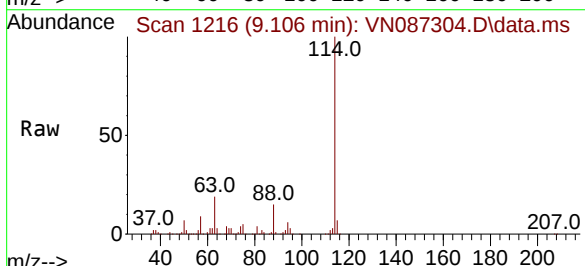


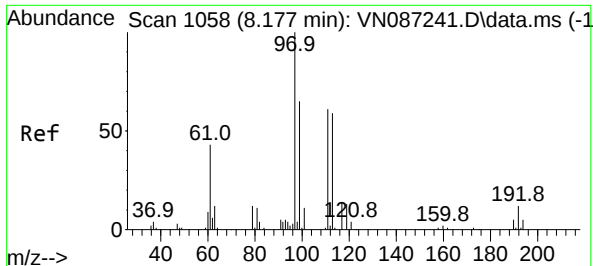

#35
Dibromofluoromethane
Concen: 53.339 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:113 Resp: 202843
Ion Ratio Lower Upper
113 100
111 102.5 81.4 122.2
192 18.1 15.1 22.7

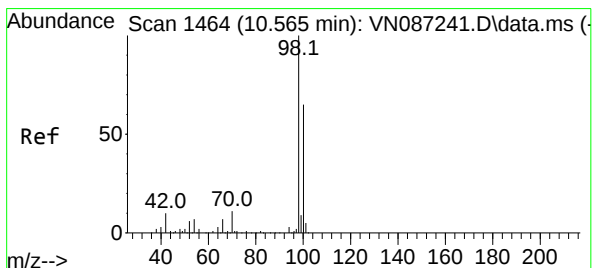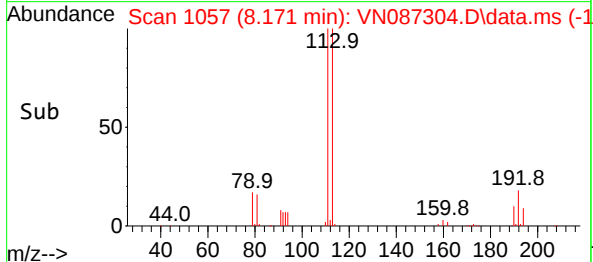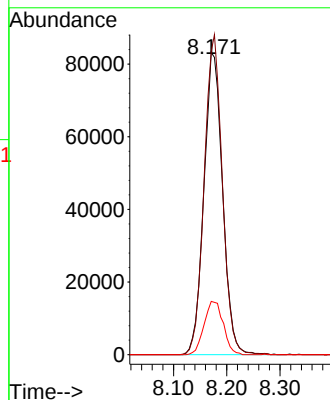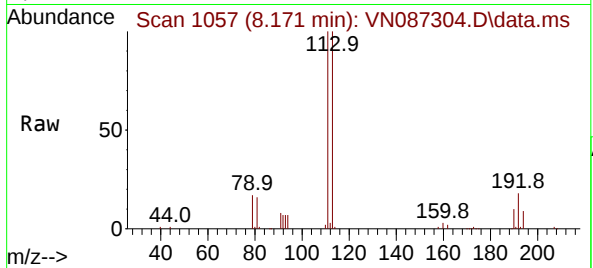

#50
Toluene-d8
Concen: 48.876 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00

Tgt Ion: 98 Resp: 724491
Ion Ratio Lower Upper
98 100
100 64.0 52.1 78.1


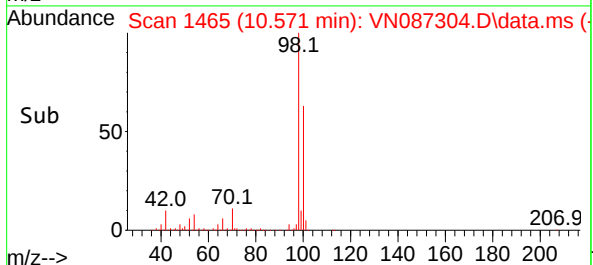
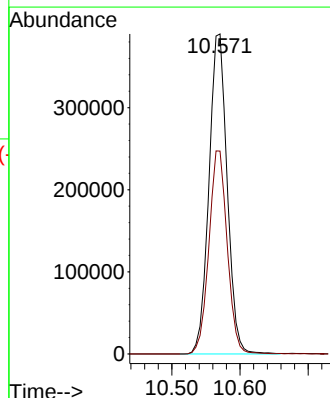
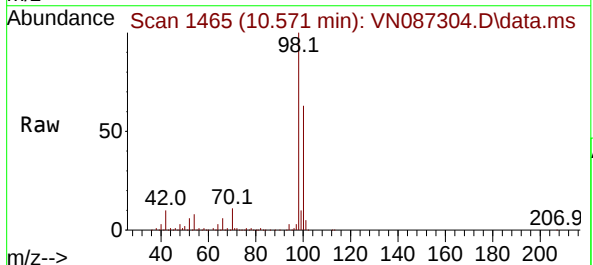


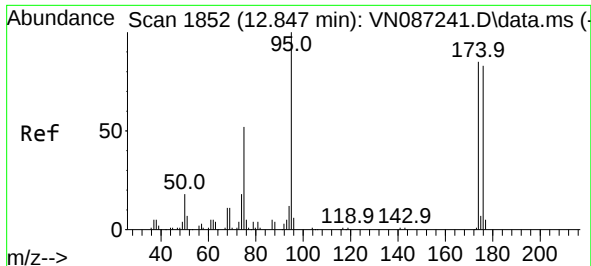

#62
4-Bromofluorobenzene
Concen: 41.881 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 95 Resp: 220885
Ion Ratio Lower Upper
95 100
174 79.9 0.0 169.6
176 75.5 0.0 161.6

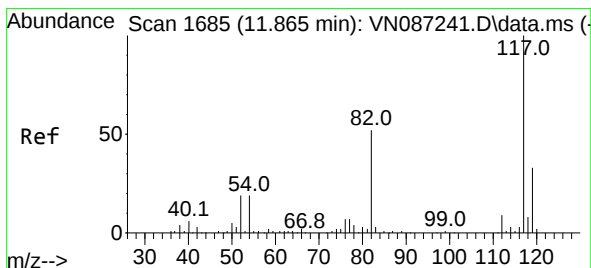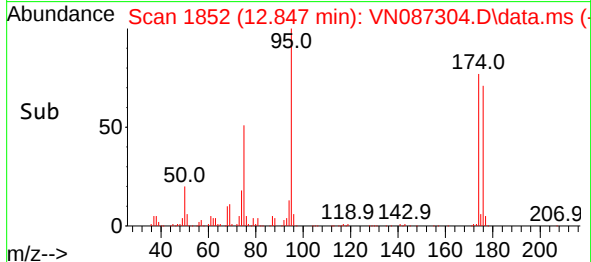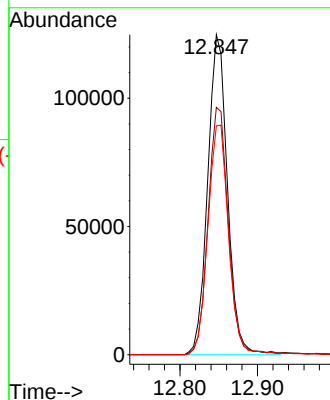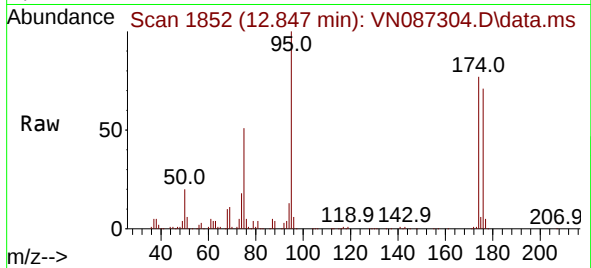

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN087304.D
Acq: 08 Jul 2025 17:00


Tgt Ion: 117 Resp: 359599
Ion Ratio Lower Upper
117 100
82 51.0 41.9 62.9
119 32.0 26.2 39.4

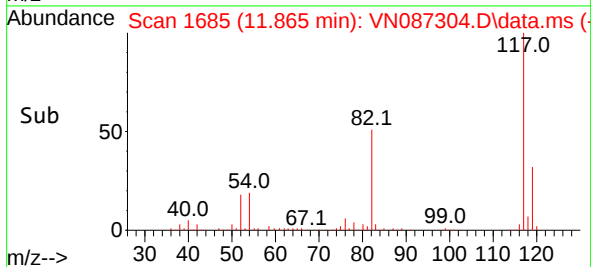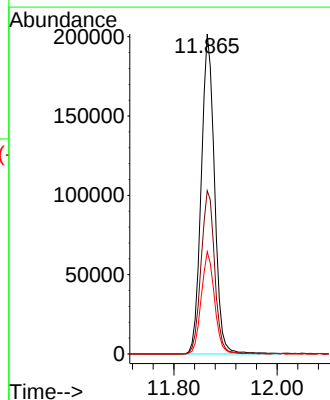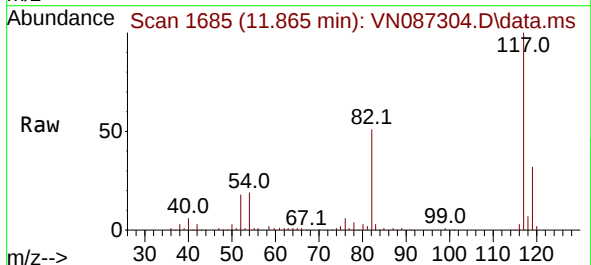

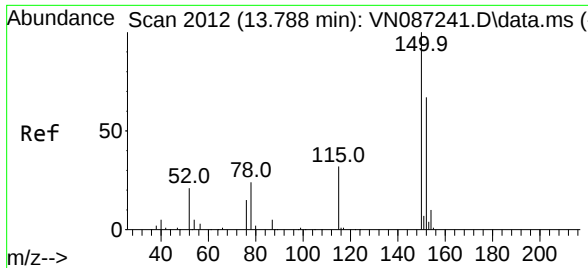

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN087304.D
 Acq: 08 Jul 2025 17:00

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

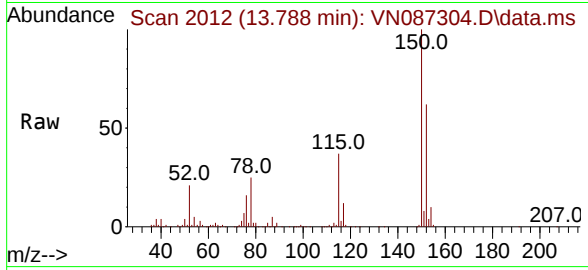

Tgt Ion:152 Resp: 255360

Ion	Ratio	Lower	Upper
152	100		
115	58.8	28.3	84.9
150	158.6	0.0	344.6

