


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070825\
Data File : VN087294.D
Acq On : 08 Jul 2025 11:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Title : SW846 8260
Last Update : Tue Jul 01 03:15:00 2025

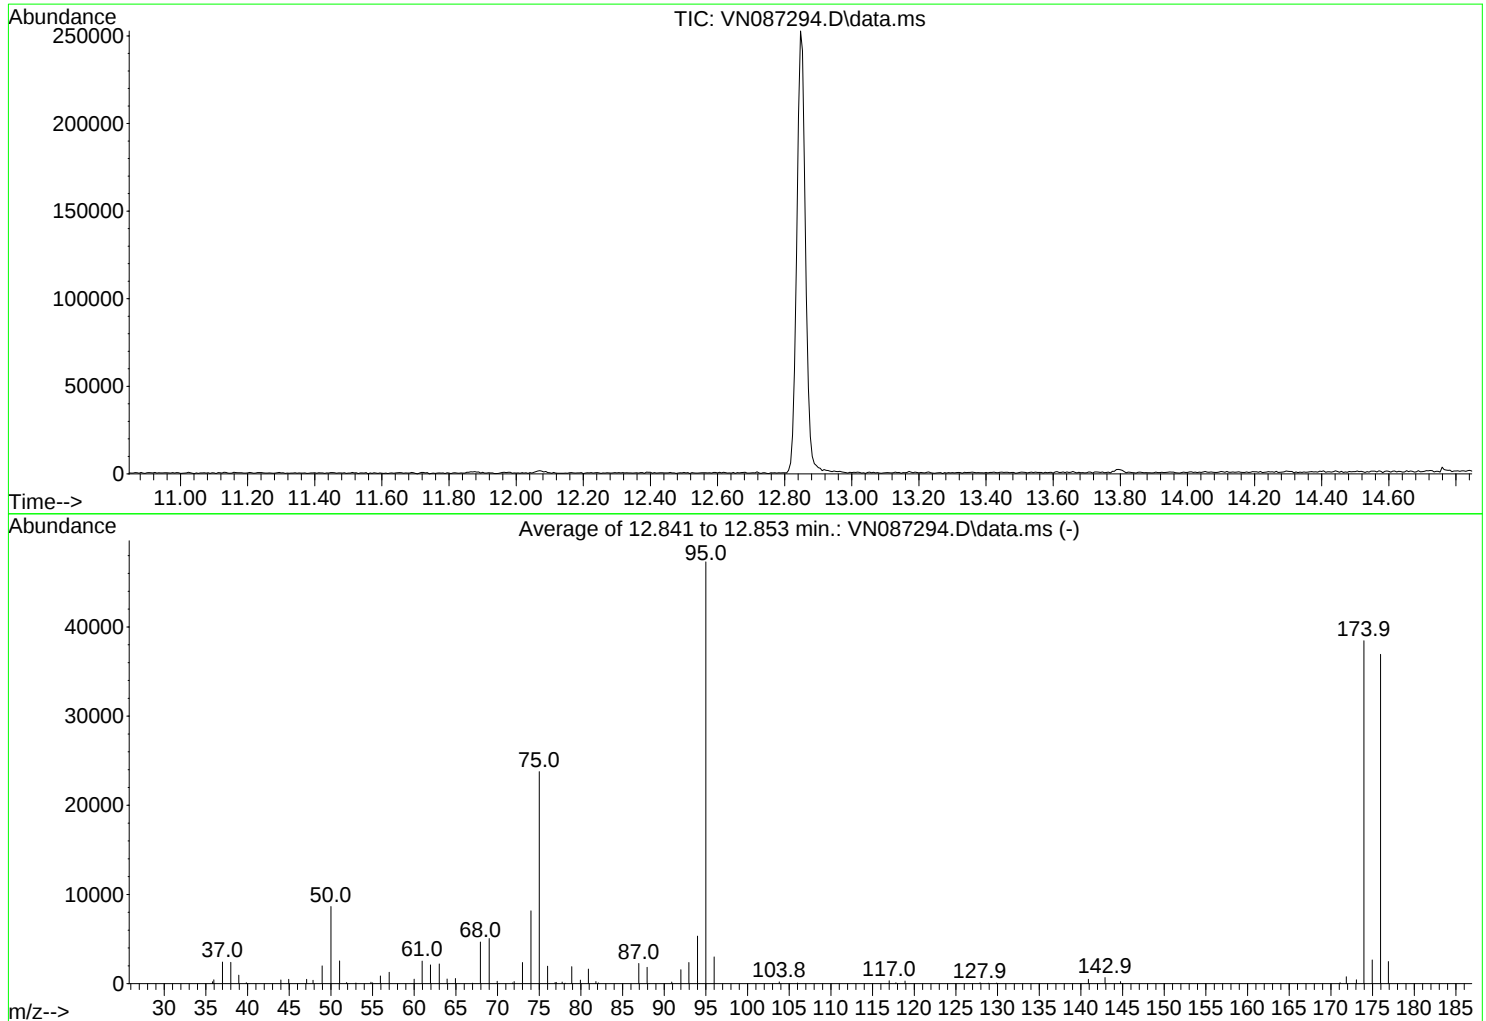

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	8652	PASS
75	95	30	60	50.3	23784	PASS
95	95	100	100	100.0	47304	PASS
96	95	5	9	6.3	2994	PASS
173	174	0.00	2	1.1	436	PASS
174	95	50	100	81.3	38456	PASS
175	174	5	9	6.9	2656	PASS
176	174	95	101	96.0	36923	PASS
177	176	5	9	6.7	2478	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	210	50.00	8652	63.00	2203	75.00	2378
35.95	426	51.05	2556	63.95	516	76.00	196
37.00	2428	51.90	134	64.95	574	76.90	12
38.00	2384	53.00	66	67.00	58	77.05	14
38.95	951	54.80	167	67.95	4674	77.75	186
39.85	115	55.00	84	69.00	5066	78.10	62
44.00	408	55.95	864	69.95	274	78.90	1900
44.95	491	57.00	1282	71.80	72	79.95	392
47.10	485	60.00	501	72.00	231	80.90	1639
47.85	380	60.95	2537	73.00	2372	81.80	230
48.95	1991	61.95	2093	74.00	8168	82.10	83

Average of 12.841 to 12.853 min.: VN087294.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2264	117.80	101	173.95	38456		
87.95	1824	118.90	281	174.95	2656		
90.90	186	127.90	111	175.95	36923		
92.00	1560	128.90	51	176.90	2478		
92.95	2364	129.90	72				
94.00	5325	140.90	484				
95.00	47304	142.90	680				
96.00	2994	144.75	235				
103.80	198	171.10	103				
106.00	71	171.85	776				
117.00	332	173.05	436				

Instrument :

MSVOA_N

ClientSampleId :

BFB