

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070919\
 Data File : VN056623.D
 Acq On : 9 Jul 2019 12:34
 Operator : JC/SP
 Sample : K3704-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EFFL-B2-9

Quant Time: Jul 09 13:40:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N070319W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Jul 03 11:05:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.19	128	47008	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.58	114	257606	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.40	117	209464	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.02	65	98387	30.36	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.20%
60) 4-Bromofluorobenzene	12.40	95	80535	25.02	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	83.40%
63) Toluene-d8	10.09	98	300153	30.84	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	102.80%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070919\
Data File : VN056623.D
Acq On : 9 Jul 2019 12:34
Operator : JC/SP
Sample : K3704-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EFFL-B2-9

Quant Time: Jul 09 13:40:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N070319W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Jul 03 11:05:14 2019
Response via : Initial Calibration

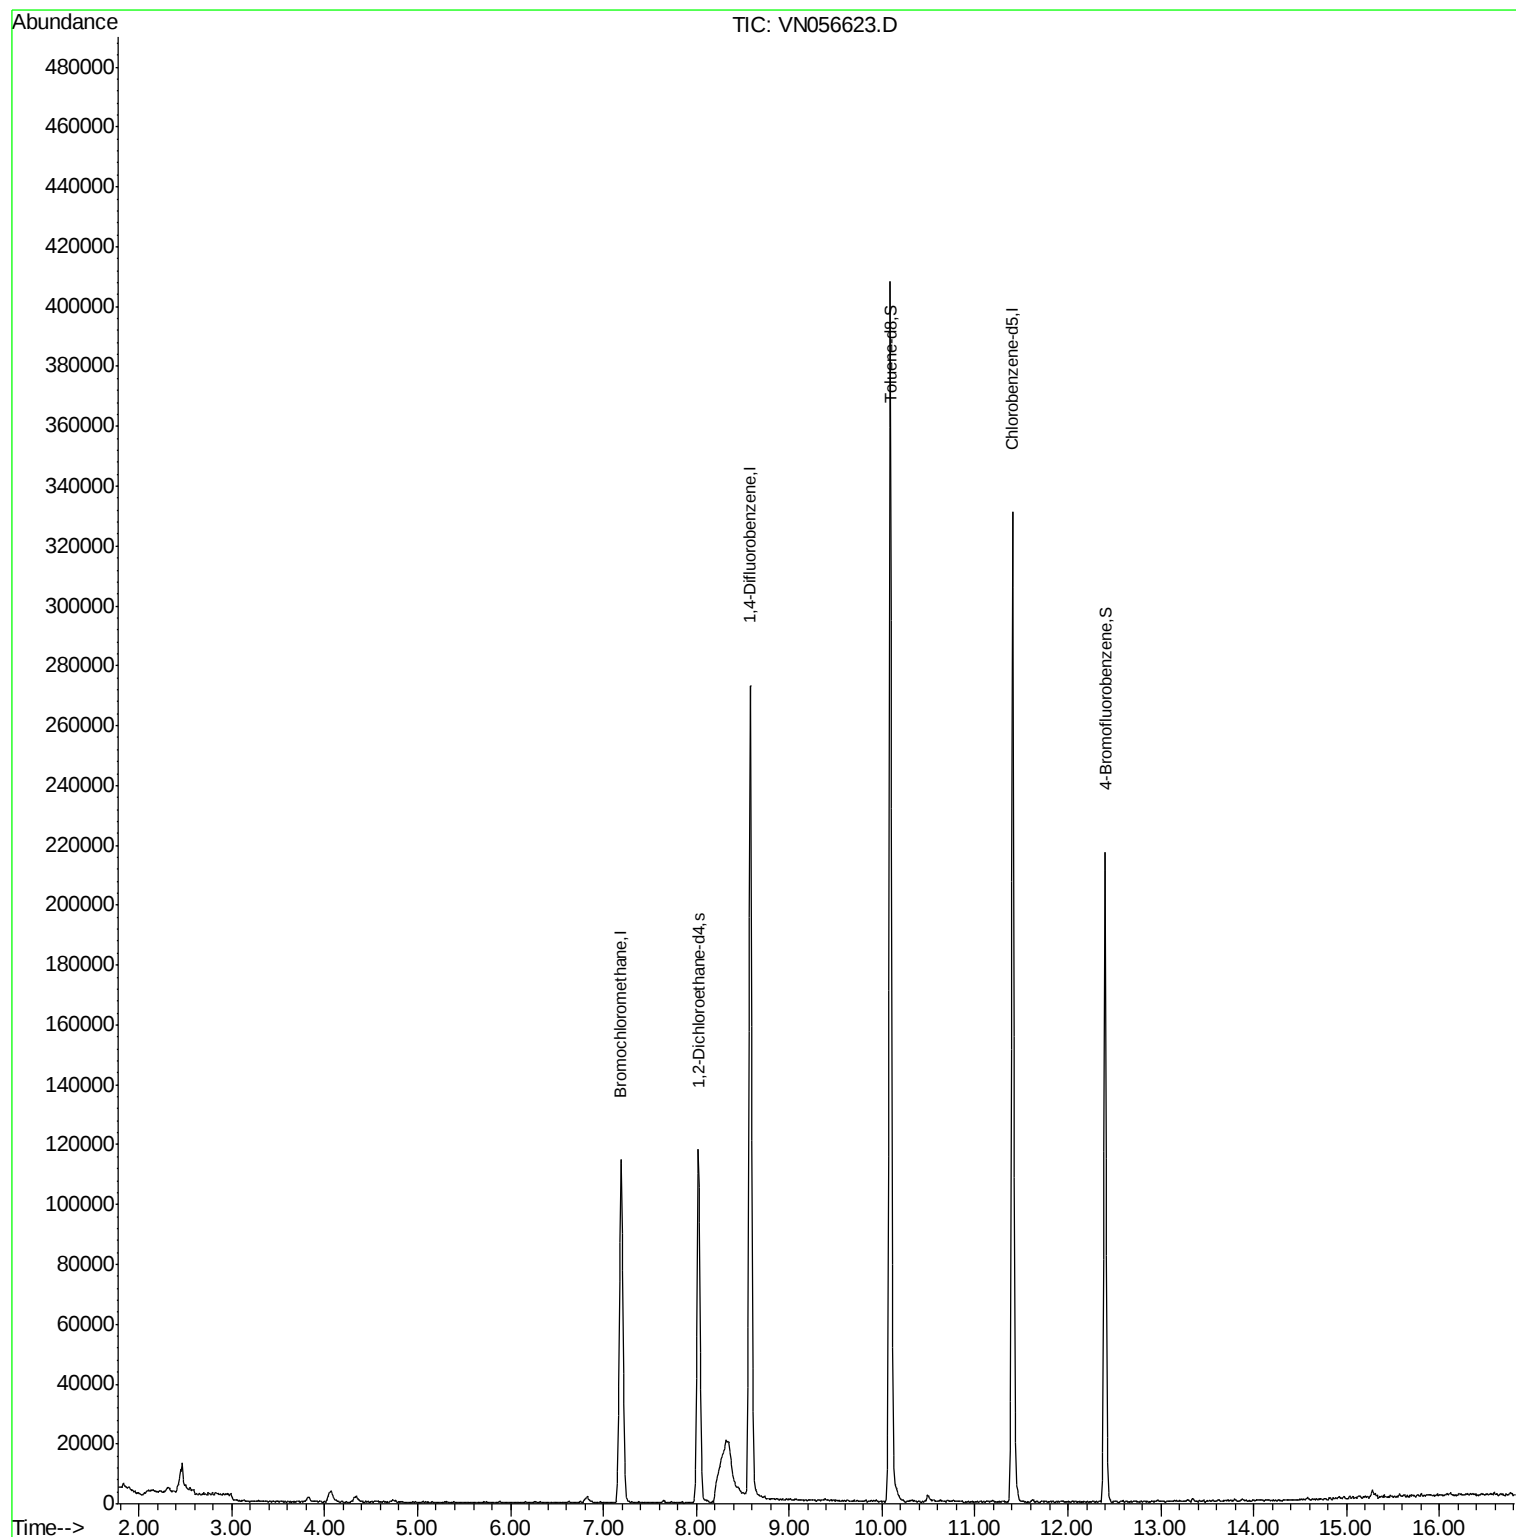

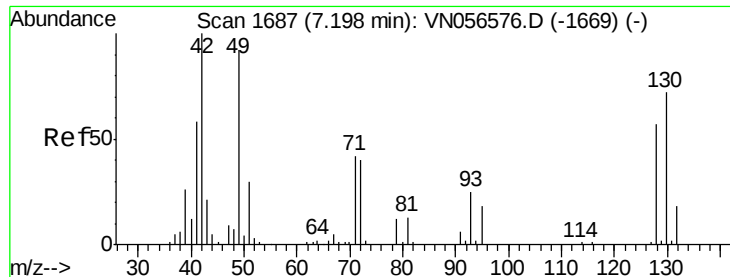

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.19 min Scan# 1685

Delta R.T. -0.01 min

Lab File: VN056623.D

Acq: 9 Jul 2019 12:34

Instrument :

MSVOA_N

ClientSampleId :

EFFL-B2-9


Tot Ion:128 Resp: 47008

Ion Ratio Lower Upper

128 100

49 163.3 0.0 355.8




130 129.1 0.0 326.3

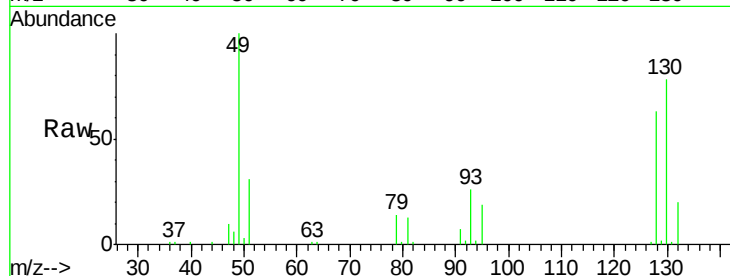

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VN0

Ion 130.00 (129.70 to 130.70): V

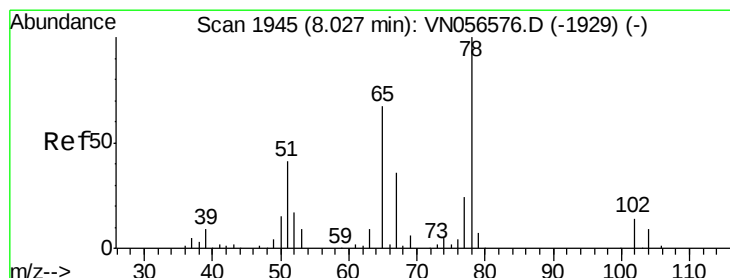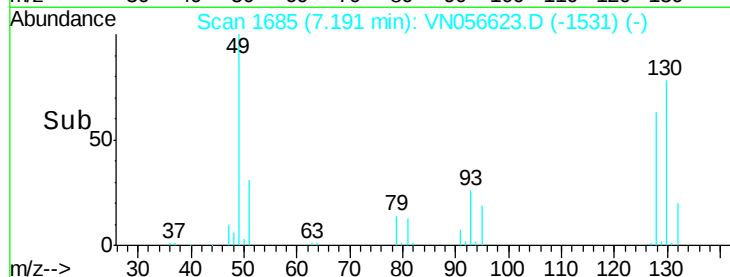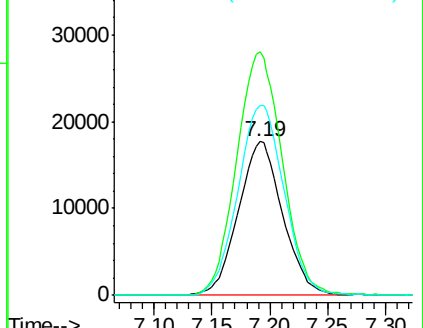

#27

1,2-Dichloroethane-d4

Concen: 30.360 ug/l

RT: 8.02 min Scan# 1944

Delta R.T. -0.00 min

Lab File: VN056623.D


Acq: 9 Jul 2019 12:34

Tgt Ion: 65 Resp: 98387

Ion Ratio Lower Upper



65 100


67 54.6 43.4 65.2

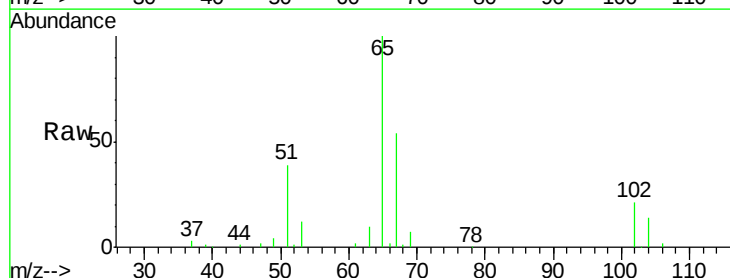

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0



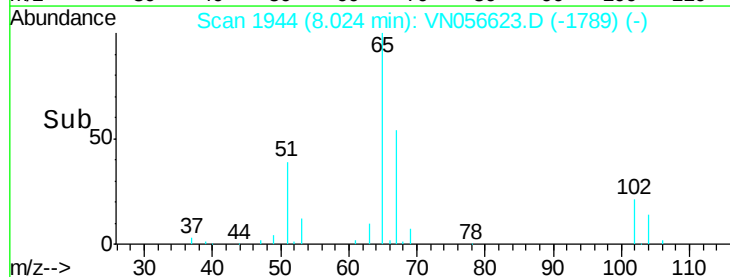
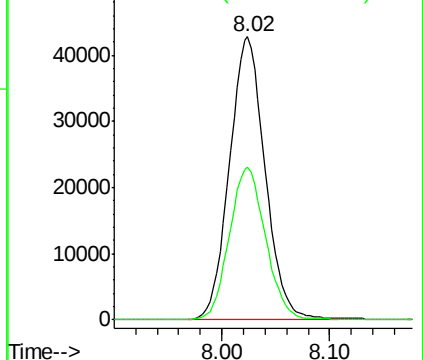


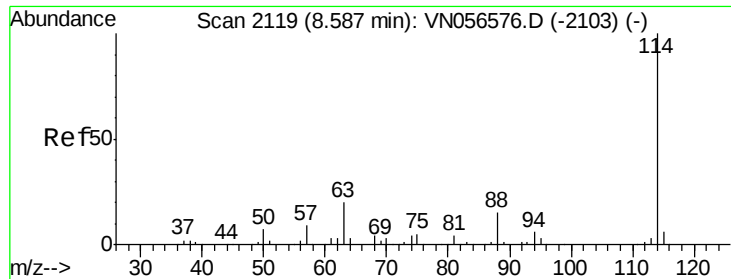

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 8.58 min Scan# 2118
Delta R.T. 0.00 min
Lab File: VN056623.D
Acq: 9 Jul 2019 12:34




Instrument :
MSVOA_N
ClientSampleId :
EFFL-B2-9


Tot Ion:114 Resp: 257606
Ion Ratio Lower Upper
114 100
63 19.5 14.7 22.1
88 15.3 11.9 17.9

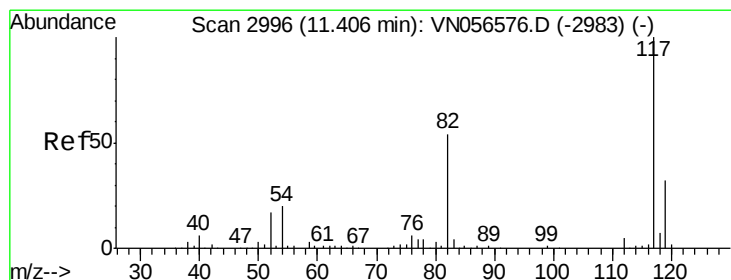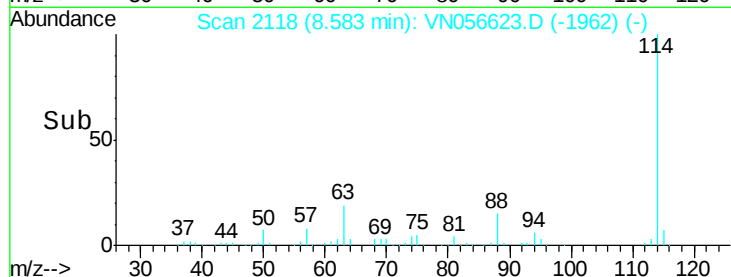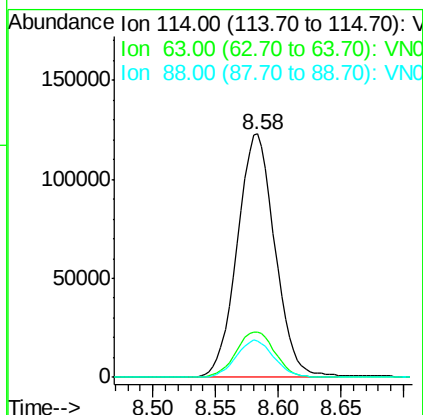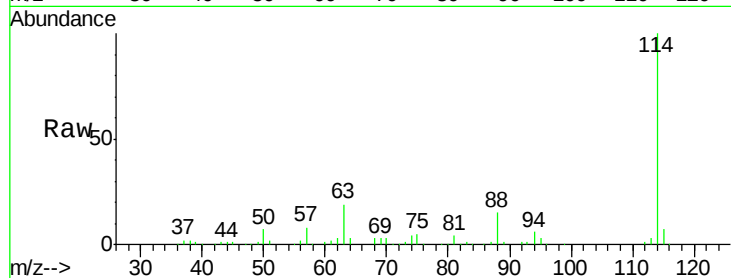

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.40 min Scan# 2995
Delta R.T. -0.00 min
Lab File: VN056623.D
Acq: 9 Jul 2019 12:34

Tgt Ion:117 Resp: 209464
Ion Ratio Lower Upper
117 100
82 53.6 41.2 61.8
119 32.0 26.2 39.2

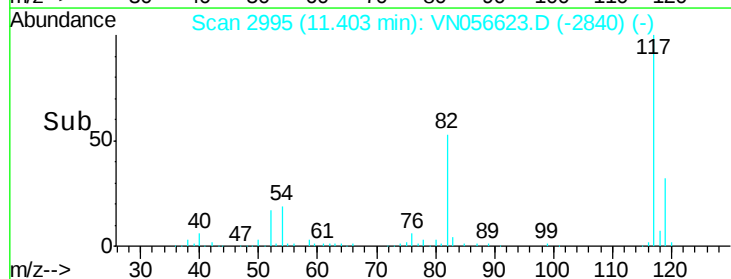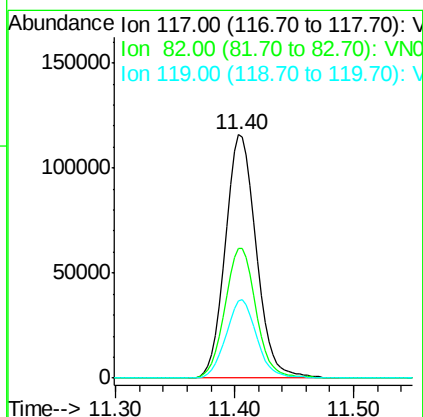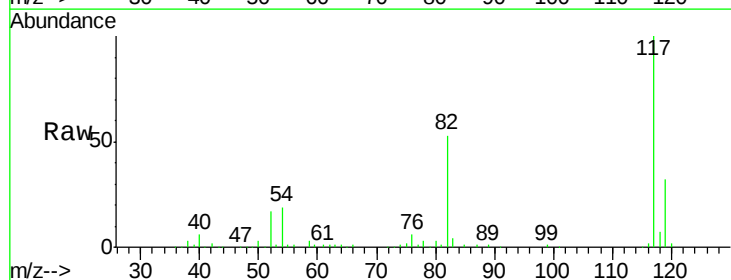

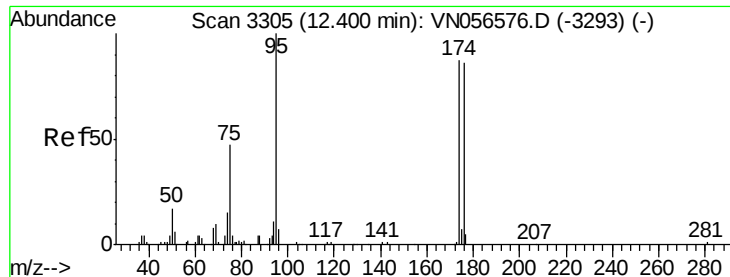

#60

4-Bromofluorobenzene

Concen: 25.021 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN056623.D

Acq: 9 Jul 2019 12:34

Instrument :

MSVOA_N

ClientSampled :

EFFL-B2-9


Tot Ion: 95 Resp: 80535

Ion Ratio Lower Upper

95 100

174 87.3 75.4 113.0




176 85.5 73.9 110.9

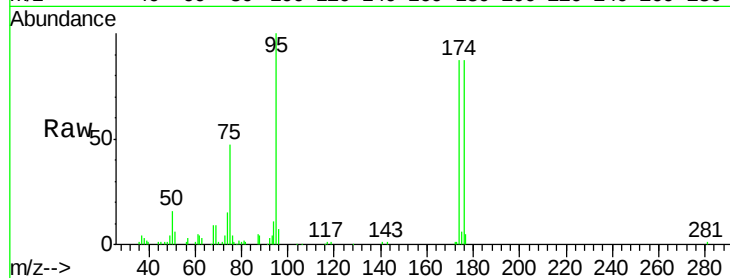

Abundance Ion 95.00 (94.70 to 95.70): VN056623.D (-3149) (-)

Ion 174.00 (173.70 to 174.70): VN056623.D (-3149) (-)

Ion 176.00 (175.70 to 176.70): VN056623.D (-3149) (-)

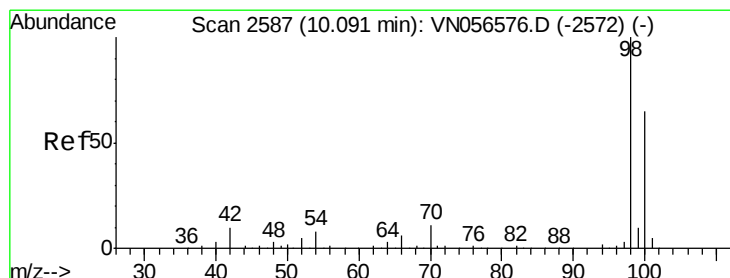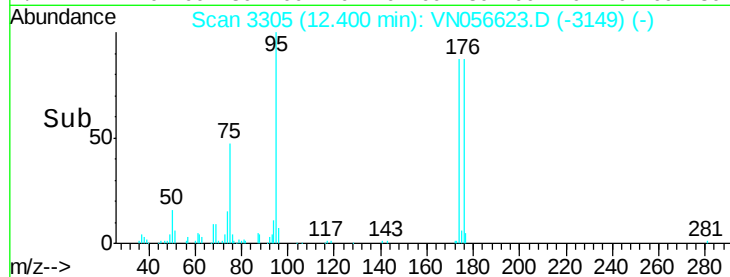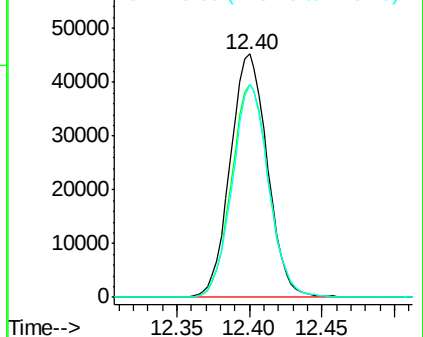

#63

Toluene-d8

Concen: 30.837 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. -0.00 min

Lab File: VN056623.D


Acq: 9 Jul 2019 12:34

Tgt Ion: 98 Resp: 300153

Ion Ratio Lower Upper

98 100

100 64.3 52.2 78.4

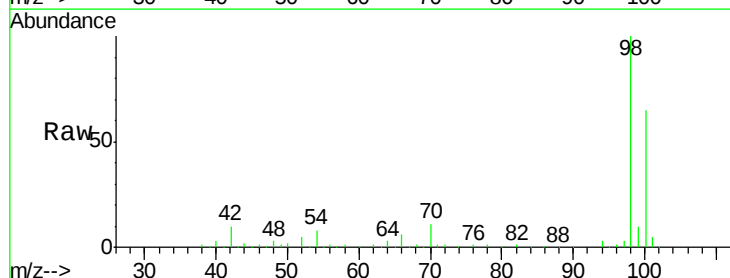

Abundance Ion 98.00 (97.70 to 98.70): VN056623.D (-2431) (-)

Ion 100.00 (99.70 to 100.70): VN056623.D (-2431) (-)

