

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070920\
 Data File : VN062469.D
 Acq On : 9 Jul 2020 21:02
 Operator : JC/MD
 Sample : PB130035TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035TB

Quant Time: Jul 10 02:08:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 00:55:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	201600	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	374923	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	361139	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	135522	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	159833	51.54	ug/l	0.00
Spiked Amount			Recovery	=	103.08%	
35) Dibromofluoromethane	7.55	113	118134	50.97	ug/l	0.00
Spiked Amount			Recovery	=	101.94%	
50) Toluene-d8	10.06	98	480902	52.56	ug/l	0.00
Spiked Amount			Recovery	=	105.12%	
62) 4-Bromofluorobenzene	12.38	95	178416	53.37	ug/l	0.00
Spiked Amount			Recovery	=	106.74%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
8) Diethyl Ether	3.38	74	471	0.307	ug/l	91
11) Tert butyl alcohol	4.72	59	401	0.780	ug/l #	74
16) Acetone	3.78	43	13707	10.412	ug/l	94
18) Methyl Acetate	4.29	43	5721	1.741	ug/l	96
20) Methylene Chloride	4.51	84	18610	6.612	ug/l	97
25) 2-Butanone	6.80	43	1809	0.941	ug/l #	53
29) Tetrahydrofuran	7.18	42	798	0.616	ug/l #	39
31) Cyclohexane	7.62	56	4690	0.996	ug/l #	1
36) 1,1-Dichloropropene	7.62	75	18095	4.790	ug/l #	51
38) Carbon Tetrachloride	7.63	117	20765	6.115	ug/l #	16
43) Isopropyl Acetate	8.13	43	76221	10.924	ug/l #	93
45) 1,2-Dichloropropane	9.24	63	1471	0.455	ug/l #	44
48) Methyl methacrylate	9.14	41	4695	1.372	ug/l #	17
51) 4-Methyl-2-Pentanone	9.95	43	7791	1.869	ug/l	99
54) cis-1,3-Dichloropropene	9.87	75	29603	6.142	ug/l #	61
56) Ethyl methacrylate	10.52	69	997	1.919	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	5275	1.129	ug/l #	43
59) 2-Hexanone	10.74	43	84582	27.957	ug/l #	53
71) Bromoform	12.37	173	1037	0.547	ug/l #	1
74) N-amyl acetate	12.00	43	3167	0.620	ug/l #	46
76) 1,2,3-Trichloropropane	12.38	75	94214	28.333	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	3465	0.403	ug/l	100
81) trans-1,4-Dichloro-2-buten	12.38	75	94214	75.835	ug/l #	10
95) Naphthalene	15.10	128	1223	Below Cal	#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070920\
Data File : VN062469.D
Acq On : 9 Jul 2020 21:02
Operator : JC/MD
Sample : PB130035TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB130035TB

Quant Time: Jul 10 02:08:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 00:55:52 2020
Response via : Initial Calibration

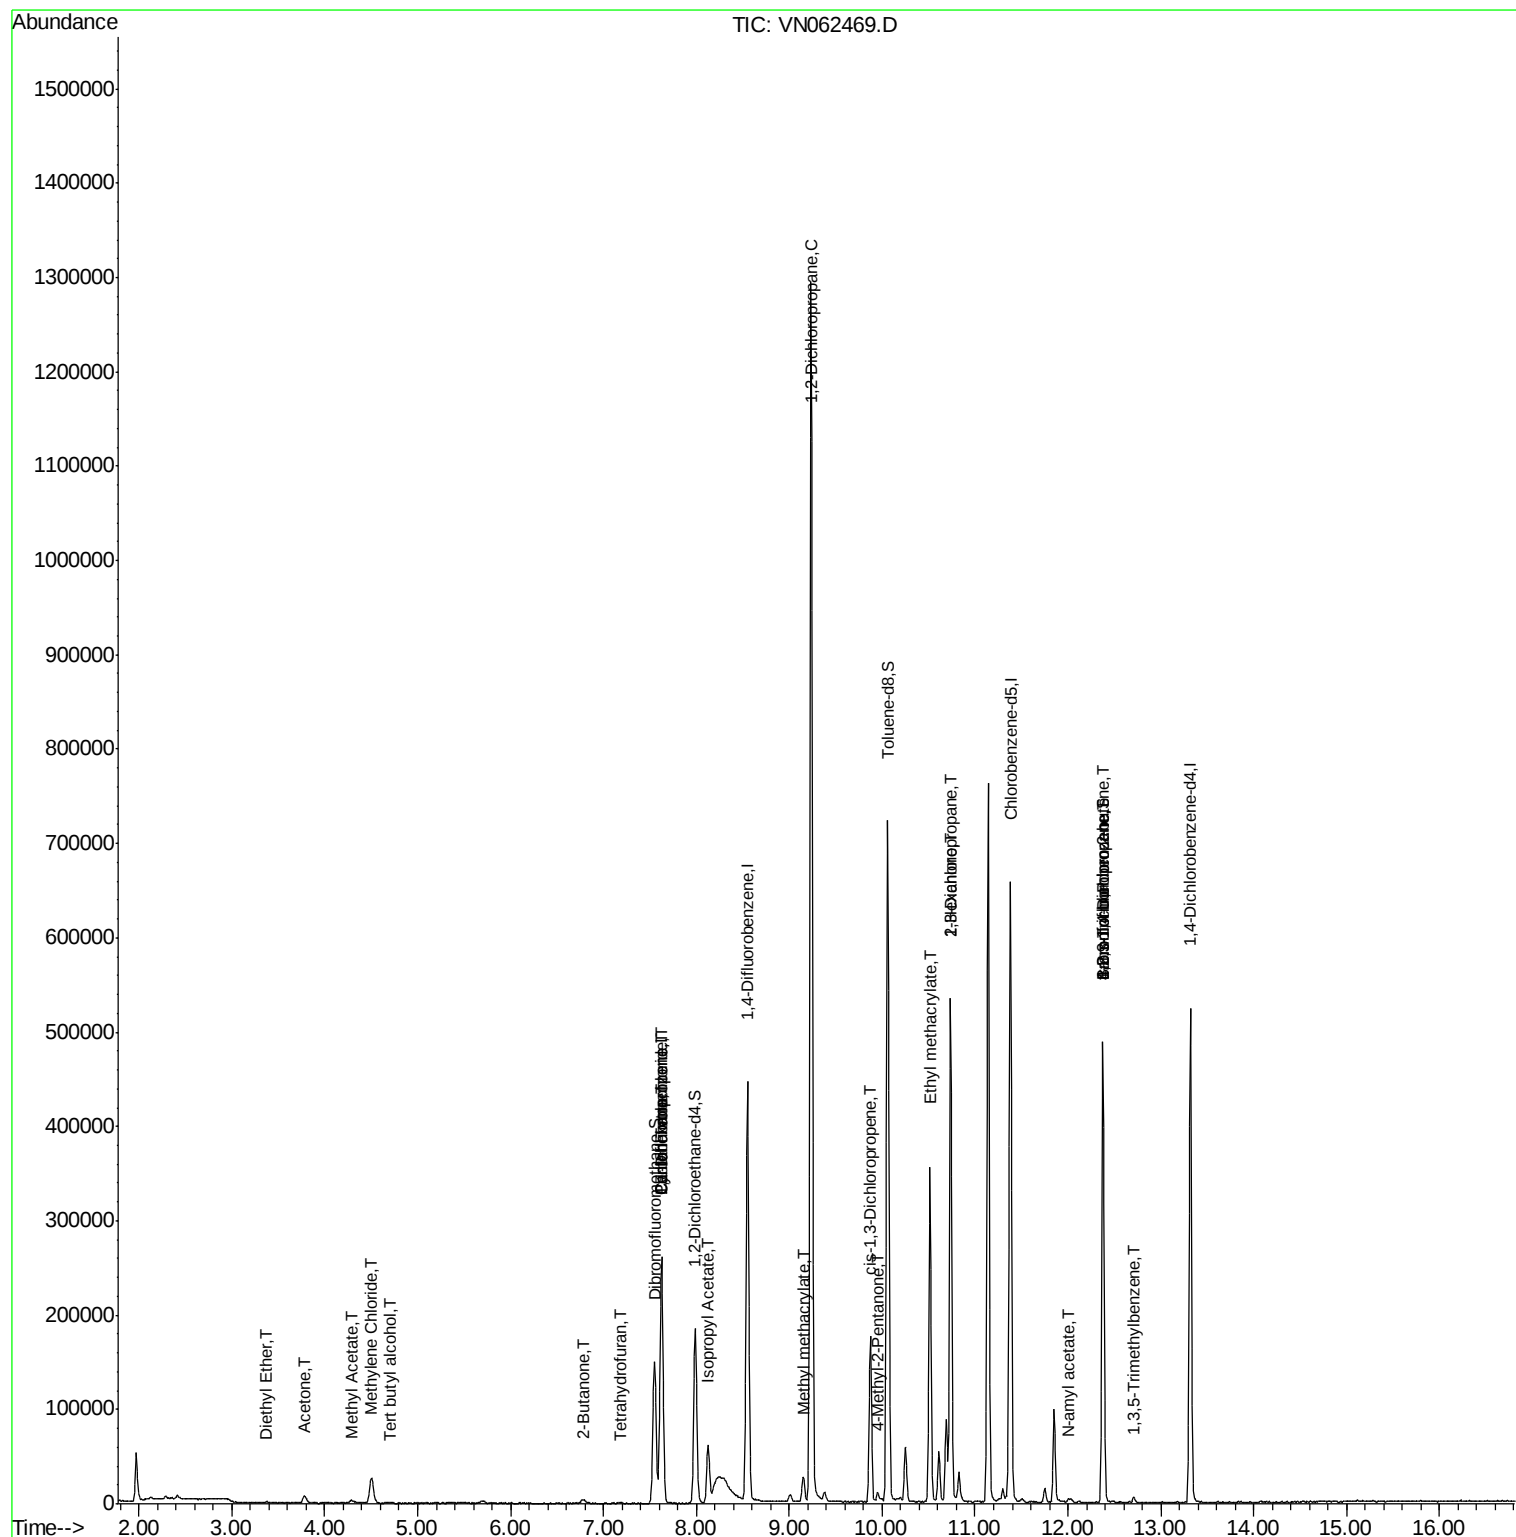



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :


PB130035TB

Tot Ion:168 Resp: 201600

Ion Ratio Lower Upper

168 100

99 61.6 48.8 73.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#8

Diethyl Ether

Concen: 0.307 ug/l

RT: 3.38 min Scan# 499

Delta R.T. 0.00 min

Lab File: VN062469.D


Acq: 9 Jul 2020 21:02

Tgt Ion: 74 Resp: 471

Ion Ratio Lower Upper

74 100

45 127.2 58.5 175.3



Abundance Ion 74.00 (73.70 to 74.70): VN

Ion 45.00 (44.70 to 45.70): VN

3.38

400


300


200

100

0

Time--> 3.34 3.36 3.38 3.40






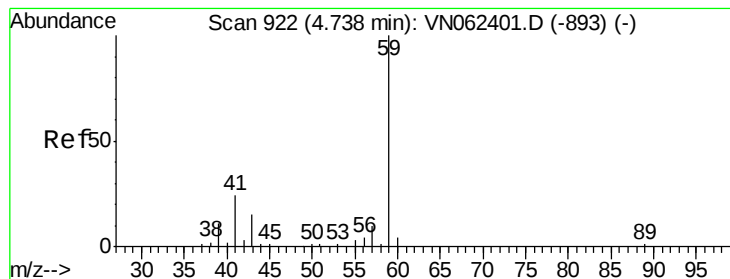


#11

Tert butyl alcohol
 Concen: 0.780 ug/l
 RT: 4.72 min Scan# 915
 Delta R.T. -0.02 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Instrument :
 MSVOA_N
 ClientSampleID :
 PB130035TB




Tot Ion: 59 Resp: 401
 Ion Ratio Lower Upper
 59 100
 57 0.0 7.8 11.6#

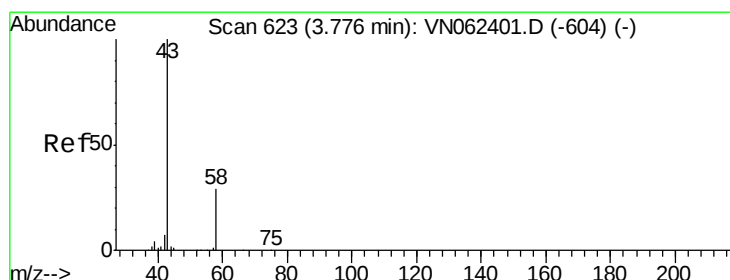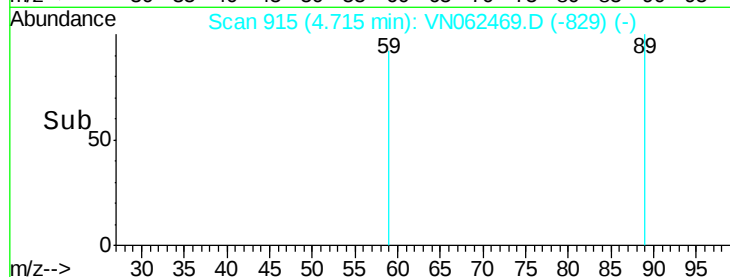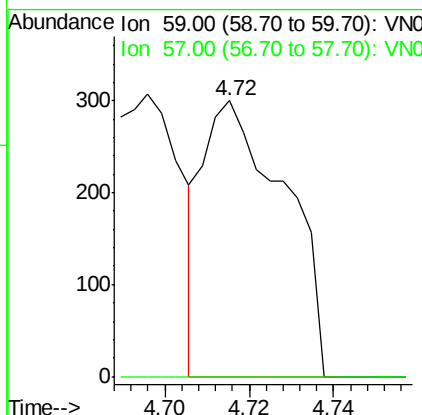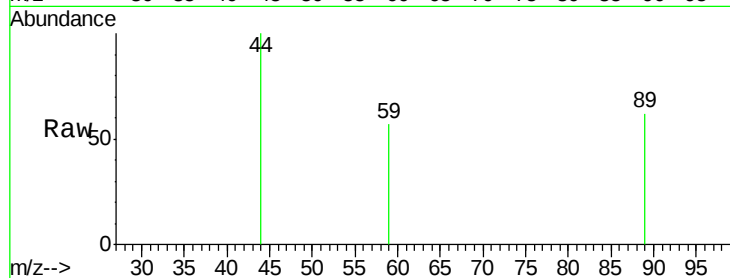


#16

Acetone
 Concen: 10.412 ug/l
 RT: 3.78 min Scan# 625
 Delta R.T. 0.01 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Tgt Ion: 43 Resp: 13707
 Ion Ratio Lower Upper
 43 100
 58 32.8 23.5 35.3


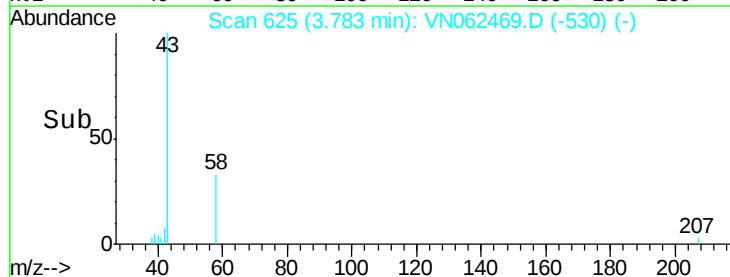
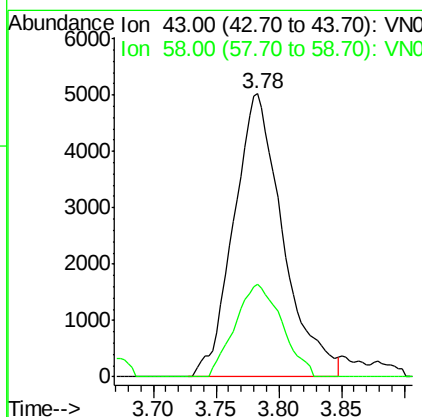
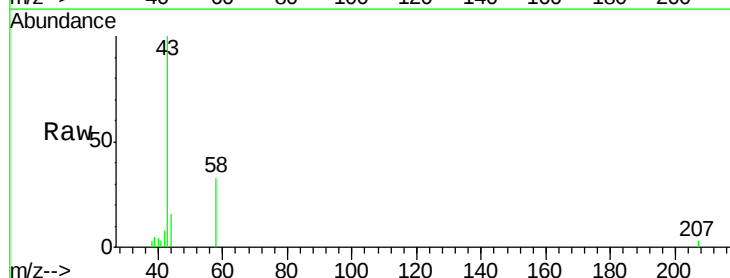




#18
Methyl Acetate
Concen: 1.741 ug/l
RT: 4.29 min Scan# 782
Delta R.T. 0.01 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02




Instrument :
MSVOA_N
ClientSampled :
PB130035TB


Tot Ion: 43 Resp: 5721
Ion Ratio Lower Upper
43 100
74 18.1 16.0 24.0

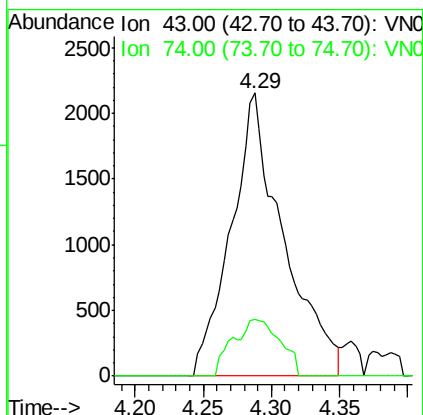

#20
Methylene Chloride
Concen: 6.612 ug/l
RT: 4.51 min Scan# 851
Delta R.T. 0.01 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion: 84 Resp: 18610
Ion Ratio Lower Upper
84 100
49 143.5 120.0 180.0
51 45.5 37.0 55.6
86 64.3 51.8 77.6



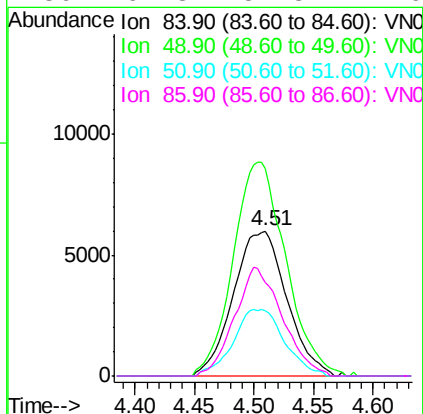





#25
2-Butanone
Concen: 0.941 ug/l
RT: 6.80 min Scan# 1563
Delta R.T. 0.01 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PB130035TB


Tot Ion: 43 Resp: 1809
Ion Ratio Lower Upper
43 100
72 0.0 17.9 26.9#

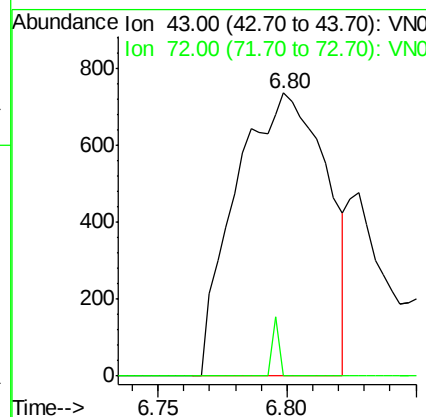

#29
Tetrahydrofuran
Concen: 0.616 ug/l
RT: 7.18 min Scan# 1683
Delta R.T. 0.02 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion: 42 Resp: 798
Ion Ratio Lower Upper
42 100
72 0.0 29.1 43.7#
71 0.0 28.1 42.1#

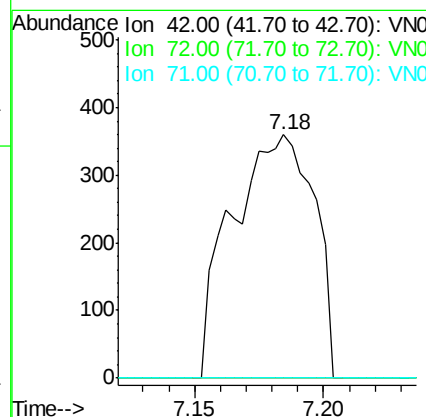







#31
Cyclohexane
Concen: 0.996 ug/l
RT: 7.62 min Scan# 1819
Delta R.T. 0.01 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Instrument :
MSVOA_N
ClientSampleId :
PB130035TB

Tot Ion: 56 Resp: 4690
Ion Ratio Lower Upper
56 100
69 170.4 24.5 36.7#
84 109.8 57.4 86.2#




Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

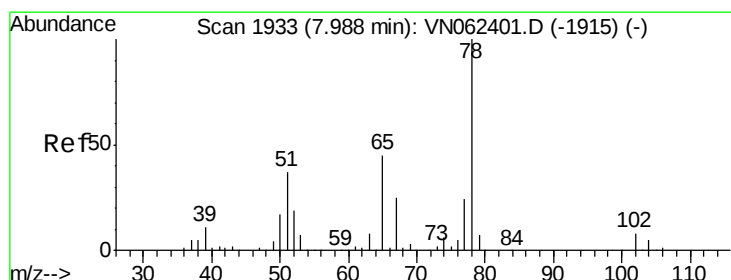
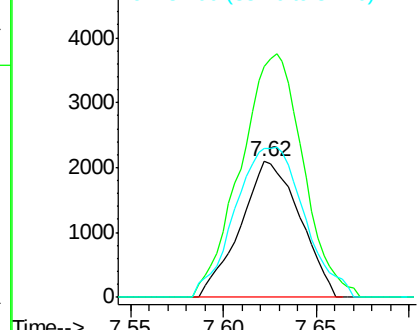



#33
1,2-Dichloroethane-d4
Concen: 51.545 ug/l
RT: 7.99 min Scan# 1933
Delta R.T. -0.00 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion: 65 Resp: 159833
Ion Ratio Lower Upper
65 100
67 53.0 0.0 107.6



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

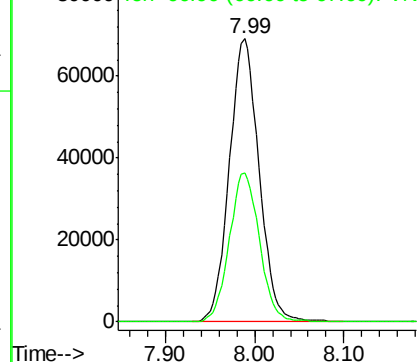







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. -0.00 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035TB

Tot Ion	Ratio	Lower	Upper
114	100		
63	23.7	0.0	48.4
88	17.5	0.0	33.8




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

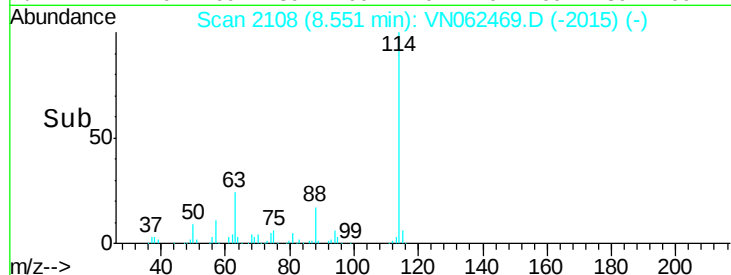
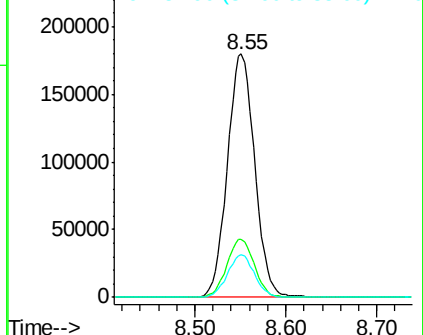



#35
 Dibromofluoromethane
 Concen: 50.974 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.5	83.1	124.7
192	18.4	14.1	21.1



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




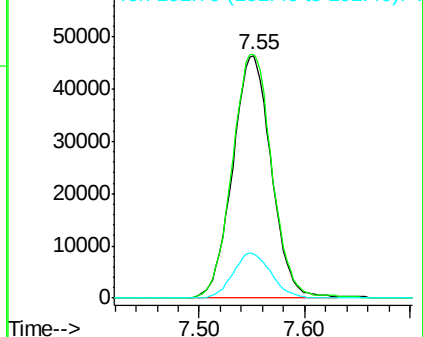




#36
 1,1-Dichloropropene
 Concen: 4.790 ug/l
 RT: 7.62 min Scan# 1819
 Delta R.T. -0.13 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035TB


Tot Ion	Ratio	Lower	Upper
75	100		
110	7.4	15.4	46.2#
77	0.0	24.1	36.1#

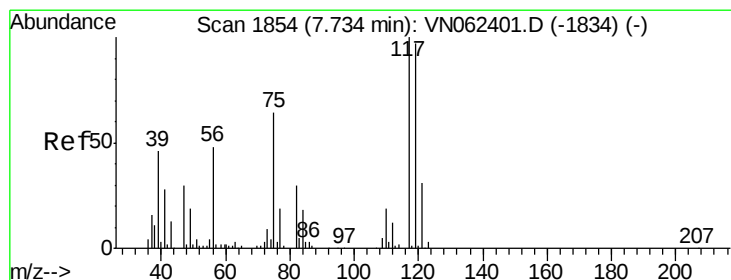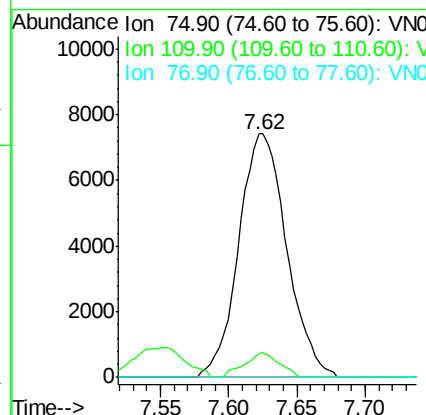

#38
 Carbon Tetrachloride
 Concen: 6.115 ug/l
 RT: 7.63 min Scan# 1821
 Delta R.T. -0.11 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.1	77.2	115.8#
121	0.0	24.8	37.2#

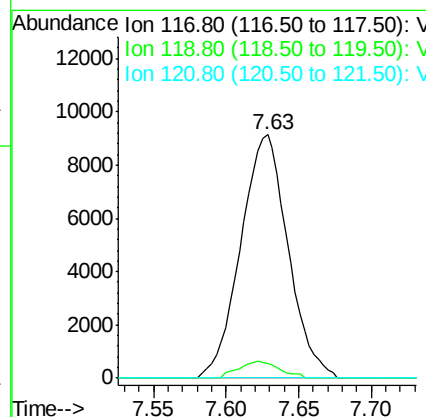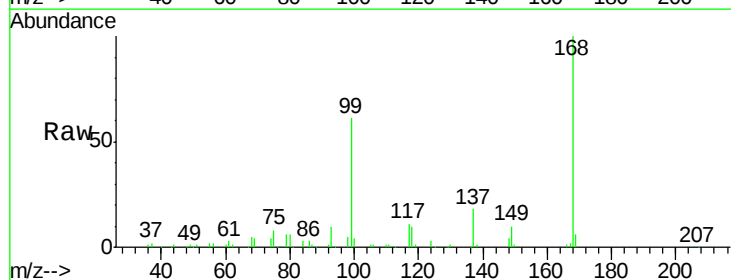



#43

Isopropyl Acetate

Concen: 10.924 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. -0.00 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PB130035TB


Tot Ion: 43 Resp: 76221

Ion Ratio Lower Upper

43 100

61 18.9 19.3 28.9#




87 10.8 8.6 13.0



Abundance Ion 43.00 (42.70 to 43.70): VN062401.D (-1957) (-)

Ion 61.00 (60.70 to 61.70): VN062401.D (-1957) (-)

Ion 87.00 (86.70 to 87.70): VN062401.D (-1957) (-)

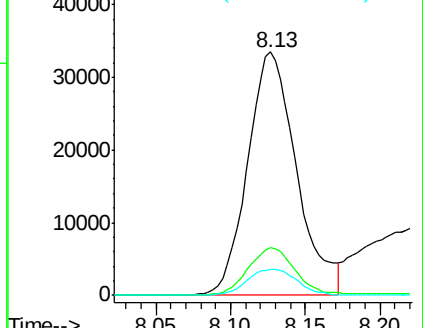

#45

1,2-Dichloropropane

Concen: 0.455 ug/l

RT: 9.24 min Scan# 2321

Delta R.T. 0.15 min

Lab File: VN062469.D


Acq: 9 Jul 2020 21:02

Tgt Ion: 63 Resp: 1471

Ion Ratio Lower Upper



63 100


65 0.0 24.6 36.8#



Abundance Ion 62.90 (62.60 to 63.60): VN062401.D (-2252) (-)

Ion 64.90 (64.60 to 65.60): VN062401.D (-2252) (-)




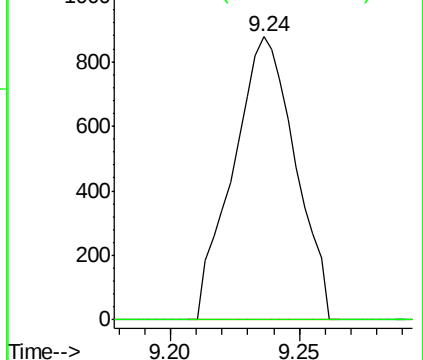




#48
Methvl methacrylate
Concen: 1.372 ug/l
RT: 9.14 min Scan# 2291
Delta R.T. -0.03 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PB130035TB


Tot Ion: 41 Resp: 4695
Ion Ratio Lower Upper
41 100
69 0.0 60.8 91.2#
39 0.0 43.5 65.3#

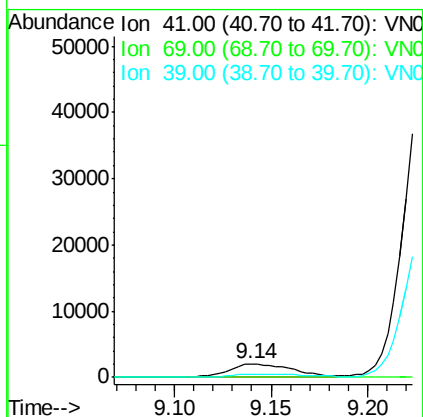

#50
Toluene-d8
Concen: 52.564 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. 0.00 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion: 98 Resp: 480902
Ion Ratio Lower Upper
98 100
100 63.7 51.5 77.3

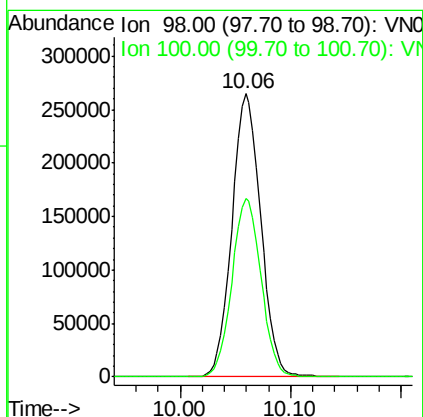



#51

4-Methyl-2-Pentanone

Concen: 1.869 ug/l

RT: 9.95 min Scan# 2544

Delta R.T. 0.00 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampled :


PB130035TB

Tot Ion: 43 Resp: 7791

Ion Ratio Lower Upper




43 100

58 36.7 29.0 43.6



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

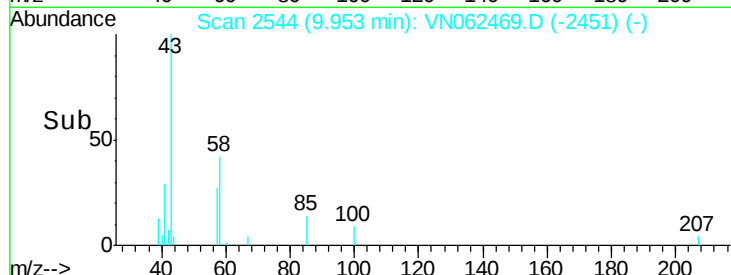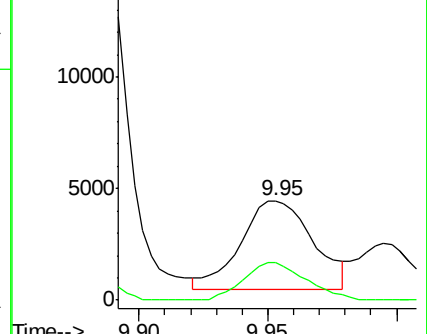

#54

cis-1,3-Dichloropropene

Concen: 6.142 ug/l

RT: 9.87 min Scan# 2519

Delta R.T. 0.06 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02


Tgt Ion: 75 Resp: 29603

Ion Ratio Lower Upper

75 100

77 0.0 24.5 36.7#



39 33.5 43.4 65.0#




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0

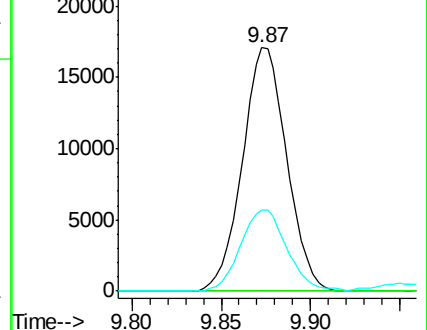



#56

Ethyl methacrylate

Concen: 1.919 ug/l

RT: 10.52 min Scan# 2719

Delta R.T. 0.12 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampled :

PB130035TB


Tot Ion: 69 Resp: 997

Ion Ratio Lower Upper

69 100

41 6693.0 59.7 89.5#

39 2570.6 30.6 45.8#




Abundance Ion 69.00 (68.70 to 69.70): VN062469.D (-2589) (-)

Ion 41.00 (40.70 to 41.70): VN062469.D (-2589) (-)

Ion 39.00 (38.70 to 39.70): VN062469.D (-2589) (-)

Time-->




Abundance Ion 69.00 (68.70 to 69.70): VN062469.D (-2589) (-)

Ion 41.00 (40.70 to 41.70): VN062469.D (-2589) (-)

Ion 39.00 (38.70 to 39.70): VN062469.D (-2589) (-)

Time-->



#57

1,3-Dichloropropane

Concen: 1.129 ug/l

RT: 10.73 min Scan# 2787

Delta R.T. 0.05 min

Lab File: VN062469.D


Acq: 9 Jul 2020 21:02

Tgt Ion: 76 Resp: 5275

Ion Ratio Lower Upper

76 100


78 0.0 25.6 38.4#



Abundance Ion 75.90 (75.60 to 76.60): VN062469.D (-2677) (-)

Ion 77.90 (77.60 to 78.60): VN062469.D (-2677) (-)


Time-->



Abundance Ion 75.90 (75.60 to 76.60): VN062469.D (-2677) (-)

Ion 77.90 (77.60 to 78.60): VN062469.D (-2677) (-)





Time-->



#59
2-Hexanone
Concen: 27.957 ug/l
RT: 10.74 min Scan# 2788
Delta R.T. 0.02 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02




Instrument :
MSVOA_N
ClientSampleId :
PB130035TB


Tot Ion: 43 Resp: 84582
Ion Ratio Lower Upper
43 100
58 17.4 25.1 75.2#

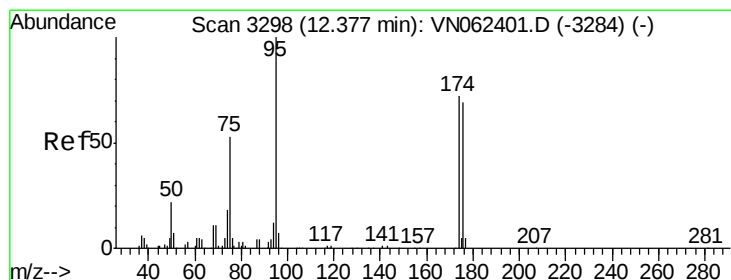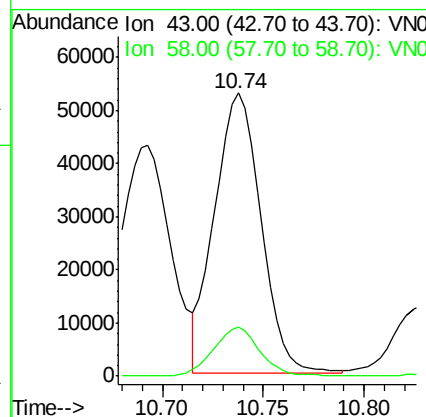

#62
4-Bromofluorobenzene
Concen: 53.365 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.00 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion: 95 Resp: 178416
Ion Ratio Lower Upper
95 100
174 69.8 0.0 141.6
176 68.2 0.0 137.2


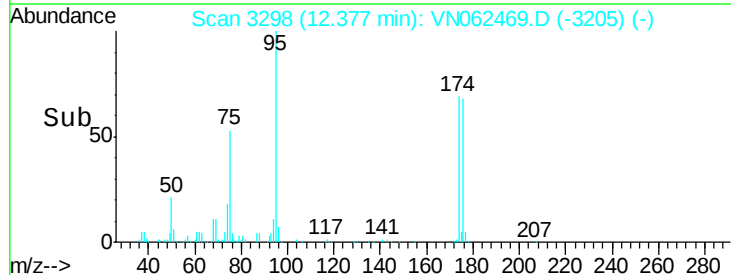
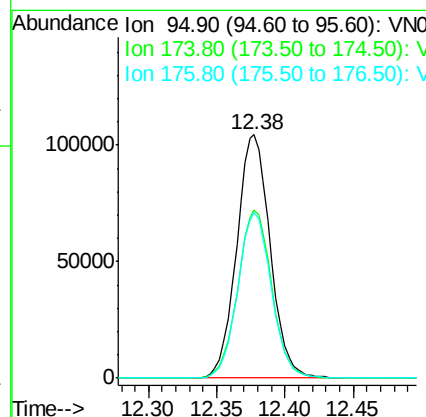





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. -0.00 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02




Instrument :
MSVOA_N
ClientSampled :
PB130035TB


Tot Ion:117 Resp: 361139
Ion Ratio Lower Upper
117 100
82 59.9 49.6 74.4
119 32.3 25.4 38.0

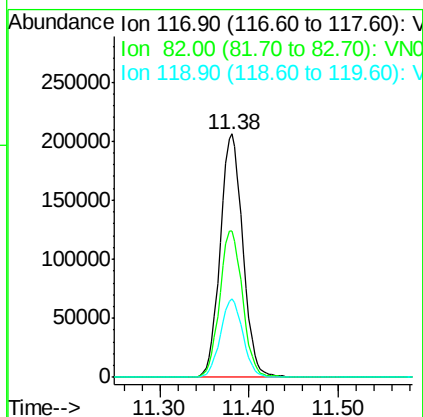

#71
Bromoform
Concen: 0.547 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. 0.27 min
Lab File: VN062469.D
Acq: 9 Jul 2020 21:02

Tgt Ion:173 Resp: 1037
Ion Ratio Lower Upper
173 100
175 747.6 23.7 71.1#
254 0.0 0.0 0.0

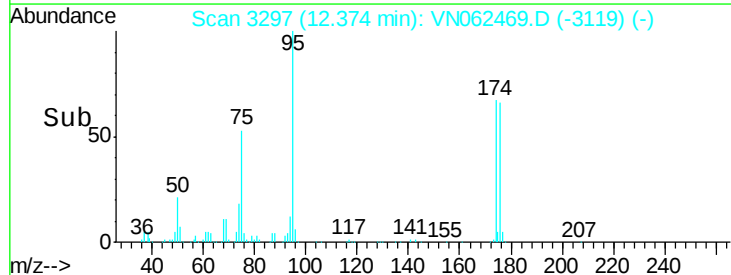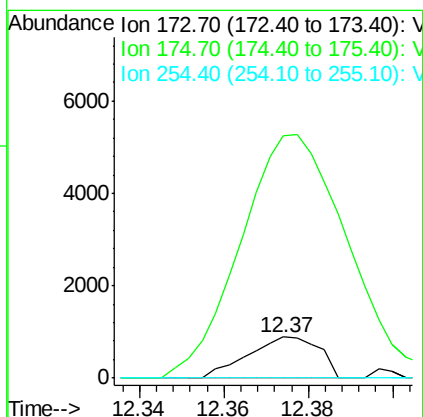



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. -0.00 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampleId :

PB130035TB


Tot Ion:152 Resp: 135522

Ion Ratio Lower Upper

152 100

115 63.3 31.4 94.2




150 160.2 0.0 347.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

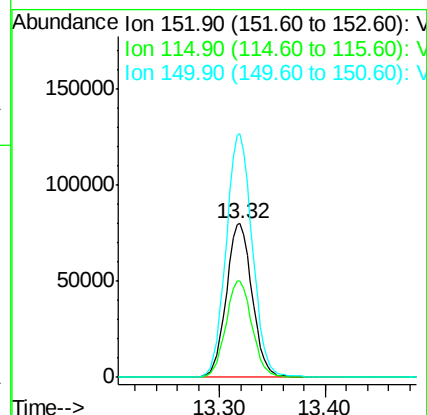

#74

N-ethyl acetate

Concen: 0.620 ug/l

RT: 12.00 min Scan# 3182

Delta R.T. -0.04 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Tgt Ion: 43 Resp: 3167


Ion Ratio Lower Upper

43 100

70 0.0 30.0 45.0#

55 0.0 18.2 27.4#

61 0.0 17.7 26.5#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V



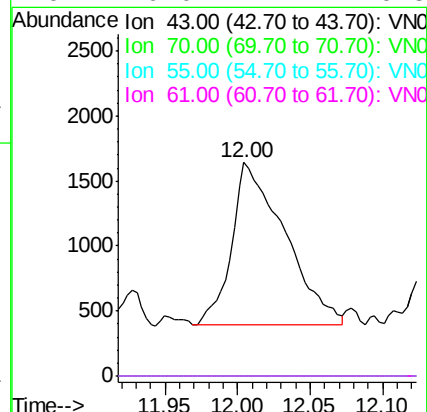





#76
 1,2,3-Trichloropropane
 Concen: 28.333 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. -0.15 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035TB


Tot Ion: 75 Resp: 94214
 Ion Ratio Lower Upper
 75 100
 77 1.2 0.0 0.0#

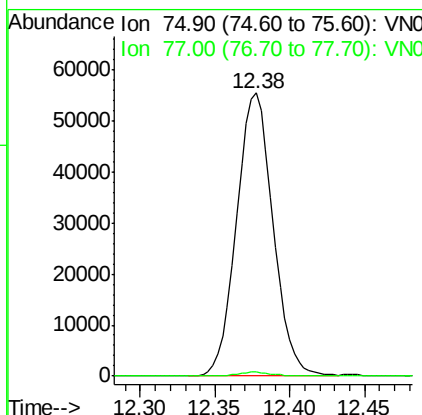

#80
 1,3,5-Trimethylbenzene
 Concen: 0.403 ug/l
 RT: 12.71 min Scan# 3402
 Delta R.T. 0.00 min
 Lab File: VN062469.D
 Acq: 9 Jul 2020 21:02

Tgt Ion: 105 Resp: 3465
 Ion Ratio Lower Upper
 105 100
 120 46.7 23.4 70.2

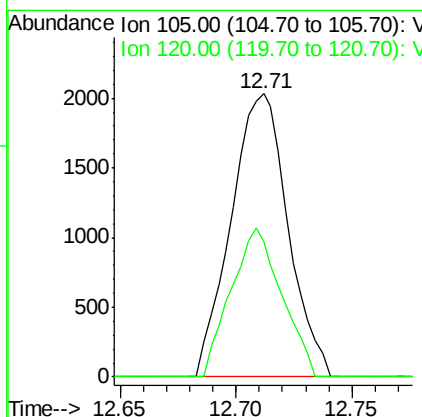



#81

trans-1,4-Dichloro-2-butene

Concen: 75.835 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.10 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02

Instrument :

MSVOA_N

ClientSampled :

PB130035TB


Tot Ion: 75 Resp: 94214

Ion Ratio Lower Upper

75 100

53 0.0 79.2 118.8#




89 0.0 34.6 52.0#



Abundance Ion 74.90 (74.60 to 75.60): VN062401.D (-3256) (-)

Ion 53.00 (52.70 to 53.70): VN062401.D (-3256) (-)

Ion 88.90 (88.60 to 89.60): VN062401.D (-3256) (-)

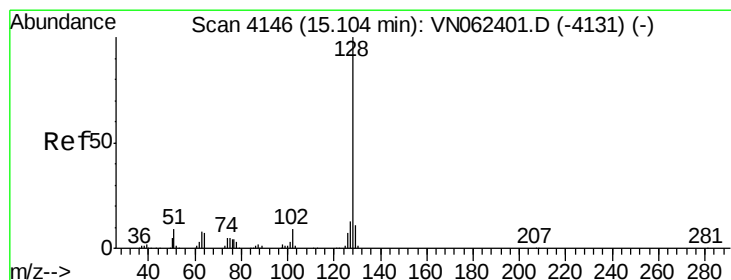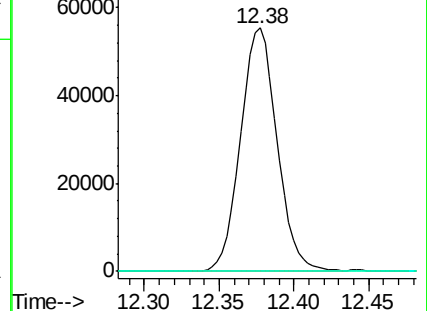

#95

Naphthalene

Concen: Below Cal

RT: 15.10 min Scan# 4146

Delta R.T. 0.00 min

Lab File: VN062469.D

Acq: 9 Jul 2020 21:02


Tgt Ion: 128 Resp: 1223

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.2#

129 0.0 8.6 12.8#



Abundance Ion 128.00 (127.70 to 128.70): VN062401.D (-4131) (-)

Ion 127.00 (126.70 to 127.70): VN062401.D (-4131) (-)

Ion 129.00 (128.70 to 129.70): VN062401.D (-4131) (-)

