

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN070920\
 Data File : VN062471.D
 Acq On : 9 Jul 2020 21:50
 Operator : JC/MD
 Sample : PB130035ZHE#02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035ZHE#02

Quant Time: Jul 10 02:23:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 00:55:52 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	206510	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	382188	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	370368	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	139567	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	160832	50.63	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.26%	
35) Dibromofluoromethane	7.55	113	119051	50.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.78%	
50) Toluene-d8	10.06	98	495038	53.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.16%	
62) 4-Bromofluorobenzene	12.38	95	183381	53.81	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.62%	
Target Compounds						
16) Acetone	3.78	43	13764	10.206	ug/l	96
18) Methyl Acetate	4.29	43	5450	1.619	ug/l #	86
20) Methylene Chloride	4.51	84	19263	6.681	ug/l	91
43) Isopropyl Acetate	8.13	43	75761	10.652	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN070920\
Data File : VN062471.D
Acq On : 9 Jul 2020 21:50
Operator : JC/MD
Sample : PB130035ZHE#02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB130035ZHE#02

Quant Time: Jul 10 02:23:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 00:55:52 2020
Response via : Initial Calibration

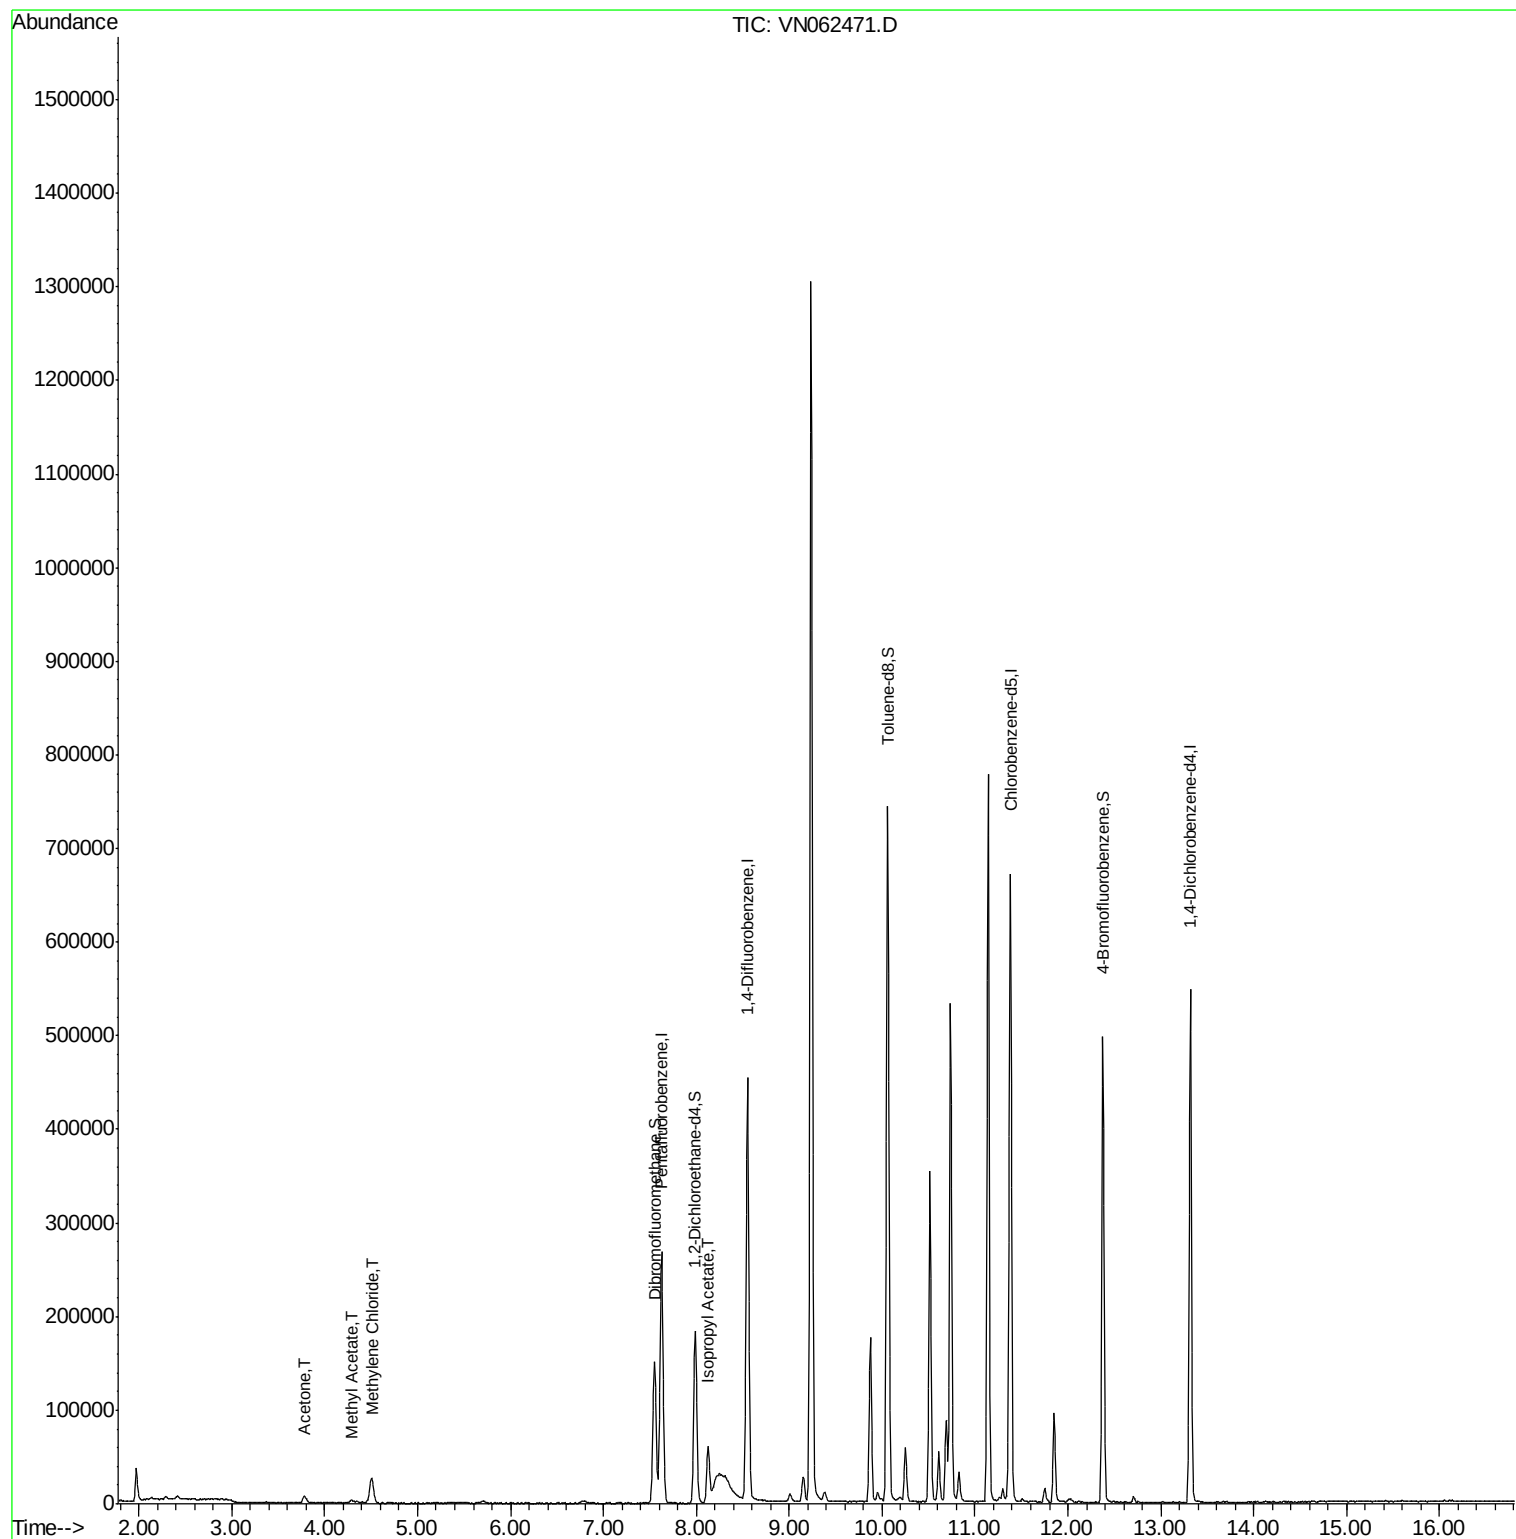

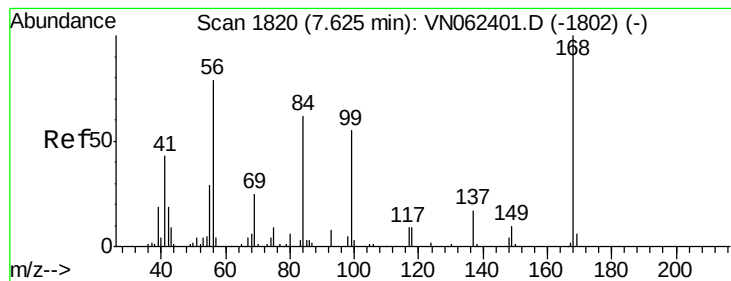

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN062471.D

Acq: 9 Jul 2020 21:50

Instrument :

MSVOA_N

ClientSampleId :


PB130035ZHE#02

Tot Ion:168 Resp: 206510

Ion Ratio Lower Upper




168 100

99 61.8 48.8 73.2

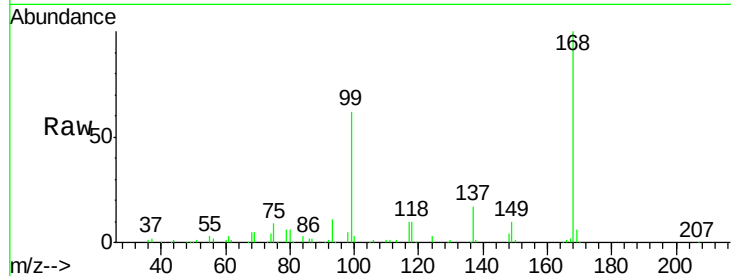

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

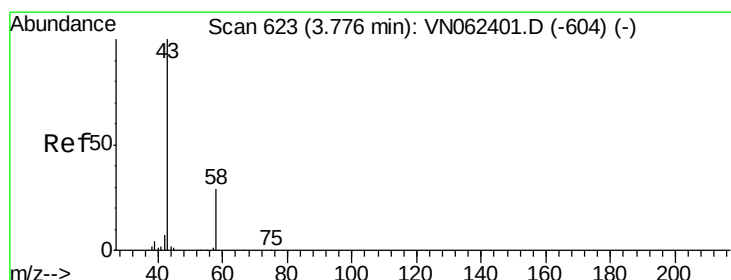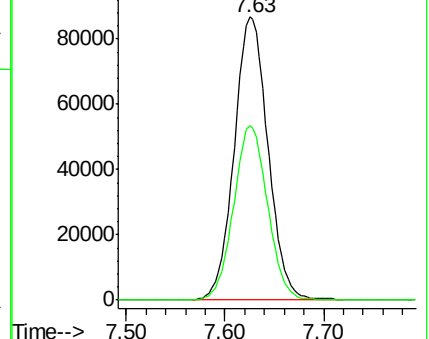

#16

Acetone

Concen: 10.206 ug/l

RT: 3.78 min Scan# 624

Delta R.T. 0.00 min

Lab File: VN062471.D


Acq: 9 Jul 2020 21:50

Tgt Ion: 43 Resp: 13764

Ion Ratio Lower Upper



43 100


58 31.4 23.5 35.3

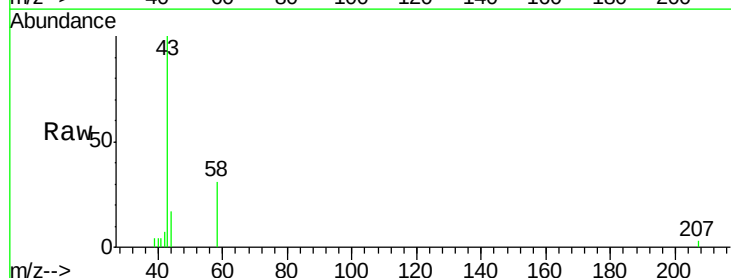

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




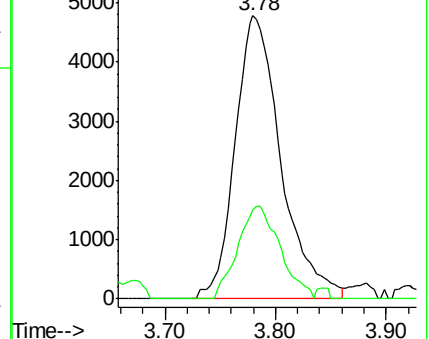




#18
Methvl Acetate
Concen: 1.619 ug/l
RT: 4.29 min Scan# 783
Delta R.T. 0.01 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50




Instrument :
MSVOA_N
ClientSampleId :
PB130035ZHE#02


Tot Ion: 43 Resp: 5450
Ion Ratio Lower Upper
43 100
74 13.8 16.0 24.0#

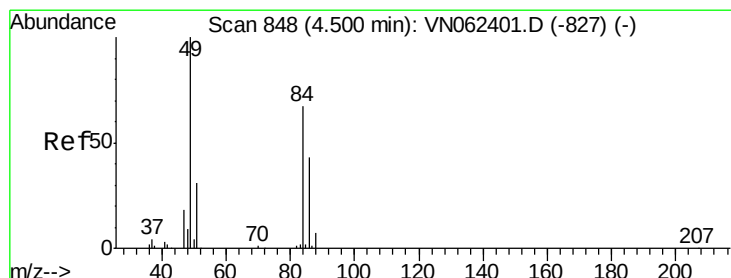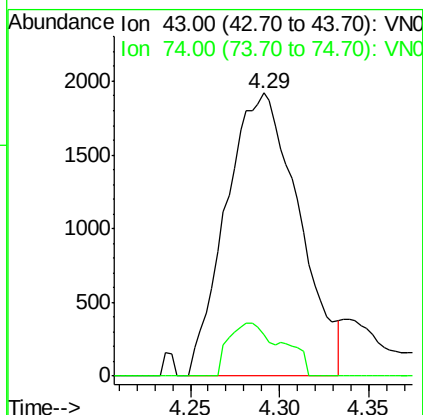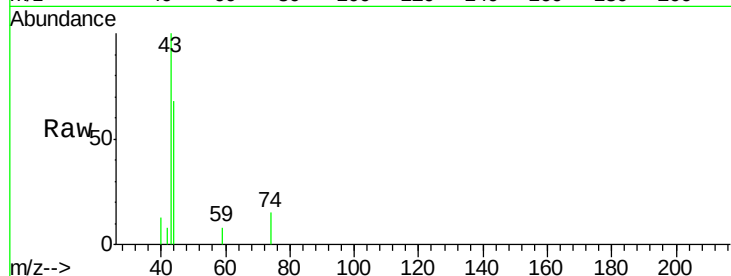

#20
Methylene Chloride
Concen: 6.681 ug/l
RT: 4.51 min Scan# 850
Delta R.T. 0.01 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50

Tgt Ion: 84 Resp: 19263
Ion Ratio Lower Upper
84 100
49 136.0 120.0 180.0
51 40.0 37.0 55.6
86 60.1 51.8 77.6



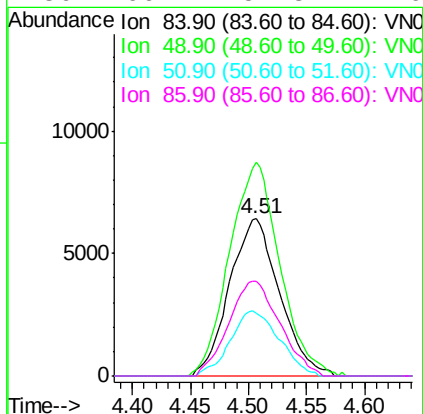
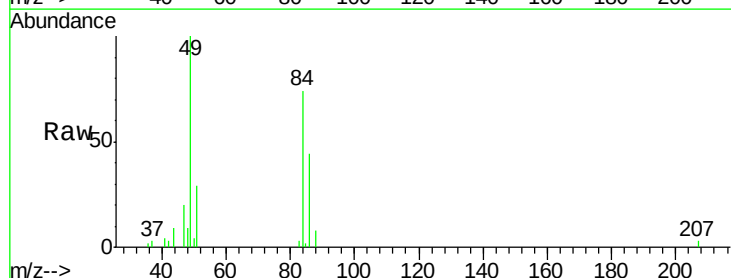


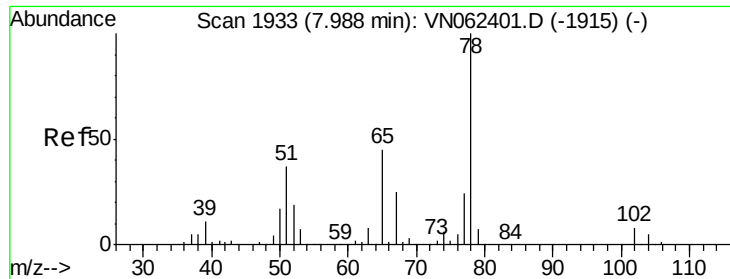

#33
 1,2-Dichloroethane-d4
 Concen: 50.634 ug/l
 RT: 7.99 min Scan# 1933
 Delta R.T. 0.00 min
 Lab File: VN062471.D
 Acq: 9 Jul 2020 21:50




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035ZHE#02


Tot Ion: 65 Resp: 160832
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 107.6

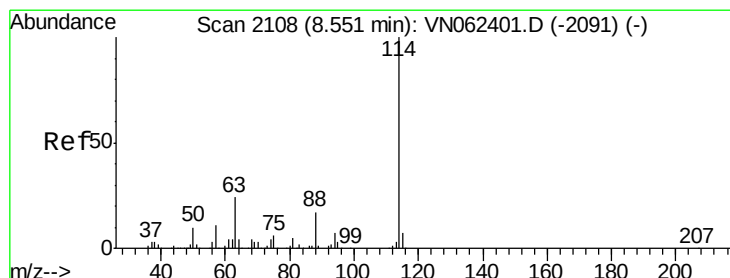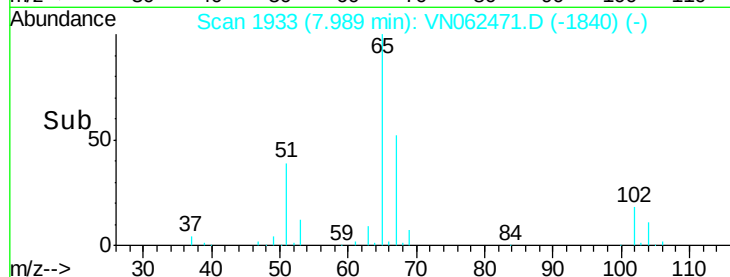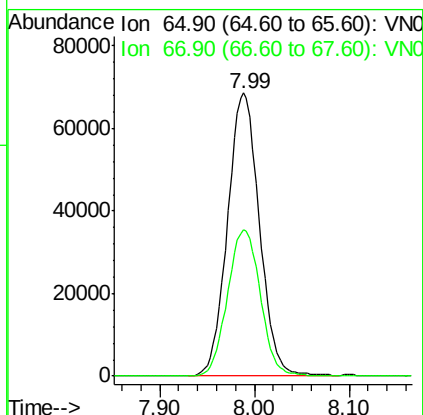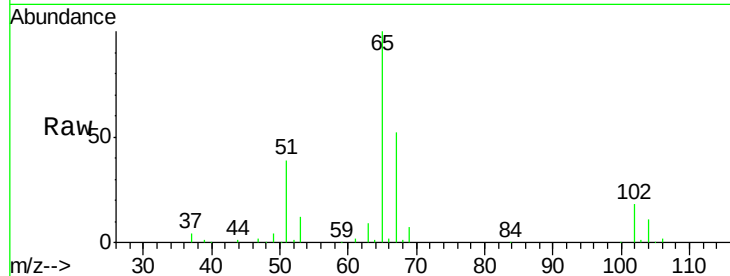

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. 0.00 min
 Lab File: VN062471.D
 Acq: 9 Jul 2020 21:50

Tgt Ion: 114 Resp: 382188
 Ion Ratio Lower Upper
 114 100
 63 24.0 0.0 48.4
 88 16.6 0.0 33.8


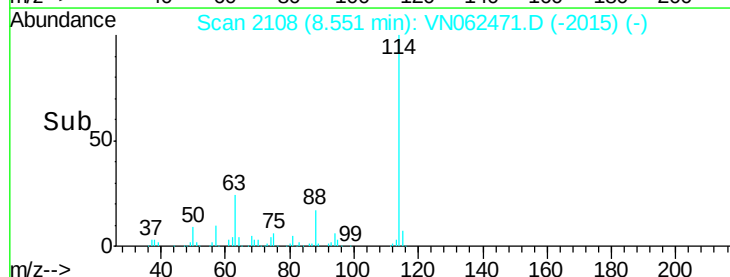
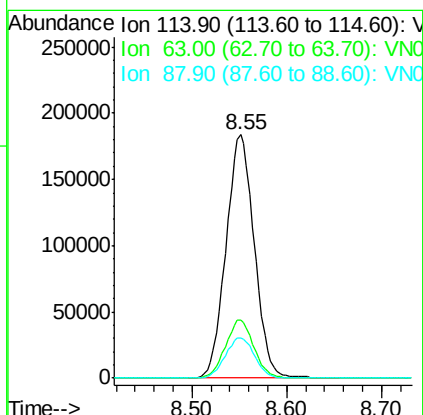
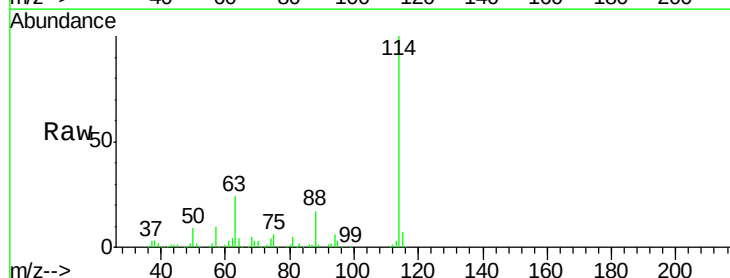




#35
 Dibromofluoromethane
 Concen: 50.393 ug/l
 RT: 7.55 min Scan# 1797
 Delta R.T. 0.00 min
 Lab File: VN062471.D
 Acq: 9 Jul 2020 21:50




Instrument :
 MSVOA_N
 ClientSampleId :
 PB130035ZHE#02


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.2	83.1	124.7
192	18.0	14.1	21.1

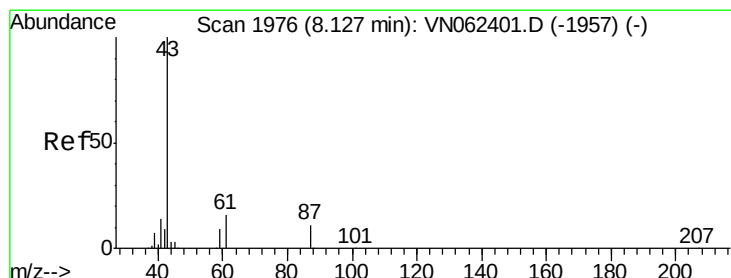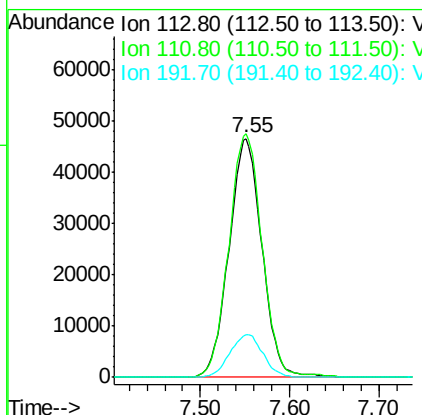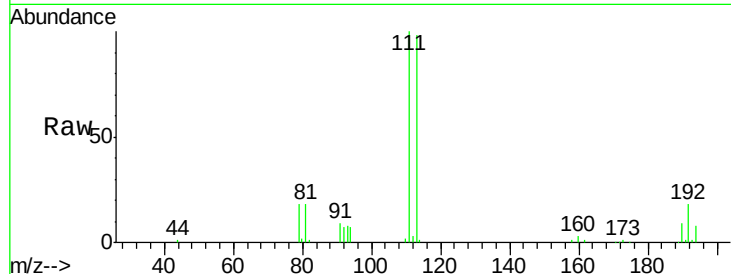

#43
 Isopropyl Acetate
 Concen: 10.652 ug/l
 RT: 8.13 min Scan# 1976
 Delta R.T. 0.00 min
 Lab File: VN062471.D
 Acq: 9 Jul 2020 21:50

Tgt Ion	Ratio	Lower	Upper
43	100		
61	18.7	19.3	28.9#
87	10.8	8.6	13.0



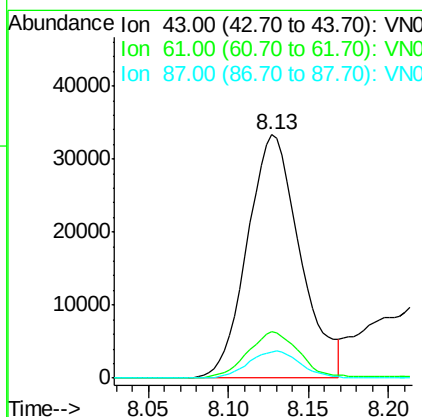
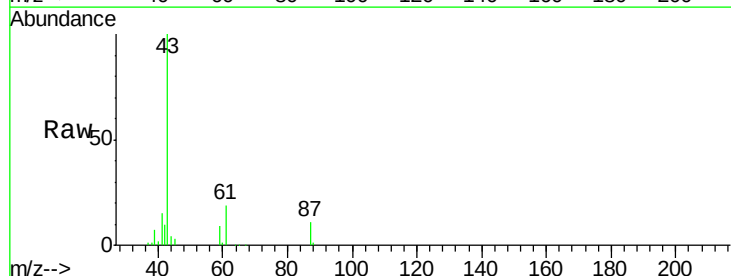


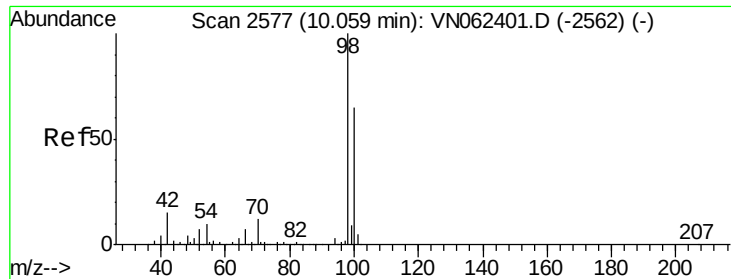

#50
Toluene-d8
Concen: 53.080 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. 0.00 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50




Instrument :
MSVOA_N
ClientSampleId :
PB130035ZHE#02


Tot Ion: 98 Resp: 495038
Ion Ratio Lower Upper
98 100
100 63.7 51.5 77.3

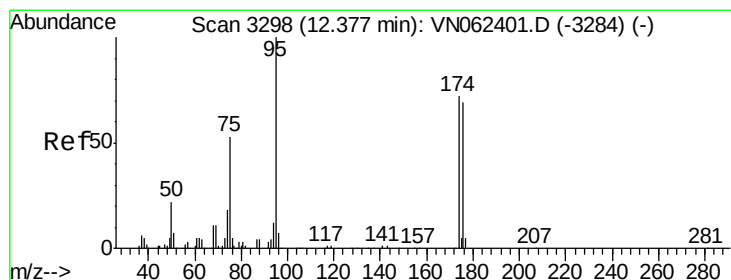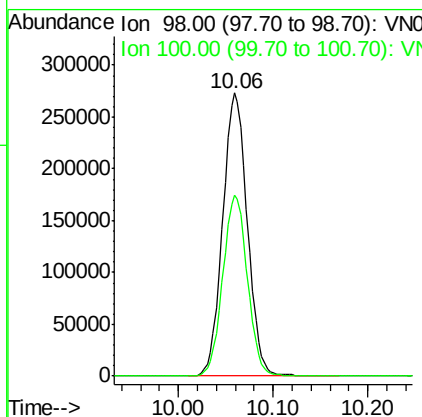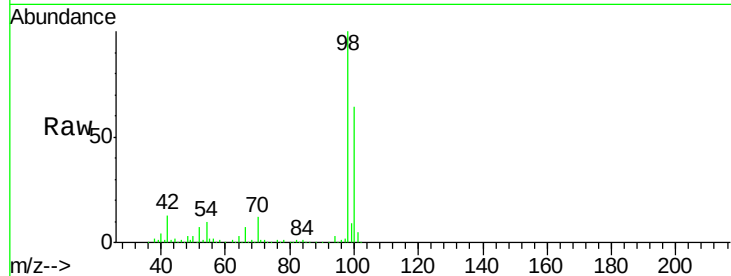

#62
4-Bromofluorobenzene
Concen: 53.807 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.00 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50

Tgt Ion: 95 Resp: 183381
Ion Ratio Lower Upper
95 100
174 69.8 0.0 141.6
176 67.3 0.0 137.2



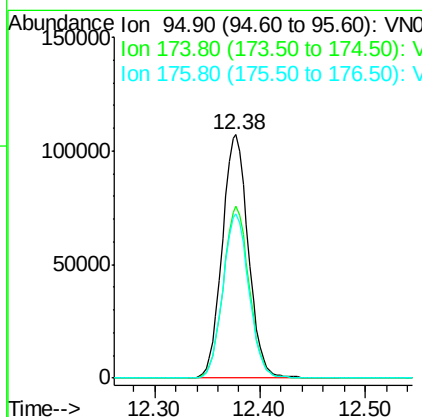
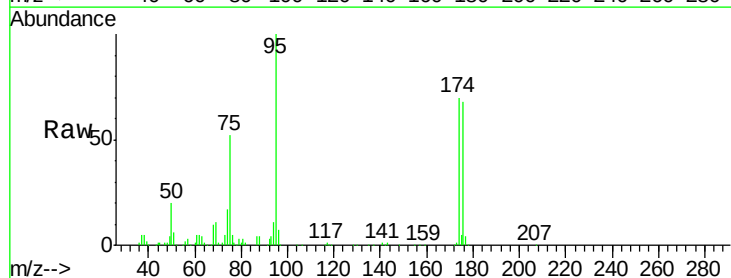


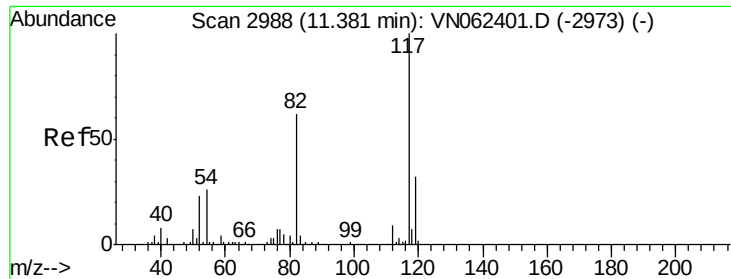

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50

Instrument :
MSVOA_N
ClientSampleId :
PB130035ZHE#02

Tot Ion:117 Resp: 370368
Ion Ratio Lower Upper
117 100
82 61.9 49.6 74.4
119 31.3 25.4 38.0

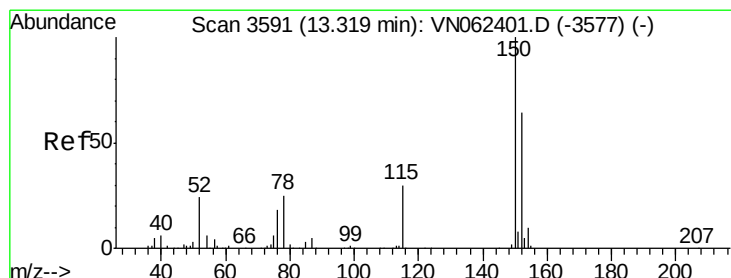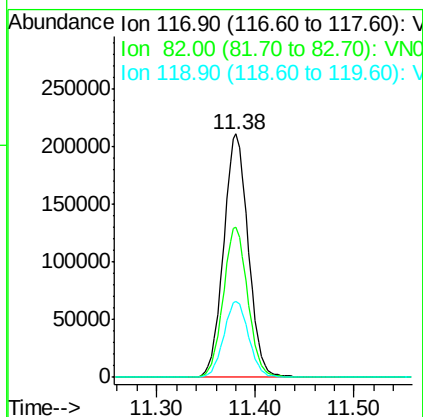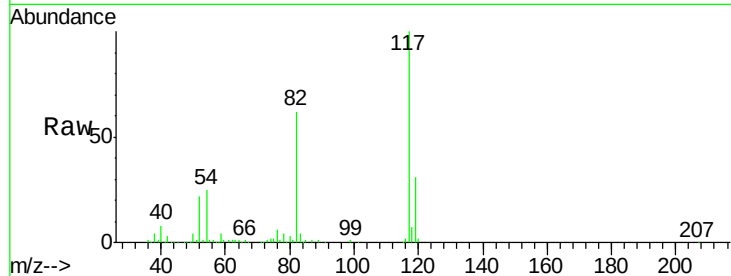

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3591
Delta R.T. 0.00 min
Lab File: VN062471.D
Acq: 9 Jul 2020 21:50

Tgt Ion:152 Resp: 139567
Ion Ratio Lower Upper
152 100
115 62.8 31.4 94.2
150 157.2 0.0 347.4

