


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN070920\
Data File : VN062446.D
Acq On : 9 Jul 2020 8:56
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Title : SW846 8260
Last Update : Fri Jul 10 00:55:52 2020

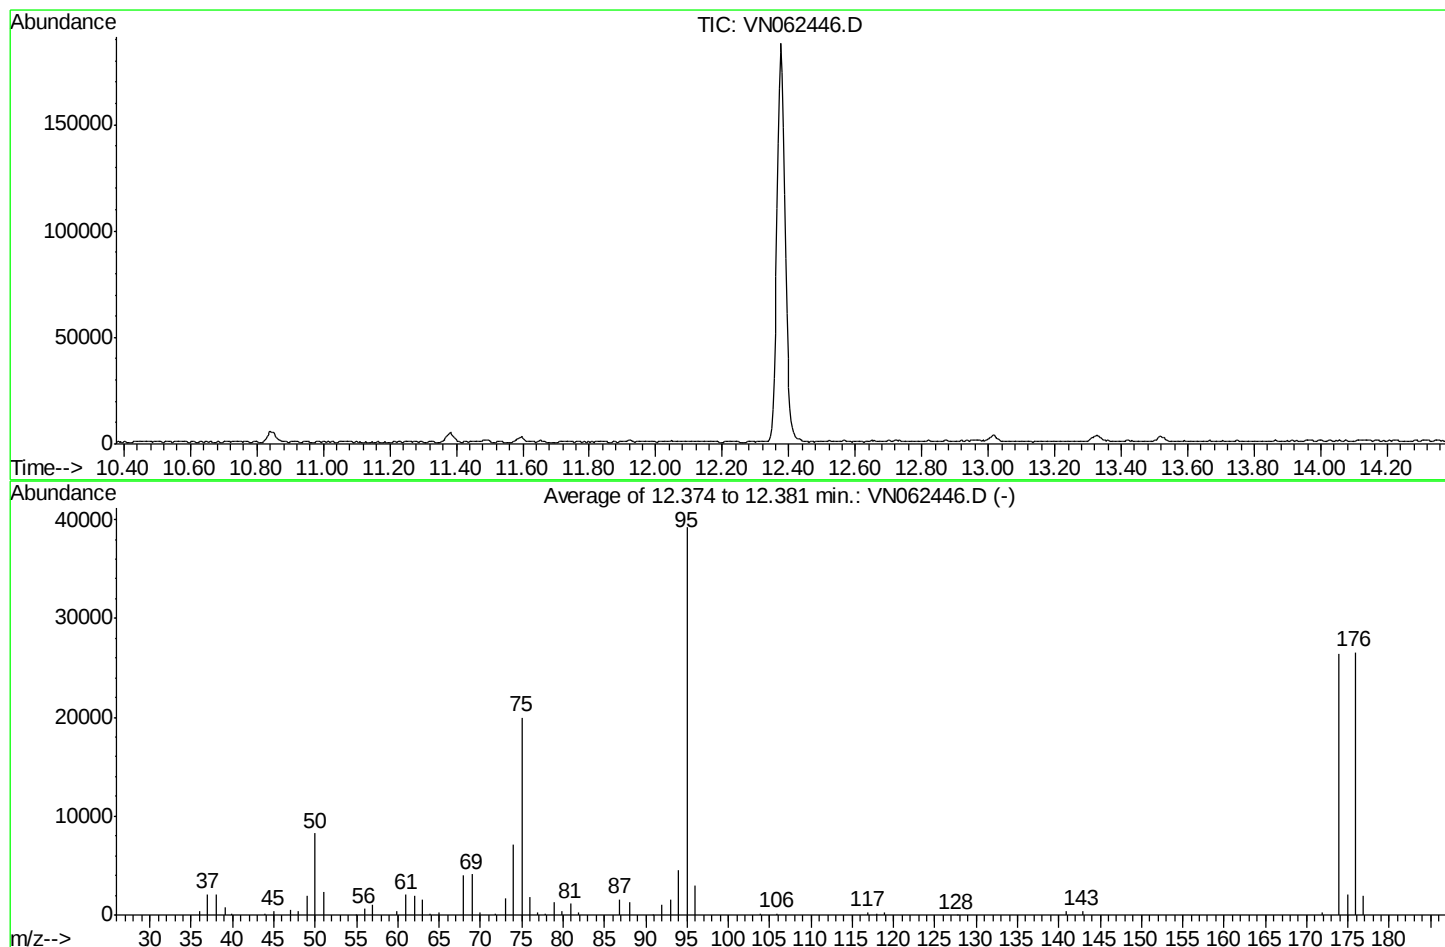

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	8249	PASS
75	95	30	60	50.9	19960	PASS
95	95	100	100	100.0	39213	PASS
96	95	5	9	7.5	2927	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.4	26440	PASS
175	174	5	9	8.0	2122	PASS
176	174	95	101	100.5	26562	PASS
177	176	5	9	7.1	1892	PASS