

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070921\
 Data File : VN067691.D
 Acq On : 9 Jul 2021 17:28
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jul 10 05:25:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	313240	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	583744	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	541558	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	196795	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	245168	51.789	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	103.580%
35) Dibromofluoromethane	8.024	113	174216	49.397	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.800%
50) Toluene-d8	10.446	98	746066	50.538	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	101.080%
62) 4-Bromofluorobenzene	12.734	95	237658	45.573	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070921\
Data File : VN067691.D
Acq On : 9 Jul 2021 17:28
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jul 10 05:25:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




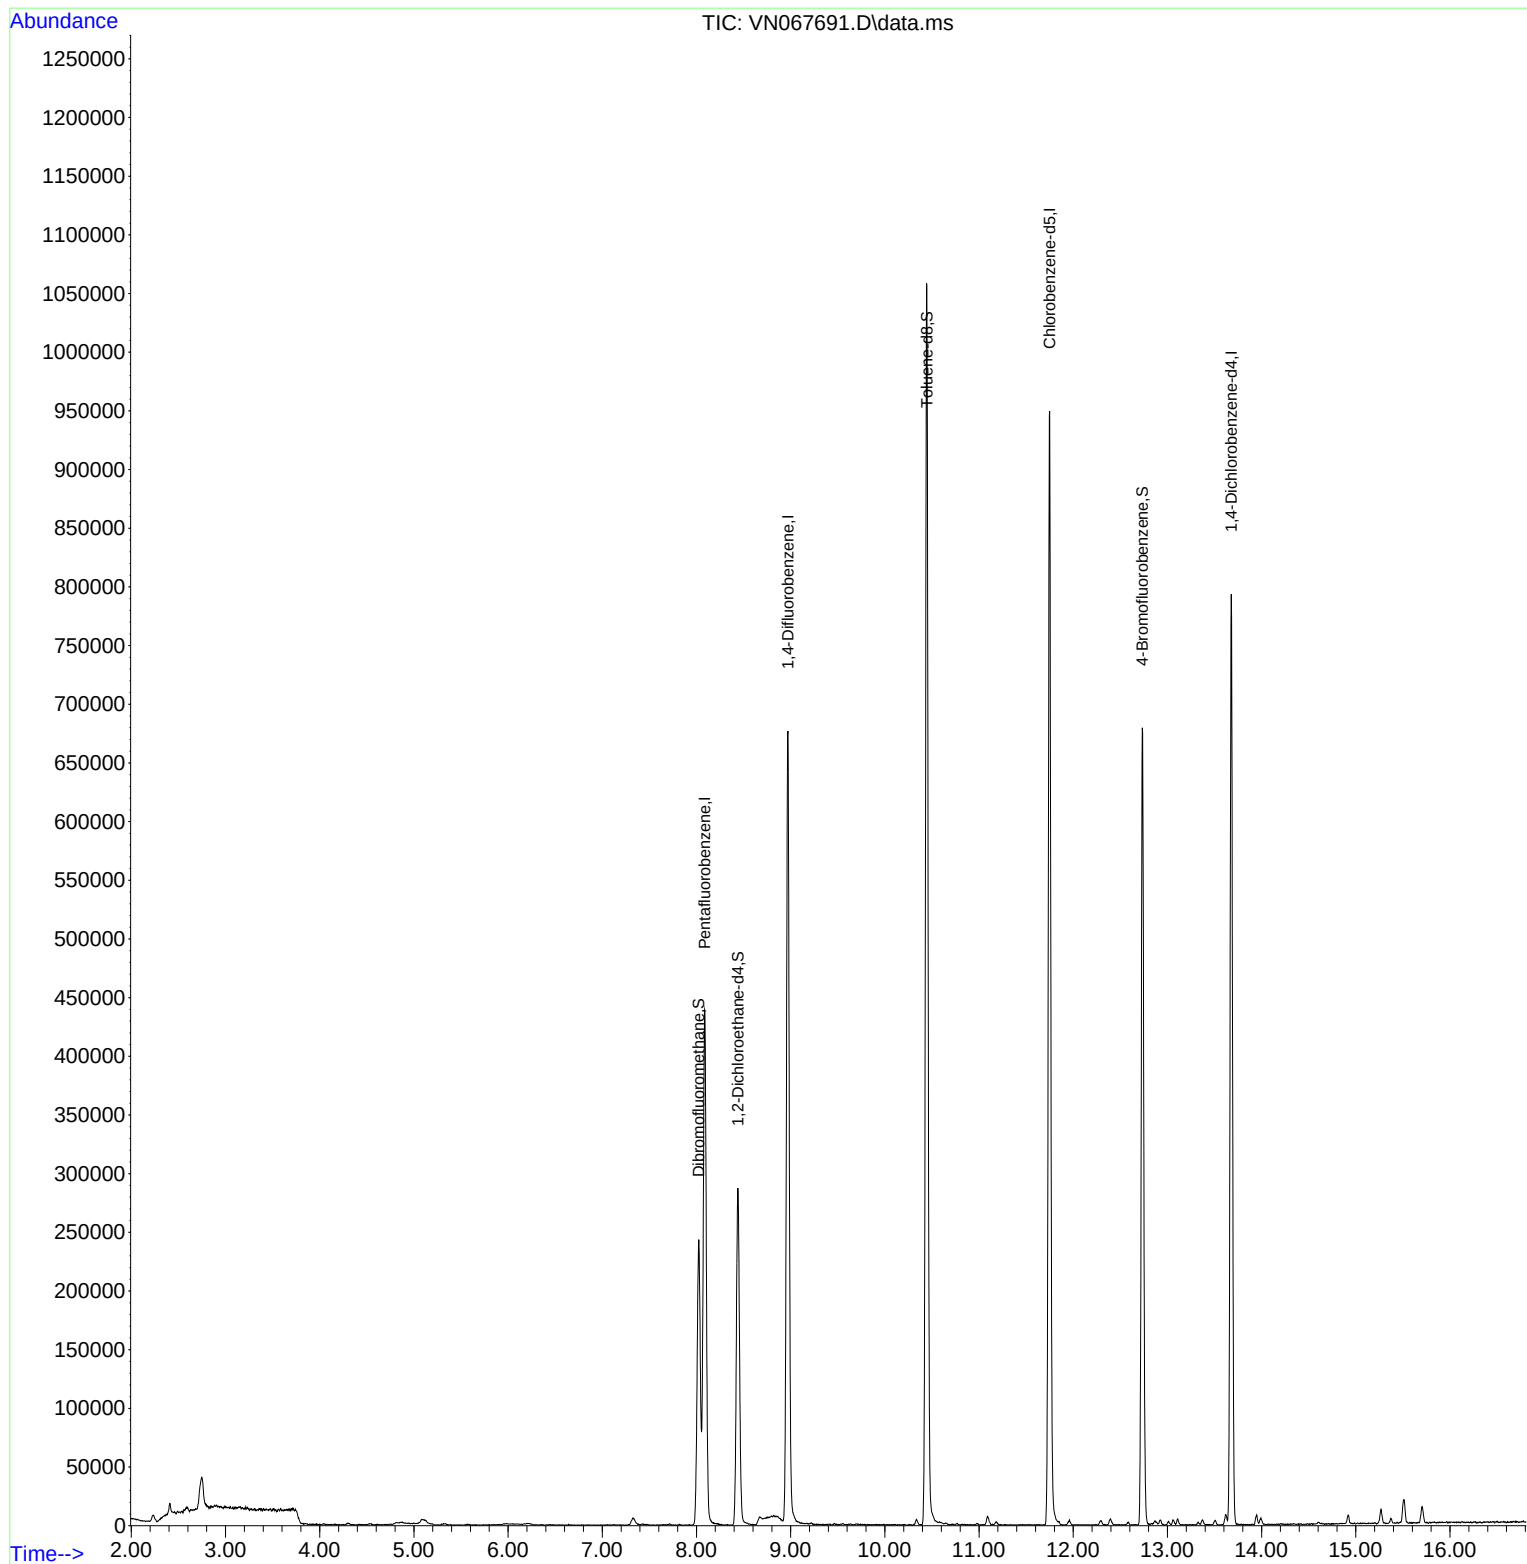


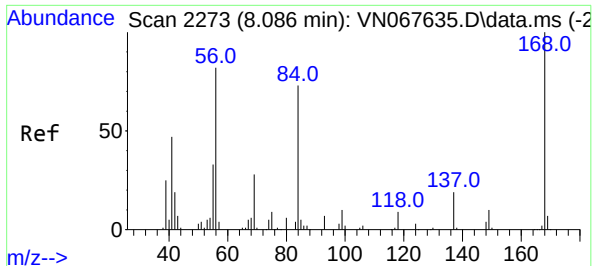

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:168 Resp: 313240
Ion Ratio Lower Upper
168 100
99 63.5 62.9 94.3

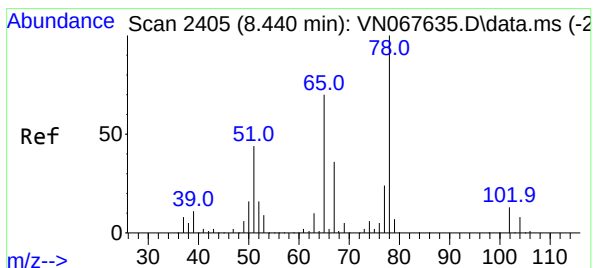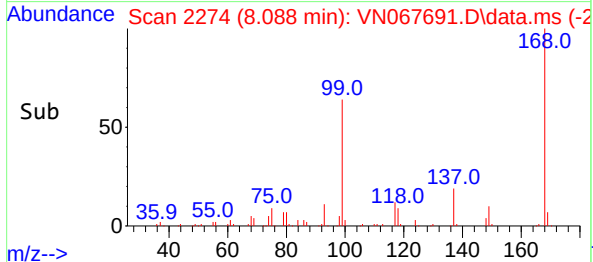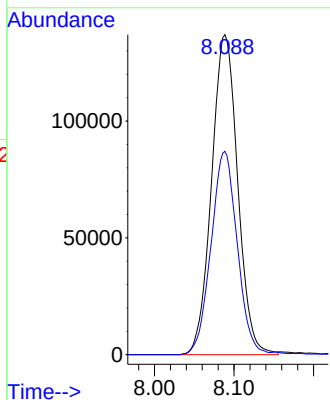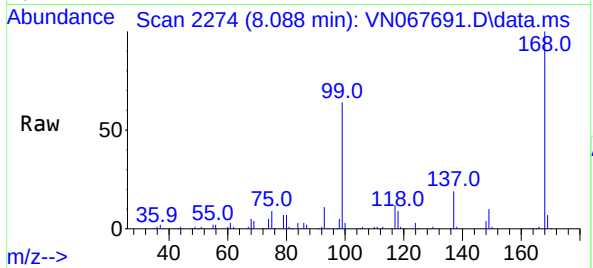

#33
1,2-Dichloroethane-d4
Concen: 51.789 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28

Tgt Ion: 65 Resp: 245168
Ion Ratio Lower Upper
65 100
67 51.0 0.0 98.6


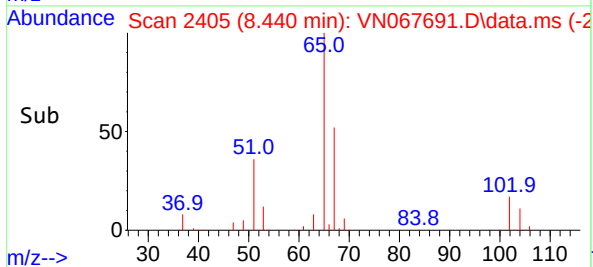
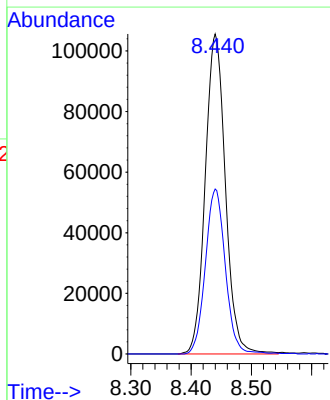
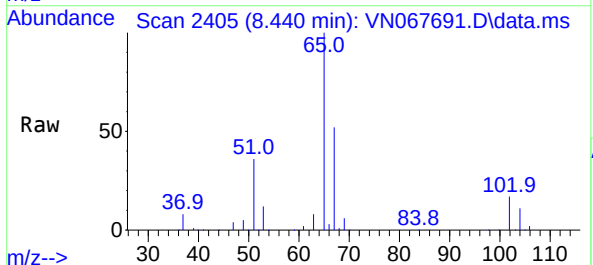


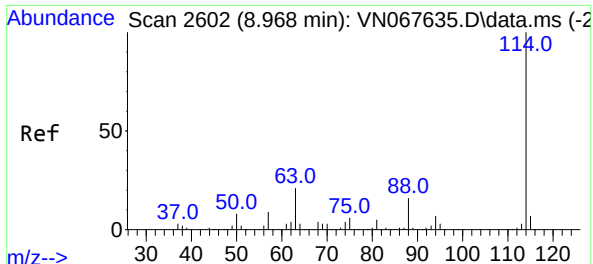

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 583744
Ion Ratio Lower Upper
114 100
63 21.7 0.0 49.0
88 14.8 0.0 36.6

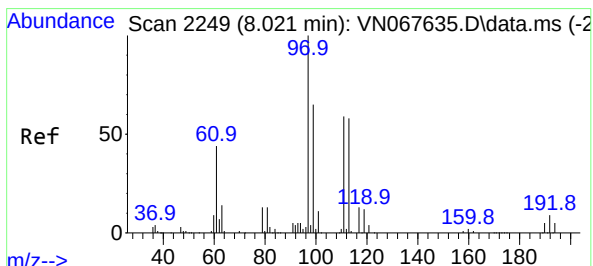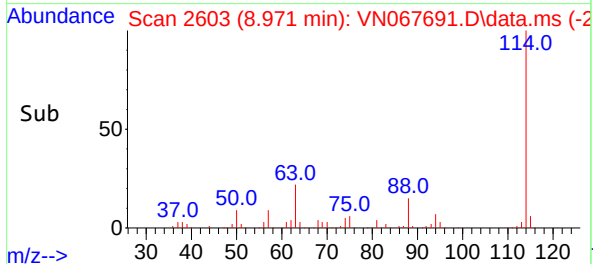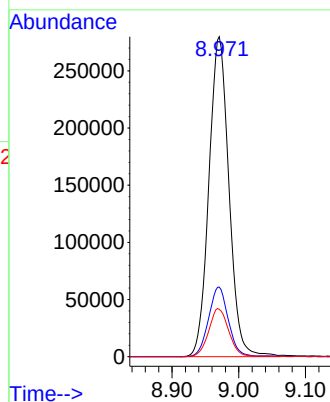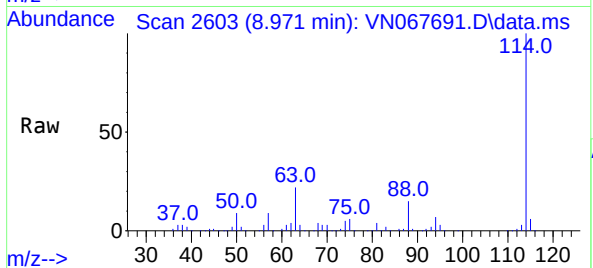

#35
Dibromofluoromethane
Concen: 49.397 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28

Tgt Ion:113 Resp: 174216
Ion Ratio Lower Upper
113 100
111 104.3 83.8 125.8
192 16.2 13.4 20.0


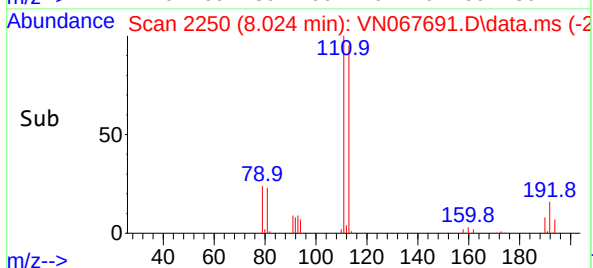
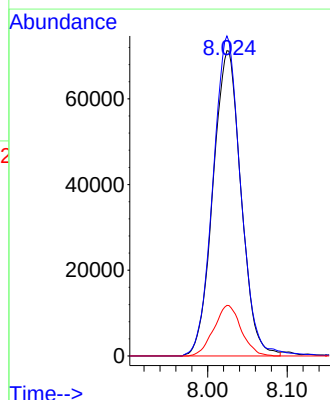
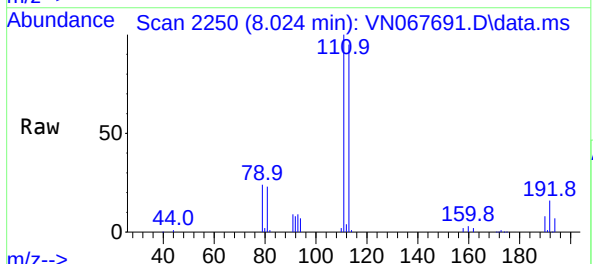


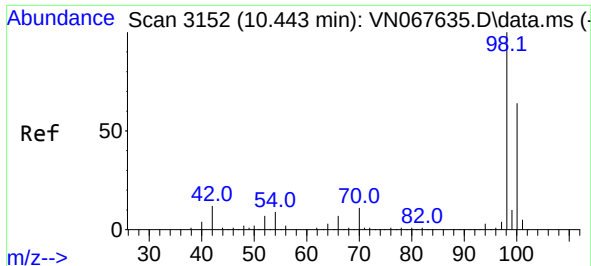

#50
Toluene-d8
Concen: 50.538 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 746066
Ion Ratio Lower Upper
98 100
100 63.3 51.7 77.5

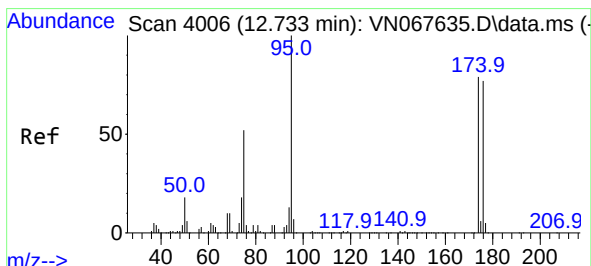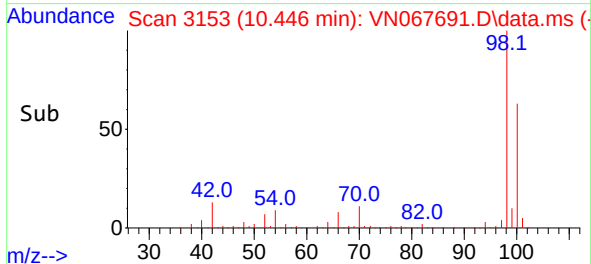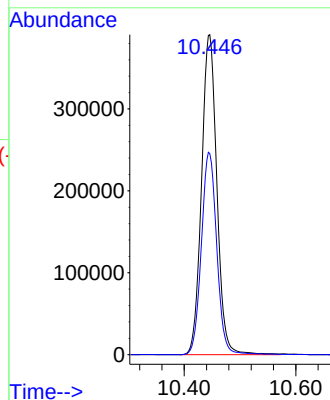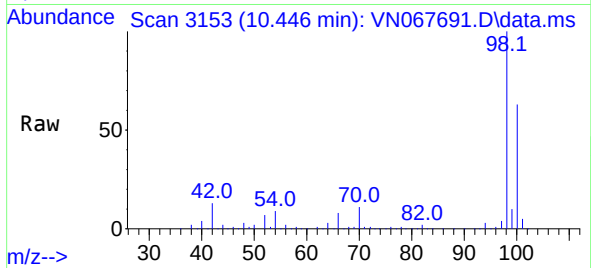

#62
4-Bromofluorobenzene
Concen: 45.573 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28

Tgt Ion: 95 Resp: 237658
Ion Ratio Lower Upper
95 100
174 70.9 0.0 122.0
176 68.0 0.0 117.6


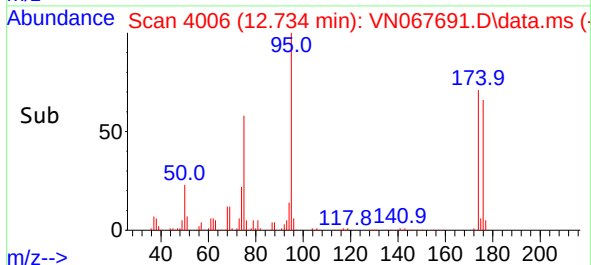
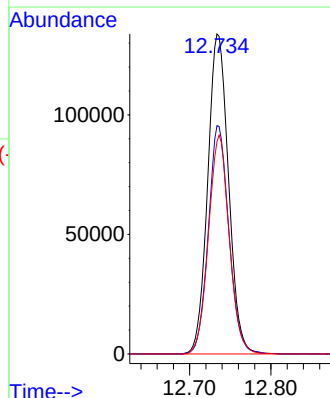
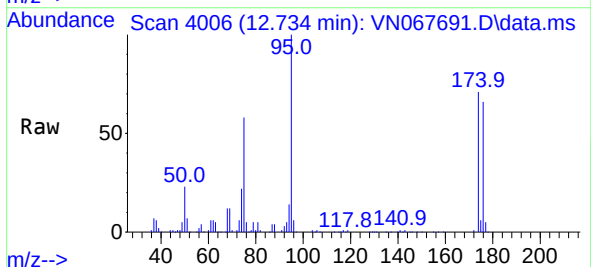


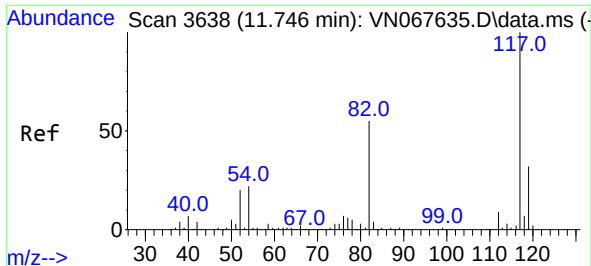

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 541558
Ion Ratio Lower Upper
117 100
82 57.4 53.1 79.7
119 32.2 25.5 38.3

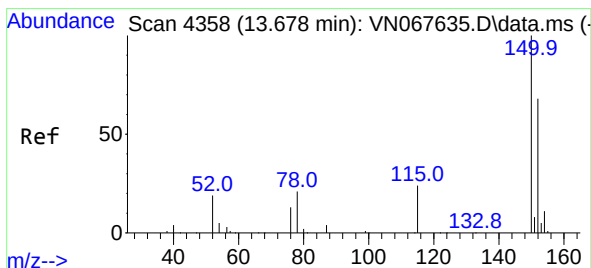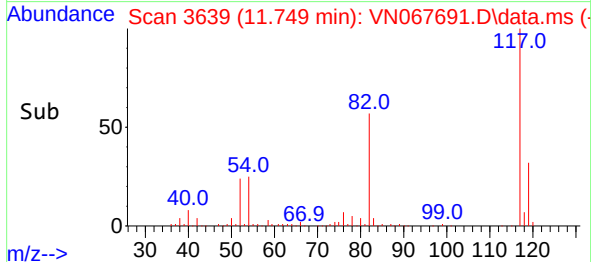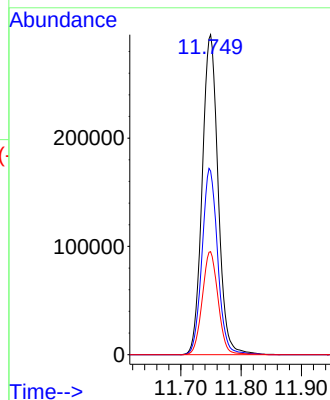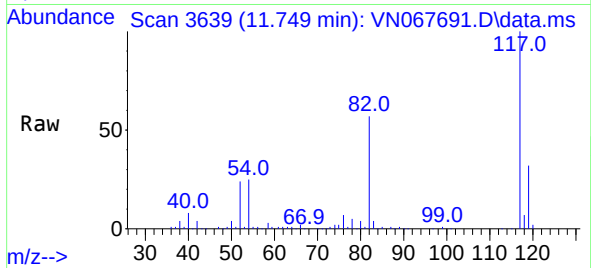

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067691.D
Acq: 9 Jul 2021 17:28

Tgt Ion:152 Resp: 196795
Ion Ratio Lower Upper
152 100
115 64.4 36.1 108.5
150 161.1 0.0 351.8

