


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070921\
 Data File : VN067676.D
 Acq On : 9 Jul 2021 9:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N070121W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jul 01 12:09:22 2021

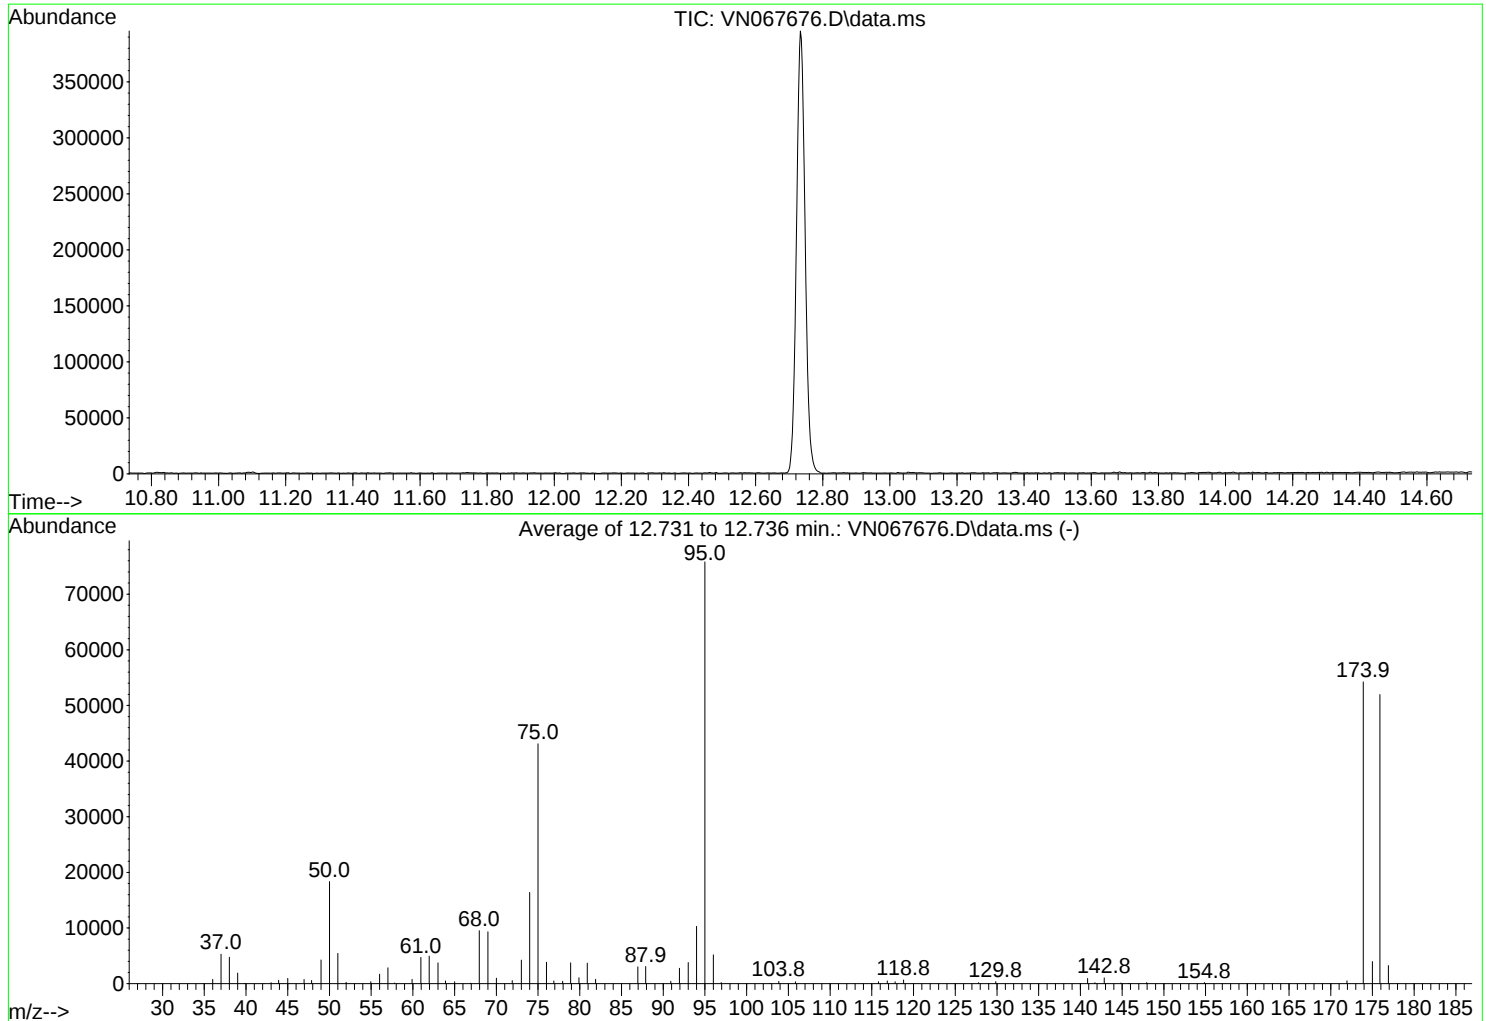

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	18355	PASS
75	95	30	60	56.9	43115	PASS
95	95	100	100	100.0	75811	PASS
96	95	5	9	6.8	5177	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.6	54248	PASS
175	174	5	9	7.3	3982	PASS
176	174	95	101	95.8	51971	PASS
177	176	5	9	6.2	3242	PASS