

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070924\
 Data File : VN082835.D
 Acq On : 09 Jul 2024 12:07
 Operator : JC\MD
 Sample : VN0709WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0709WBL01

Quant Time: Jul 10 01:19:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	106108	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	200923	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	199910	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	88074	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	82334	55.354	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.700%
35) Dibromofluoromethane	8.171	113	66918	51.904	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.800%
50) Toluene-d8	10.571	98	239687	50.334	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.660%
62) 4-Bromofluorobenzene	12.853	95	82747	48.375	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	96.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070924\
Data File : VN082835.D
Acq On : 09 Jul 2024 12:07
Operator : JC\MD
Sample : VN0709WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0709WBL01


Quant Time: Jul 10 01:19:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration

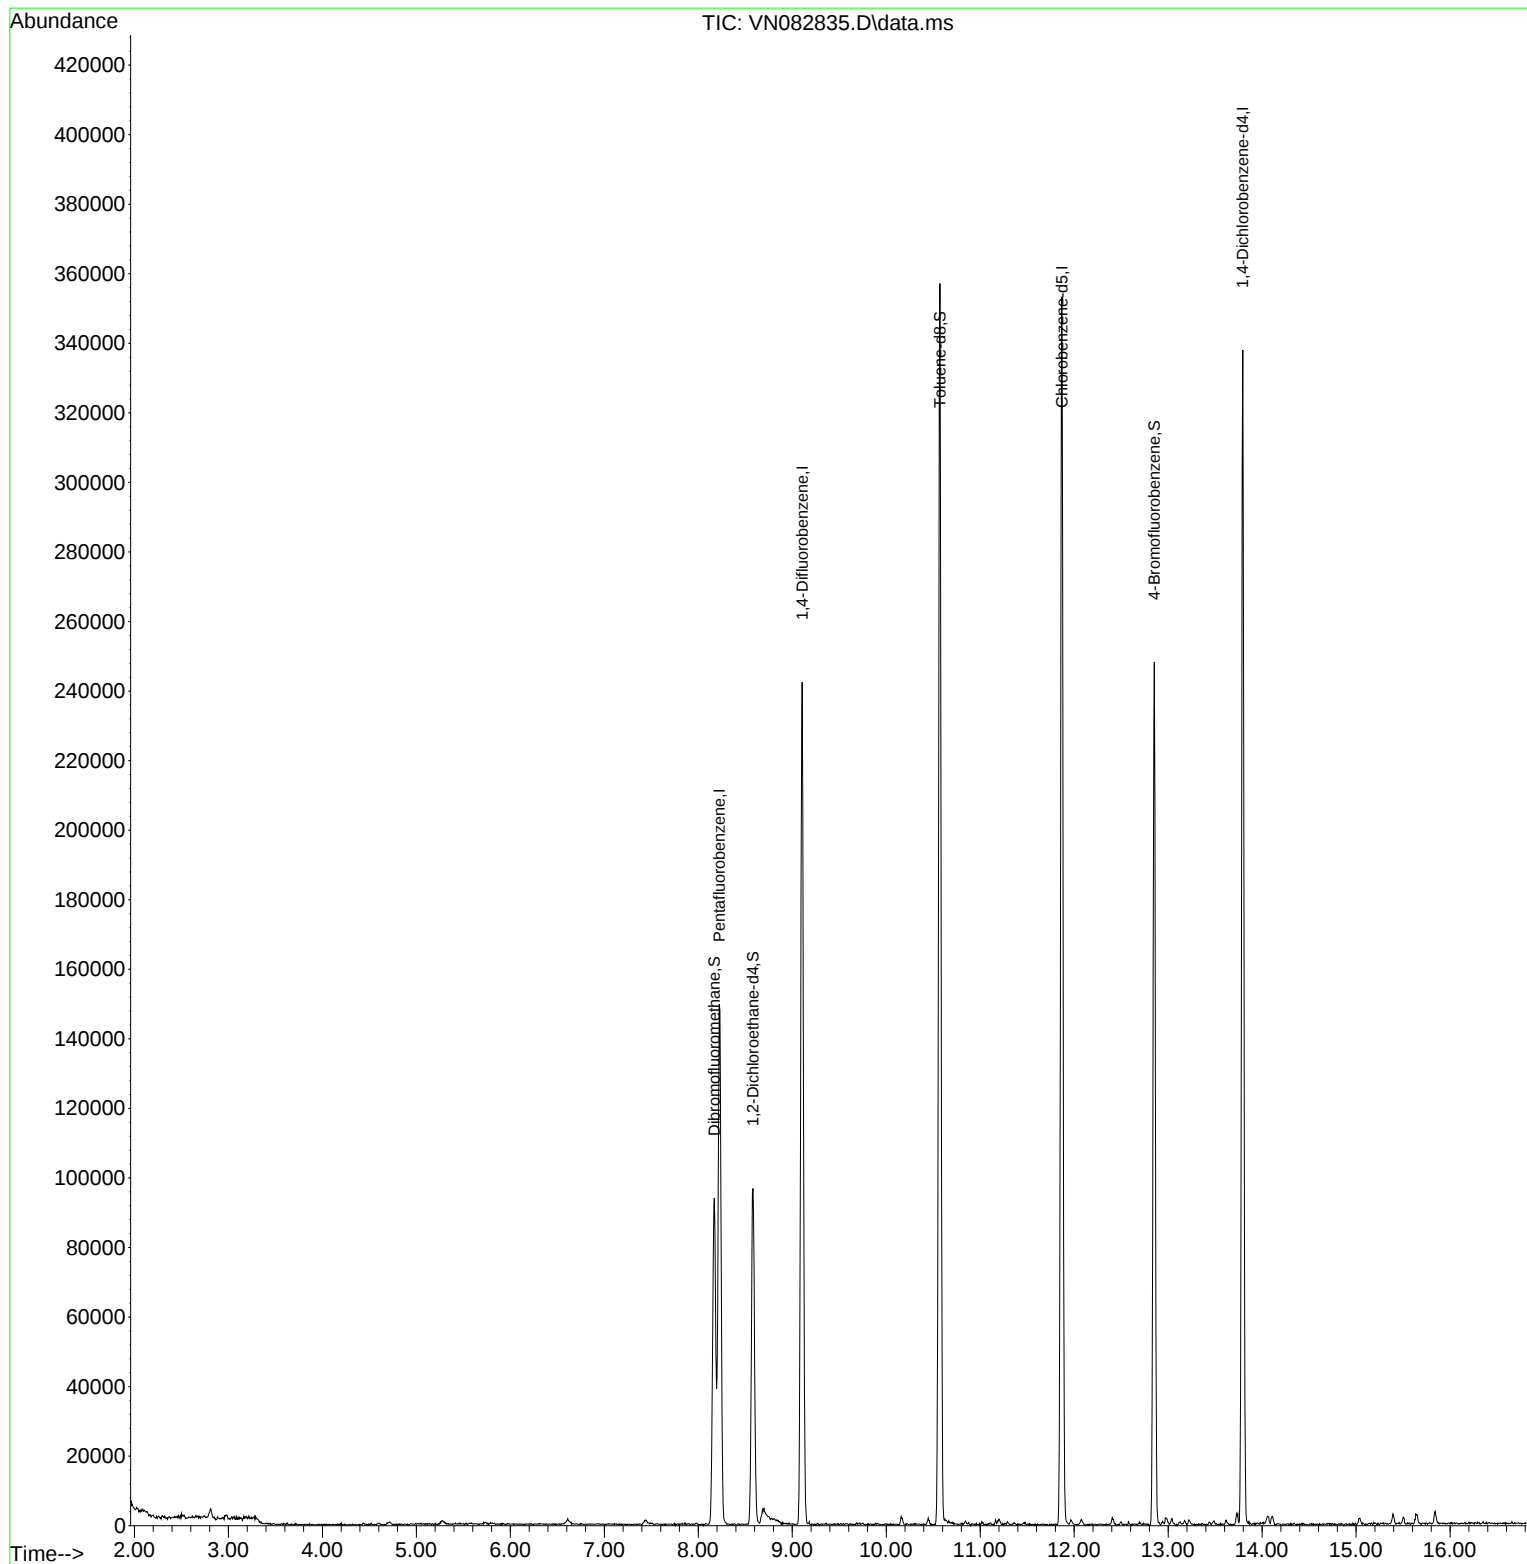



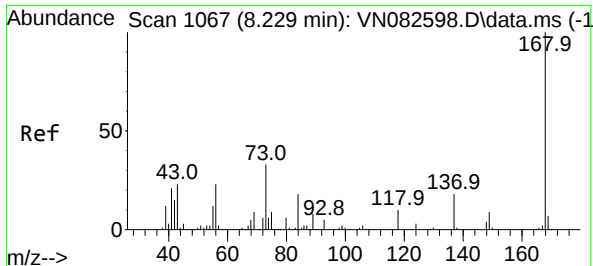


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.005 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Instrument :
MSVOA_N
ClientSampleId :
VN0709WBL01



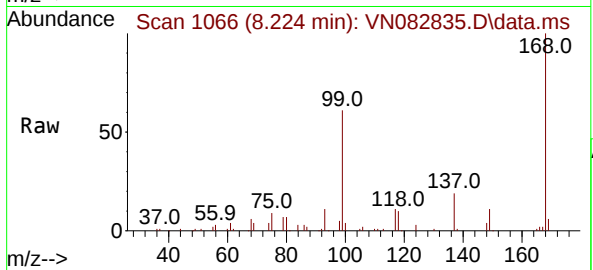



Tgt Ion:168 Resp: 106108
Ion Ratio Lower Upper
168 100
99 61.0 48.2 72.4

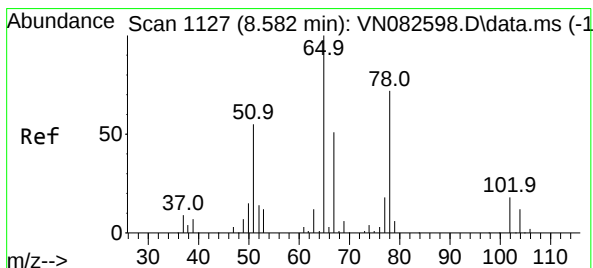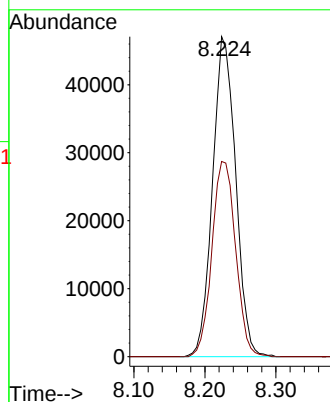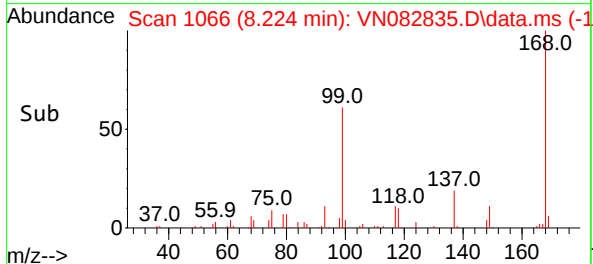

#33
1,2-Dichloroethane-d4
Concen: 55.354 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07


Tgt Ion: 65 Resp: 82334
Ion Ratio Lower Upper
65 100
67 49.8 0.0 104.4

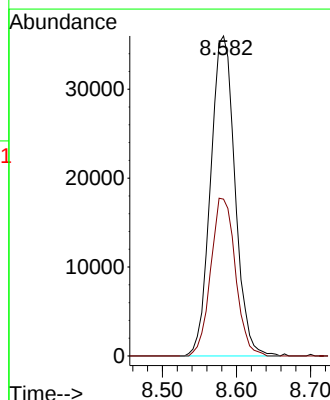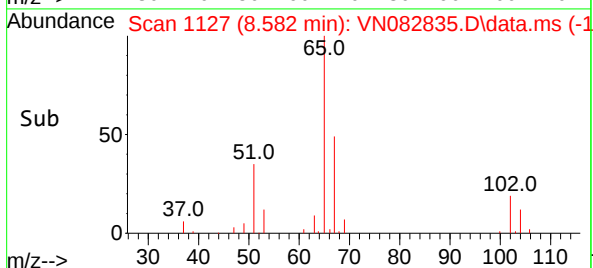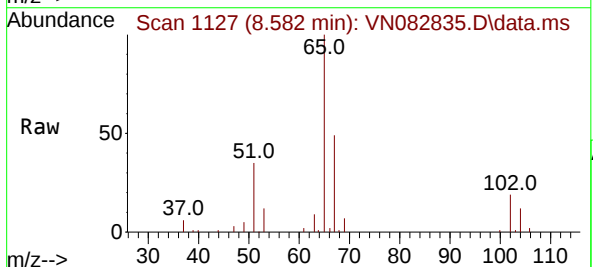



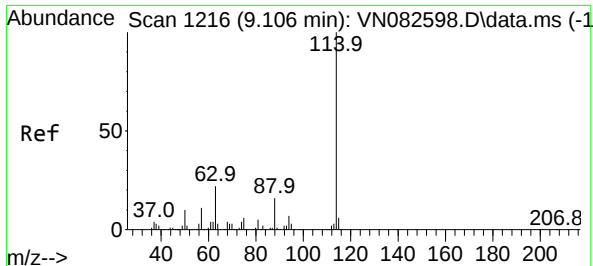


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Instrument :
MSVOA_N
ClientSampleId :
VN0709WBL01



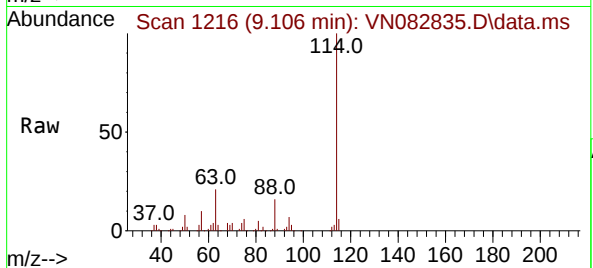



Tgt Ion:114 Resp: 200923
Ion Ratio Lower Upper
114 100
63 21.0 0.0 44.6
88 16.0 0.0 31.4

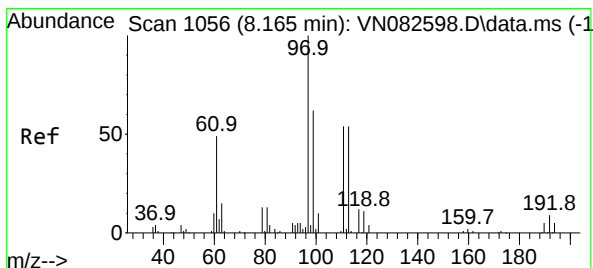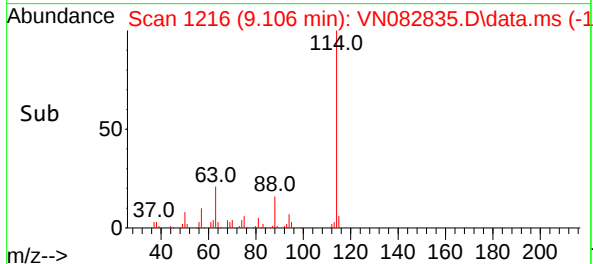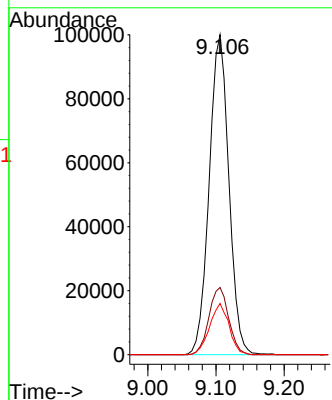

#35
Dibromofluoromethane
Concen: 51.904 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Tgt Ion:113 Resp: 66918
Ion Ratio Lower Upper
113 100
111 102.9 82.4 123.6
192 18.2 14.9 22.3


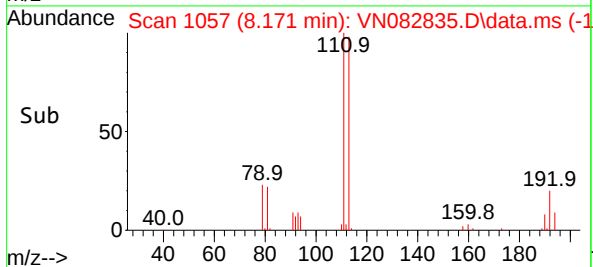
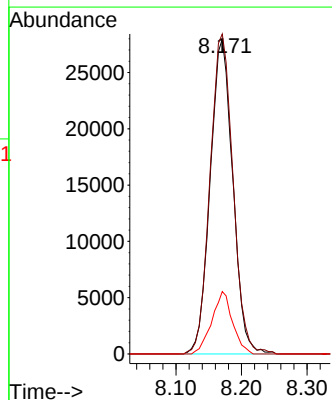
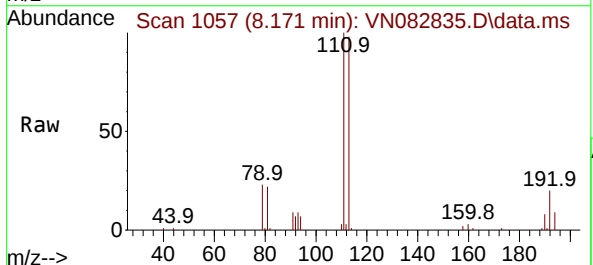


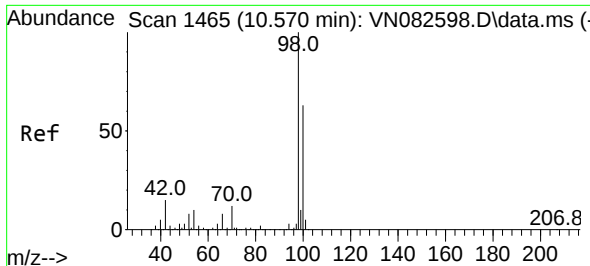

#50
Toluene-d8
Concen: 50.334 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07




Instrument :
MSVOA_N
ClientSampleId :
VN0709WBL01


Tgt Ion: 98 Resp: 239687
Ion Ratio Lower Upper
98 100
100 63.1 51.5 77.3

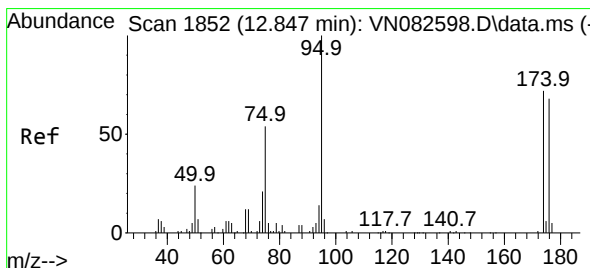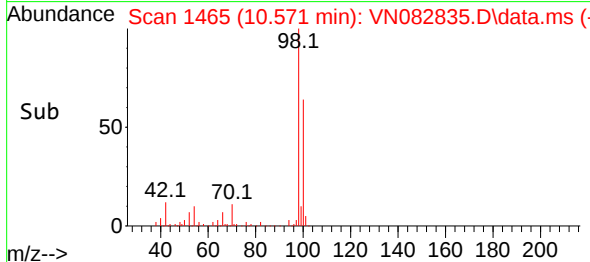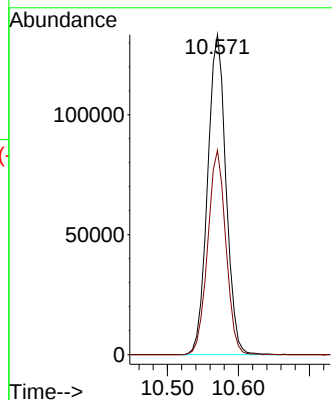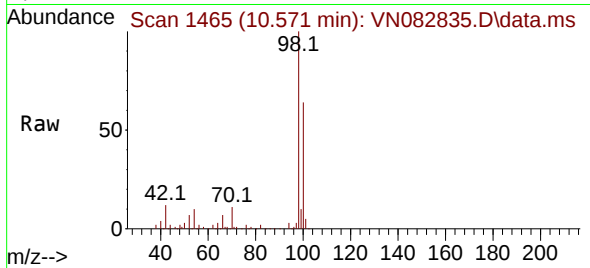

#62
4-Bromofluorobenzene
Concen: 48.375 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Tgt Ion: 95 Resp: 82747
Ion Ratio Lower Upper
95 100
174 75.8 0.0 159.2
176 73.4 0.0 147.6


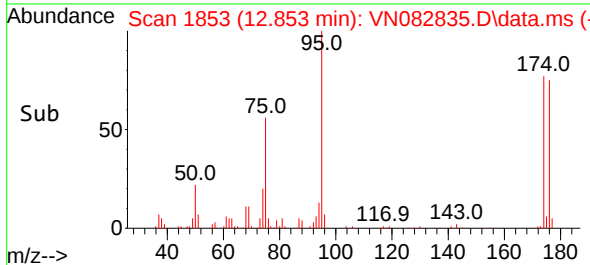
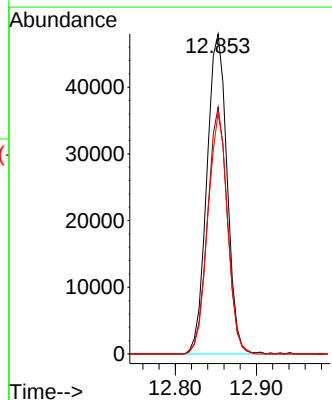
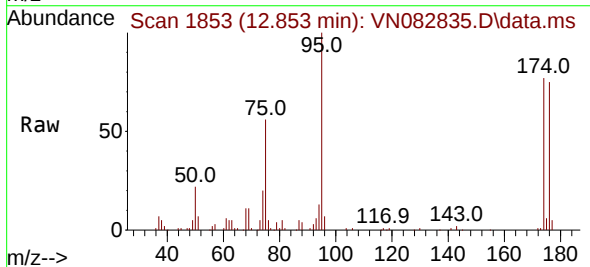


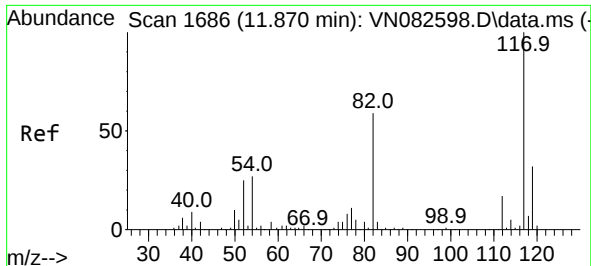

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Instrument :
MSVOA_N
ClientSampleId :
VN0709WBL01

Tgt Ion:117 Resp: 199910
Ion Ratio Lower Upper
117 100
82 57.6 47.5 71.3
119 33.2 25.6 38.4

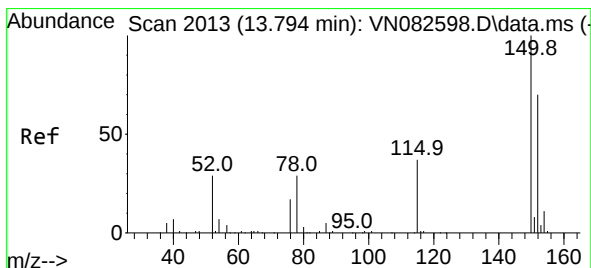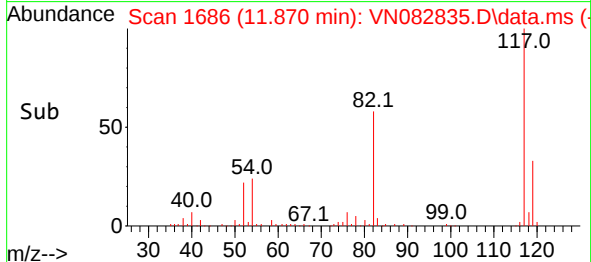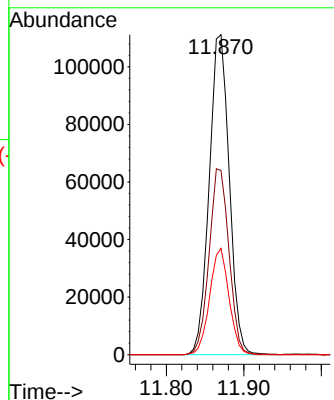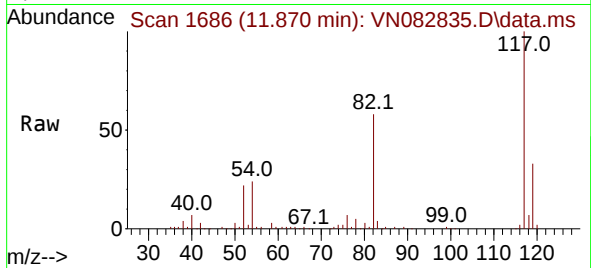

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082835.D
Acq: 09 Jul 2024 12:07

Tgt Ion:152 Resp: 88074
Ion Ratio Lower Upper
152 100
115 61.2 30.6 91.6
150 157.4 0.0 348.6

