
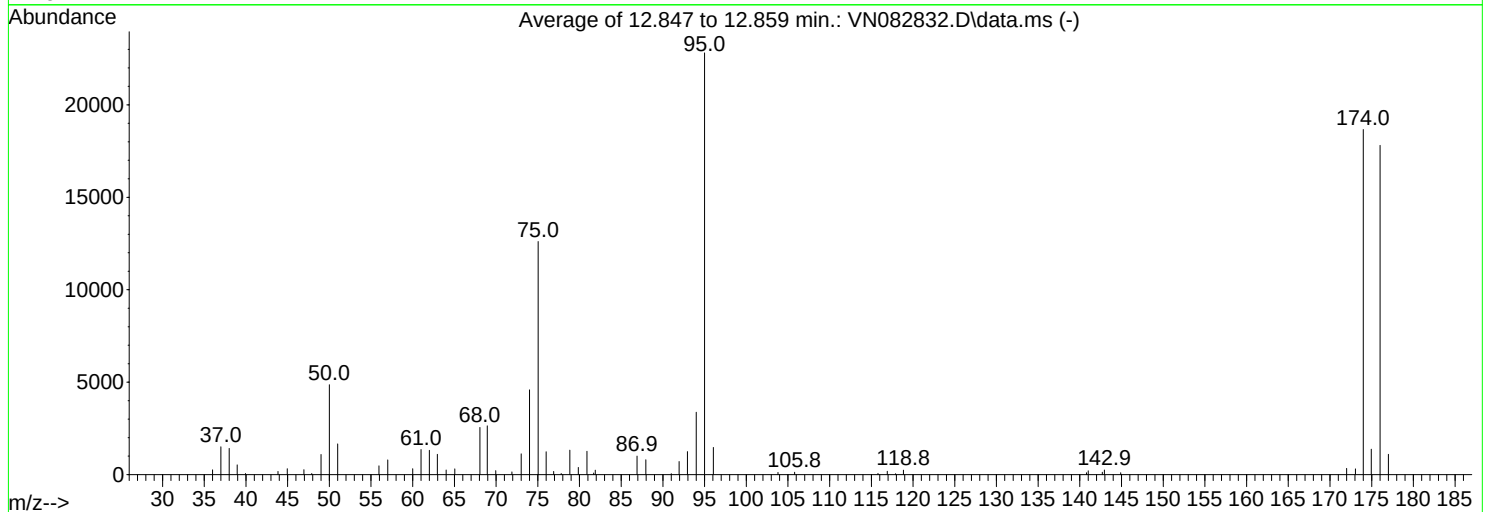


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070924\
Data File : VN082832.D
Acq On : 09 Jul 2024 09:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

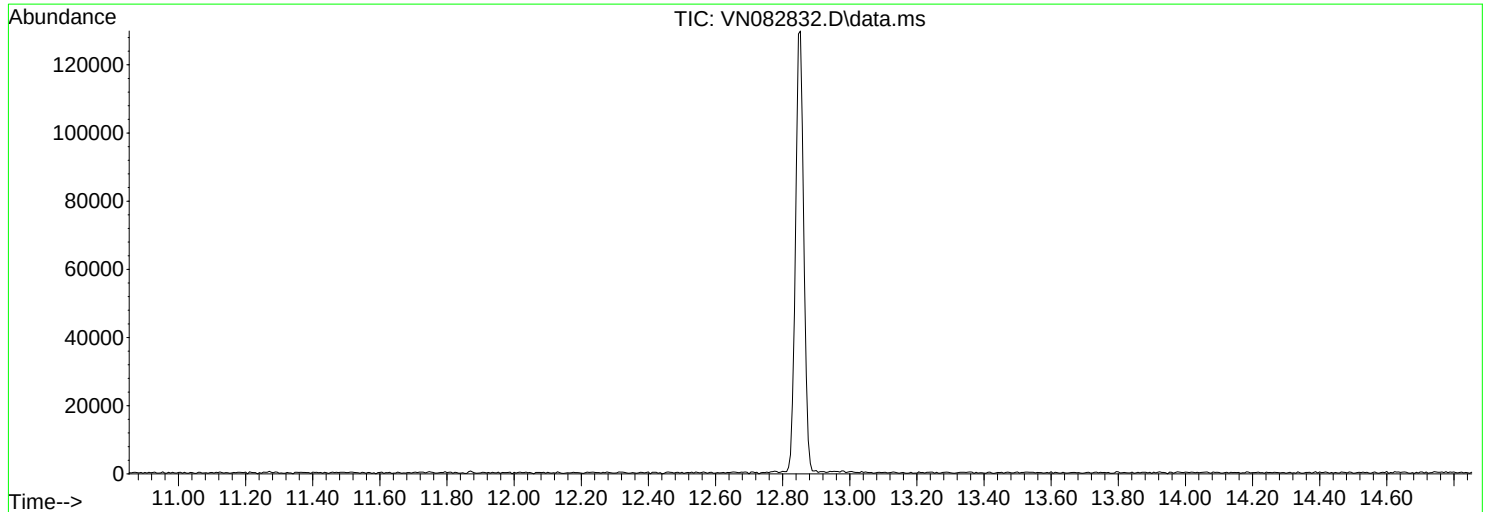

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	4860	PASS
75	95	30	60	55.3	12609	PASS
95	95	100	100	100.0	22811	PASS
96	95	5	9	6.5	1472	PASS
173	174	0.00	2	1.6	308	PASS
174	95	50	100	81.8	18667	PASS
175	174	5	9	7.4	1377	PASS
176	174	95	101	95.4	17810	PASS
177	176	5	9	6.2	1098	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	258	51.00	1658	69.95	216	81.70	81
37.00	1502	55.95	479	71.90	151	81.90	241
38.00	1422	57.00	798	73.00	1127	86.90	100
38.95	530	60.00	318	74.00	4585	87.95	80
39.95	63	61.00	1363	75.05	12609	91.00	53
43.85	172	62.00	1319	76.00	1237	91.95	706
44.95	322	62.95	1101	76.90	170	92.95	1250
46.95	266	64.00	249	77.80	59	94.00	3379
47.90	59	65.05	313	78.85	1327	95.00	22811
49.00	1094	68.05	2553	79.85	392	96.05	1472
50.00	4860	68.95	2640	80.90	1264	103.80	119

Average of 12.847 to 12.859 min.: VN082832.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.80	129	173.05	308				
115.80	70	174.00	18667				
116.90	179	174.95	1377				
117.90	51	176.00	17810				
118.85	244	177.00	1098				
140.80	108						
141.00	205						
142.70	131						
142.95	255						
144.90	108						
172.00	334						

Instrument :

MSVOA_N

ClientSampleId :

BFB