


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071019\
Data File : VN056632.D
Acq On : 10 Jul 2019 8:41
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071019SIM-VINYL.M
Title : SW846 8260
Last Update : Thu Jul 11 04:54:57 2019

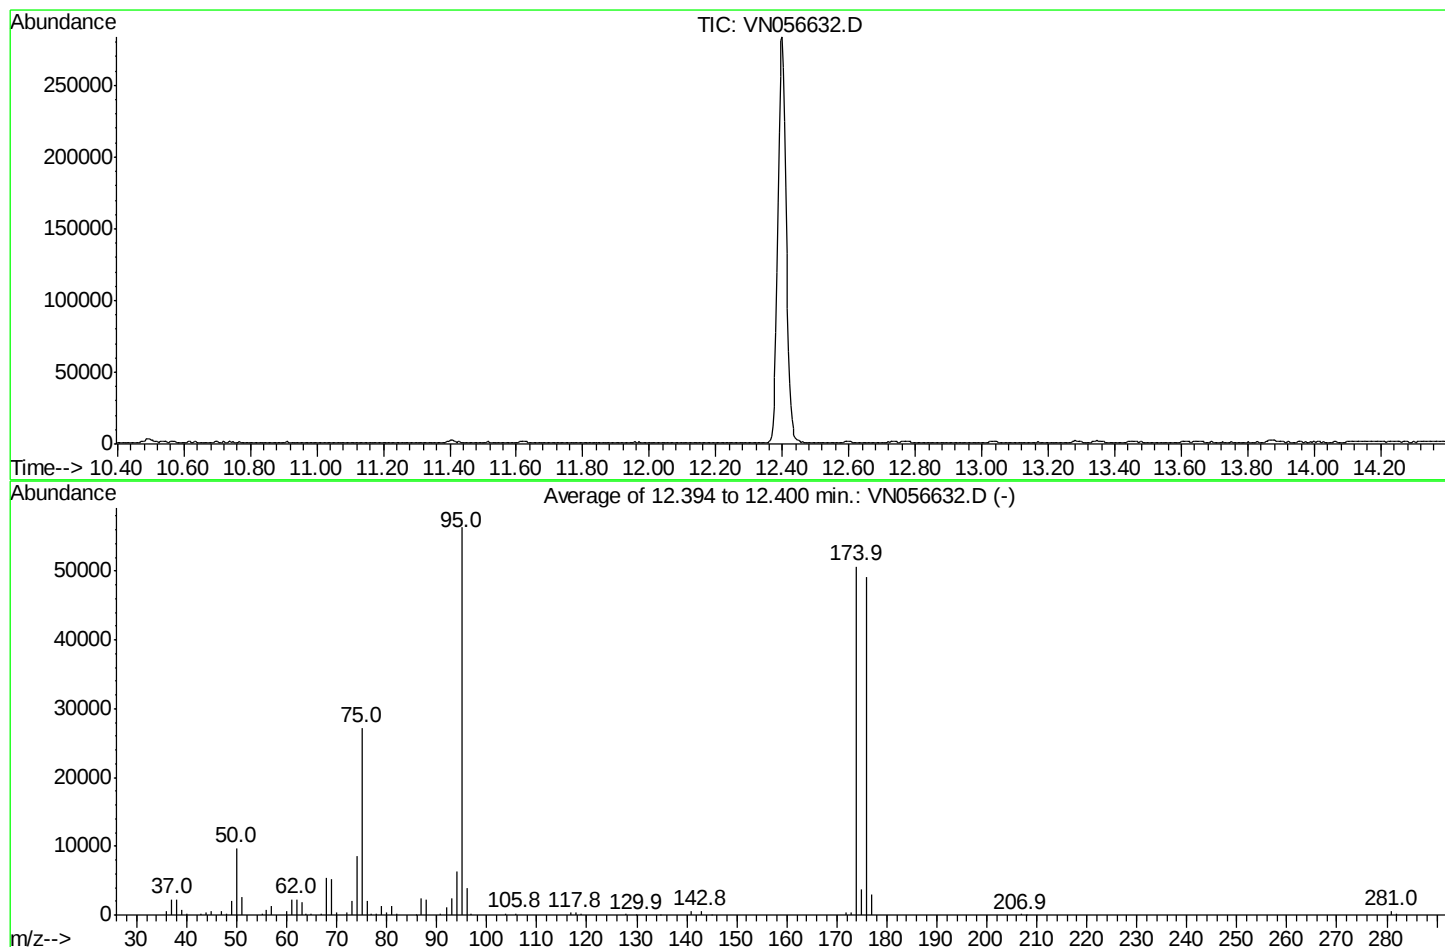

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	9722	PASS
75	95	30	60	48.2	27170	PASS
95	95	100	100	100.0	56354	PASS
96	95	5	9	7.0	3932	PASS
173	174	0.00	2	0.8	407	PASS
174	95	50	100	90.0	50701	PASS
175	174	5	9	7.3	3714	PASS
176	174	95	101	96.8	49096	PASS
177	176	5	9	6.2	3056	PASS