


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071020\
 Data File : VN062483.D
 Acq On : 10 Jul 2020 9:31
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
 Title : SW846 8260
 Last Update : Fri Jul 10 00:55:52 2020

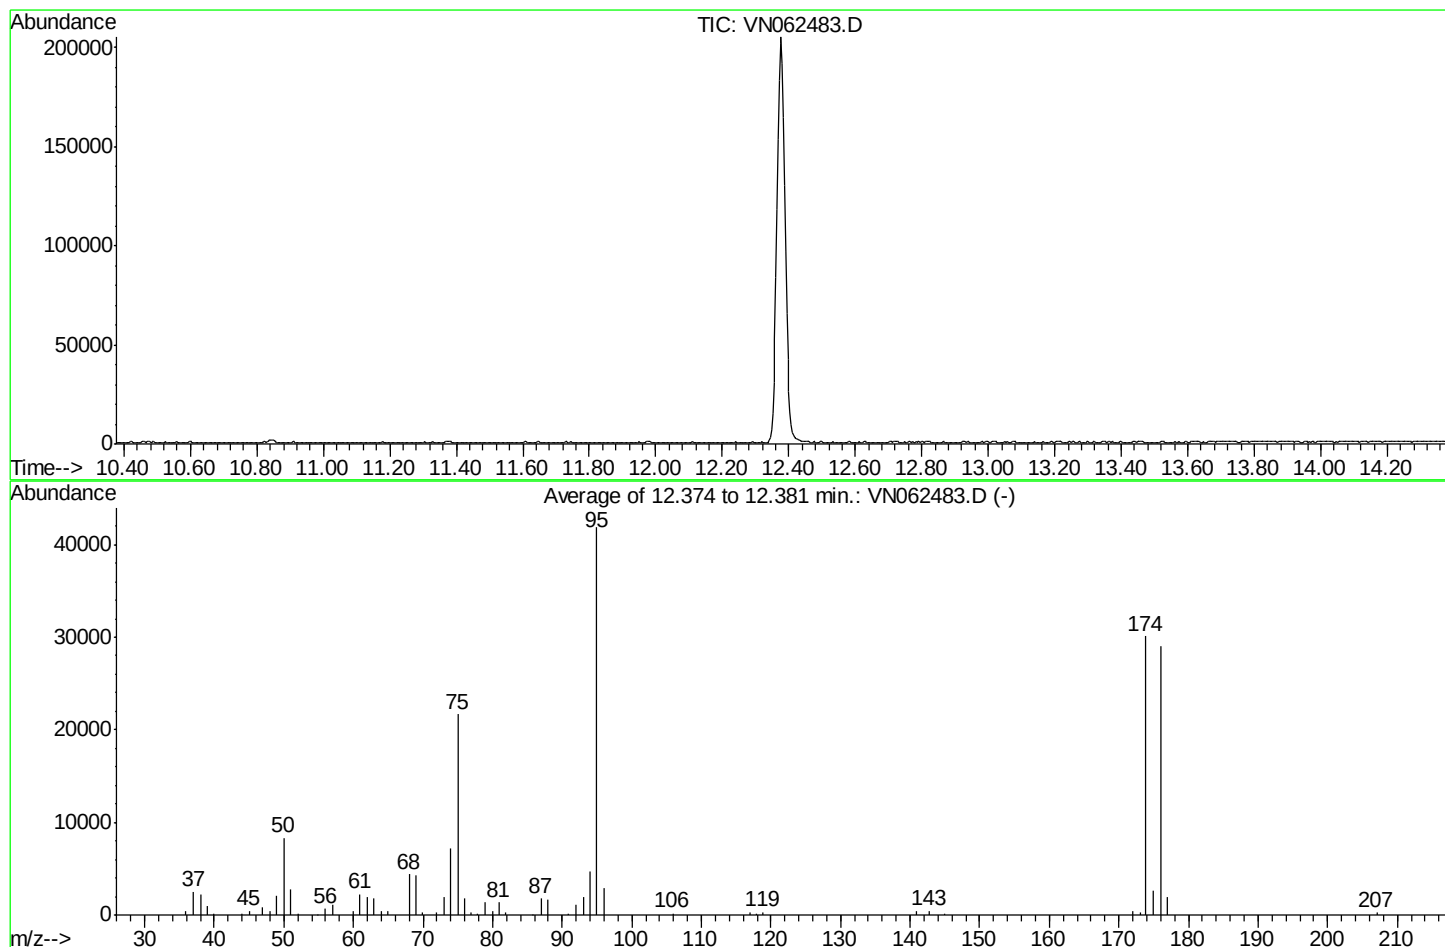

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	8342	PASS
75	95	30	60	51.8	21690	PASS
95	95	100	100	100.0	41869	PASS
96	95	5	9	6.8	2843	PASS
173	174	0.00	2	0.9	263	PASS
174	95	50	100	72.0	30125	PASS
175	174	5	9	8.6	2593	PASS
176	174	95	101	96.6	29098	PASS
177	176	5	9	6.4	1876	PASS