
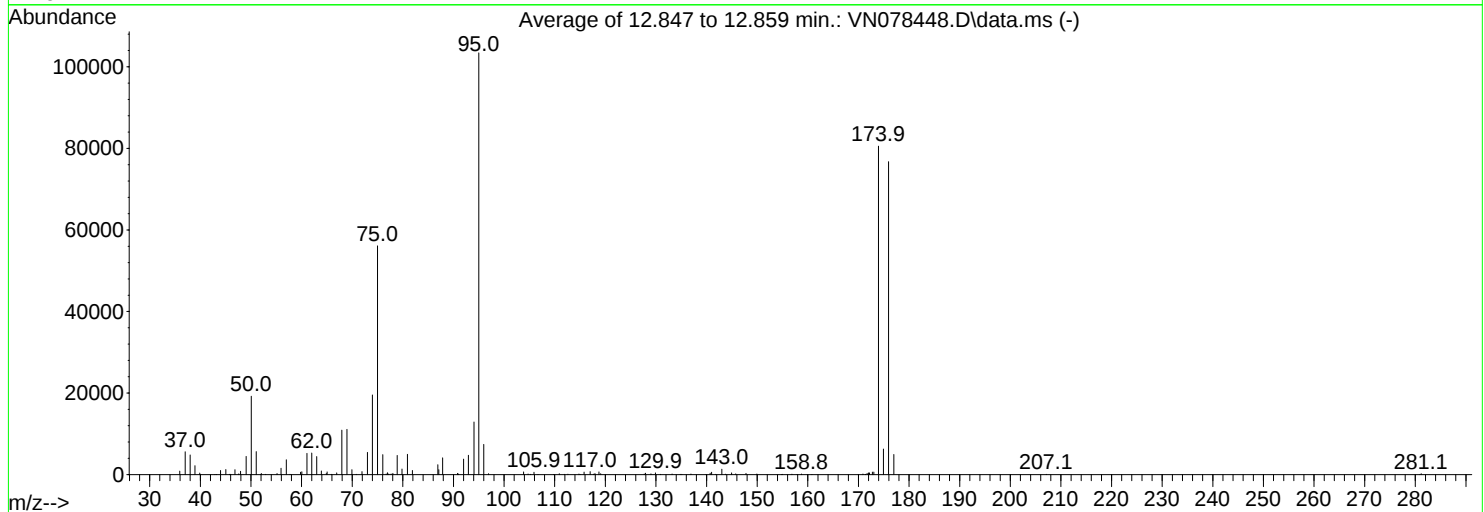


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071023\
Data File : VN078448.D
Acq On : 10 Jul 2023 11:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

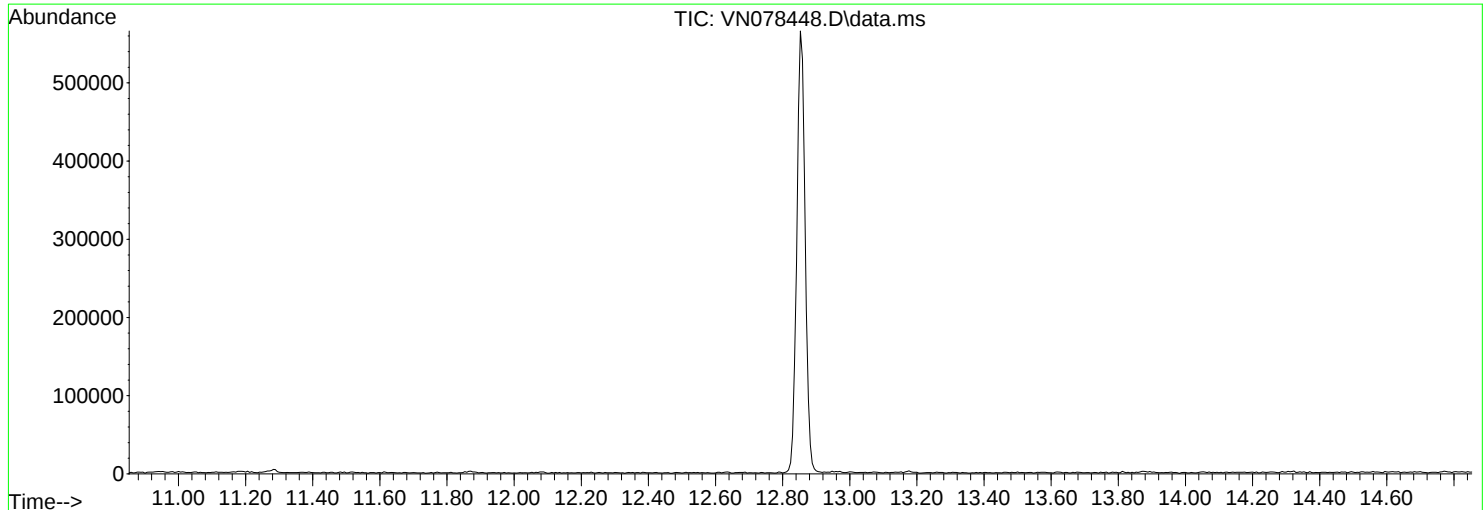

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	19208	PASS
75	95	30	60	54.2	56091	PASS
95	95	100	100	100.0	103427	PASS
96	95	5	9	7.2	7423	PASS
173	174	0.00	2	0.8	641	PASS
174	95	50	100	77.9	80544	PASS
175	174	5	9	7.8	6283	PASS
176	174	95	101	95.3	76741	PASS
177	176	5	9	6.5	4951	PASS

Average of 12.847 to 12.859 min.: VN078448.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	874	46.85	1210	57.00	3666	66.95	441
37.00	5615	47.60	206	57.70	64	67.95	1089
38.00	4833	47.95	818	59.80	583	68.95	1112
38.95	2217	49.05	4476	60.05	719	69.95	122
39.90	413	50.05	19208	61.05	5238	70.80	82
42.90	59	51.05	5657	62.00	5293	71.95	741
43.20	62	51.90	90	63.00	4452	73.00	5445
44.00	1027	52.05	290	63.90	907	74.00	19544
45.05	1263	52.90	73	64.90	281	75.00	56091
45.80	85	55.15	274	65.05	674	76.05	4914
46.00	79	55.95	1573	65.90	78	76.70	151

Average of 12.847 to 12.859 min.: VN078448.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	459	90.80	304	105.90	587	117.95	293
77.20	142	91.00	168	106.70	57	118.75	682
77.70	144	92.00	3802	109.80	58	119.10	220
78.05	325	92.95	4751	110.90	226	127.70	153
78.90	4702	94.05	12926	111.90	65	127.95	367
79.85	1371	95.00	103427	112.60	108	129.00	218
80.90	4972	96.00	7423	114.80	152	129.90	435
81.90	1032	96.95	239	115.00	52	130.90	69
86.90	2440	103.85	679	115.80	642	133.20	152
87.10	1236	104.75	170	117.00	757	134.80	74
87.85	4112	105.20	67	117.70	112	135.10	68

Average of 12.847 to 12.859 min.: VN078448.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
136.90	173	154.80	63	172.75	641		
139.90	56	155.00	89	173.05	632		
140.70	366	156.85	131	173.95	80544		
141.00	588	157.90	62	174.95	6283		
141.80	64	158.75	177	175.95	76741		
143.00	1330	160.80	54	177.00	4951		
143.70	100	170.90	140	207.10	83		
144.95	420	171.40	84	280.90	57		
145.75	218	171.70	310	281.15	251		
147.80	308	172.00	427				
149.95	168	172.20	421				