

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071024\
 Data File : VN082849.D
 Acq On : 10 Jul 2024 12:37
 Operator : JC\MD
 Sample : VN0710MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0710MBL01

Quant Time: Jul 11 03:45:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	90565	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	171124	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	169756	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	71381	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	78655	61.956	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	123.920%
35) Dibromofluoromethane	8.165	113	63848	58.146	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	116.300%
50) Toluene-d8	10.571	98	220966	54.483	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.960%
62) 4-Bromofluorobenzene	12.853	95	72020	49.436	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	98.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071024\
Data File : VN082849.D
Acq On : 10 Jul 2024 12:37
Operator : JC\MD
Sample : VN0710MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0710MBL01


Quant Time: Jul 11 03:45:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration

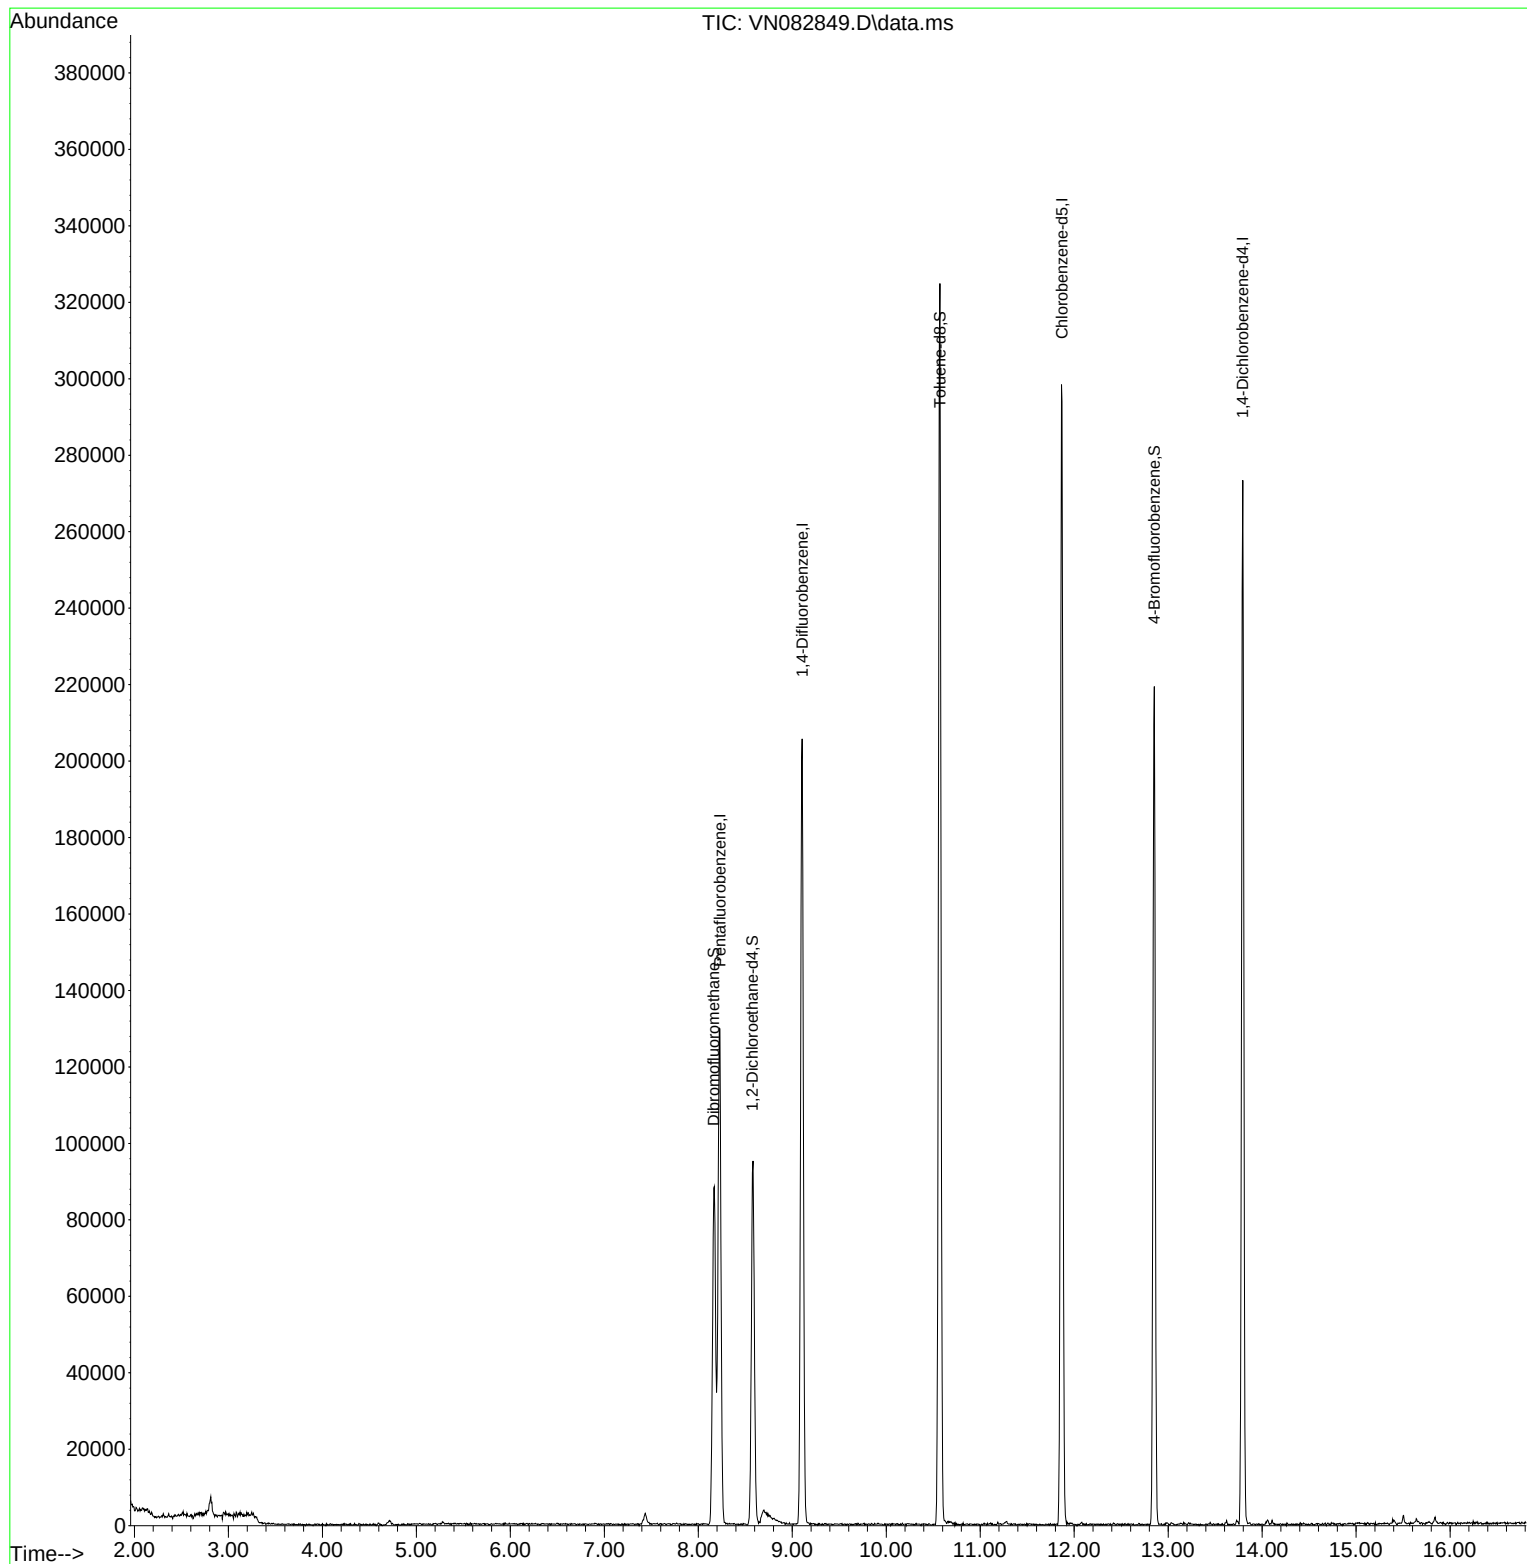



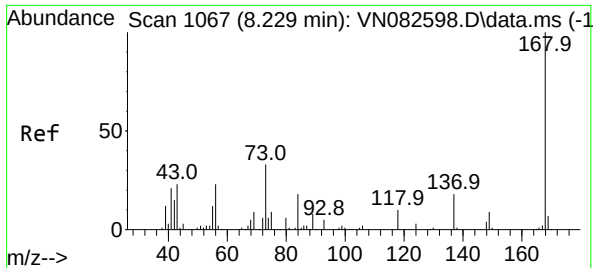


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Instrument :
MSVOA_N
ClientSampleId :
VN0710MBL01



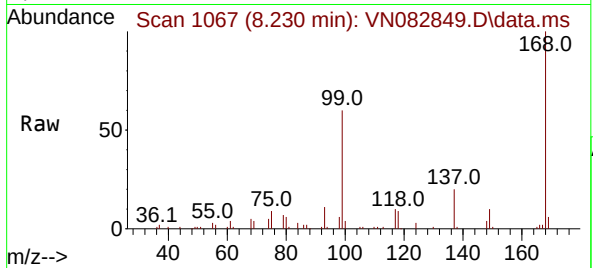



Tgt Ion:168 Resp: 90565
Ion Ratio Lower Upper
168 100
99 59.9 48.2 72.4

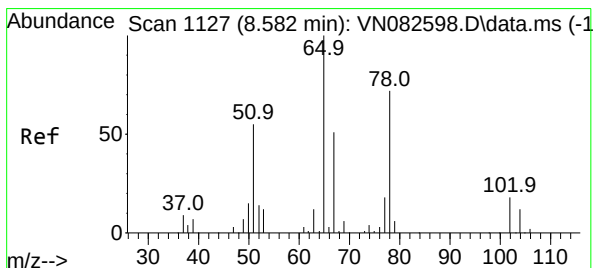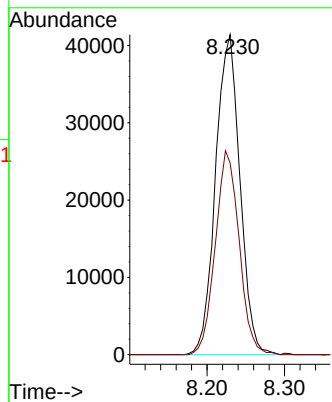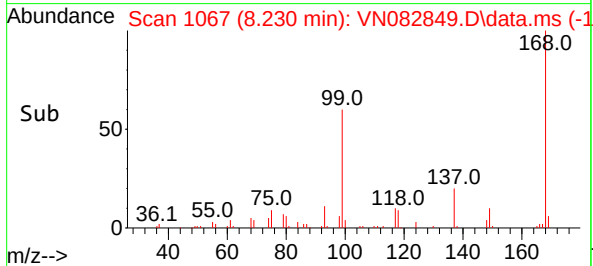

#33
1,2-Dichloroethane-d4
Concen: 61.956 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Tgt Ion: 65 Resp: 78655
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.4


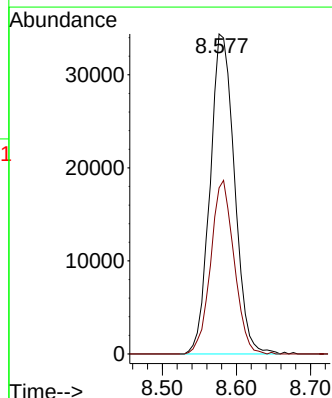
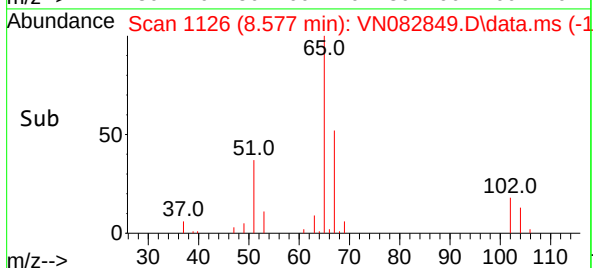
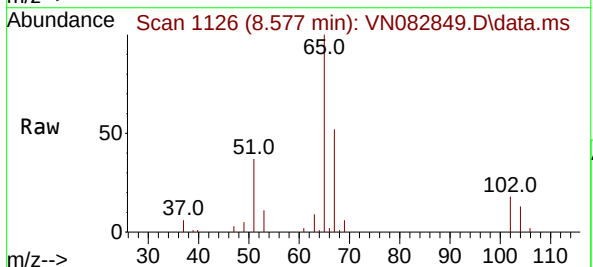


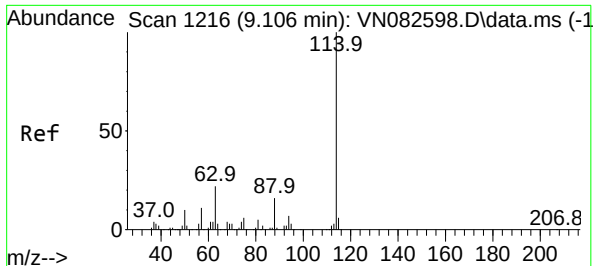

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37




Instrument :
MSVOA_N
ClientSampleId :
VN0710MBL01


Tgt Ion	Ratio	Lower	Upper
114	100		
63	21.6	0.0	44.6
88	15.5	0.0	31.4

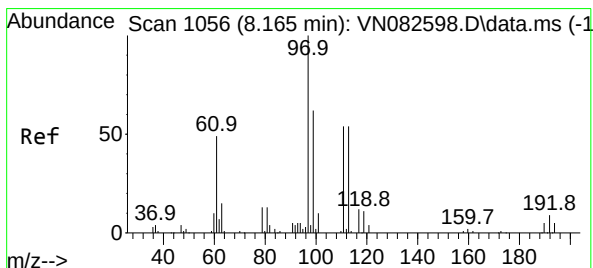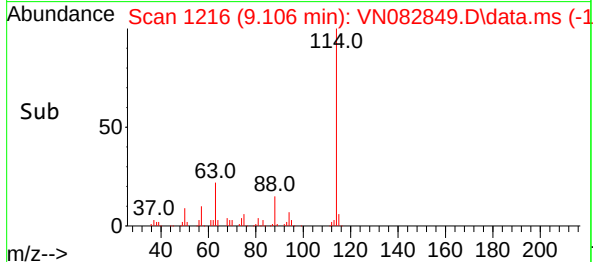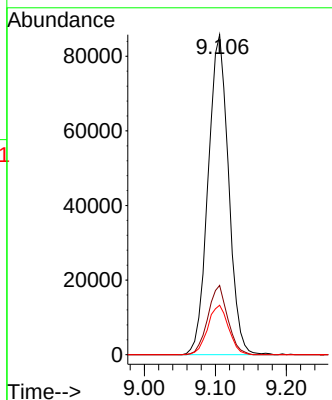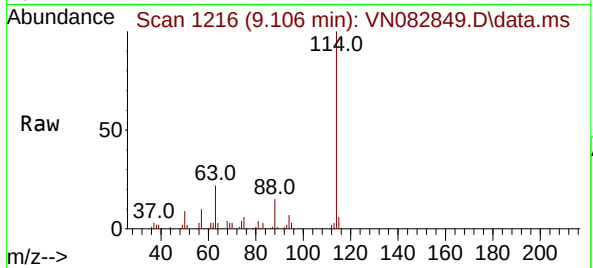

#35
Dibromofluoromethane
Concen: 58.146 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Tgt Ion	Ratio	Lower	Upper
113	100		
111	101.9	82.4	123.6
192	18.0	14.9	22.3


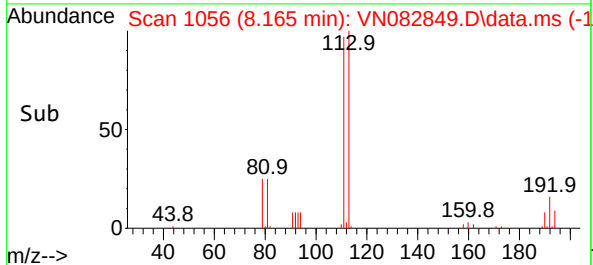
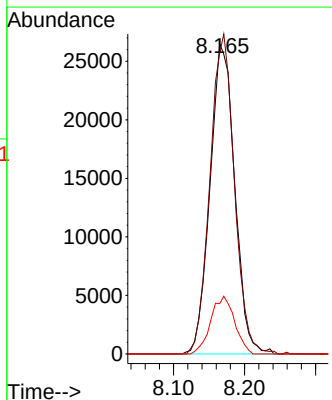
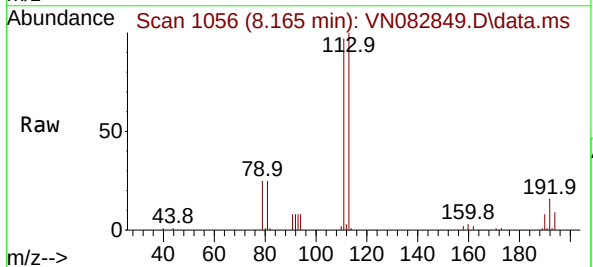


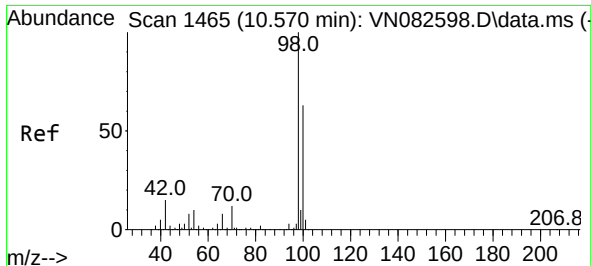

#50
Toluene-d8
Concen: 54.483 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37




Instrument :
MSVOA_N
ClientSampleId :
VN0710MBL01


Tgt Ion: 98 Resp: 220966
Ion Ratio Lower Upper
98 100
100 64.0 51.5 77.3

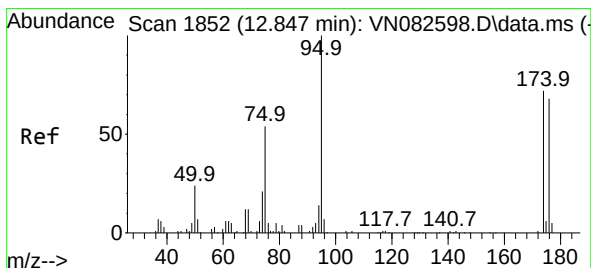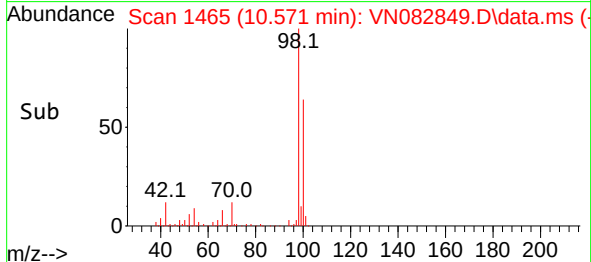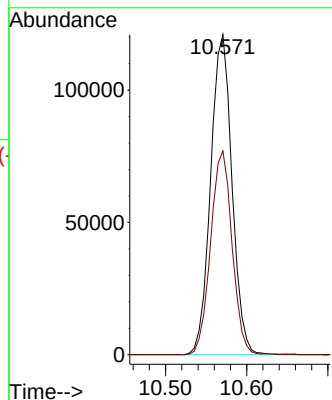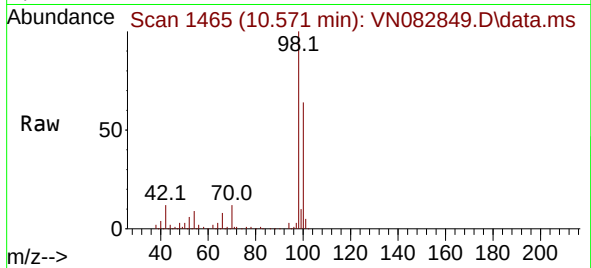

#62
4-Bromofluorobenzene
Concen: 49.436 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Tgt Ion: 95 Resp: 72020
Ion Ratio Lower Upper
95 100
174 78.9 0.0 159.2
176 75.6 0.0 147.6


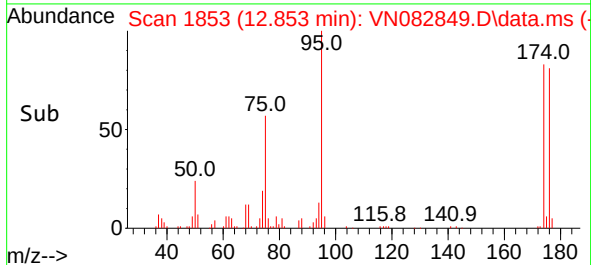
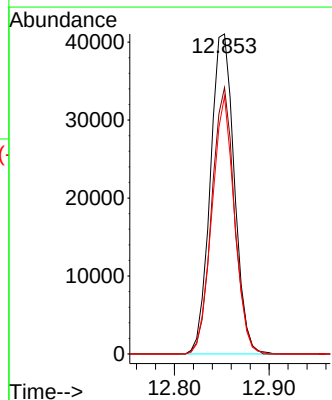
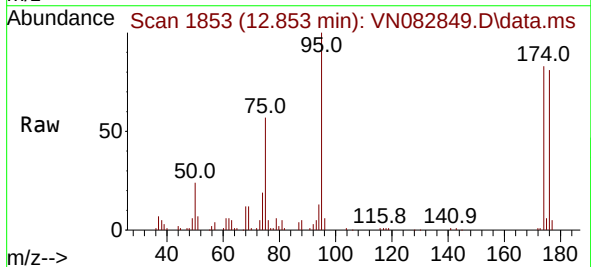


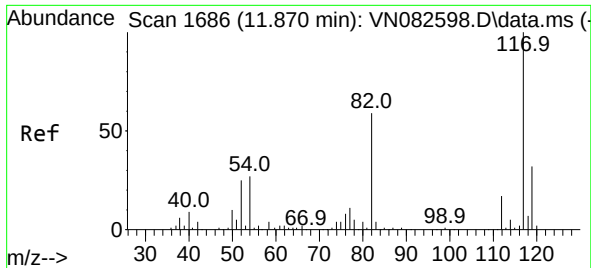

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.001 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Instrument :
MSVOA_N
ClientSampleId :
VN0710MBL01

Tgt Ion:117 Resp: 169756
Ion Ratio Lower Upper
117 100
82 54.4 47.5 71.3
119 32.2 25.6 38.4

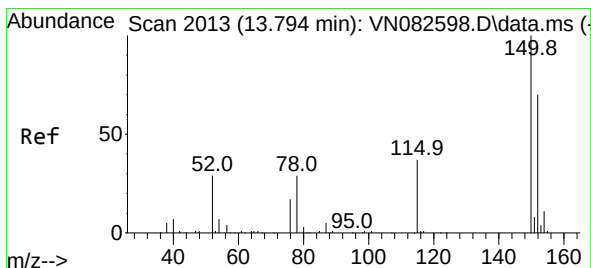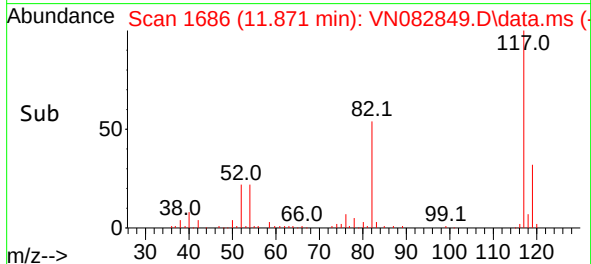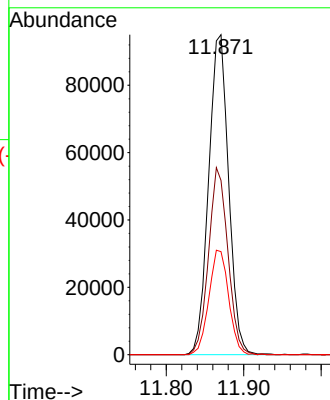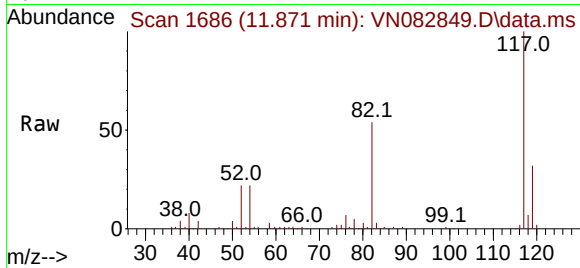

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082849.D
Acq: 10 Jul 2024 12:37

Tgt Ion:152 Resp: 71381
Ion Ratio Lower Upper
152 100
115 61.0 30.6 91.6
150 156.9 0.0 348.6

