



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071024\
Data File : VN082847.D
Acq On : 10 Jul 2024 10:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

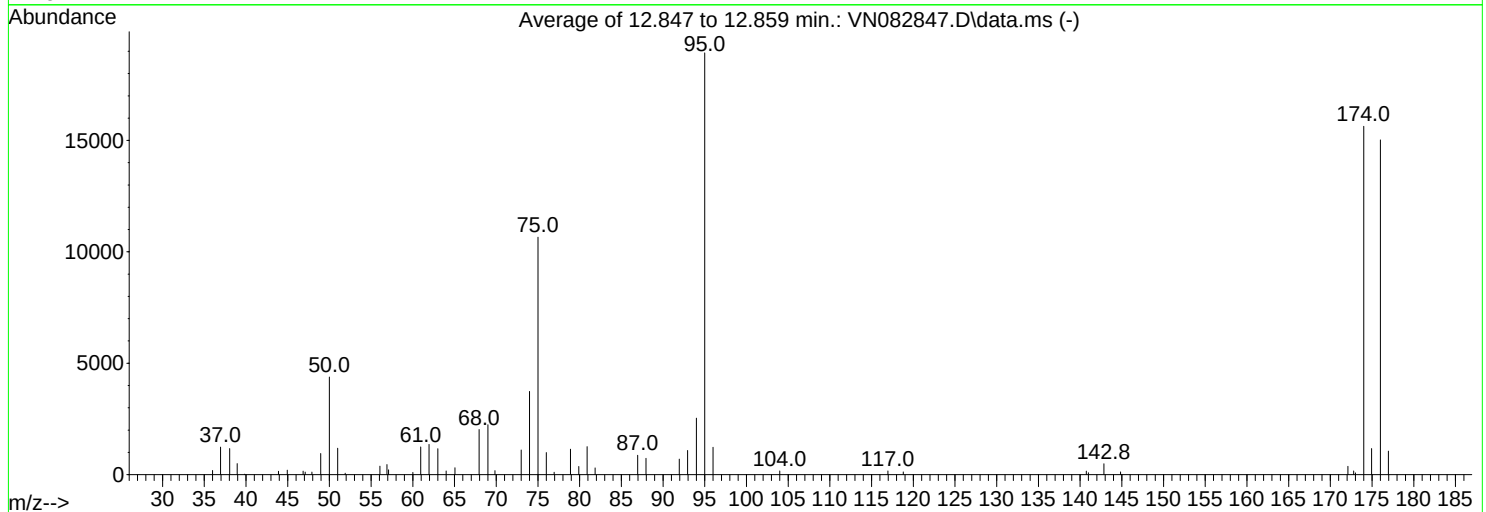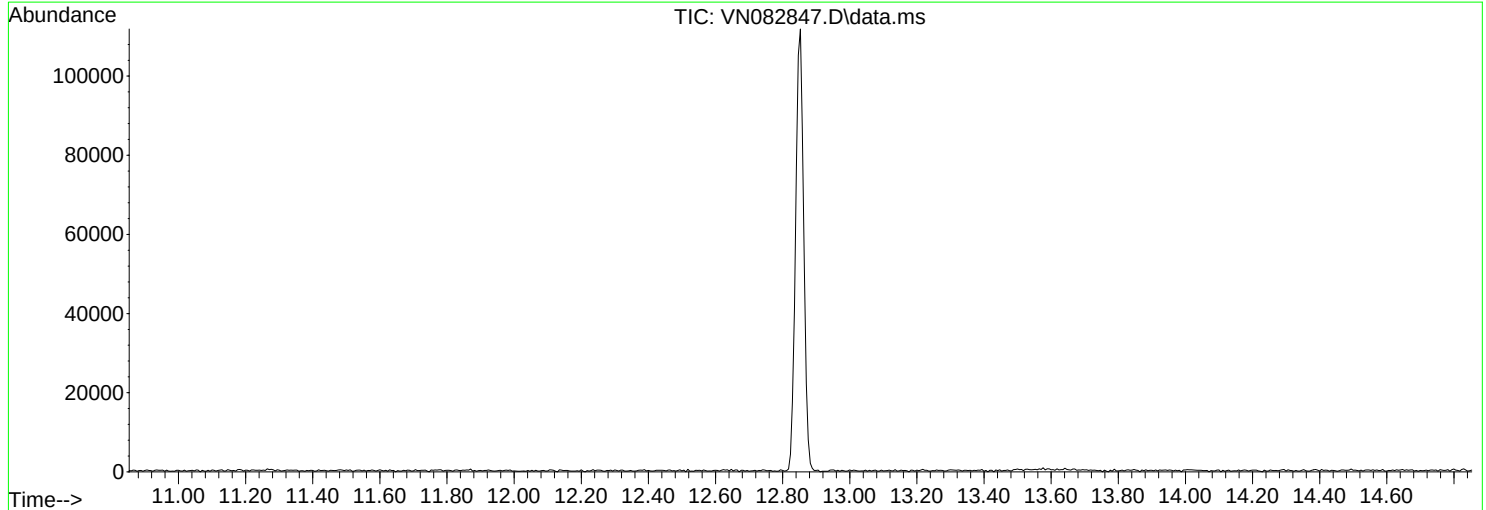

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	4381	PASS
75	95	30	60	56.3	10657	PASS
95	95	100	100	100.0	18930	PASS
96	95	5	9	6.5	1225	PASS
173	174	0.00	2	1.1	166	PASS
174	95	50	100	82.6	15634	PASS
175	174	5	9	7.5	1173	PASS
176	174	95	101	96.1	15026	PASS
177	176	5	9	7.0	1057	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	190	50.00	4381	65.05	311	80.90	1254
36.95	1235	51.00	1186	67.95	2025	81.85	301
38.05	1170	51.90	63	69.00	2241	86.95	86
38.95	493	56.05	382	69.85	181	87.95	73
39.85	21	56.90	454	73.00	1106	91.95	699
43.90	153	57.10	215	74.00	3734	92.95	1082
44.95	202	60.00	101	75.00	10657	94.00	2536
46.85	159	60.95	1241	76.00	988	95.00	18930
47.10	113	61.95	1358	76.95	111	96.00	1225
47.90	118	63.00	1160	78.90	1143	104.00	168
48.95	949	64.00	164	79.90	370	116.95	167

Average of 12.847 to 12.859 min.: VN082847.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.80	122	176.95	1057				
140.75	161						
141.00	84						
142.85	485						
144.85	121						
172.10	376						
172.80	166						
173.00	81						
174.00	15634						
174.95	1173						
176.00	15026						

Instrument :

MSVOA_N

ClientSampleId :

BFB