
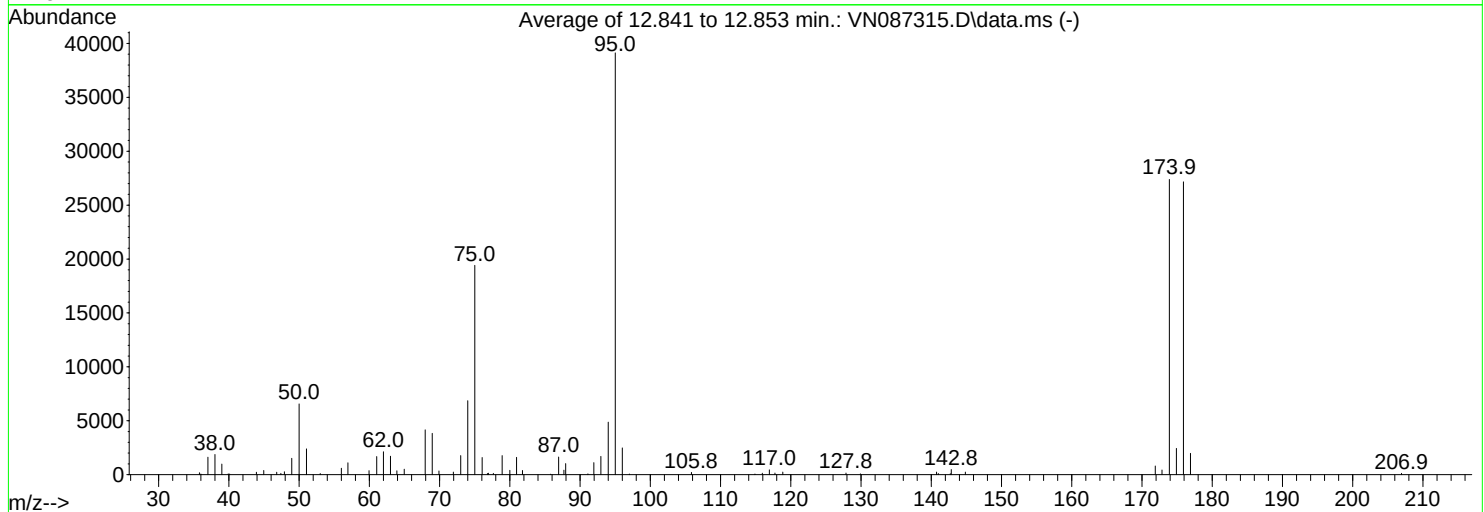


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071025\
Data File : VN087315.D
Acq On : 10 Jul 2025 08:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N062525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jun 25 10:49:56 2025

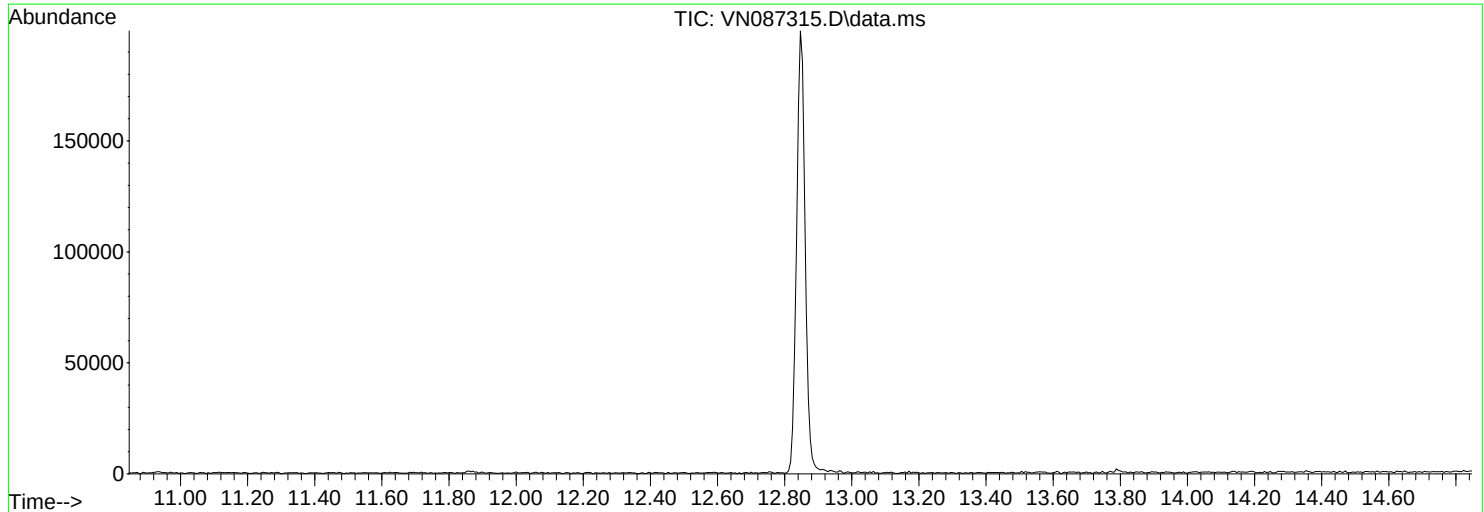

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	6567	PASS
75	95	30	60	49.6	19411	PASS
95	95	100	100	100.0	39128	PASS
96	95	5	9	6.3	2482	PASS
173	174	0.00	2	1.6	439	PASS
174	95	50	100	70.0	27389	PASS
175	174	5	9	8.9	2431	PASS
176	174	95	101	99.2	27160	PASS
177	176	5	9	7.3	1974	PASS