


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071118\
Data File : VN049753.D
Acq On : 11 Jul 2018 9:37
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N063017W.M
Title : SW846 8260
Last Update : Fri Jun 30 12:03:08 2017

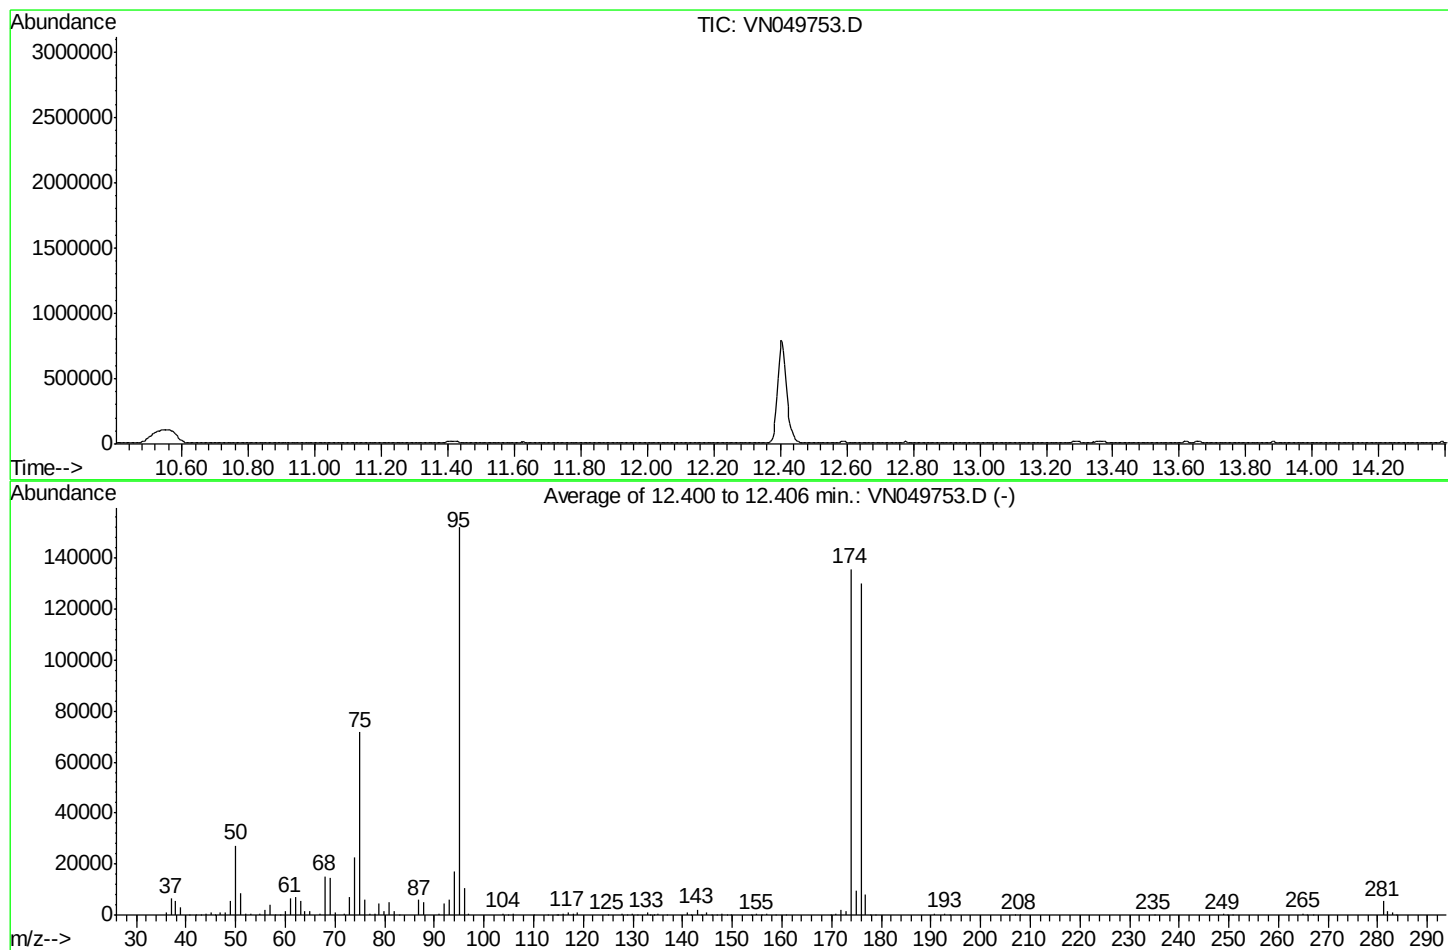

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3347

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	27205	PASS
75	95	30	60	47.1	71600	PASS
95	95	100	100	100.0	152106	PASS
96	95	5	9	6.9	10547	PASS
173	174	0.00	2	1.1	1460	PASS
174	95	50	100	89.2	135741	PASS
175	174	5	9	7.2	9727	PASS
176	174	95	101	95.7	129845	PASS
177	176	5	9	6.2	8102	PASS