


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071119\
Data File : VN056658.D
Acq On : 11 Jul 2019 8:22
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071019SIM-VINYL.M
Title : SW846 8260
Last Update : Thu Jul 11 04:54:57 2019

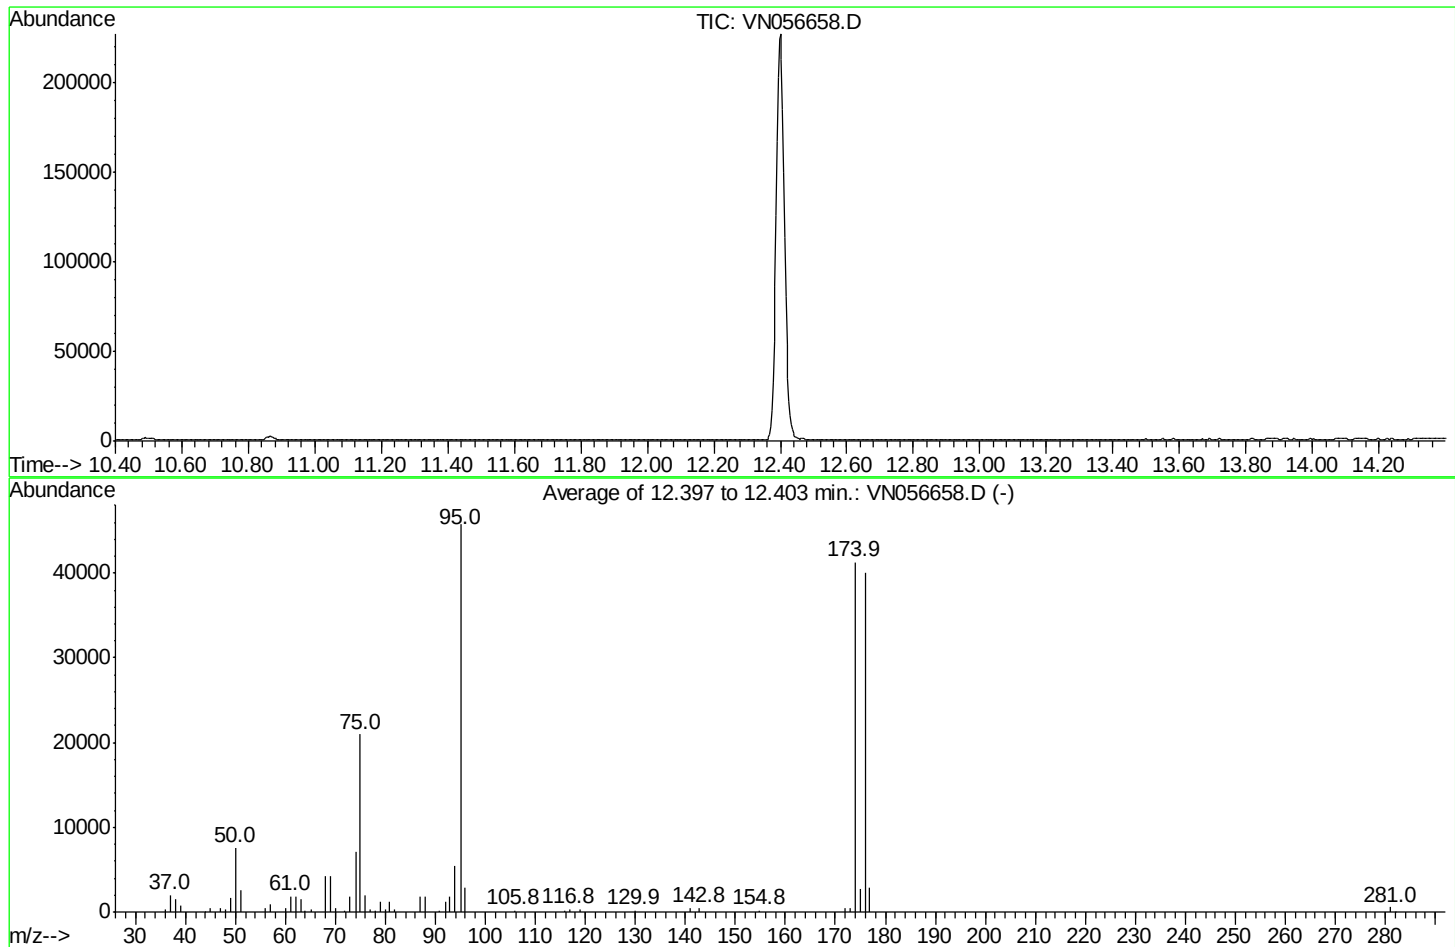

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	7604	PASS
75	95	30	60	45.8	20938	PASS
95	95	100	100	100.0	45757	PASS
96	95	5	9	6.4	2907	PASS
173	174	0.00	2	1.1	437	PASS
174	95	50	100	90.3	41322	PASS
175	174	5	9	6.5	2672	PASS
176	174	95	101	97.1	40106	PASS
177	176	5	9	7.2	2903	PASS