


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071119\
 Data File : VN056662.D
 Acq On : 11 Jul 2019 12:03
 Operator : JC/SP
 Sample : K3636-07
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SP19-LF3MW3

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071019SIM-VINYL.M
 Title : SW846 8260
 Last Update : Thu Jul 11 04:54:57 2019

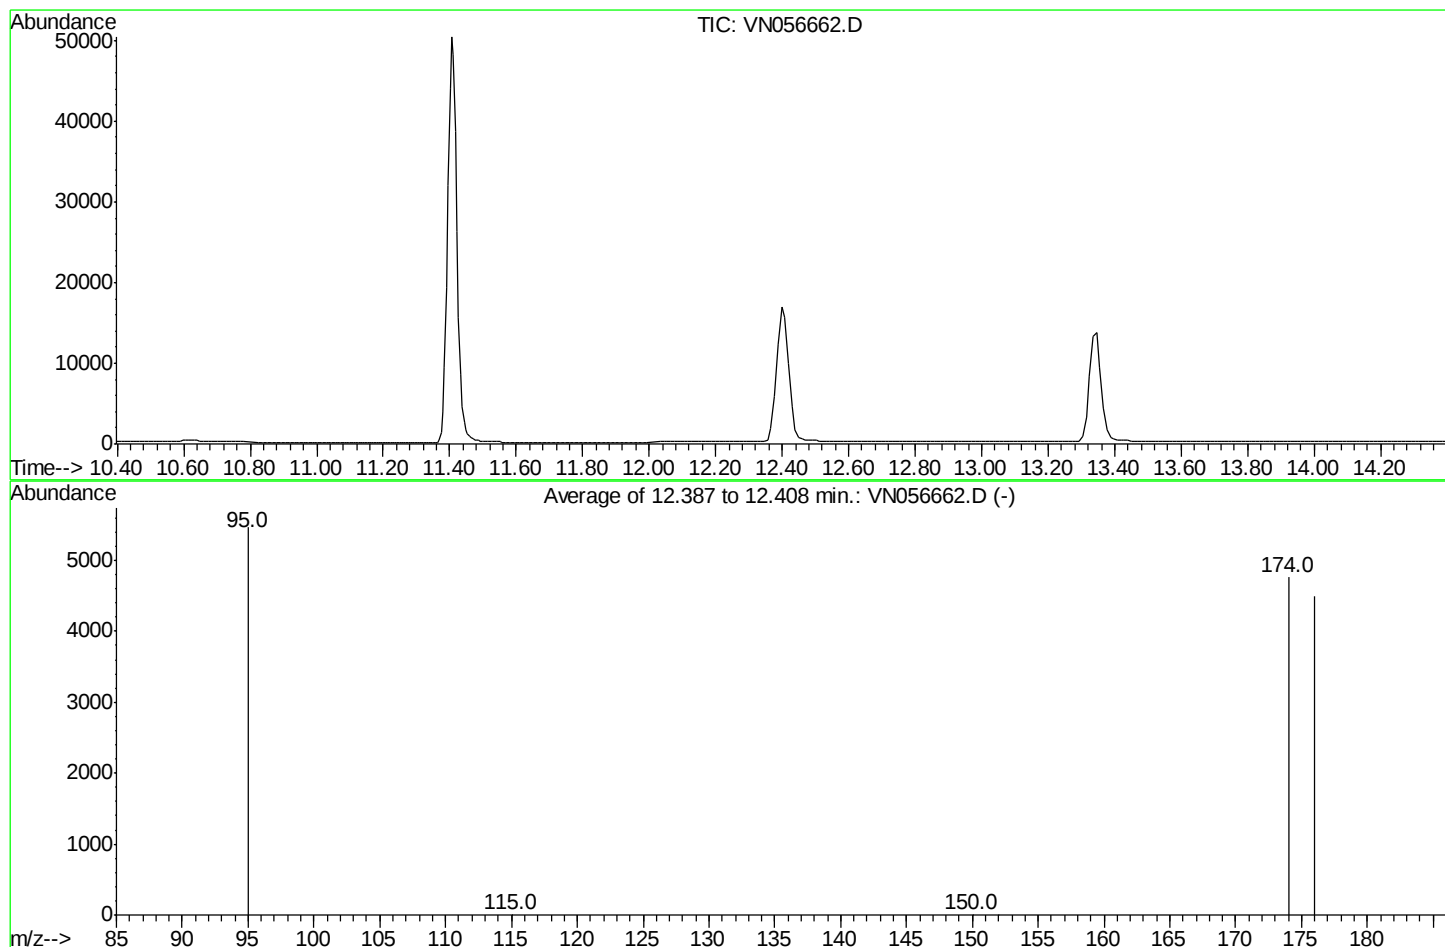

AutoFind: Scans 1772, 1773, 1774; Background Corrected with Scan 1765

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	0.0	0	FAIL *
75	95	30	60	0.0	0	FAIL *
95	95	100	100	100.0	5466	PASS
96	95	5	9	0.0	0	FAIL *
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.1	4760	PASS
175	174	5	9	0.0	0	FAIL *
176	174	95	101	94.2	4486	FAIL *
177	176	5	9	0.0	0	FAIL *