

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071122\
 Data File : VN073410.D
 Acq On : 11 Jul 2022 11:08
 Operator : JC\MD
 Sample : VN0711WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0711WBL01

Quant Time: Jul 12 07:23:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	313043	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	520355	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.680	117	472075	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.610	152	222226	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	216735	47.960	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.920%
35) Dibromofluoromethane	7.951	113	178589	51.586	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.180%
50) Toluene-d8	10.380	98	586030	47.661	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.320%
62) 4-Bromofluorobenzene	12.669	95	244642	51.773	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071122\
Data File : VN073410.D
Acq On : 11 Jul 2022 11:08
Operator : JC\MD
Sample : VN0711WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0711WBL01

Quant Time: Jul 12 07:23:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




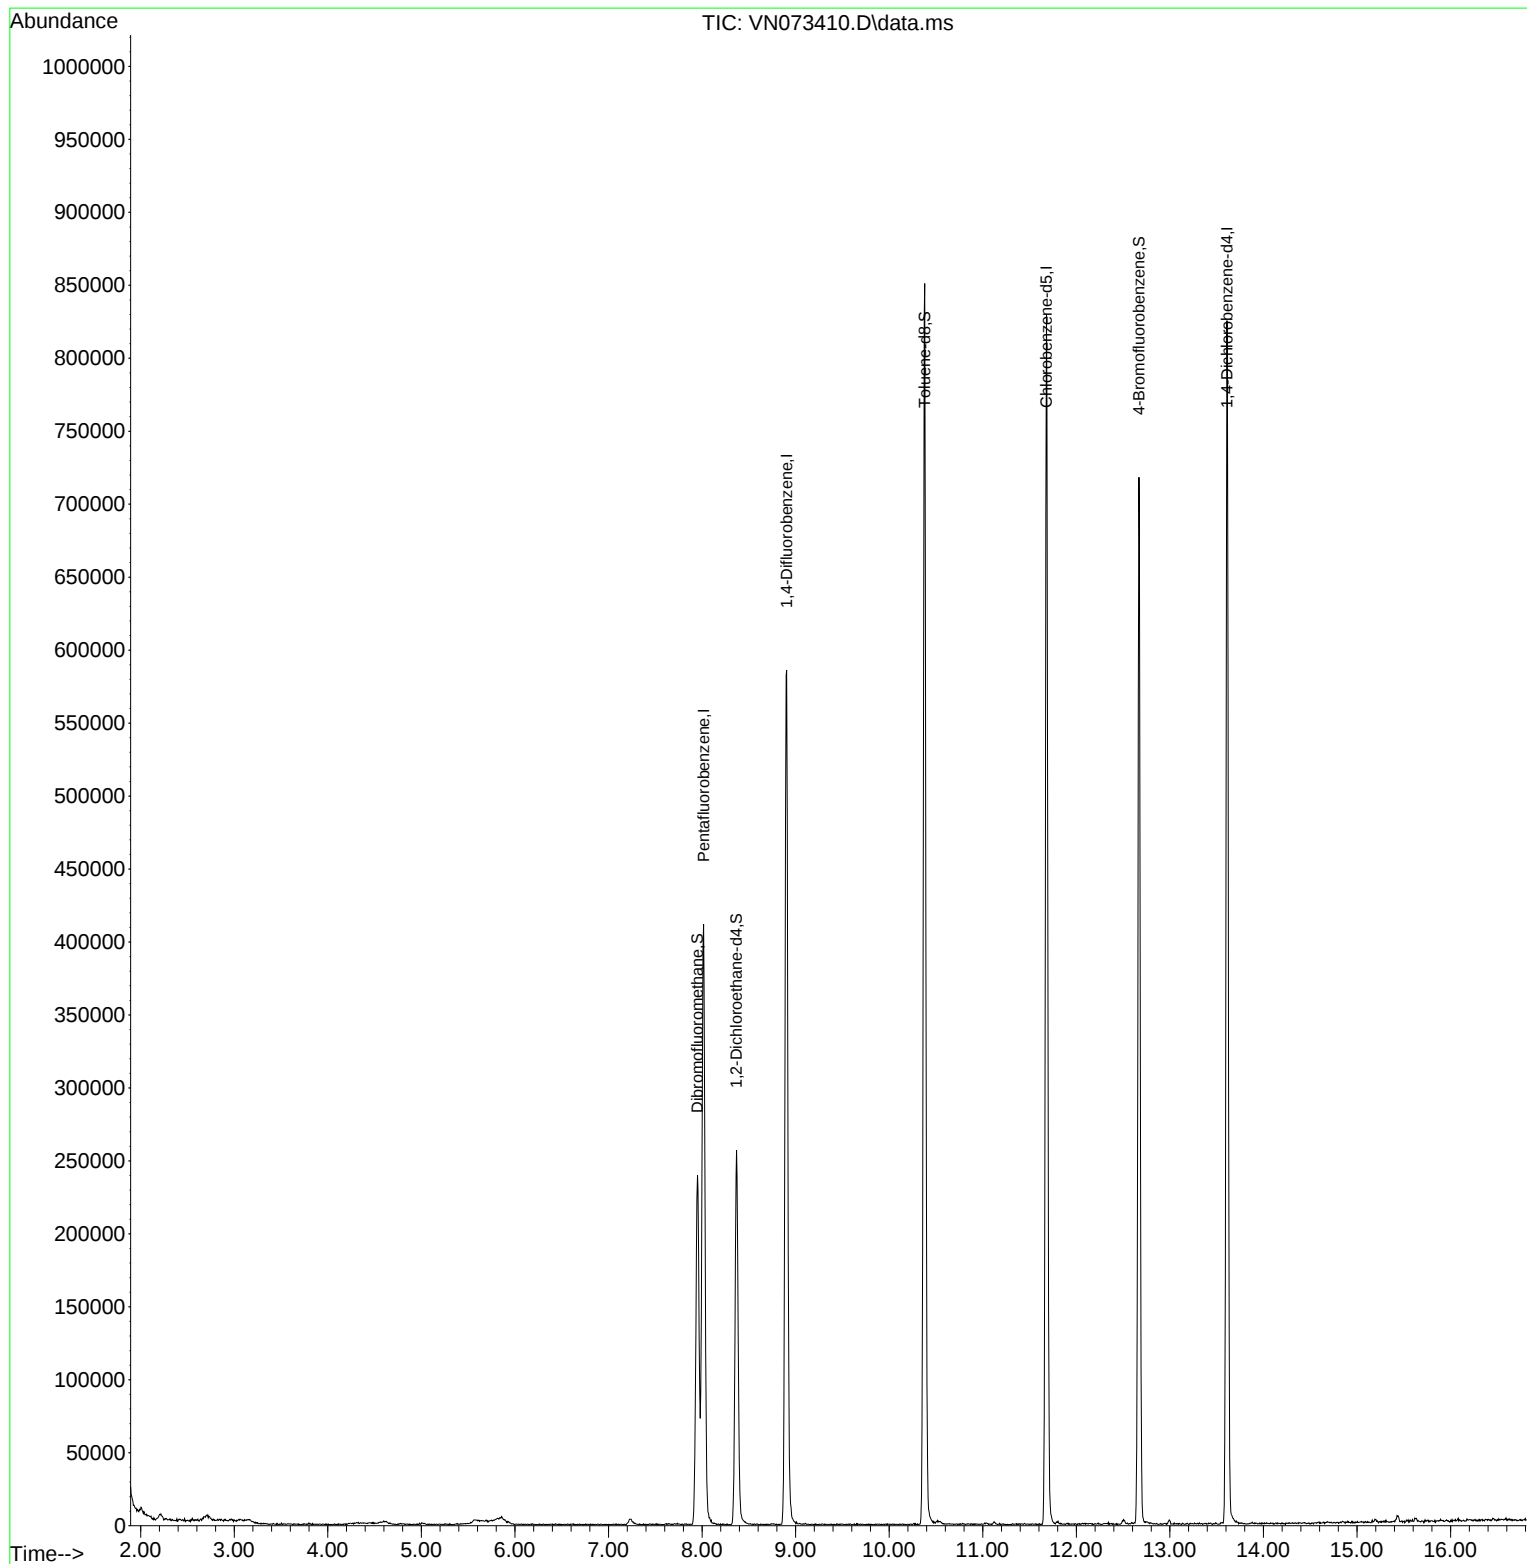


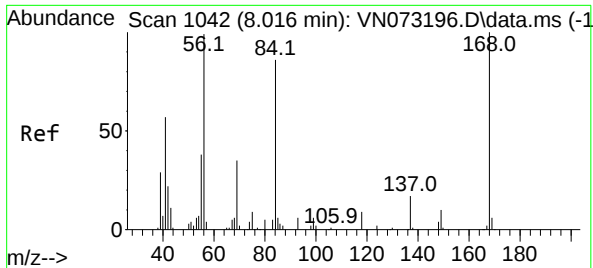

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08




Instrument :
MSVOA_N
ClientSampleId :
VN0711WBL01


Tgt Ion:168 Resp: 313043
Ion Ratio Lower Upper
168 100
99 59.1 42.3 63.5

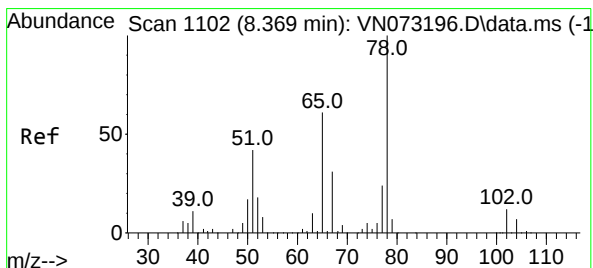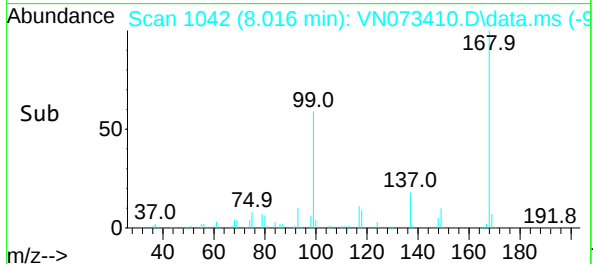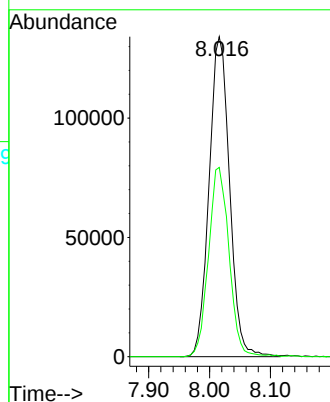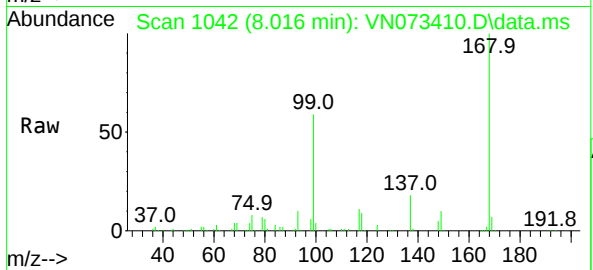

#33
1,2-Dichloroethane-d4
Concen: 47.960 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08

Tgt Ion: 65 Resp: 216735
Ion Ratio Lower Upper
65 100
67 50.9 0.0 104.8

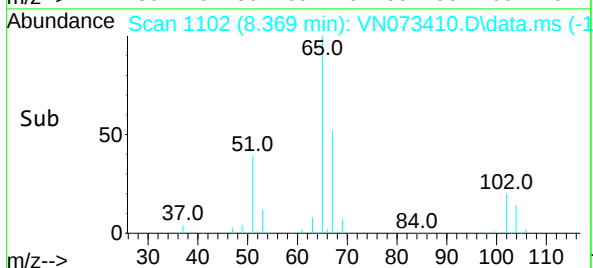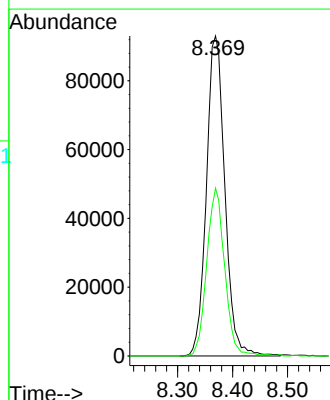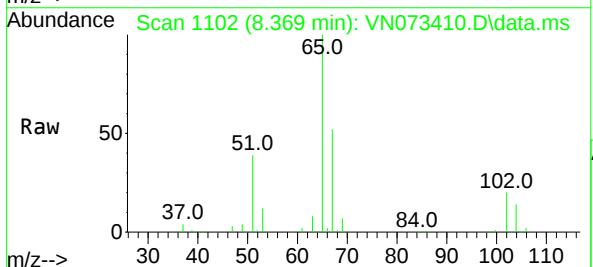

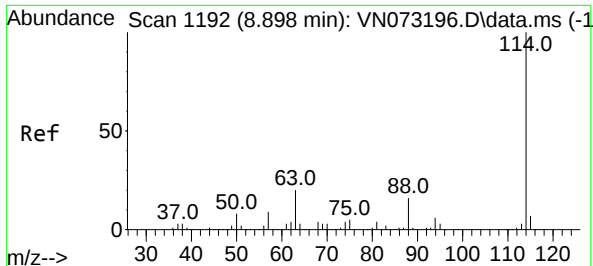

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN073410.D

Acq: 11 Jul 2022 11:08

Instrument :

MSVOA_N

ClientSampleId :

VN0711WBL01





Tgt Ion:114 Resp: 520355

Ion Ratio Lower Upper

114 100

63 21.3 0.0 40.0

88 16.2 0.0 32.6

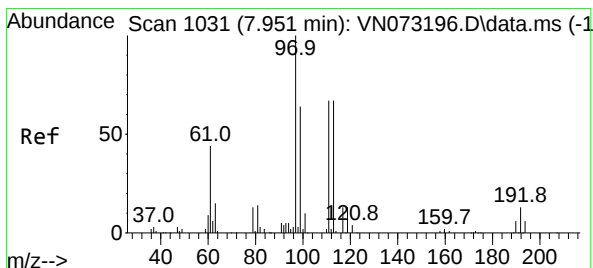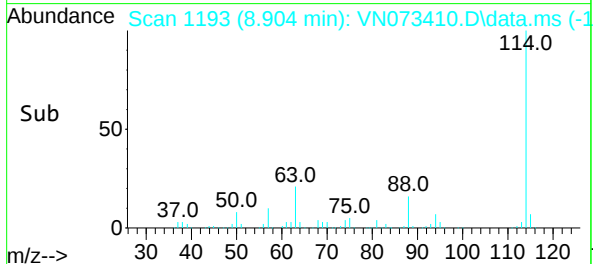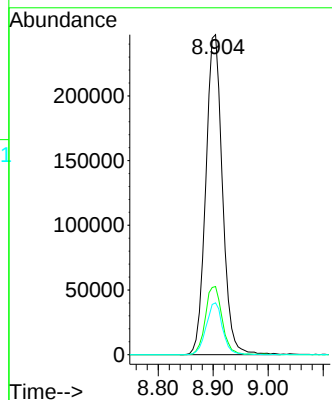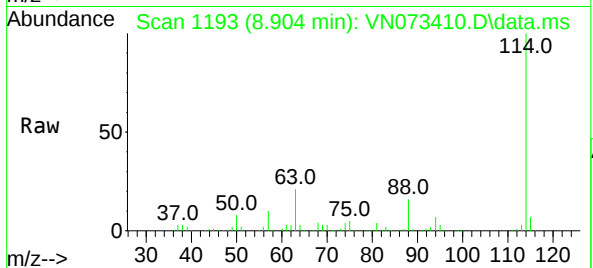

#35

Dibromofluoromethane

Concen: 51.586 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073410.D

Acq: 11 Jul 2022 11:08




Tgt Ion:113 Resp: 178589


Ion Ratio Lower Upper

113 100

111 103.6 81.4 122.0

192 18.5 17.0 25.6


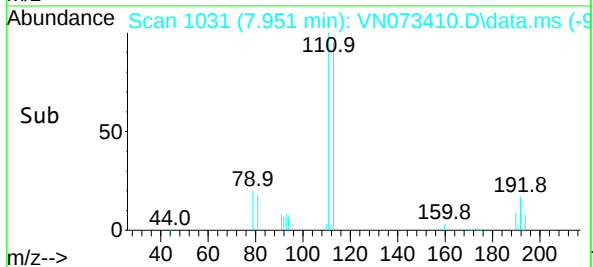
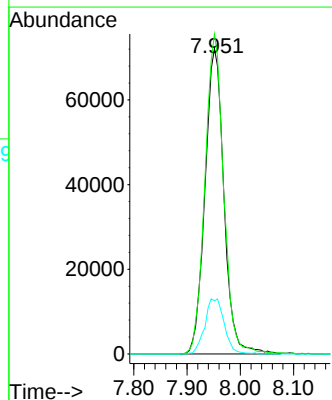
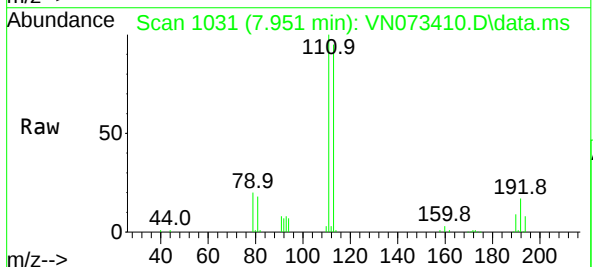


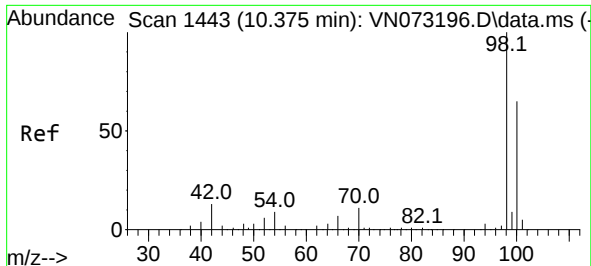

#50
Toluene-d8
Concen: 47.661 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.005 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08




Instrument :
MSVOA_N
ClientSampleId :
VN0711WBL01


Tgt Ion: 98 Resp: 586030
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

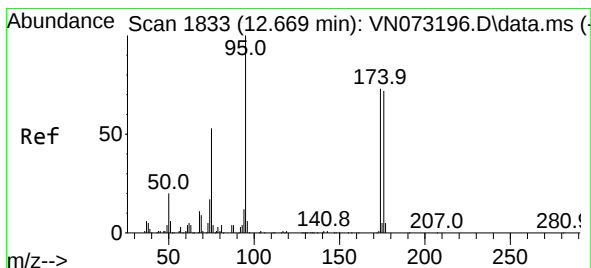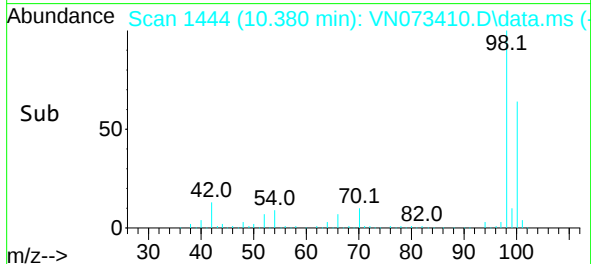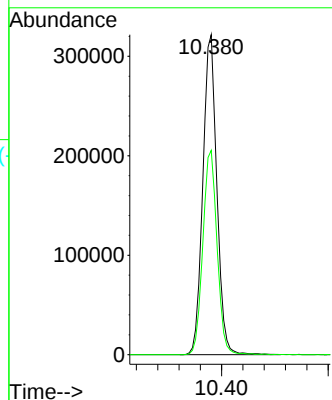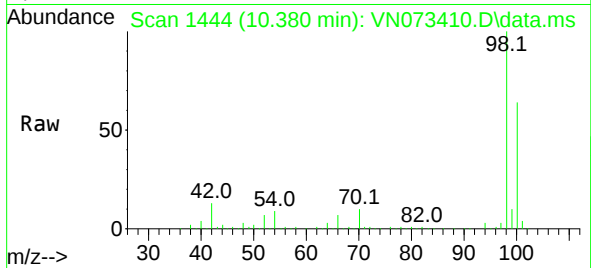

#62
4-Bromofluorobenzene
Concen: 51.773 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08

Tgt Ion: 95 Resp: 244642
Ion Ratio Lower Upper
95 100
174 76.0 0.0 167.6
176 73.5 0.0 163.4


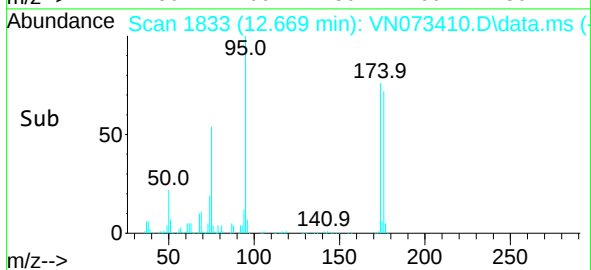
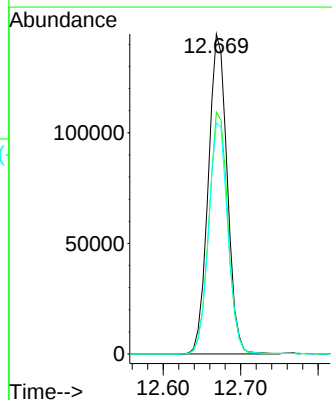
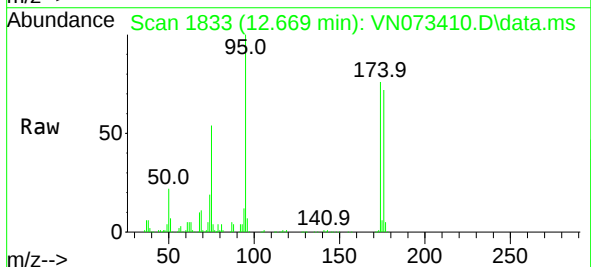


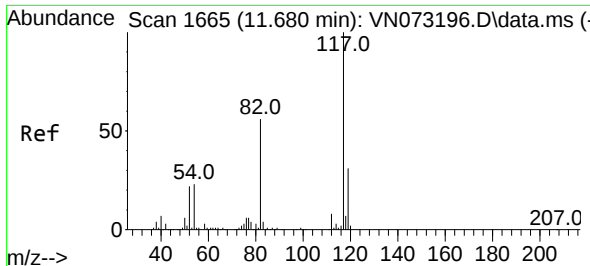

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.680 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08

Instrument :
MSVOA_N
ClientSampleId :
VN0711WBL01

Tgt Ion:117 Resp: 472075
Ion Ratio Lower Upper
117 100
82 56.3 44.2 66.2
119 32.3 25.4 38.0

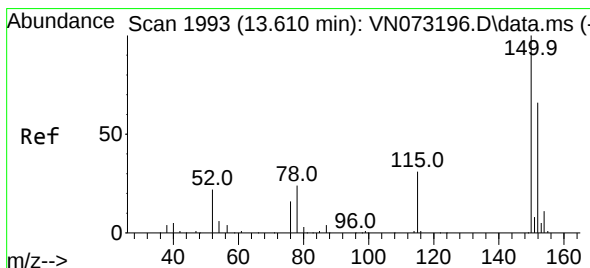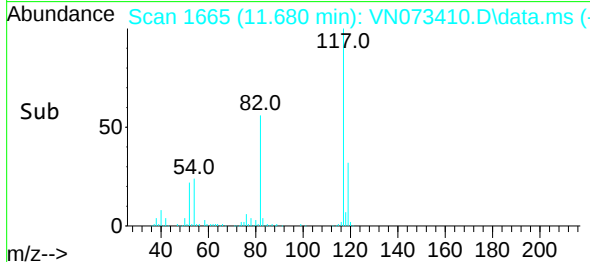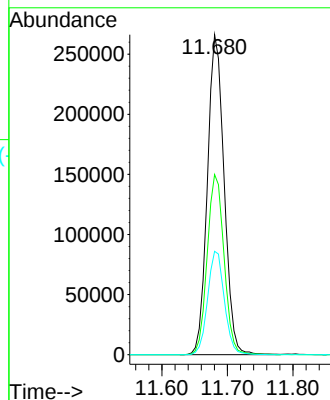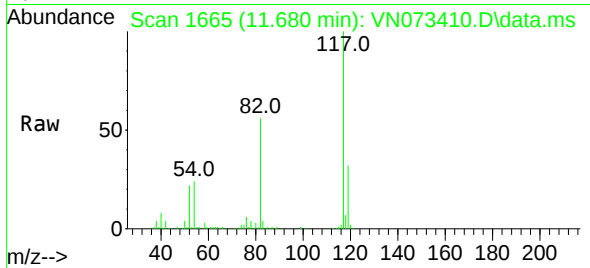

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.610 min Scan# 1993
Delta R.T. -0.000 min
Lab File: VN073410.D
Acq: 11 Jul 2022 11:08

Tgt Ion:152 Resp: 222226
Ion Ratio Lower Upper
152 100
115 60.3 28.9 86.7
150 157.9 0.0 356.2

