

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071122\
 Data File : VN073417.D
 Acq On : 11 Jul 2022 14:17
 Operator : JC\MD
 Sample : N3651-09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SW-1

Quant Time: Jul 12 07:26:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	281748	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	477228	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	441235	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	213185	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	188498	46.344	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.680%
35) Dibromofluoromethane	7.951	113	155638	49.019	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.040%
50) Toluene-d8	10.380	98	503297	44.631	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.260%
62) 4-Bromofluorobenzene	12.674	95	221517	51.116	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.240%
Target Compounds						
16) Acetone	4.240	43	8533	3.738	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071122\
Data File : VN073417.D
Acq On : 11 Jul 2022 14:17
Operator : JC\MD
Sample : N3651-09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SW-1

Quant Time: Jul 12 07:26:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




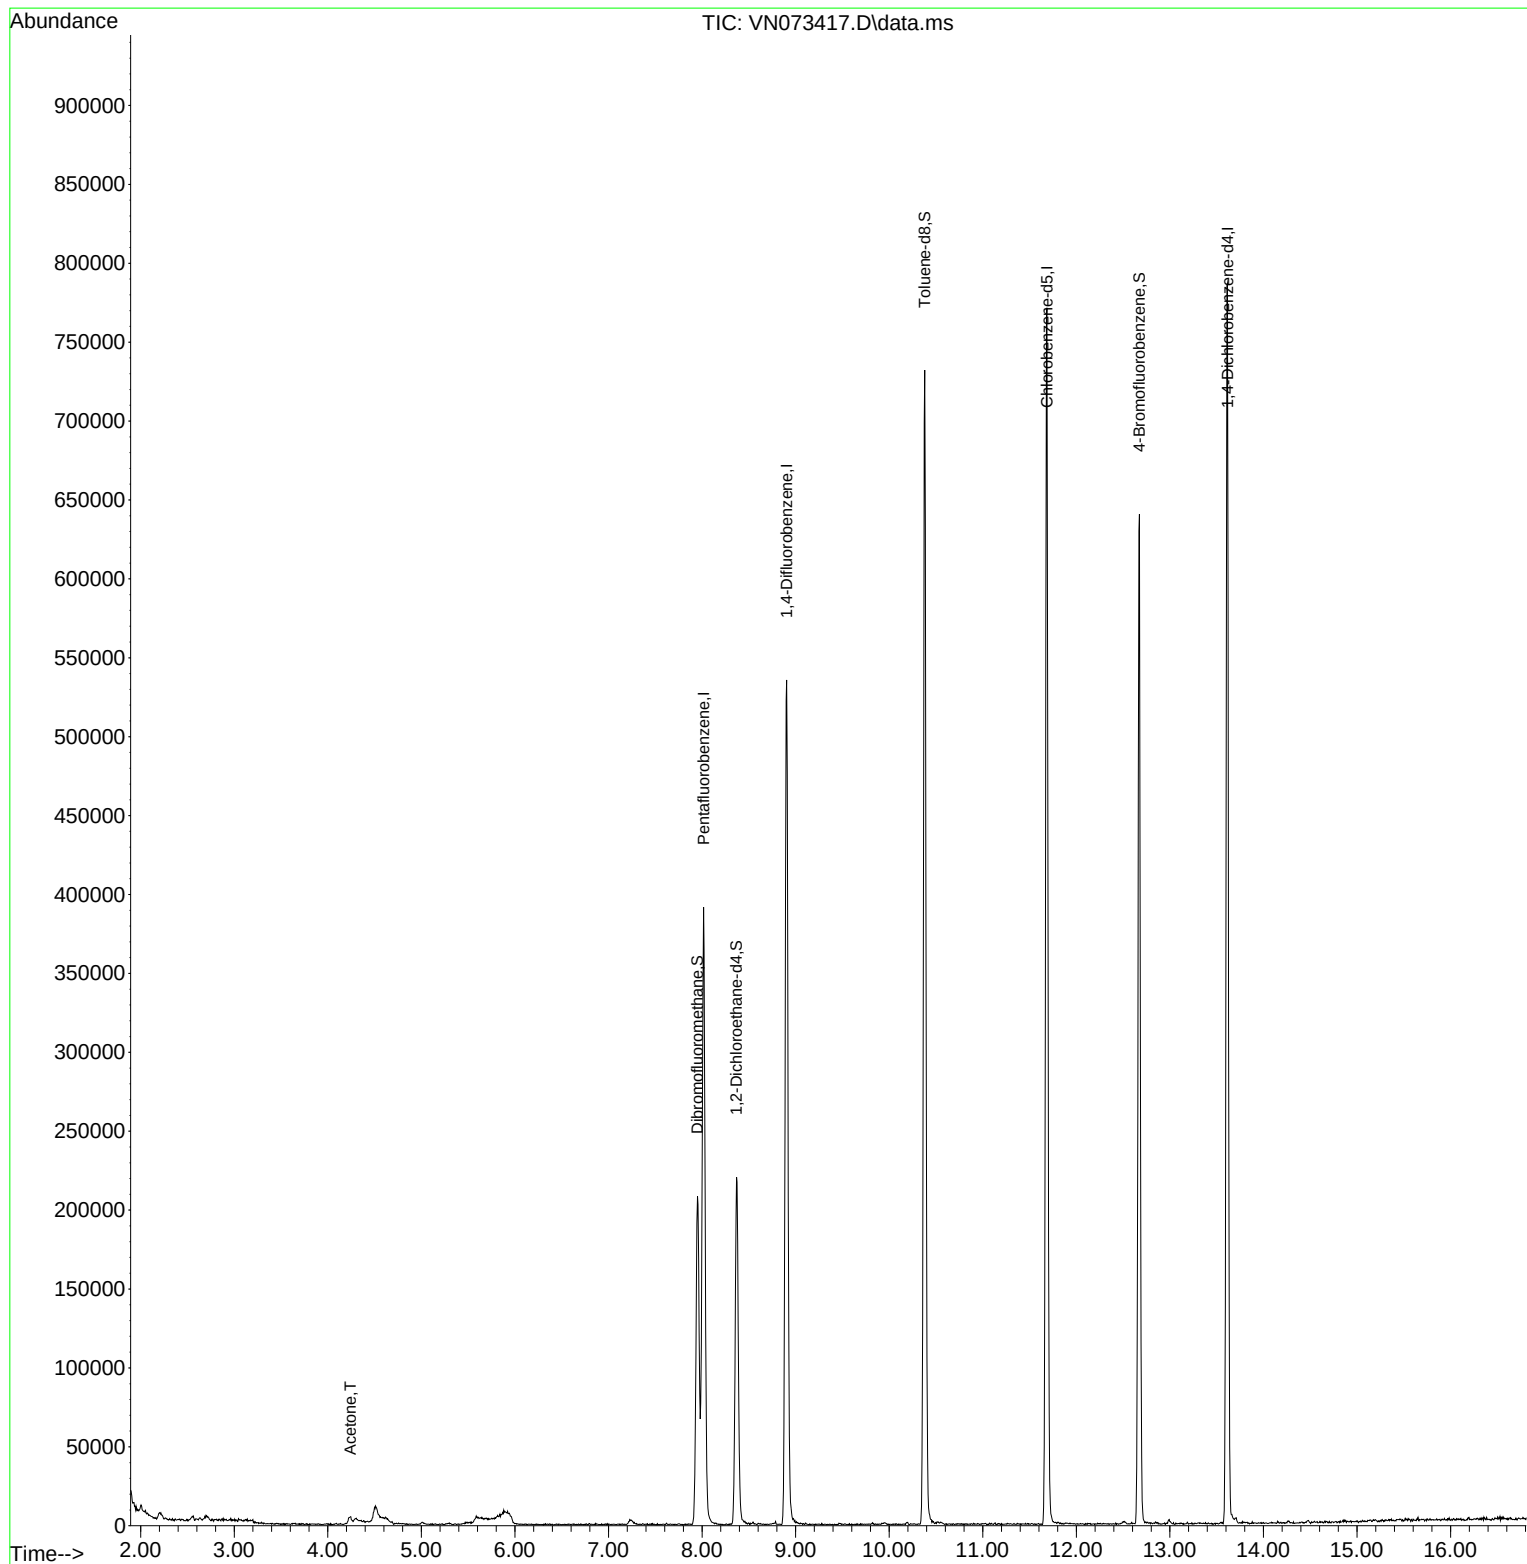


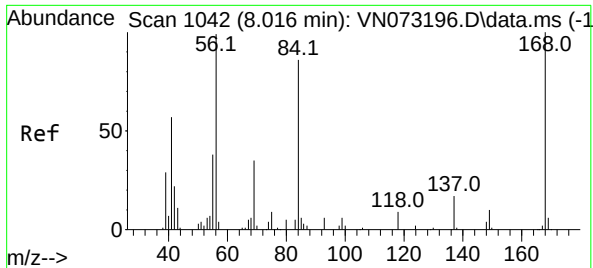

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17




Instrument :
MSVOA_N
ClientSampleId :
SW-1


Tgt Ion:168 Resp: 281748
Ion Ratio Lower Upper
168 100
99 60.3 42.3 63.5

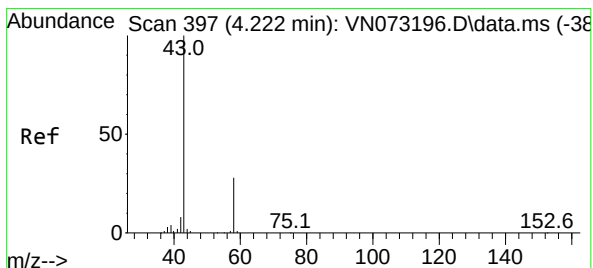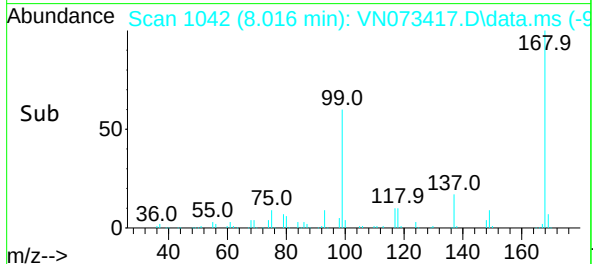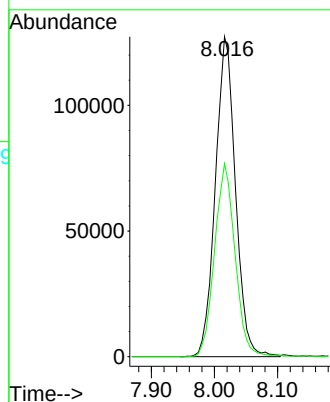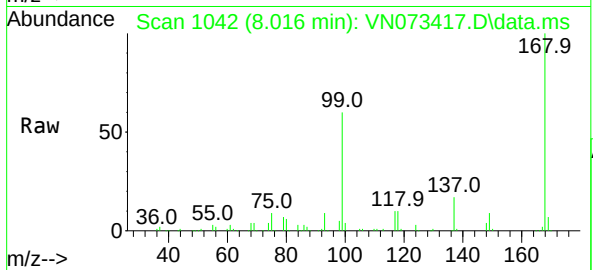

#16
Acetone
Concen: 3.738 ug/l
RT: 4.240 min Scan# 400
Delta R.T. 0.018 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17

Tgt Ion: 43 Resp: 8533
Ion Ratio Lower Upper
43 100
58 31.2 26.0 39.0

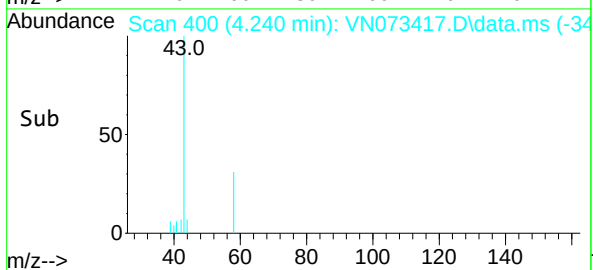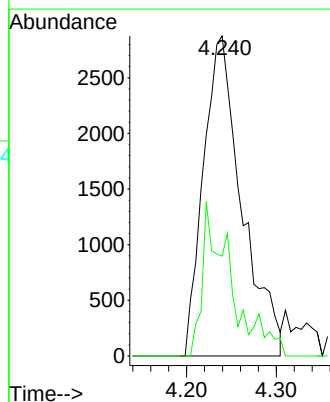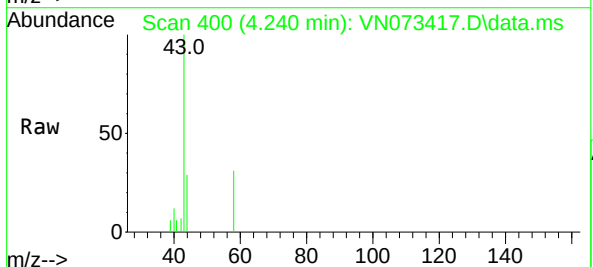

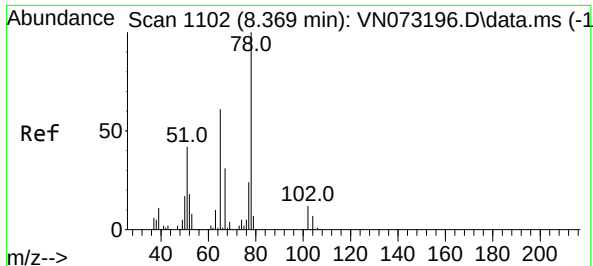

#33

1,2-Dichloroethane-d4

Concen: 46.344 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073417.D

Acq: 11 Jul 2022 14:17

Instrument :

MSVOA_N

ClientSampleId :





SW-1

Tgt Ion: 65 Resp: 188498

Ion Ratio Lower Upper

65 100

67 51.2 0.0 104.8

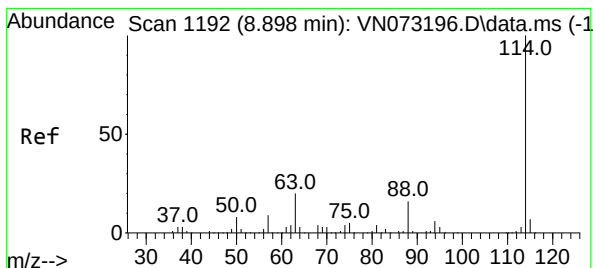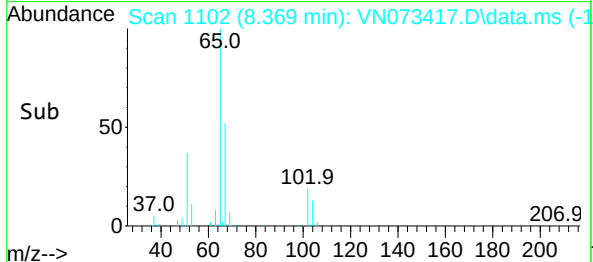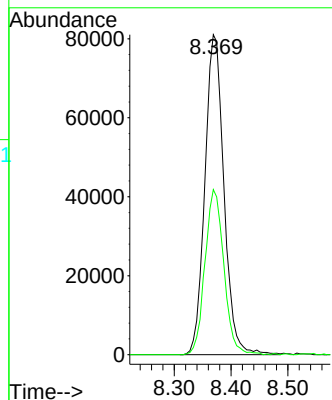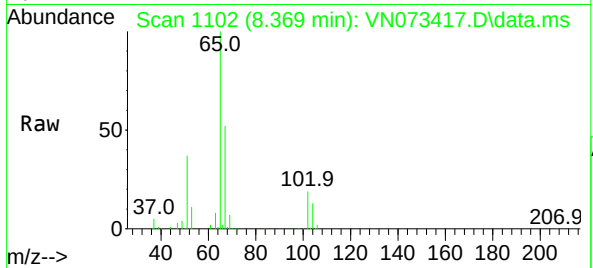

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073417.D

Acq: 11 Jul 2022 14:17




Tgt Ion: 114 Resp: 477228


Ion Ratio Lower Upper

114 100

63 21.6 0.0 40.0

88 15.6 0.0 32.6


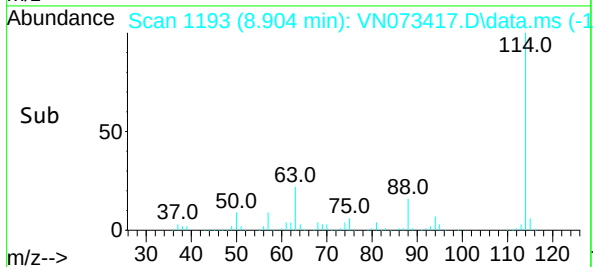
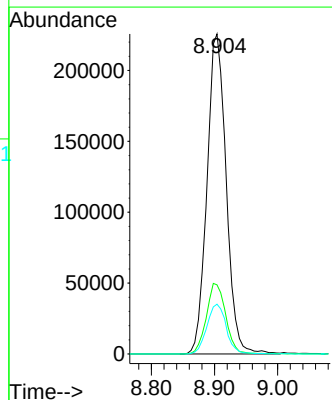
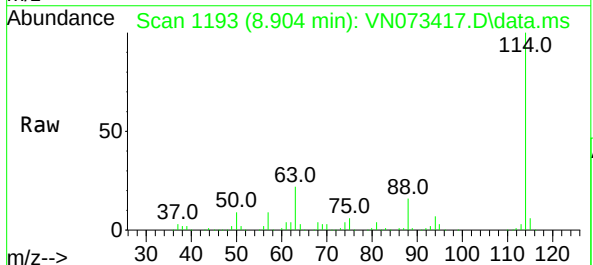


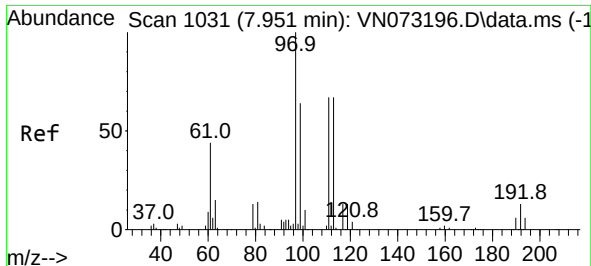

#35
Dibromofluoromethane
Concen: 49.019 ug/l
RT: 7.951 min Scan# 1031
Delta R.T. 0.000 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17




Instrument :
MSVOA_N
ClientSampleId :
SW-1


Tgt Ion:113 Resp: 155638
Ion Ratio Lower Upper
113 100
111 103.1 81.4 122.0
192 18.4 17.0 25.6

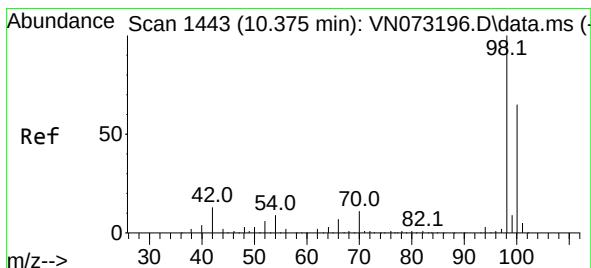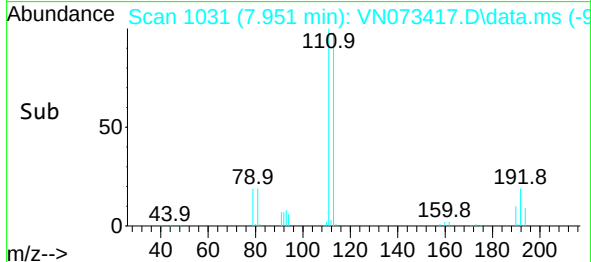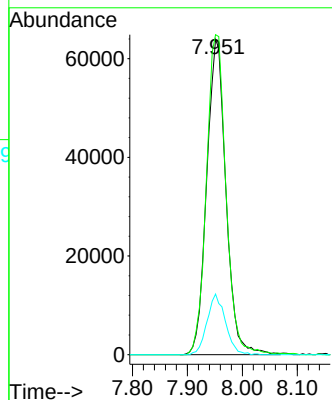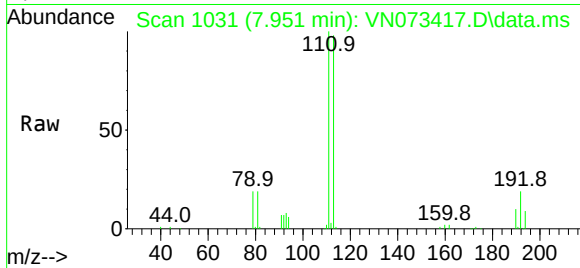

#50
Toluene-d8
Concen: 44.631 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.005 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17

Tgt Ion: 98 Resp: 503297
Ion Ratio Lower Upper
98 100
100 65.9 52.6 78.8


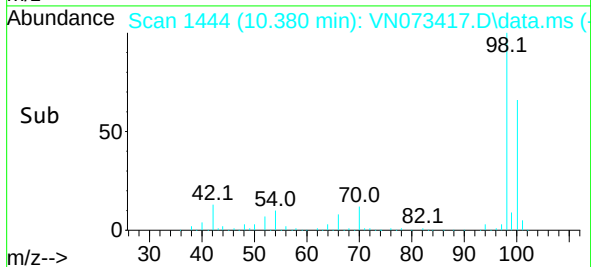
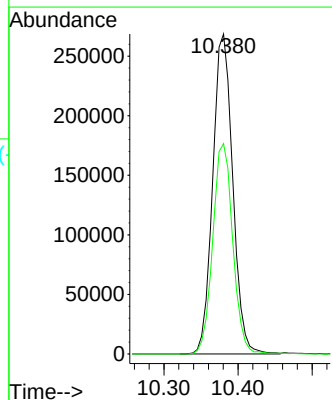
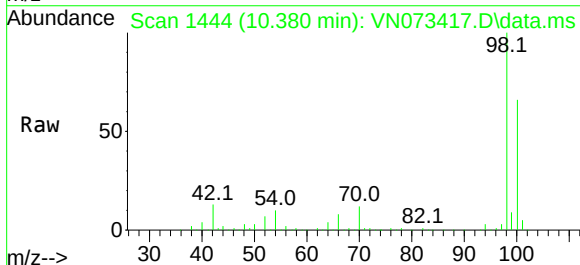


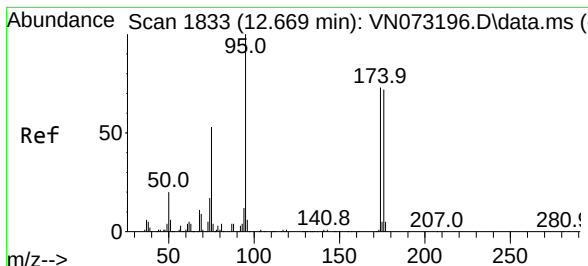

#62
4-Bromofluorobenzene
Concen: 51.116 ug/l
RT: 12.674 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17




Instrument :
MSVOA_N
ClientSampleId :
SW-1


Tgt Ion: 95 Resp: 221517
Ion Ratio Lower Upper
95 100
174 74.9 0.0 167.6
176 72.0 0.0 163.4

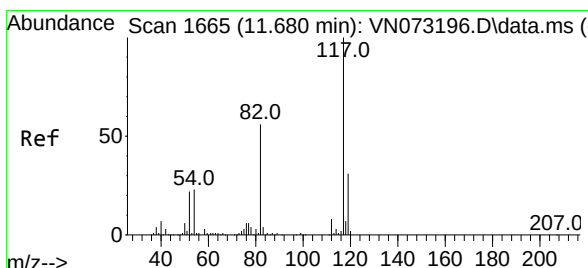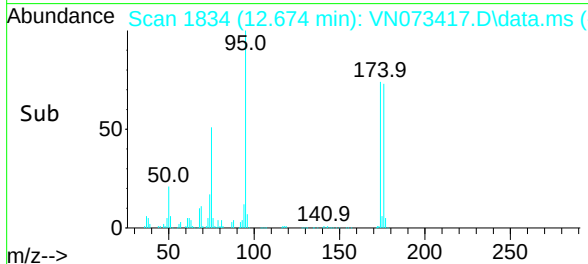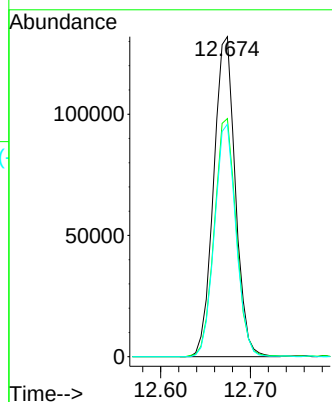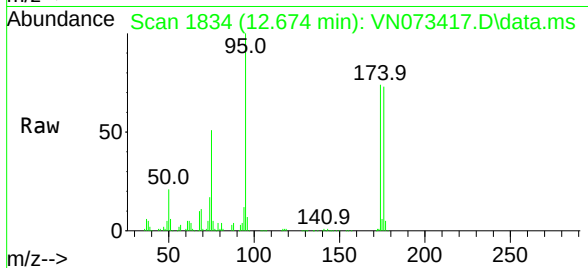

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.006 min
Lab File: VN073417.D
Acq: 11 Jul 2022 14:17

Tgt Ion: 117 Resp: 441235
Ion Ratio Lower Upper
117 100
82 57.8 44.2 66.2
119 31.6 25.4 38.0

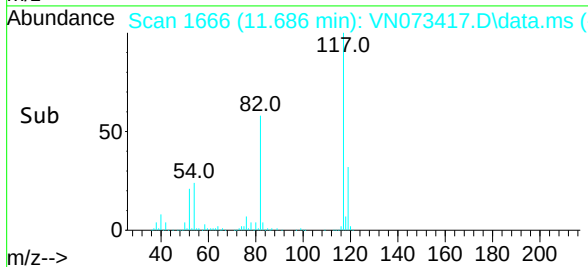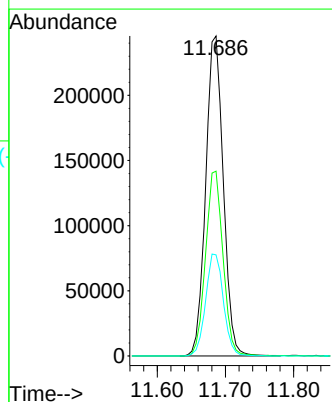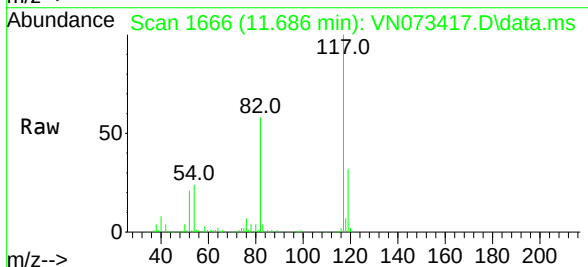

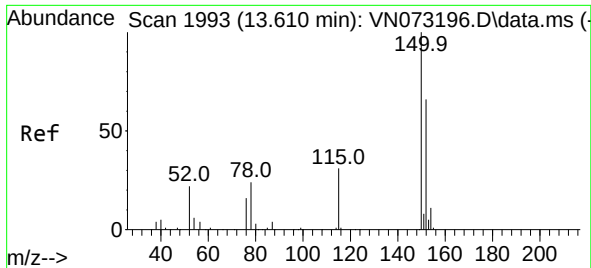

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.615 min Scan# 1994
 Delta R.T. 0.005 min
 Lab File: VN073417.D
 Acq: 11 Jul 2022 14:17

Instrument :
 MSVOA_N
 ClientSampleId :
 SW-1

Tgt Ion:152 Resp: 213185
 Ion Ratio Lower Upper
 152 100
 115 60.6 28.9 86.7
 150 158.3 0.0 356.2

