
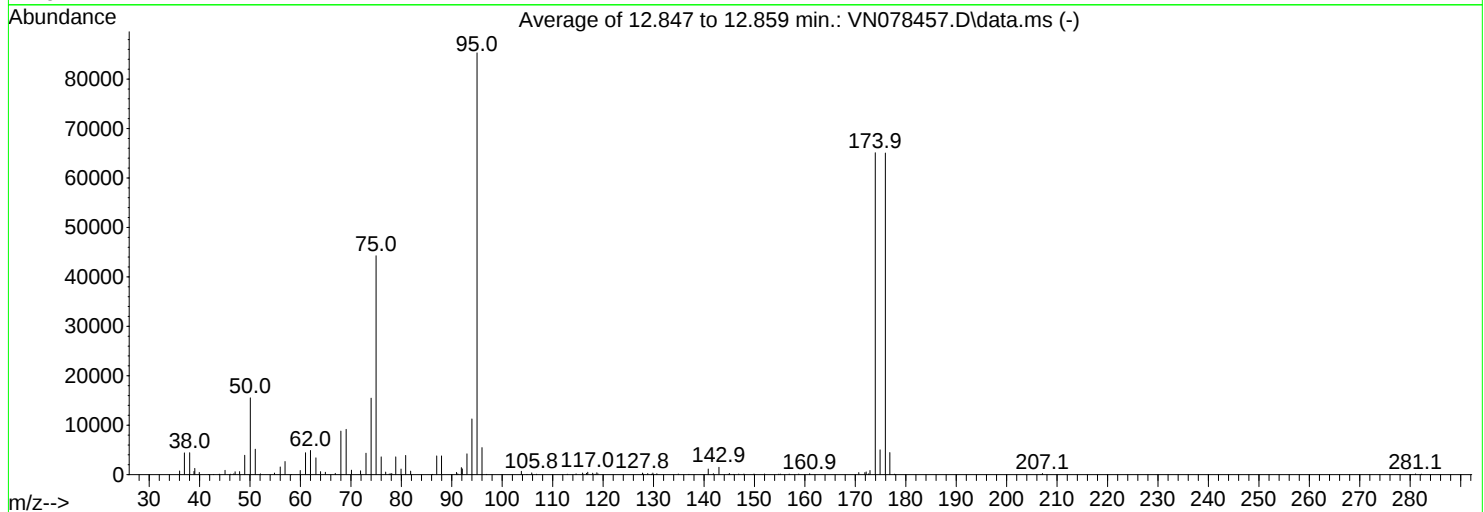


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071123\
Data File : VN078457.D
Acq On : 11 Jul 2023 11:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

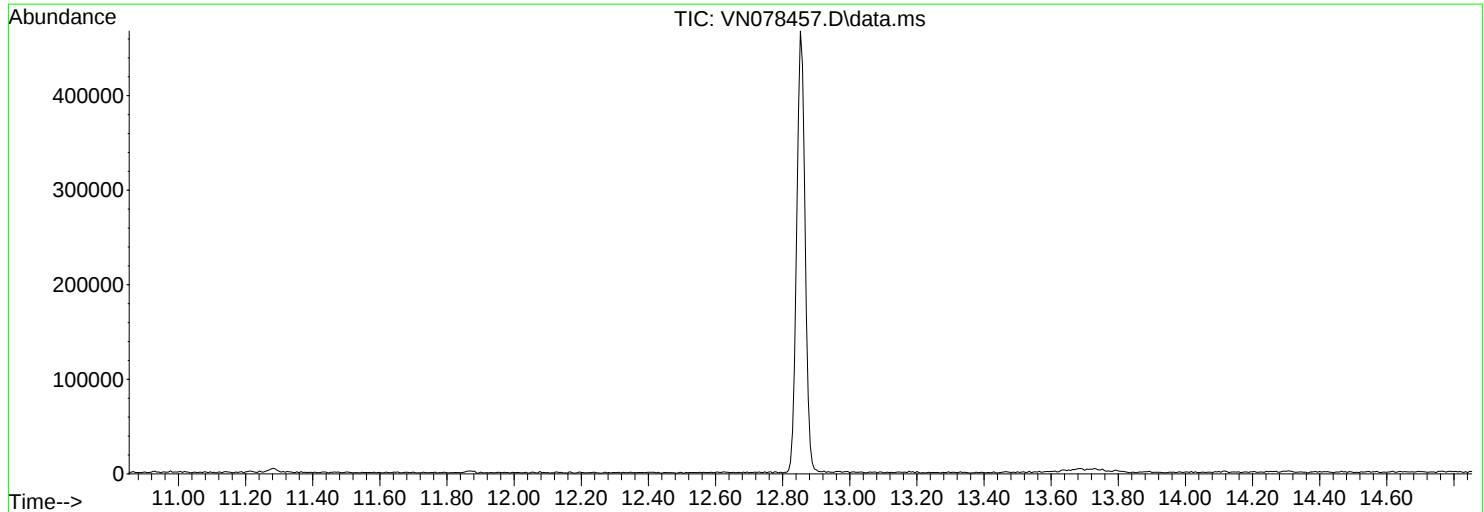

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	15542	PASS
75	95	30	60	51.9	44277	PASS
95	95	100	100	100.0	85307	PASS
96	95	5	9	6.4	5478	PASS
173	174	0.00	2	1.3	836	PASS
174	95	50	100	76.3	65125	PASS
175	174	5	9	7.7	5018	PASS
176	174	95	101	99.9	65032	PASS
177	176	5	9	6.9	4473	PASS

Average of 12.847 to 12.859 min.: VN078457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	737	46.80	171	59.95	847	73.00	435
37.00	4400	47.05	574	61.00	4420	74.00	1546
38.05	4429	47.95	616	62.00	4878	75.00	4427
38.90	639	48.95	3918	63.05	3406	76.00	360
39.05	1271	50.05	15542	64.00	618	76.90	534
39.95	467	51.05	5156	64.95	503	77.60	130
41.80	50	52.05	156	66.90	268	77.80	151
42.80	51	54.85	314	68.00	8798	78.10	227
43.90	102	56.00	1559	69.05	9166	78.90	3594
45.05	882	56.95	2667	70.10	895	79.95	1137
46.10	99	58.20	51	71.90	777	80.85	3889

Instrument :

MSVOA_N

ClientSampleId :

BFB

Average of 12.847 to 12.859 min.: VN078457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	731	96.00	5478	117.95	289	137.00	61
86.20	61	96.90	56	118.40	98	140.85	1122
87.00	3781	103.80	685	118.75	389	141.85	207
87.95	3788	104.90	61	119.00	152	142.95	1481
90.95	443	105.85	365	127.80	324	144.80	86
91.20	151	106.80	101	128.00	91	145.05	238
91.90	1433	112.90	87	128.85	226	145.90	61
92.10	1152	114.65	149	129.60	88	146.90	143
93.00	4221	115.95	341	129.85	324	147.90	126
94.00	11265	116.70	244	130.65	207	149.90	121
95.00	85307	116.95	499	134.90	135	152.00	118

Average of 12.847 to 12.859 min.: VN078457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.80	94	174.90	5018				
155.10	136	175.95	65032				
156.90	139	176.85	4473				
158.80	132	177.80	111				
160.95	195	206.80	64				
170.70	419	207.10	237				
171.90	434	281.05	169				
172.15	557	282.20	88				
172.60	157						
172.90	836						
173.95	65125						