

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071124\
 Data File : VN082871.D
 Acq On : 11 Jul 2024 13:06
 Operator : JC\MD
 Sample : P3184-03RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP(00187-00189-00186)

Quant Time: Jul 12 01:05:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	123118	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	229424	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	232483	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	103996	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	90047	52.175	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.360%			
35) Dibromofluoromethane	8.165	113	73740	50.090	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.180%			
50) Toluene-d8	10.571	98	278526	51.224	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.440%			
62) 4-Bromofluorobenzene	12.847	95	102891	52.679	ug/l	0.00
Spiked Amount 50.000	Range 64 - 133		Recovery = 105.360%			
Target Compounds					Qvalue	
11) Tert butyl alcohol	5.530	59	16510	56.876	ug/l	95
16) Acetone	4.436	43	23697	38.999	ug/l	99
17) Carbon Disulfide	4.712	76	4778	1.272	ug/l #	90
18) Methyl Acetate	5.024	43	606	0.377	ug/l #	56
20) Methylene Chloride	5.283	84	12246	8.345	ug/l #	85
25) 2-Butanone	7.500	43	3498	3.813	ug/l	94
29) Tetrahydrofuran	7.847	42	246	0.426	ug/l #	62
31) Cyclohexane	8.224	56	3226	1.430	ug/l #	5
32) 1,1,1-Trichloroethane	8.171	97	535	0.218	ug/l #	45
36) 1,1-Dichloropropene	8.224	75	10889	5.365	ug/l #	51
37) Ethyl Acetate	7.565	43	2140	1.036	ug/l #	76
38) Carbon Tetrachloride	8.224	117	13760	5.630	ug/l #	15
40) Benzene	8.606	78	6690	1.072	ug/l	98
43) Isopropyl Acetate	8.694	43	84162	19.808	ug/l #	92
45) 1,2-Dichloropropane	9.735	63	535	0.367	ug/l #	44
48) Methyl methacrylate	9.659	41	2561	1.581	ug/l #	50
51) 4-Methyl-2-Pentanone	10.447	43	6855	3.346	ug/l #	79
52) Toluene	10.629	92	20610	5.284	ug/l	97
54) cis-1,3-Dichloropropene	10.359	75	22548	8.813	ug/l #	65
57) 1,3-Dichloropropane	11.206	76	1933	0.761	ug/l #	43
59) 2-Hexanone	11.171	43	44158	28.992	ug/l #	28
67) Ethyl Benzene	11.965	91	3707	0.443	ug/l	91
68) m/p-Xylenes	12.071	106	4538	1.436	ug/l	93
69) o-Xylene	12.400	106	2166	0.715	ug/l	99
71) Bromoform	12.847	173	508	0.365	ug/l #	1
74) N-amyl acetate	12.465	43	880	0.282	ug/l #	46
76) 1,2,3-Trichloropropane	12.847	75	56994	31.788	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	56994	62.517	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.476	105	2206	0.354	ug/l	96
95) Naphthalene	15.641	128	7023	1.113	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071124\
Data File : VN082871.D
Acq On : 11 Jul 2024 13:06
Operator : JC\MD
Sample : P3184-03RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Quant Time: Jul 12 01:05:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration

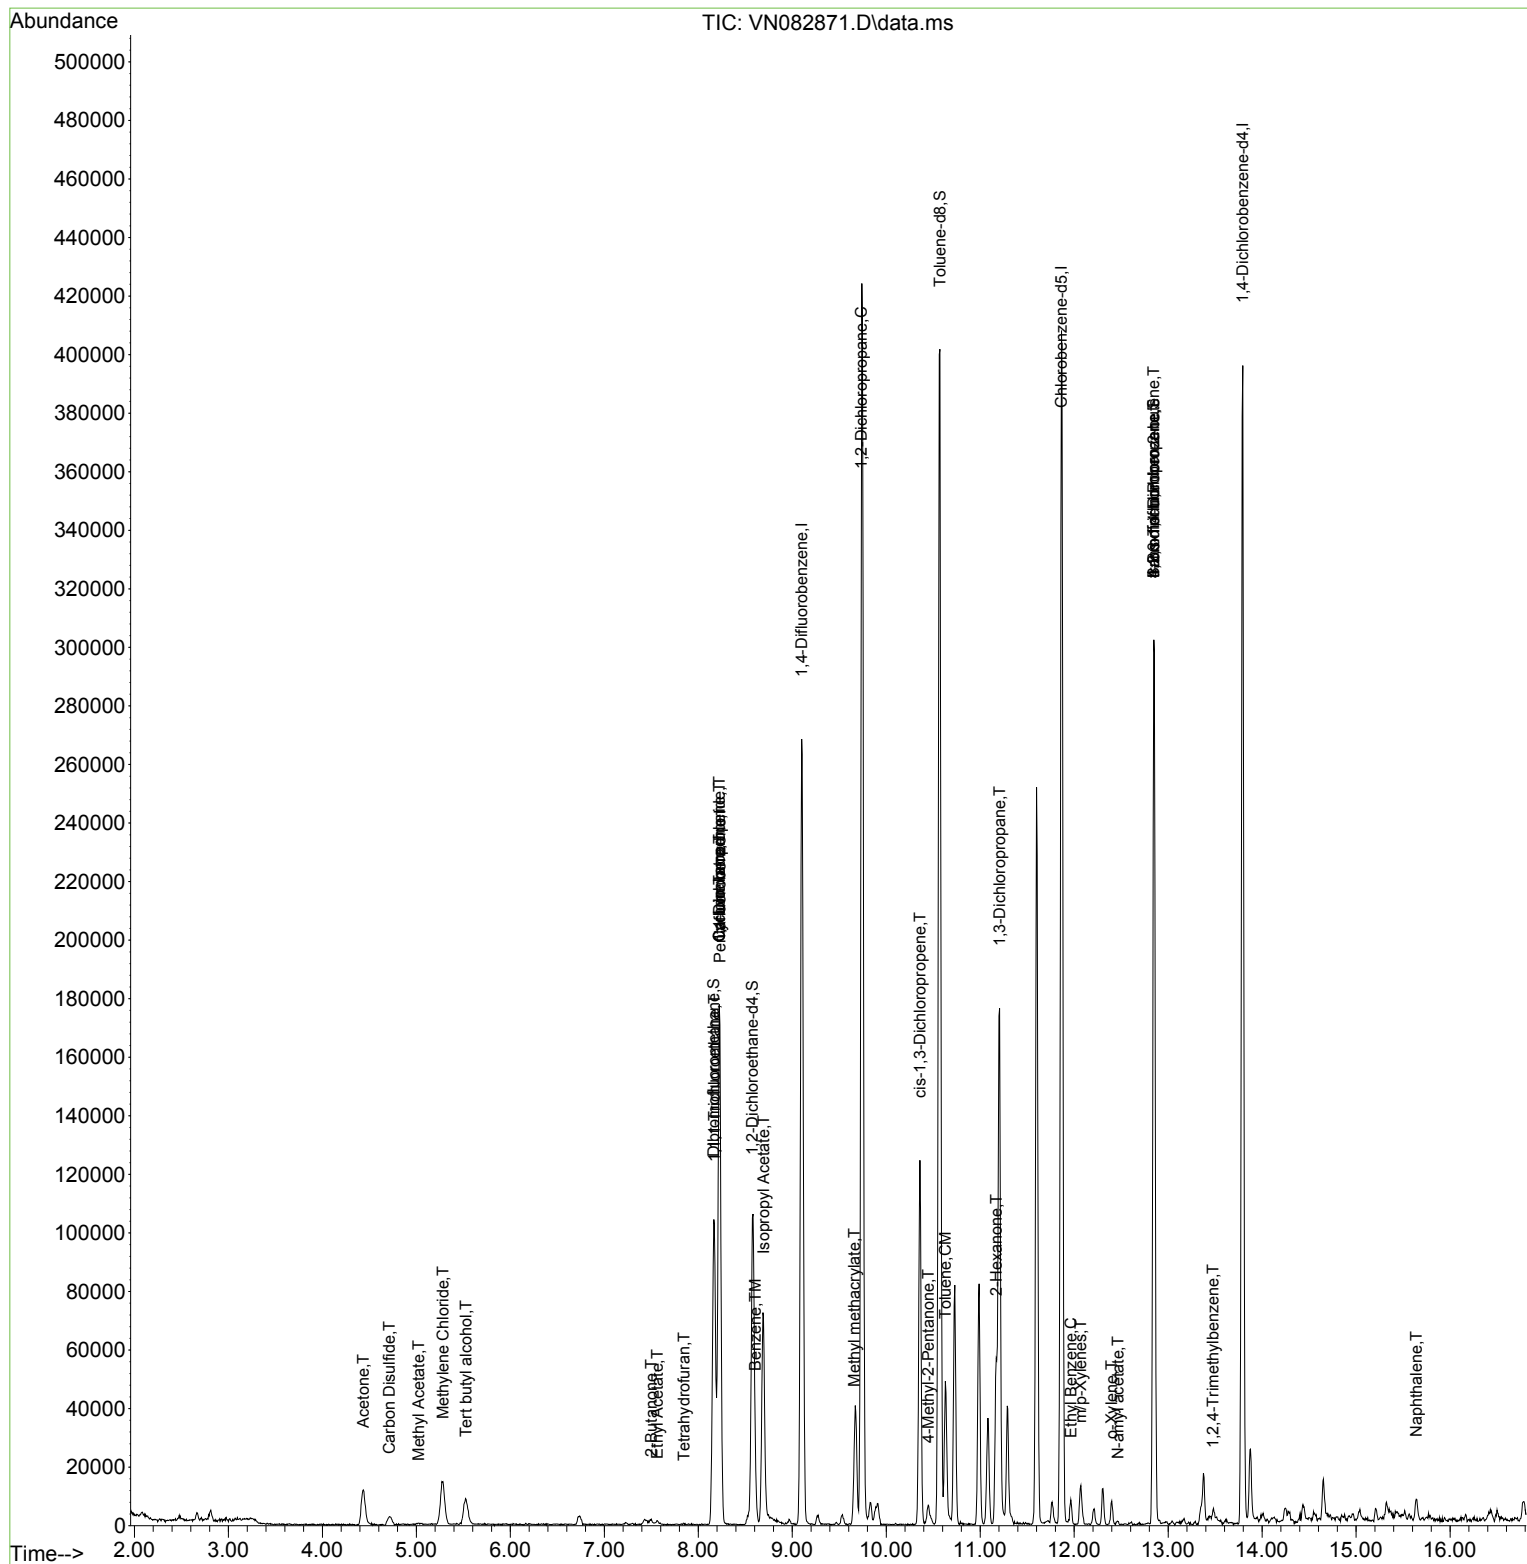






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)







Tgt Ion:168 Resp: 123118
Ion Ratio Lower Upper
168 100
99 59.1 48.2 72.4

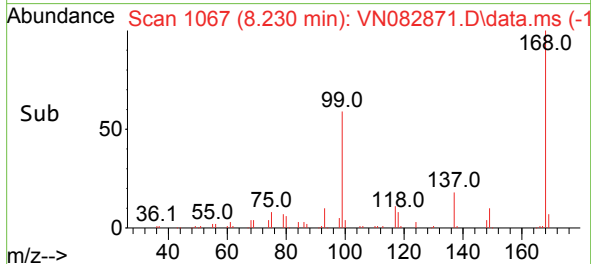

#11
Tert butyl alcohol
Concen: 56.876 ug/l
RT: 5.530 min Scan# 608
Delta R.T. 0.006 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 59 Resp: 16510
Ion Ratio Lower Upper
59 100
57 9.3 8.9 13.3

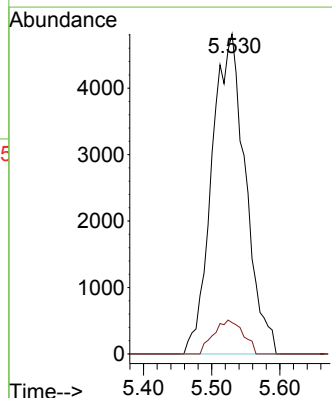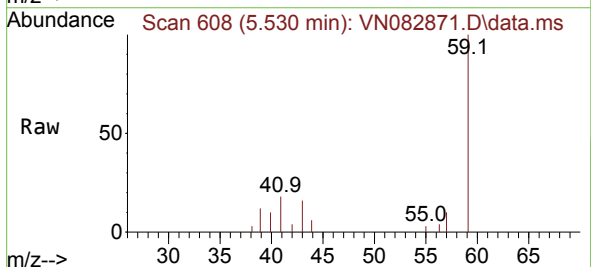



#16

Acetone

Concen: 38.999 ug/l

RT: 4.436 min Scan# 41

Delta R.T. 0.006 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :





COMP(00187-00189-00186)

Tgt Ion: 43 Resp: 23697

Ion Ratio Lower Upper

43 100

58 27.5 21.8 32.6

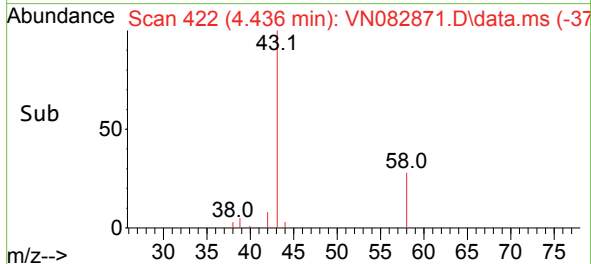

#17

Carbon Disulfide

Concen: 1.272 ug/l

RT: 4.712 min Scan# 469

Delta R.T. 0.000 min

Lab File: VN082871.D




Acq: 11 Jul 2024 13:06


Tgt Ion: 76 Resp: 4778

Ion Ratio Lower Upper

76 100


78 12.7 7.2 10.8#

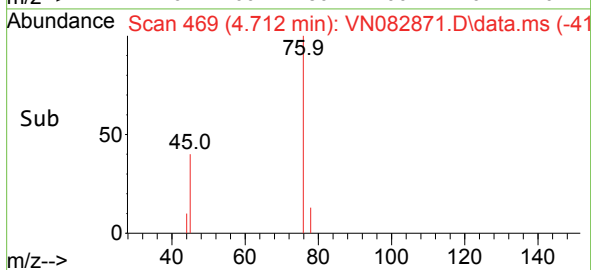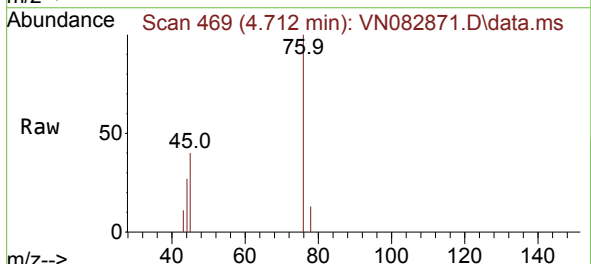






#18
Methyl Acetate
Concen: 0.377 ug/l
RT: 5.024 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)







Tgt Ion: 43 Resp: 606
Ion Ratio Lower Upper
43 100
74 0.0 16.3 24.5#

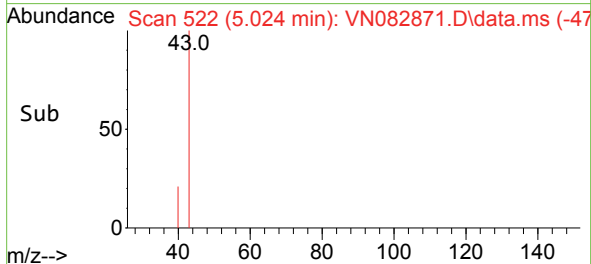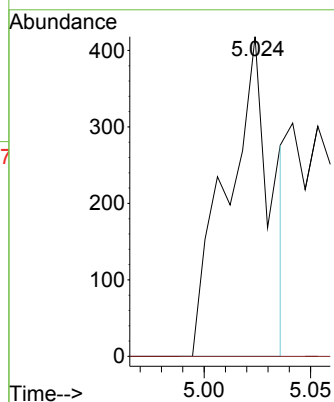

#20
Methylene Chloride
Concen: 8.345 ug/l
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 84 Resp: 12246
Ion Ratio Lower Upper
84 100
49 119.3 119.6 179.4#
51 39.5 34.8 52.2
86 66.3 52.9 79.3

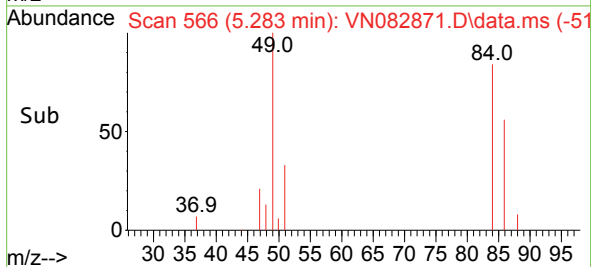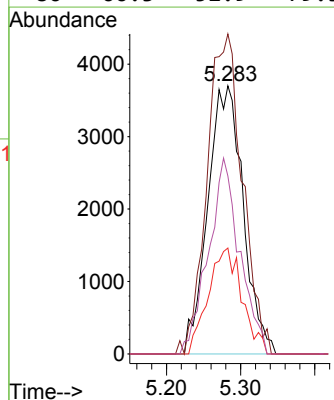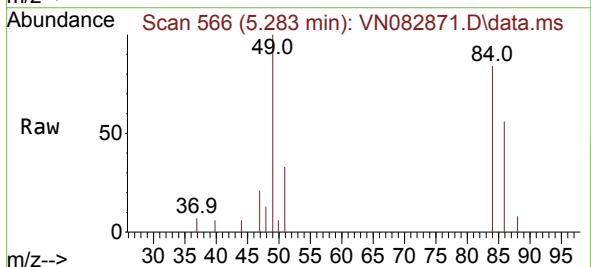

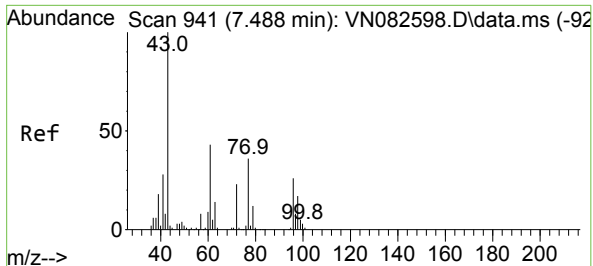

#25

2-Butanone

Concen: 3.813 ug/l

RT: 7.500 min Scan# 941

Delta R.T. 0.012 min

Lab File: VN082871.D


Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :

COMP(00187-00189-00186)



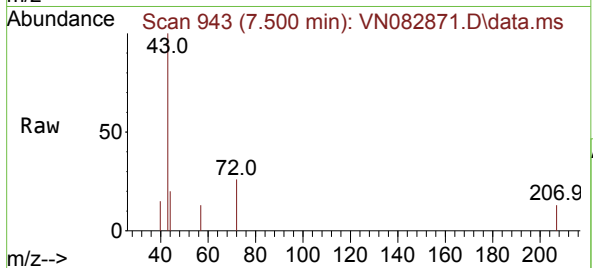


Tgt Ion: 43 Resp: 3498

Ion Ratio Lower Upper

43 100

72 25.6 18.2 27.2

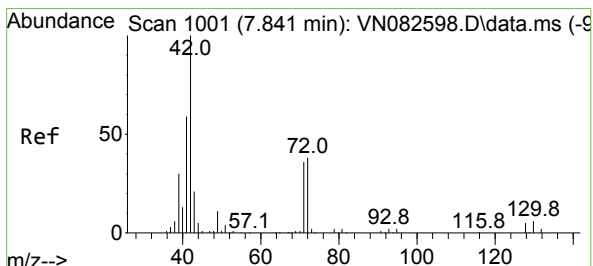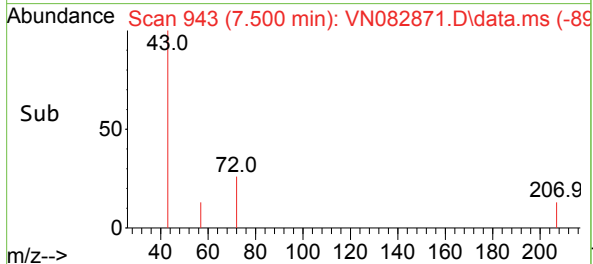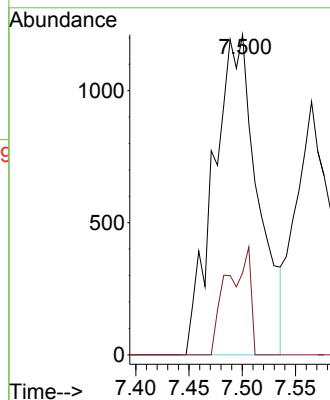

#29

Tetrahydrofuran

Concen: 0.426 ug/l

RT: 7.847 min Scan# 1002

Delta R.T. 0.006 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06




Tgt Ion: 42 Resp: 246


Ion Ratio Lower Upper

42 100

72 27.2 30.0 45.0#


71 0.0 28.3 42.5#

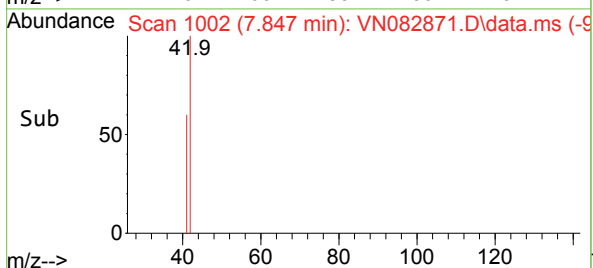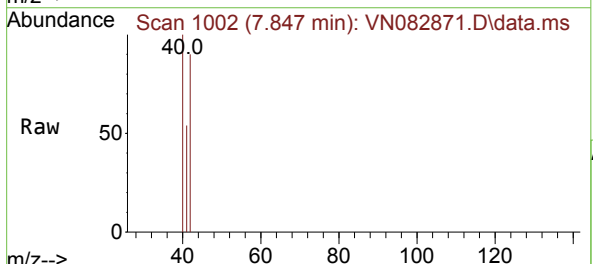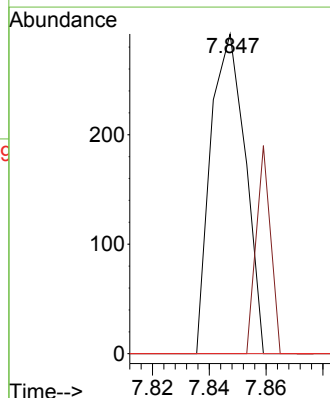






#31
Cyclohexane
Concen: 1.430 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.035 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)







Tgt Ion: 56 Resp: 3226
Ion Ratio Lower Upper
56 100
69 144.5 24.5 36.7#
84 129.9 66.0 99.0#

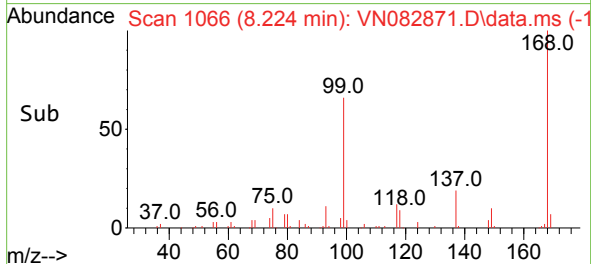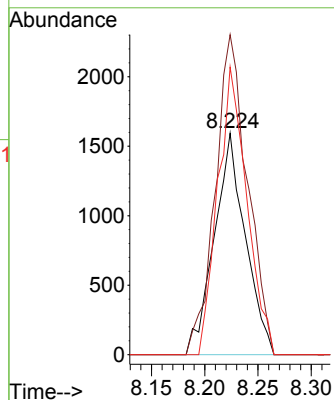

#32
1,1,1-Trichloroethane
Concen: 0.218 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 97 Resp: 535
Ion Ratio Lower Upper
97 100
99 0.0 52.0 78.0#
61 37.4 42.1 63.1#

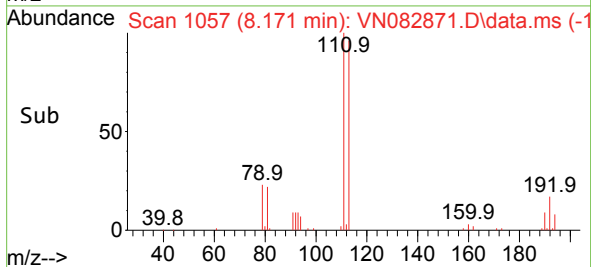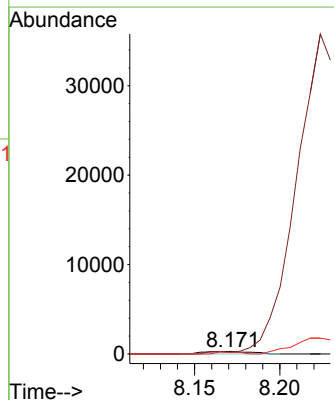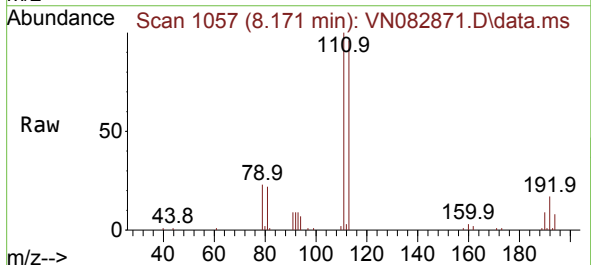



#33

1,2-Dichloroethane-d4

Concen: 52.175 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.005 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :





COMP(00187-00189-00186)

Tgt Ion: 65 Resp: 90047

Ion Ratio Lower Upper

65 100

67 50.1 0.0 104.4

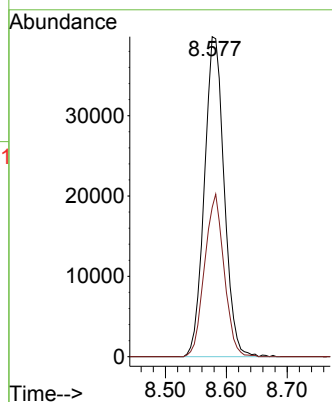

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. -0.006 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06




Tgt Ion: 114 Resp: 229424


Ion Ratio Lower Upper

114 100

63 20.9 0.0 44.6

88 15.9 0.0 31.4


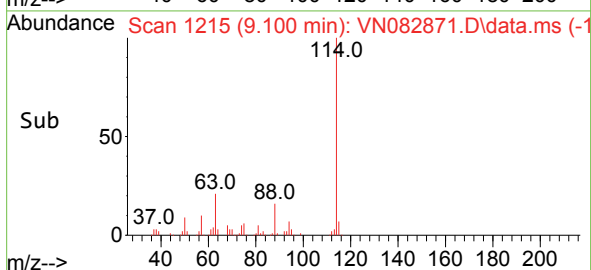






#35
Dibromofluoromethane
Concen: 50.090 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion:113 Resp: 73740
Ion Ratio Lower Upper
113 100
111 102.7 82.4 123.6
192 18.2 14.9 22.3

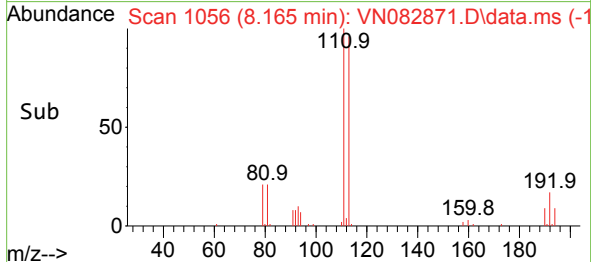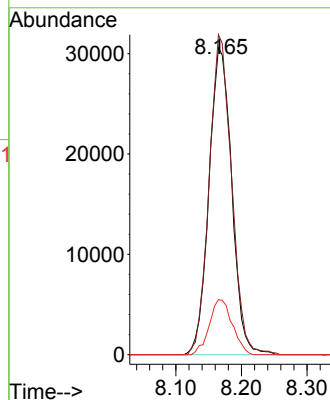

#36
1,1-Dichloropropene
Concen: 5.365 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 75 Resp: 10889
Ion Ratio Lower Upper
75 100
110 8.9 16.3 48.9#
77 0.0 24.6 37.0#

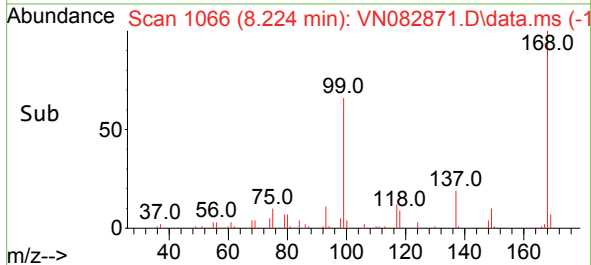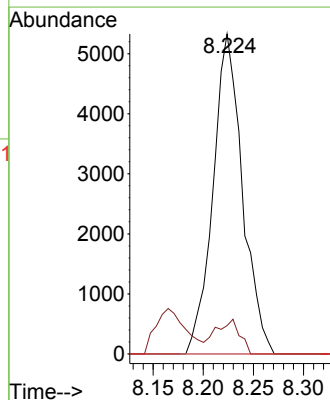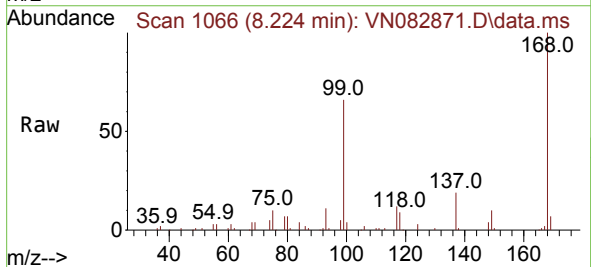



#37

Ethyl Acetate

Concen: 1.036 ug/l

RT: 7.565 min Scan# 91

Delta R.T. -0.000 min

Lab File: VN082871.D


Acq: 11 Jul 2024 13:06

Instrument :




MSVOA_N

ClientSampleId :

COMP(00187-00189-00186)



Tgt Ion:	43	Resp:	2140
Ion	Ratio	Lower	Upper
43	100		
61	2.8	9.3	13.9#
70	0.0	7.0	10.6#

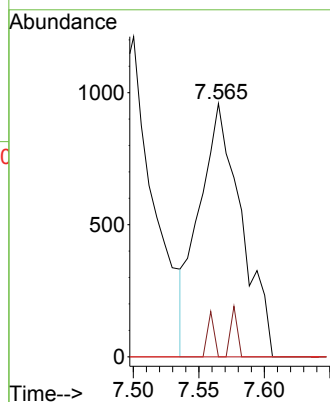

#38

Carbon Tetrachloride

Concen: 5.630 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.141 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Tgt Ion:	117	Resp:	13760
Ion	Ratio	Lower	Upper
117	100		
119	3.2	74.9	112.3#
121	0.0	24.3	36.5#


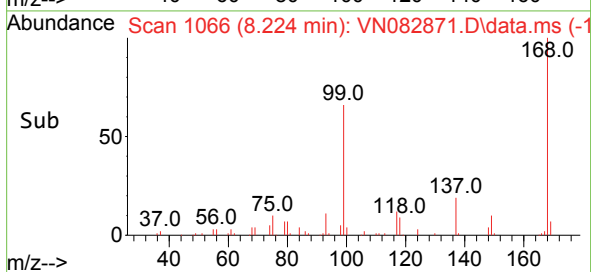

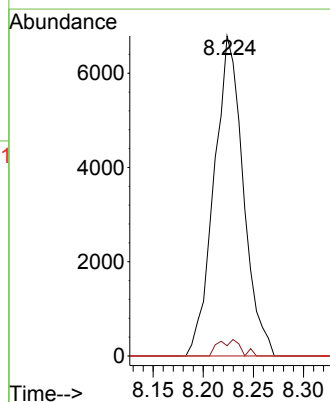




#40
Benzene
Concen: 1.072 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 78 Resp: 6690
Ion Ratio Lower Upper
78 100
77 24.8 19.0 28.4

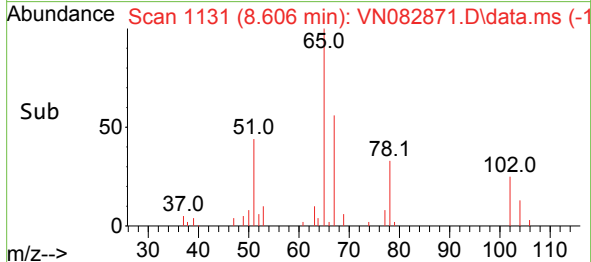

#43
Isopropyl Acetate
Concen: 19.808 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 43 Resp: 84162
Ion Ratio Lower Upper
43 100
61 18.2 17.8 26.6
87 12.9 8.2 12.2#

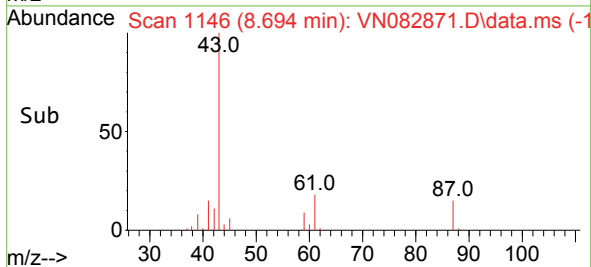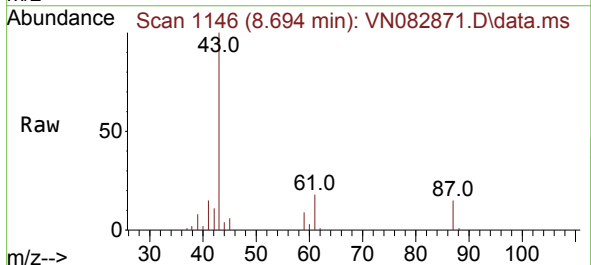



#45

1,2-Dichloropropane

Concen: 0.367 ug/l

RT: 9.735 min Scan# 11

Delta R.T. 0.112 min

Lab File: VN082871.D


Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :

COMP(00187-00189-00186)






Tgt Ion: 63 Resp: 535

Ion Ratio Lower Upper

63 100

65 0.0 24.4 36.6#

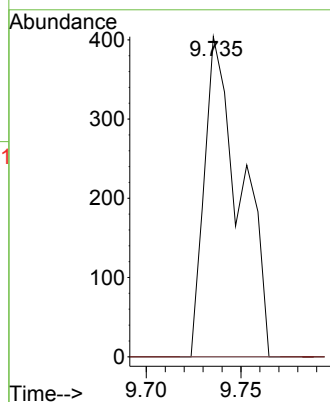

#48

Methyl methacrylate

Concen: 1.581 ug/l

RT: 9.659 min Scan# 1310

Delta R.T. -0.023 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06




Tgt Ion: 41 Resp: 2561


Ion Ratio Lower Upper

41 100

69 0.0 56.3 84.5#

39 71.3 50.3 75.5


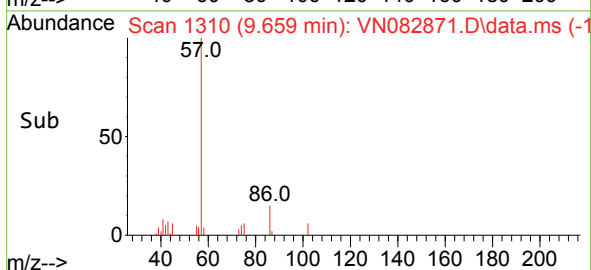

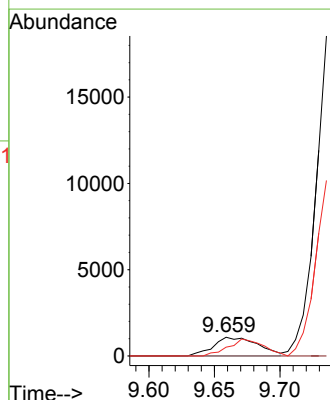


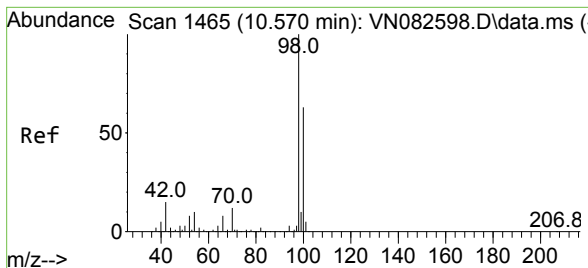

#50
Toluene-d8
Concen: 51.224 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 98 Resp: 278526
Ion Ratio Lower Upper
98 100
100 64.5 51.5 77.3

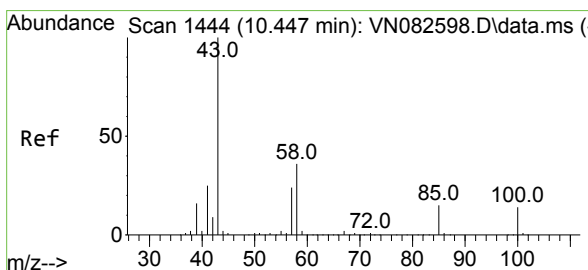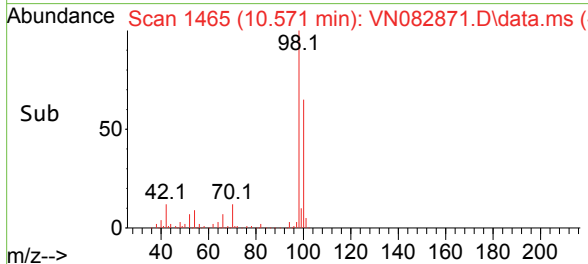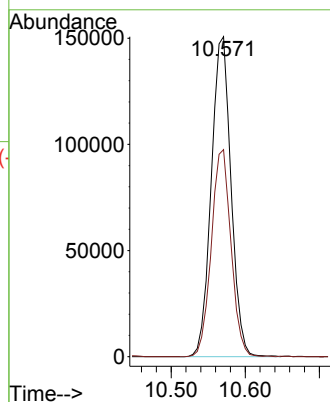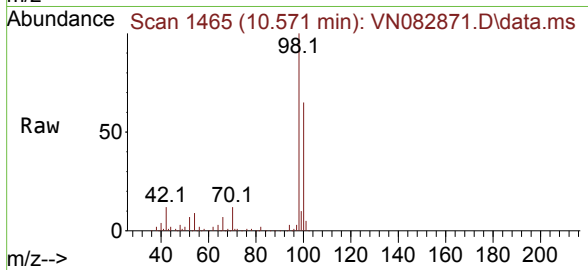

#51
4-Methyl-2-Pentanone
Concen: 3.346 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 43 Resp: 6855
Ion Ratio Lower Upper
43 100
58 22.8 28.2 42.4#


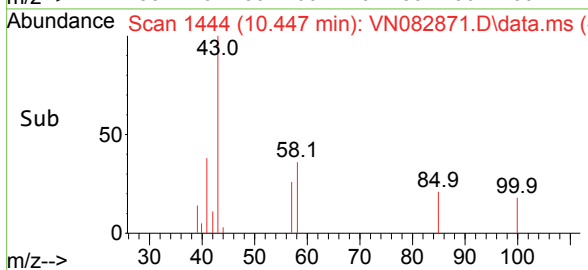
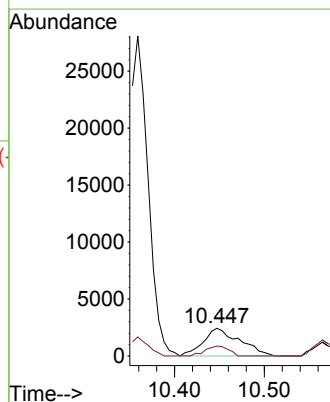
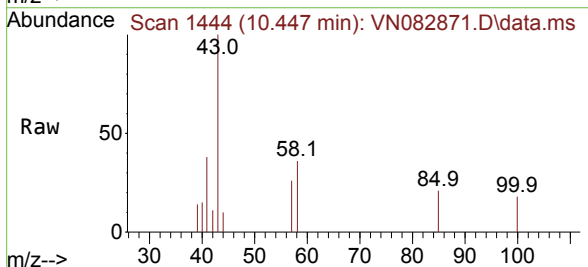


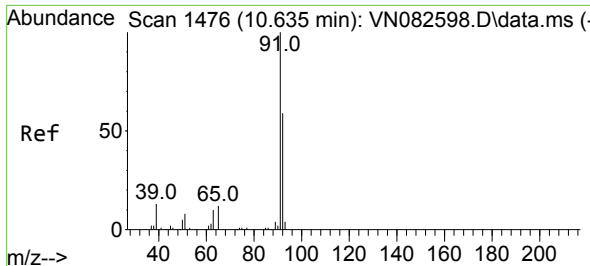

#52
Toluene
Concen: 5.284 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 92 Resp: 20610
Ion Ratio Lower Upper
92 100
91 169.9 139.4 209.0

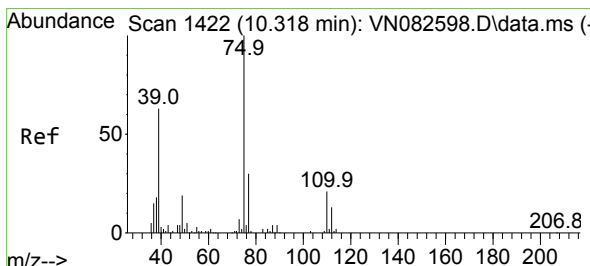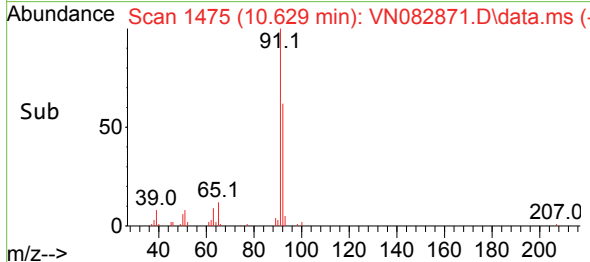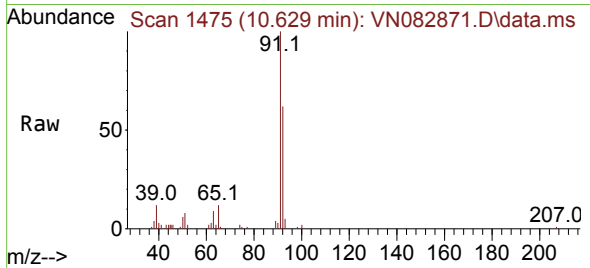

#54
cis-1,3-Dichloropropene
Concen: 8.813 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.041 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 75 Resp: 22548
Ion Ratio Lower Upper
75 100
77 0.0 24.3 36.5#
39 43.2 50.5 75.7#

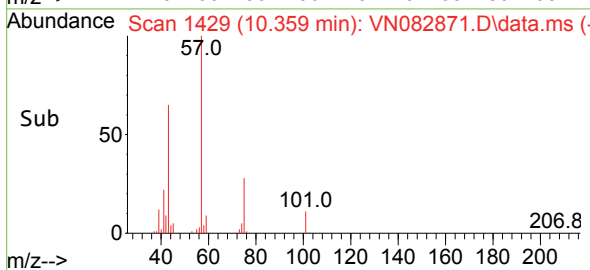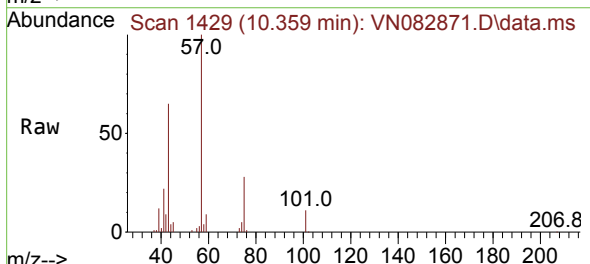

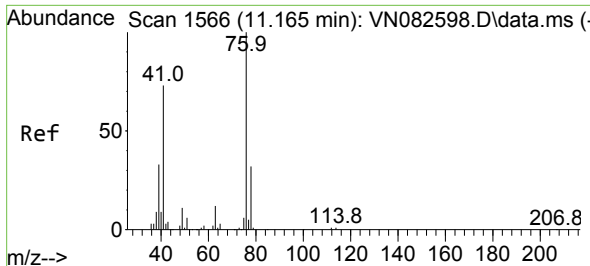

#57

1,3-Dichloropropane

Concen: 0.761 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.041 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :





COMP(00187-00189-00186)

Tgt Ion: 76 Resp: 1933

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

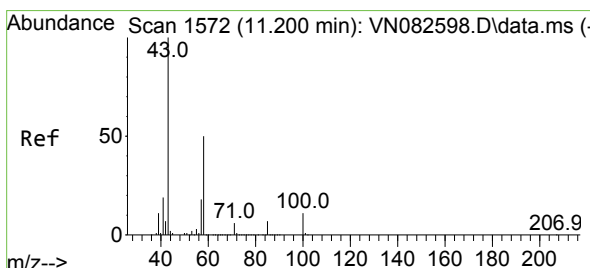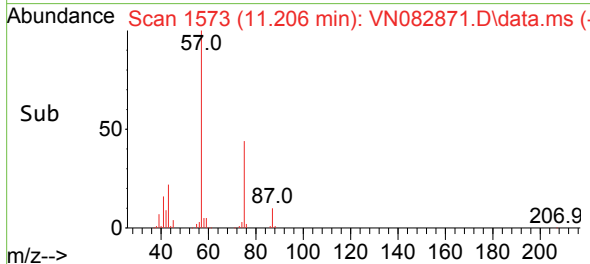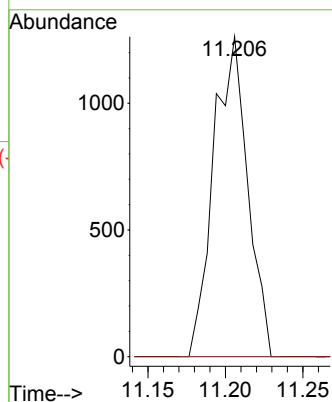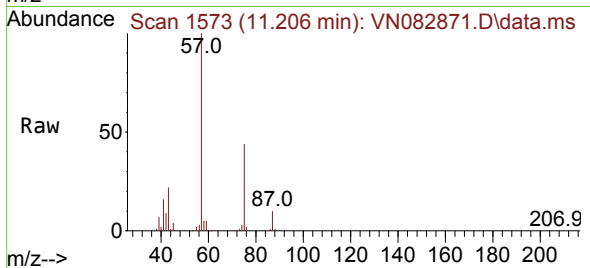

#59

2-Hexanone

Concen: 28.992 ug/l

RT: 11.171 min Scan# 1567

Delta R.T. -0.029 min

Lab File: VN082871.D




Acq: 11 Jul 2024 13:06


Tgt Ion: 43 Resp: 44158

Ion Ratio Lower Upper

43 100

58 0.0 24.6 73.8#


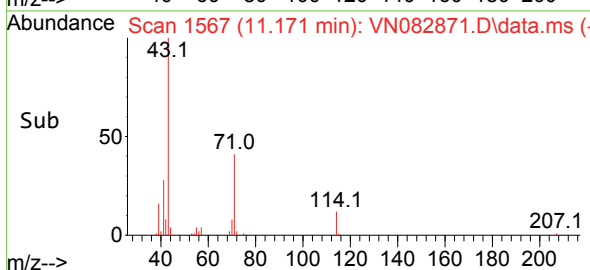

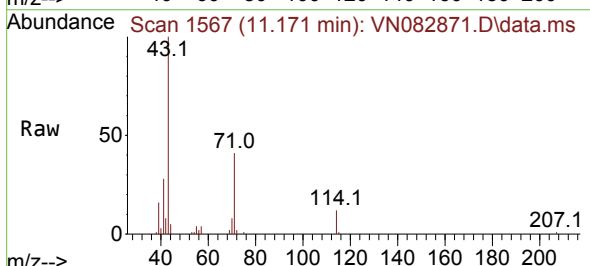




#62
4-Bromofluorobenzene
Concen: 52.679 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 95 Resp: 102891
Ion Ratio Lower Upper
95 100
174 76.6 0.0 159.2
176 72.8 0.0 147.6

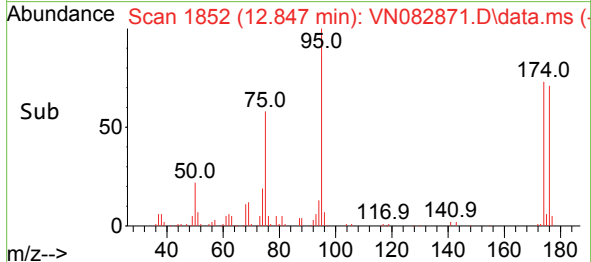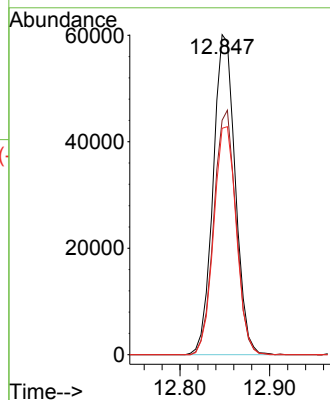

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.005 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 117 Resp: 232483
Ion Ratio Lower Upper
117 100
82 58.9 47.5 71.3
119 31.9 25.6 38.4


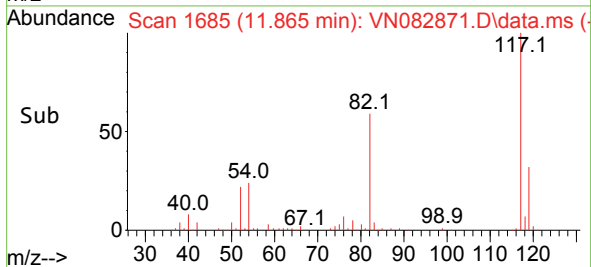
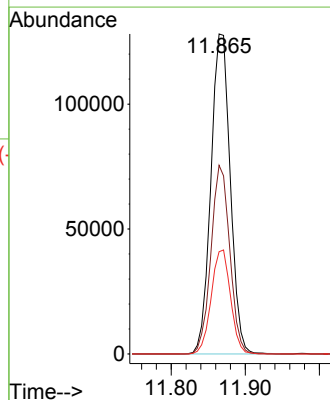
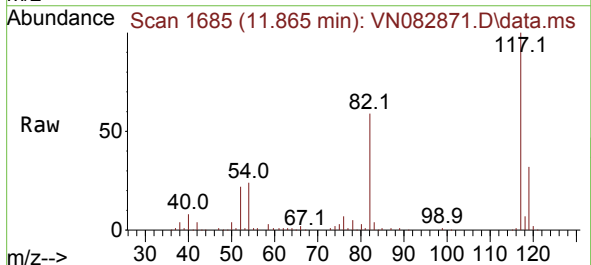




#67
Ethyl Benzene
Concen: 0.443 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.001 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 91 Resp: 3707
Ion Ratio Lower Upper
91 100
106 25.4 24.0 36.0

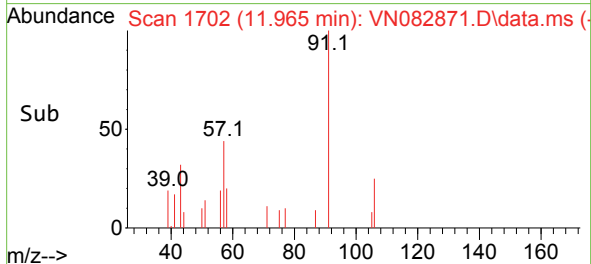

#68
m/p-Xylenes
Concen: 1.436 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.001 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 106 Resp: 4538
Ion Ratio Lower Upper
106 100
91 196.4 166.1 249.1


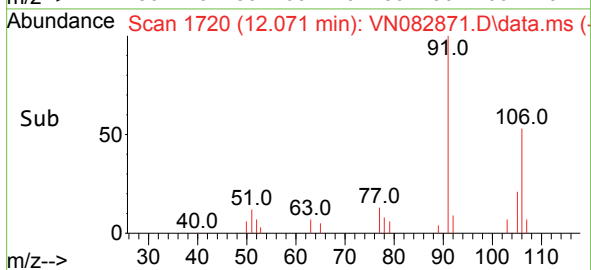

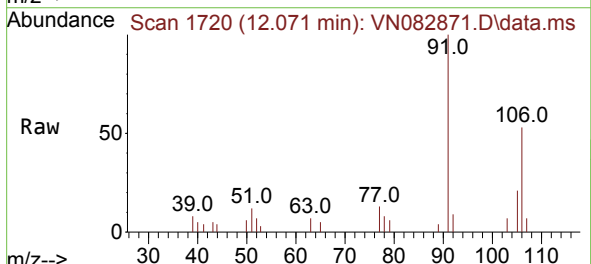




#69
o-Xylene
Concen: 0.715 ug/l
RT: 12.400 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion:106 Resp: 2166
Ion Ratio Lower Upper
106 100
91 224.7 111.3 333.9

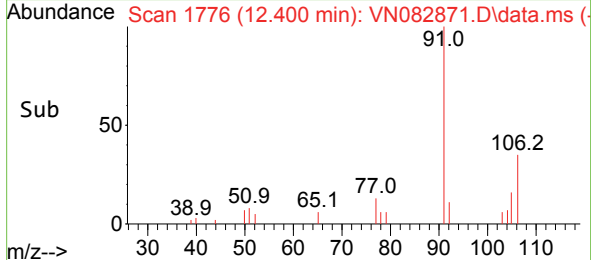

#71
Bromoform
Concen: 0.365 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.265 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion:173 Resp: 508
Ion Ratio Lower Upper
173 100
175 1016.5 24.0 72.0#
254 0.0 0.0 0.0


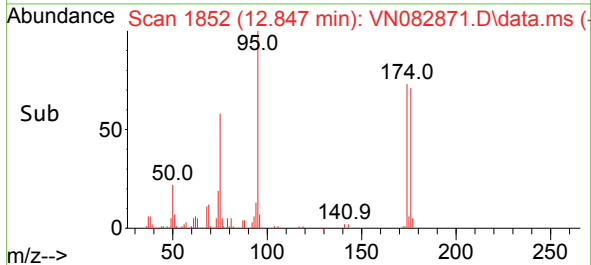

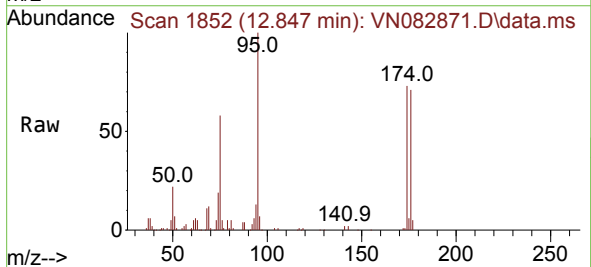


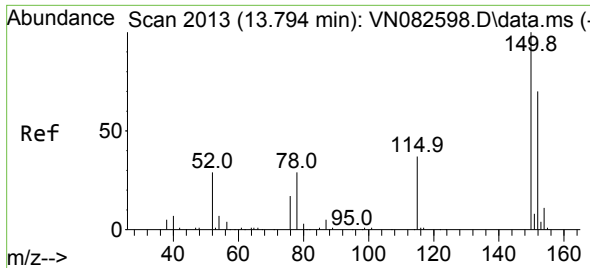

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN082871.D
 Acq: 11 Jul 2024 13:06




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP(00187-00189-00186)


Tgt Ion:152 Resp: 103996
 Ion Ratio Lower Upper
 152 100
 115 60.7 30.6 91.6
 150 158.9 0.0 348.6

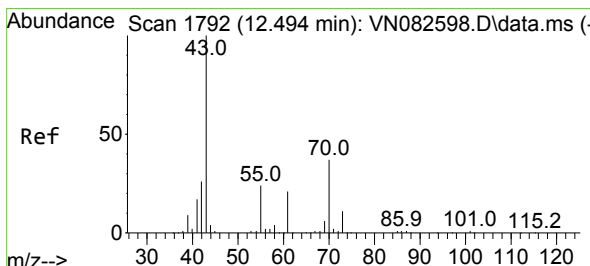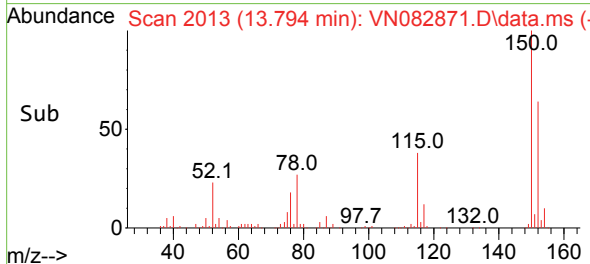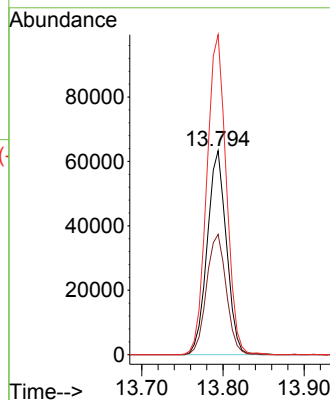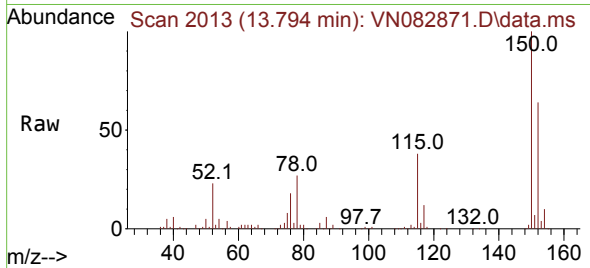

#74
 N-ethyl acetate
 Concen: 0.282 ug/l
 RT: 12.465 min Scan# 1787
 Delta R.T. -0.029 min
 Lab File: VN082871.D
 Acq: 11 Jul 2024 13:06

Tgt Ion: 43 Resp: 880
 Ion Ratio Lower Upper
 43 100
 70 0.0 29.8 44.6#
 55 0.0 18.7 28.1#
 61 0.0 17.4 26.0#


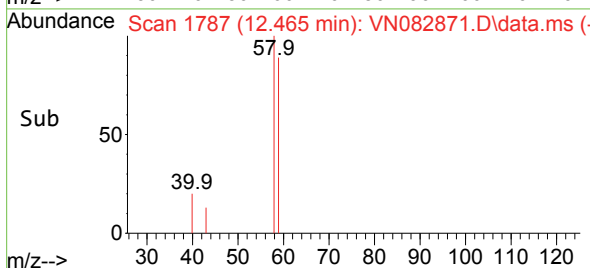
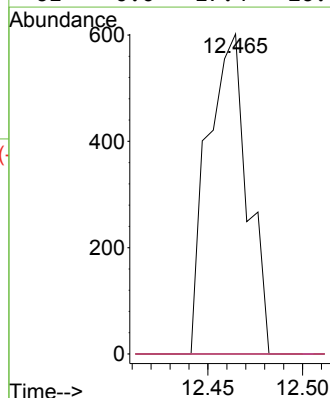
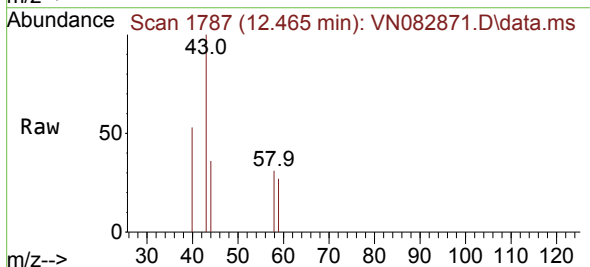




#76
1,2,3-Trichloropropane
Concen: 31.788 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06




Instrument :
MSVOA_N
ClientSampleId :
COMP(00187-00189-00186)


Tgt Ion: 75 Resp: 56994
Ion Ratio Lower Upper
75 100
77 1.1 110.9 332.6#

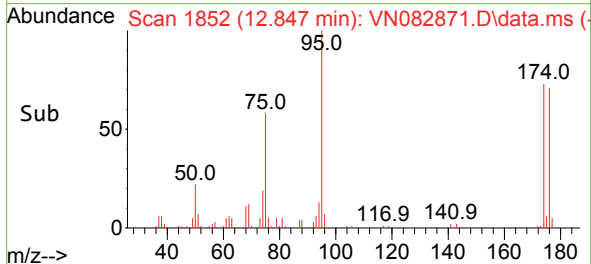

#81
trans-1,4-Dichloro-2-butene
Concen: 62.517 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.106 min
Lab File: VN082871.D
Acq: 11 Jul 2024 13:06

Tgt Ion: 75 Resp: 56994
Ion Ratio Lower Upper
75 100
53 0.0 88.4 132.6#
89 0.0 36.3 54.5#

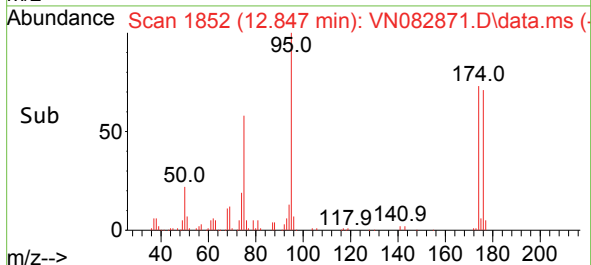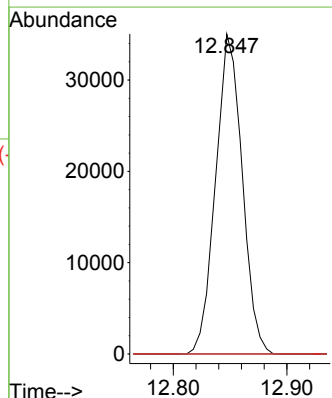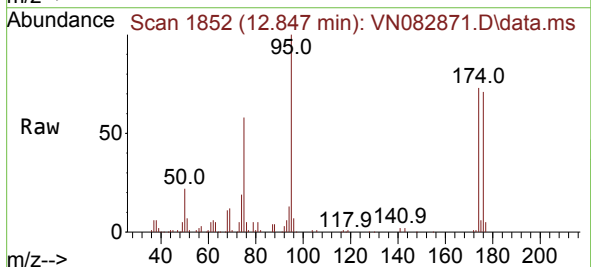



#84

1,2,4-Trimethylbenzene

Concen: 0.354 ug/l

RT: 13.476 min Scan# 1959

Delta R.T. -0.006 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Instrument :

MSVOA_N

ClientSampleId :





COMP(00187-00189-00186)

Tgt Ion:105 Resp: 2206

Ion Ratio Lower Upper

105 100

120 46.6 21.9 65.8

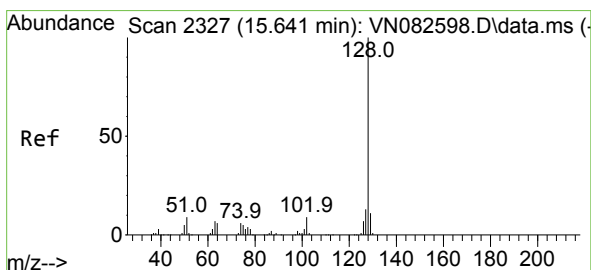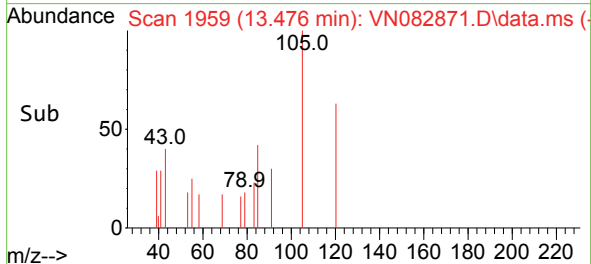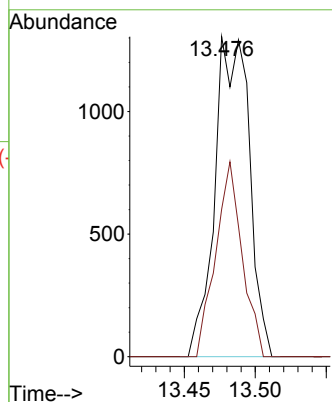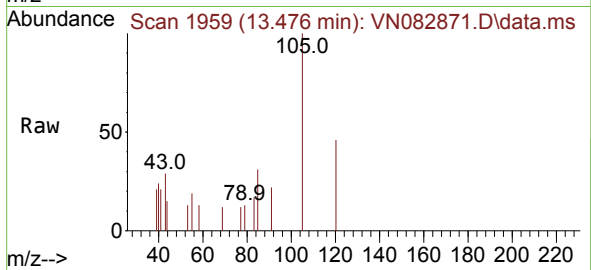

#95

Naphthalene

Concen: 1.113 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. -0.000 min

Lab File: VN082871.D

Acq: 11 Jul 2024 13:06

Tgt Ion:128 Resp: 7023

Ion Ratio Lower Upper

128 100

127 12.7 10.6 16.0

129 6.7 8.6 12.8#

