
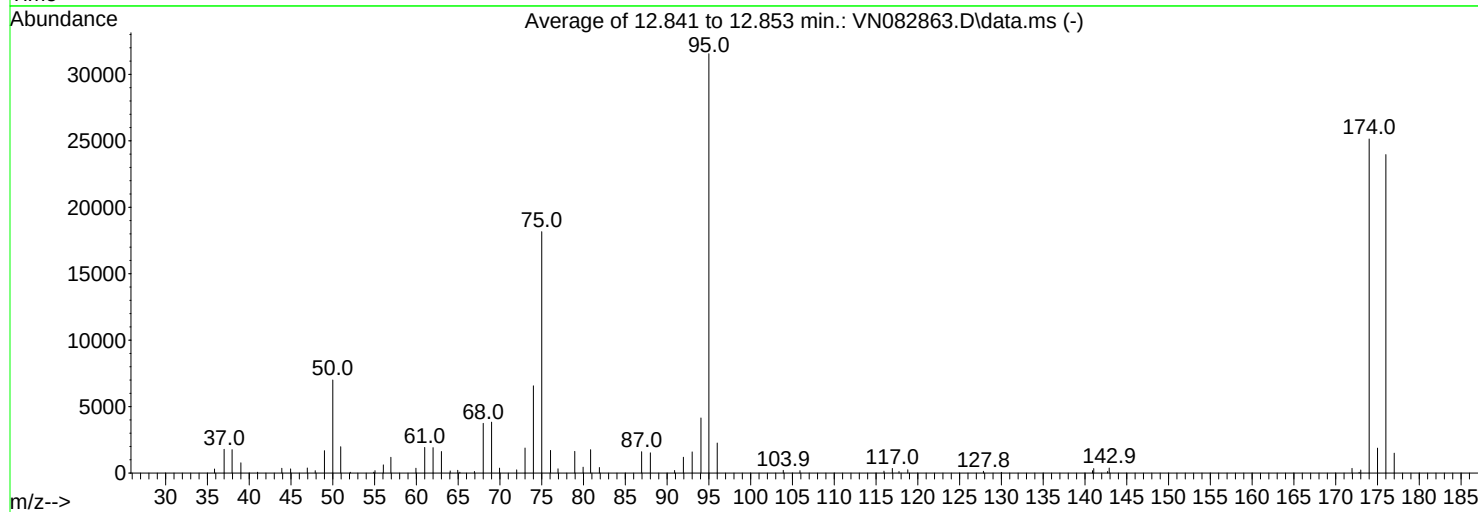


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071124\
Data File : VN082863.D
Acq On : 11 Jul 2024 09:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

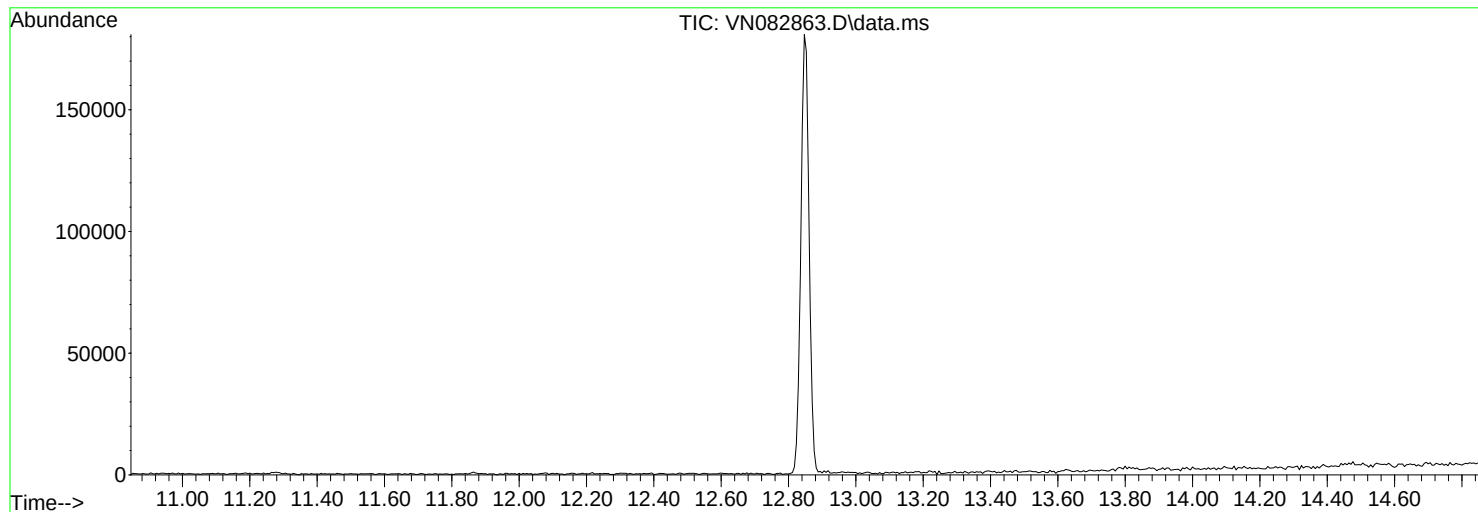

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	7002	PASS
75	95	30	60	57.6	18164	PASS
95	95	100	100	100.0	31555	PASS
96	95	5	9	7.2	2262	PASS
173	174	0.00	2	0.9	233	PASS
174	95	50	100	79.7	25141	PASS
175	174	5	9	7.5	1880	PASS
176	174	95	101	95.3	23965	PASS
177	176	5	9	6.3	1501	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	306	50.95	1982	64.95	208	76.95	320
37.00	1789	52.10	61	65.20	66	78.95	1635
37.95	1762	54.90	67	66.95	120	79.95	442
39.00	773	55.05	186	68.00	3743	80.85	1758
41.00	66	56.05	619	69.00	3835	81.90	419
43.90	363	56.95	1191	69.95	372	86.95	1608
44.95	314	59.95	367	72.00	242	88.00	1527
46.95	383	61.00	1931	73.00	1887	90.90	197
47.90	183	62.00	1916	74.00	6569	91.95	1192
49.00	1688	63.00	1622	75.00	18164	93.00	1595
50.00	7002	64.05	165	76.05	1707	94.05	4146

Average of 12.841 to 12.853 min.: VN082863.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	31555	141.05	341				
96.00	2262	142.70	115				
103.90	207	142.90	381				
105.90	187	171.95	355				
115.95	148	172.80	59				
116.95	351	173.00	233				
117.75	114	174.00	25141				
118.80	251	175.00	1880				
127.85	136	176.00	23965				
130.00	57	177.00	1501				
140.90	182						

Instrument :

MSVOA_N

ClientSampleId :

BFB