


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071218\
Data File : VN049775.D
Acq On : 12 Jul 2018 16:13
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071218W.M
Title : SW846 8260
Last Update : Thu Jul 12 15:51:38 2018

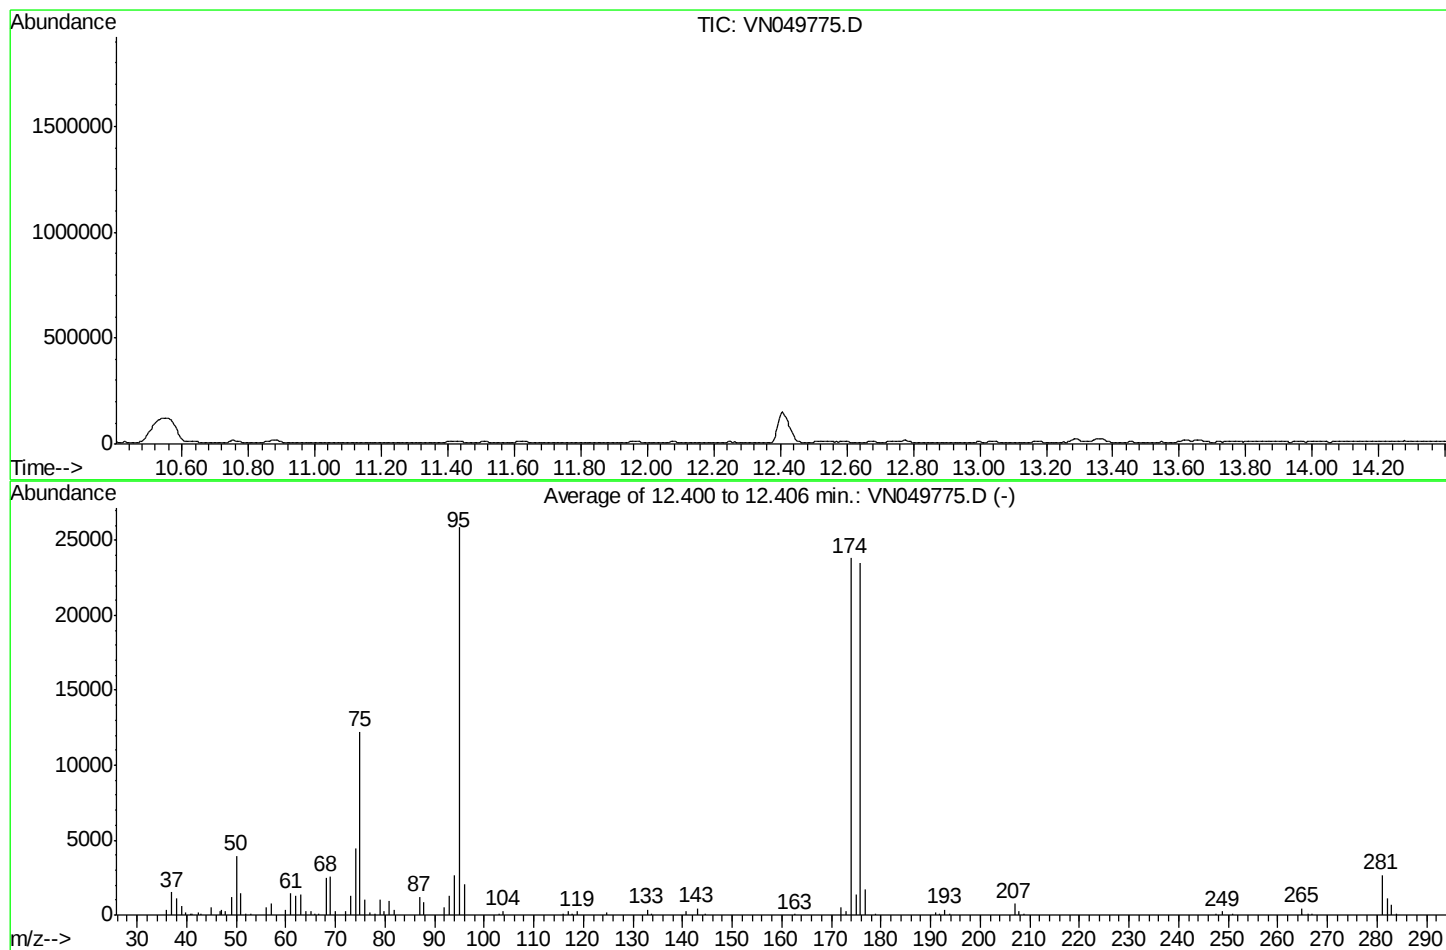

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3350

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	3969	PASS
75	95	30	60	47.2	12226	PASS
95	95	100	100	100.0	25877	PASS
96	95	5	9	7.9	2040	PASS
173	174	0.00	2	1.2	281	PASS
174	95	50	100	92.0	23800	PASS
175	174	5	9	5.7	1355	PASS
176	174	95	101	98.7	23501	PASS
177	176	5	9	7.4	1747	PASS