

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071219\
 Data File : VN056674.D
 Acq On : 11 Jul 2019 18:52
 Operator : JC/SP
 Sample : K3740-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-23

Quant Time: Jul 12 09:06:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 03:45:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	270919	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	480822	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	502075	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	184612	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	160031	53.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.60%	
35) Dibromofluoromethane	7.59	113	143903	47.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.96%	
50) Toluene-d8	10.09	98	611914	52.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.86%	
62) 4-Bromofluorobenzene	12.40	95	214245	55.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.12%	
Target Compounds						
16) Acetone	3.82	43	20317	13.505	ug/l	99
20) Methylene Chloride	4.55	84	6177	1.311	ug/l	95
43) Isopropyl Acetate	8.17	43	15483	2.414	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN071219\
Data File : VN056674.D
Acq On : 11 Jul 2019 18:52
Operator : JC/SP
Sample : K3740-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP-23

Quant Time: Jul 12 09:06:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N061919W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 03:45:40 2019
Response via : Initial Calibration

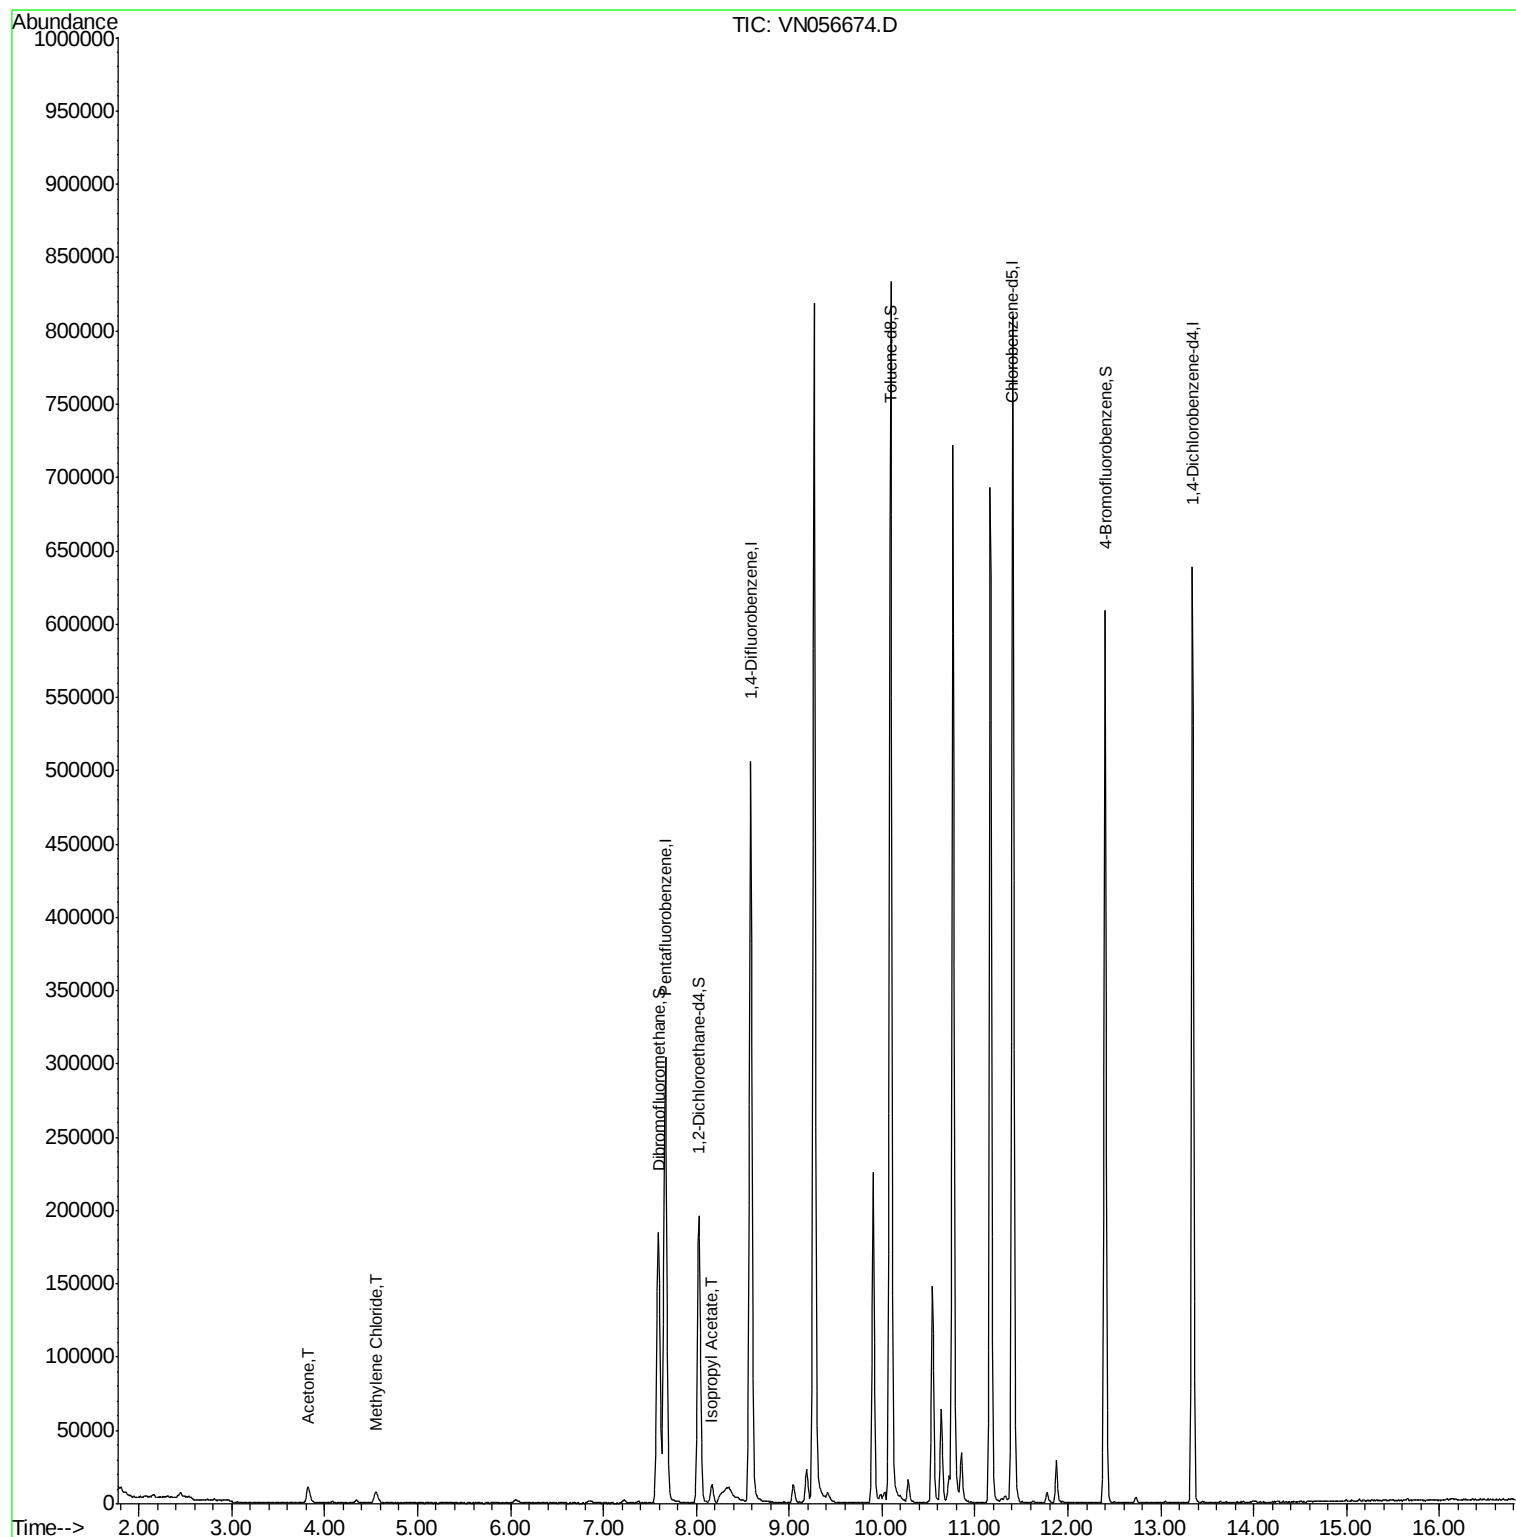

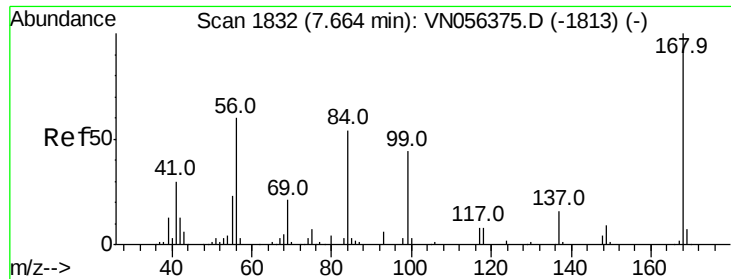

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN056674.D

Acq: 11 Jul 2019 18:52

Instrument :

MSVOA_N

ClientSampleId :


COMP-23

Tot Ion:168 Resp: 270919




Ion Ratio Lower Upper

168 100

99 49.3 40.6 61.0

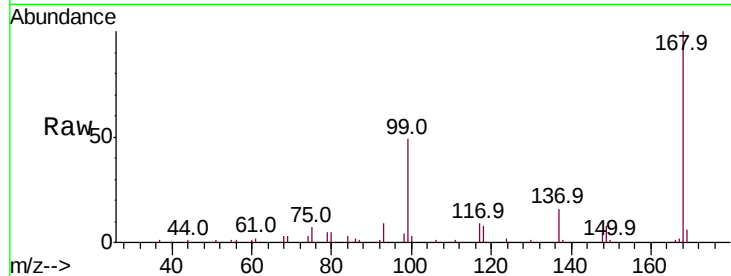

Abundance Ion 167.90 (167.60 to 168.60): VN056674.D (-1739) (-)

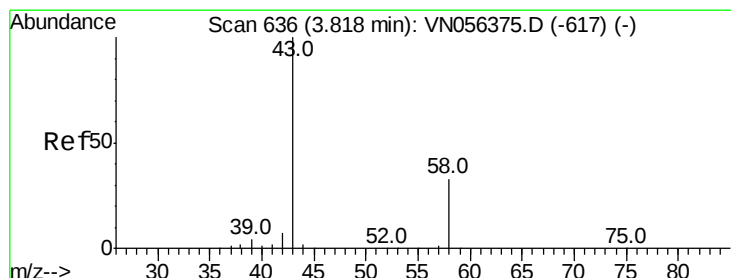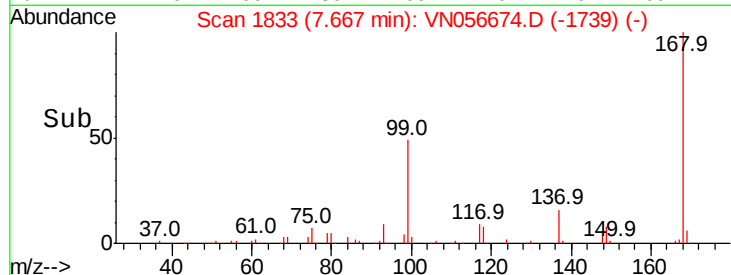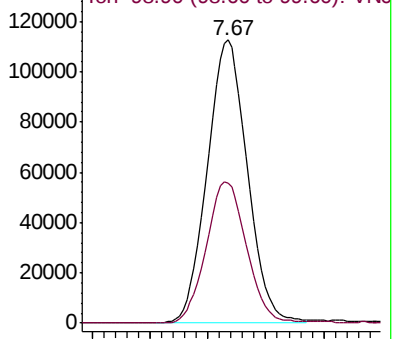

#16

Acetone

Concen: 13.505 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.00 min

Lab File: VN056674.D


Acq: 11 Jul 2019 18:52

Tgt Ion: 43 Resp: 20317



Ion Ratio Lower Upper


43 100

58 32.3 26.4 39.6

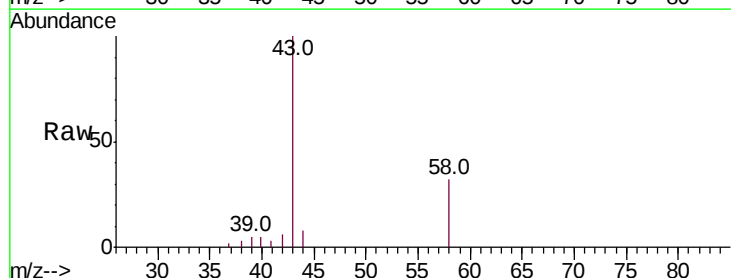

Abundance Ion 43.00 (42.70 to 43.70): VN056674.D (-543) (-)



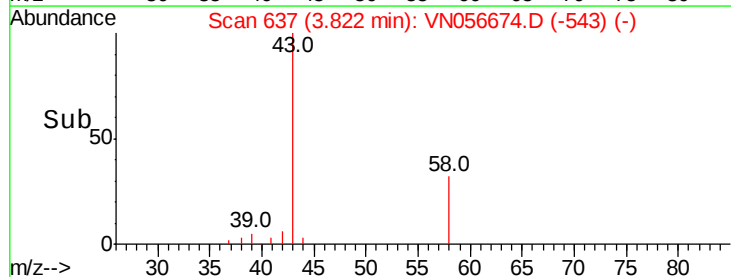
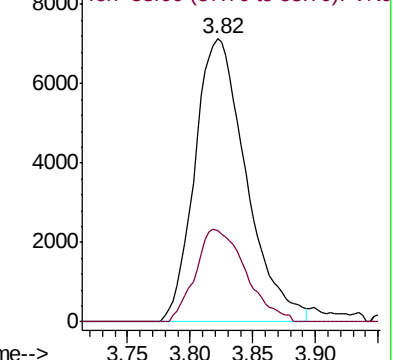


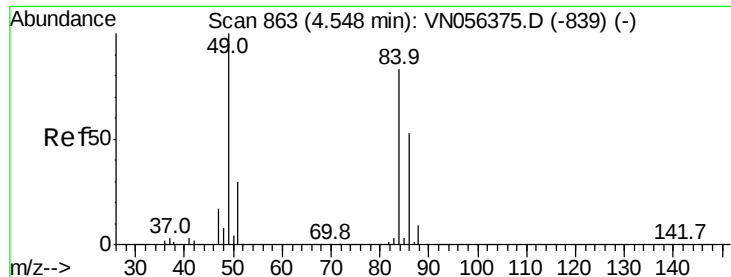

#20
Methvlene Chloride
Concen: 1.311 ug/l
RT: 4.55 min Scan# 863
Delta R.T. 0.00 min
Lab File: VN056674.D
Acq: 11 Jul 2019 18:52




Instrument :
MSVOA_N
ClientSampled :
COMP-23


Tot Ion: 84 Resp: 6177
Ion Ratio Lower Upper
84 100
49 113.0 96.4 144.6
51 40.5 28.6 43.0
86 65.2 51.4 77.2

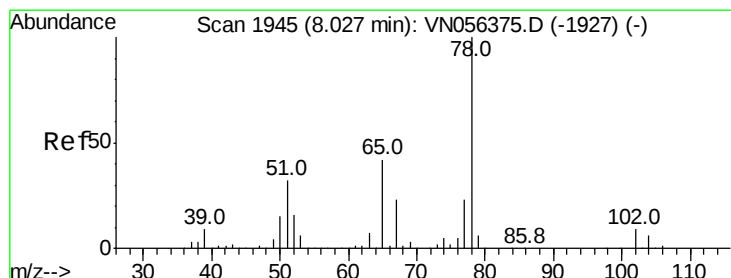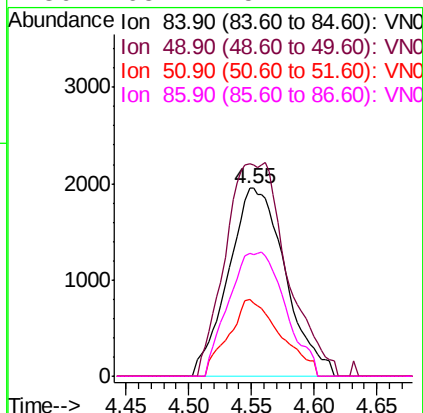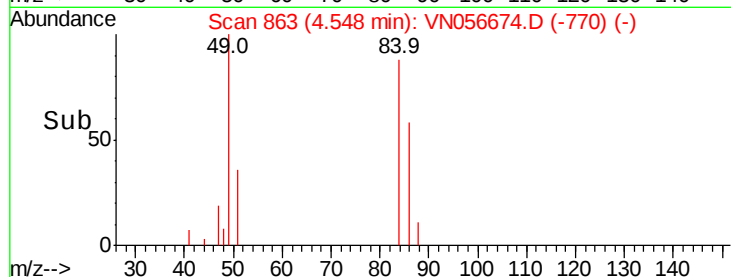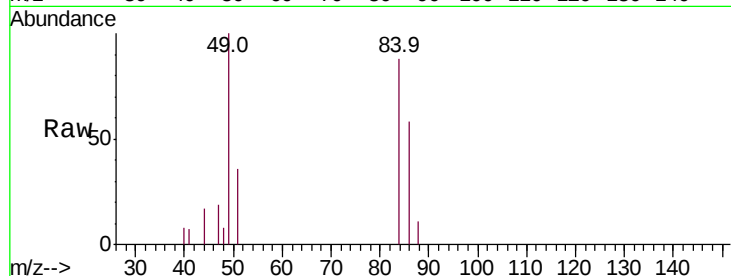

#33
1,2-Dichloroethane-d4
Concen: 53.297 ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN056674.D
Acq: 11 Jul 2019 18:52

Tgt Ion: 65 Resp: 160031
Ion Ratio Lower Upper
65 100
67 54.9 0.0 109.0

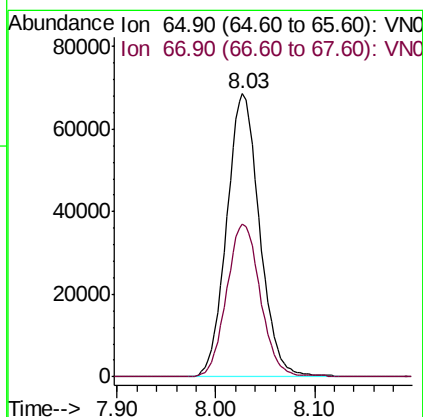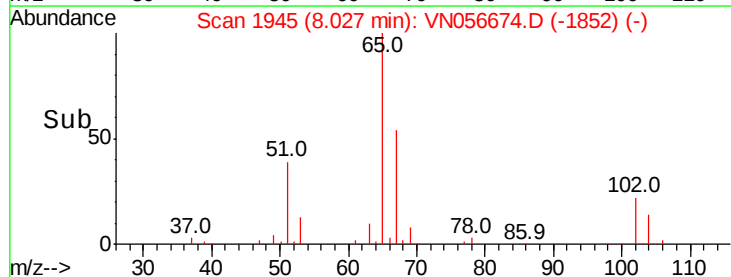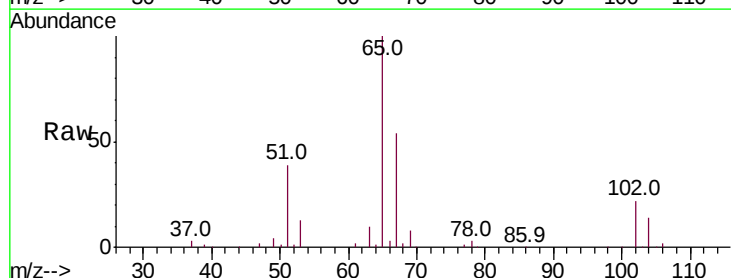


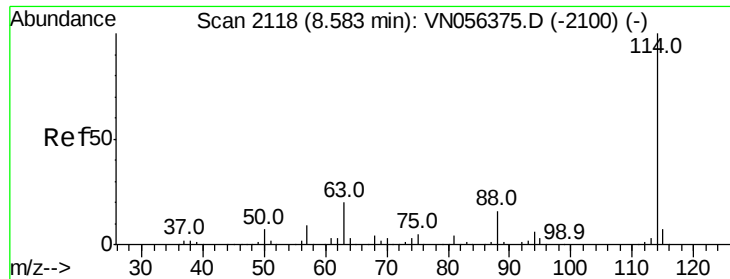




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN056674.D
 Acq: 11 Jul 2019 18:52

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-23

Tot Ion:114 Resp: 480822
 Ion Ratio Lower Upper
 114 100
 63 20.0 0.0 39.2
 88 15.6 0.0 31.4

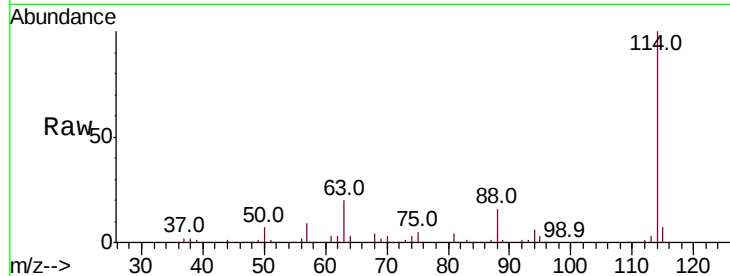


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

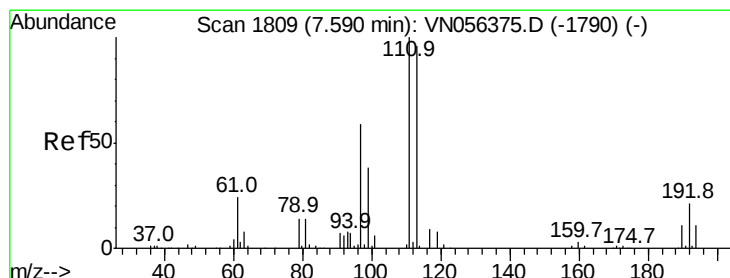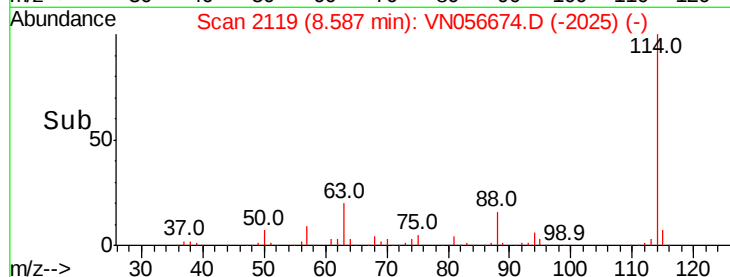
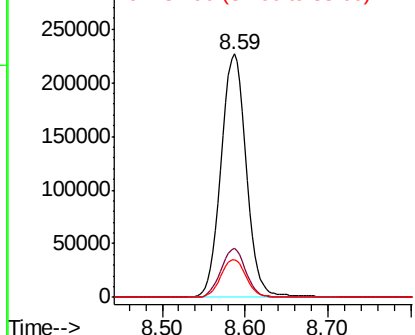



#35
 Dibromofluoromethane
 Concen: 47.975 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN056674.D
 Acq: 11 Jul 2019 18:52

Tgt Ion:113 Resp: 143903
 Ion Ratio Lower Upper
 113 100
 111 103.4 82.9 124.3
 192 22.4 17.7 26.5

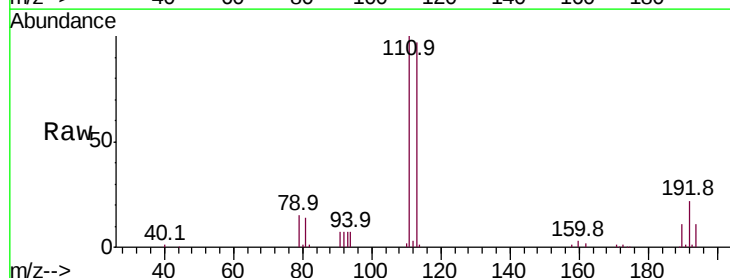

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

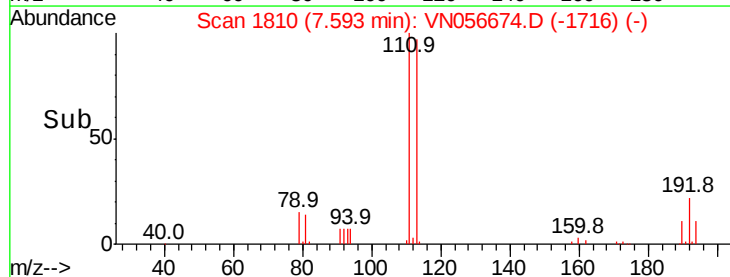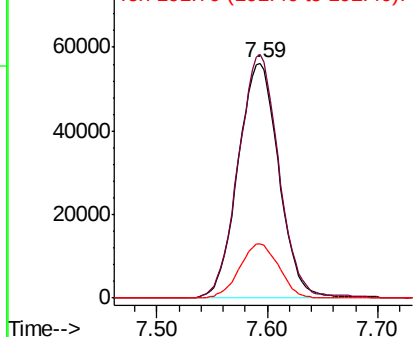

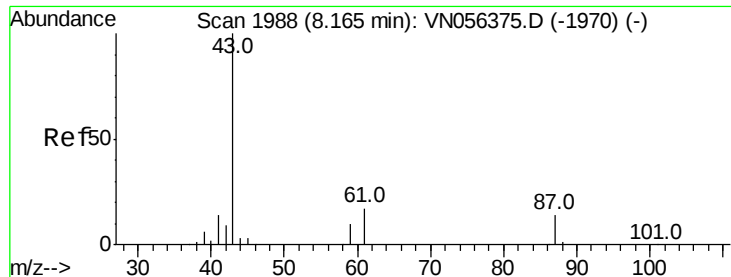

#43

Isopropyl Acetate

Concen: 2.414 ug/l

RT: 8.17 min Scan# 1988

Delta R.T. 0.00 min

Lab File: VN056674.D

Acq: 11 Jul 2019 18:52

Instrument :

MSVOA_N

ClientSampleId :

COMP-23


Tot Ion: 43 Resp: 15483

Ion Ratio Lower Upper

43 100

61 19.4 22.0 33.0#




87 12.6 11.0 16.4

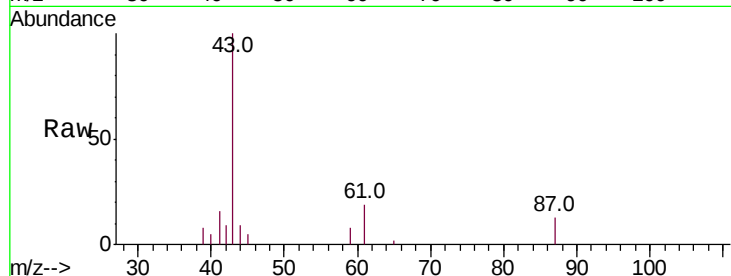

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

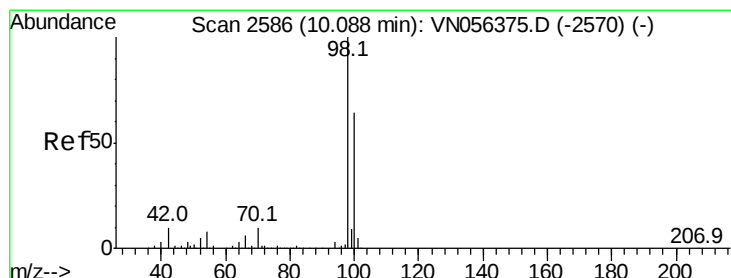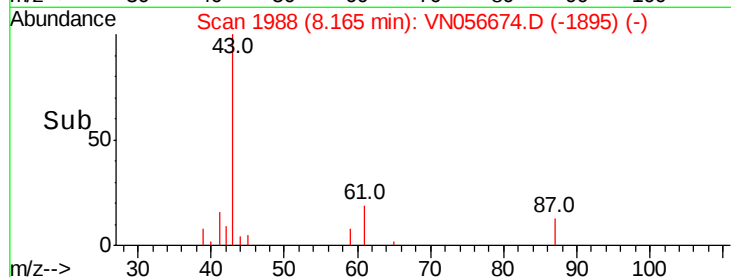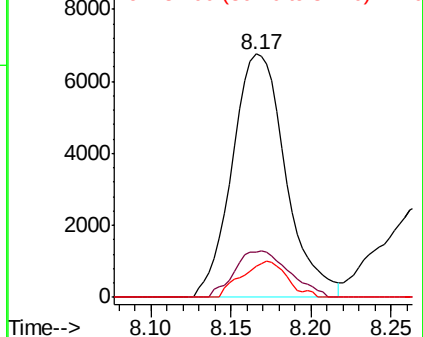

#50

Toluene-d8

Concen: 52.428 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN056674.D


Acq: 11 Jul 2019 18:52

Tgt Ion: 98 Resp: 611914

Ion Ratio Lower Upper



98 100


100 64.1 52.2 78.2

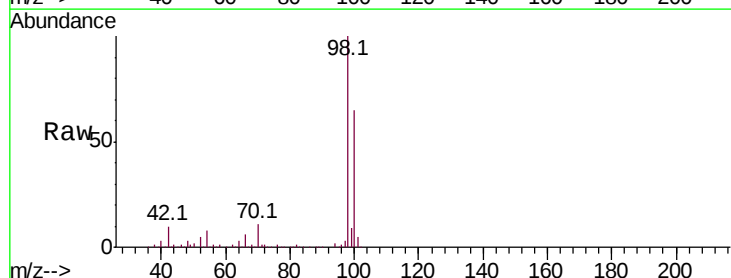

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0



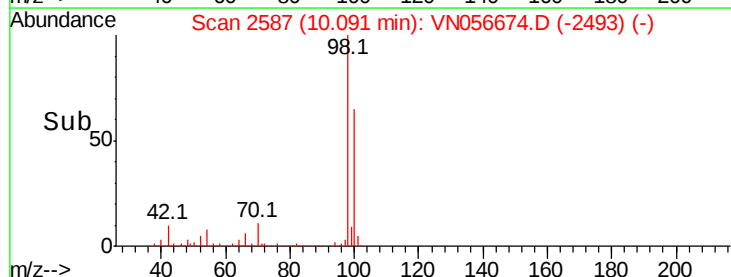
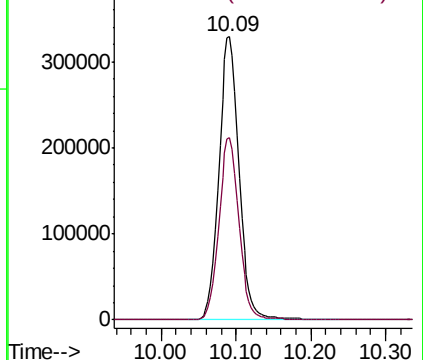


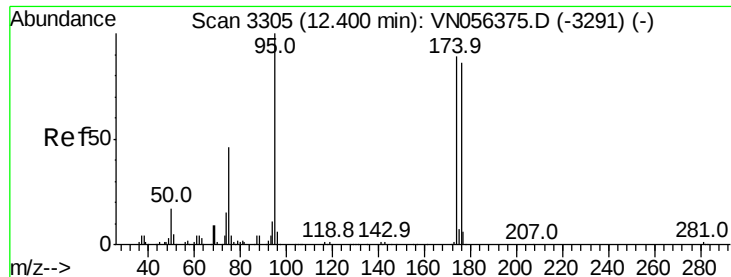

#62
4-Bromofluorobenzene
Concen: 55.065 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN056674.D
Acq: 11 Jul 2019 18:52




Instrument :
MSVOA_N
ClientSampleId :
COMP-23


Tot Ion: 95 Resp: 214245
Ion Ratio Lower Upper
95 100
174 91.0 0.0 179.4
176 87.4 0.0 173.4

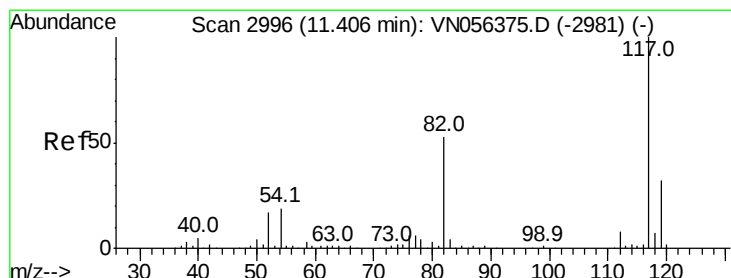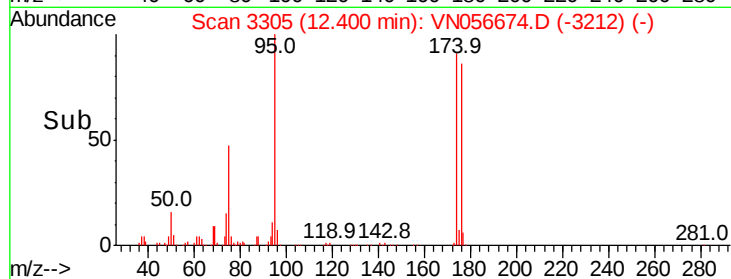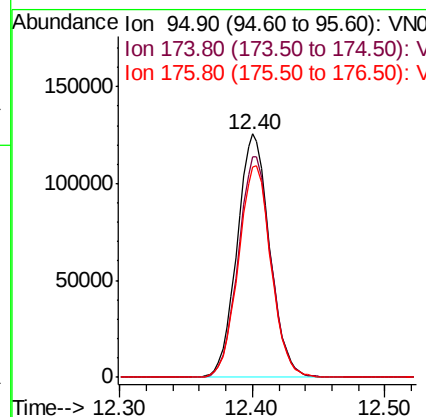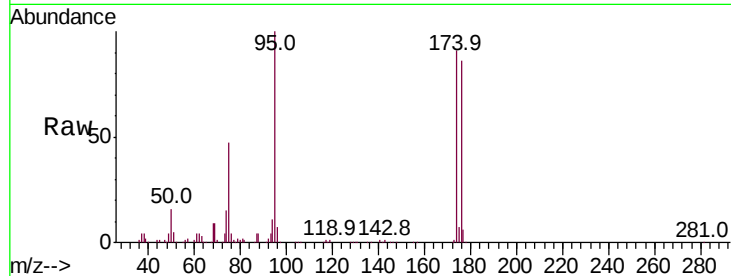

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN056674.D
Acq: 11 Jul 2019 18:52

Tgt Ion: 117 Resp: 502075
Ion Ratio Lower Upper
117 100
82 54.1 42.0 63.0
119 32.8 25.3 37.9

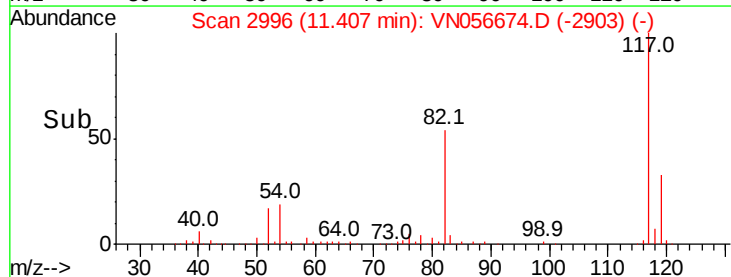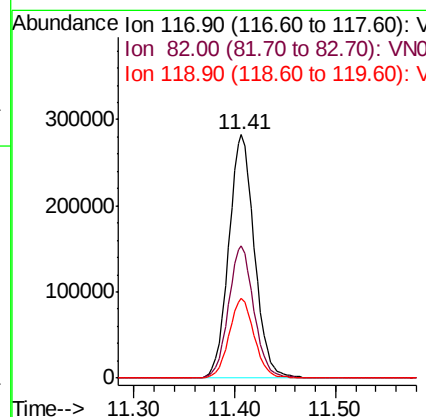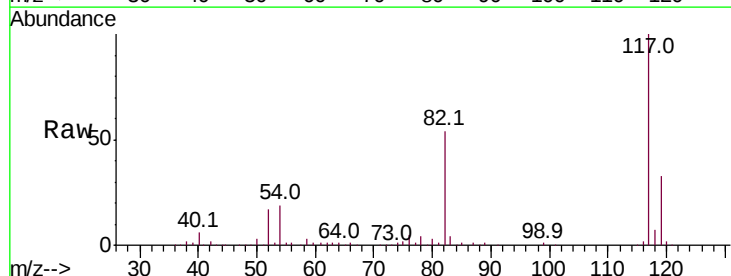

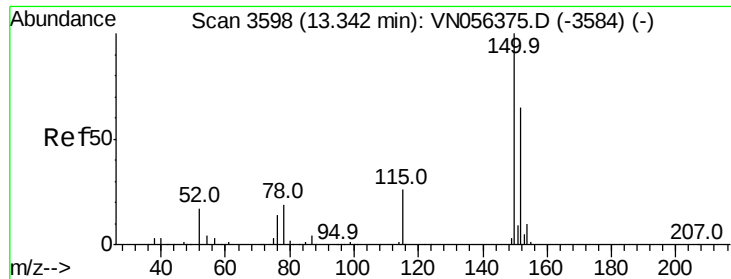

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN056674.D

Acq: 11 Jul 2019 18:52

Instrument :

MSVOA_N

ClientSampleId :

COMP-23


Tot Ion:152 Resp: 184612

Ion Ratio Lower Upper

152 100

115 55.5 28.1 84.4

150 156.1 0.0 348.4

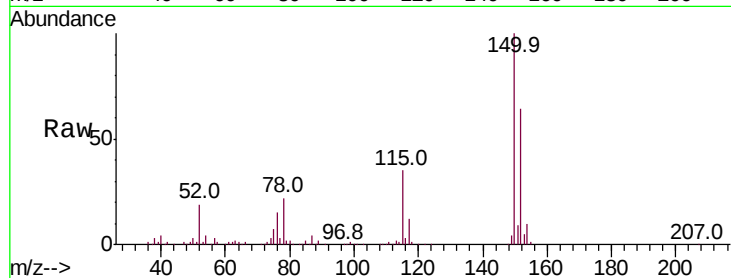

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

