
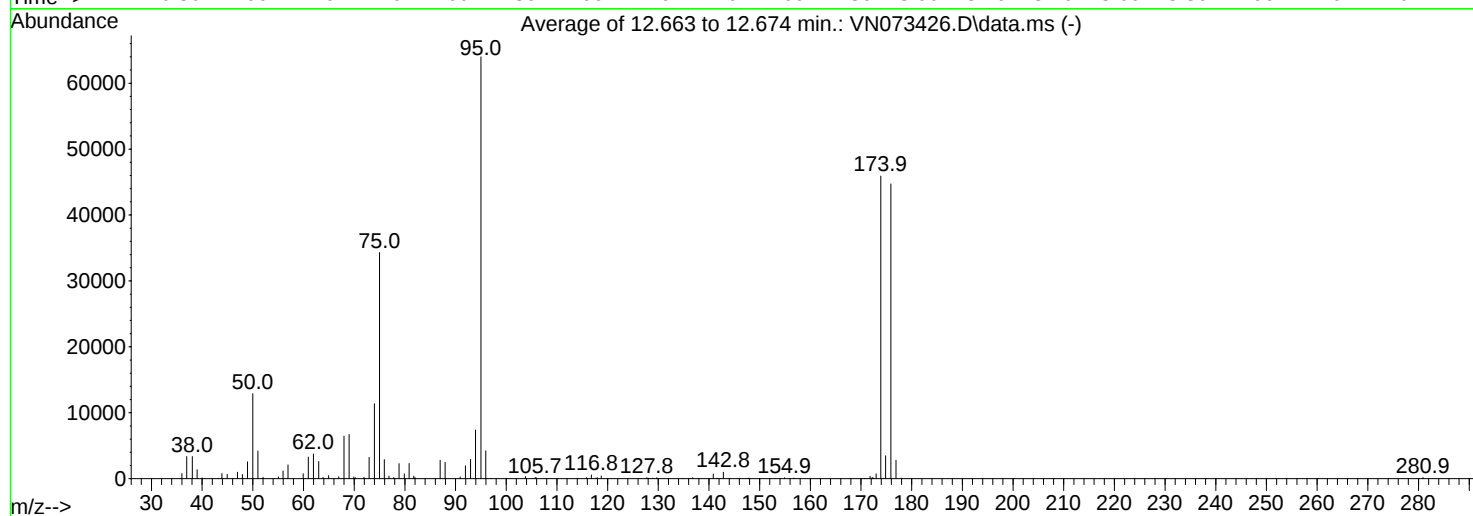


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071222\
 Data File : VN073426.D
 Acq On : 12 Jul 2022 09:24
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Title : SW846 8260
 Last Update : Wed Jun 29 01:54:03 2022

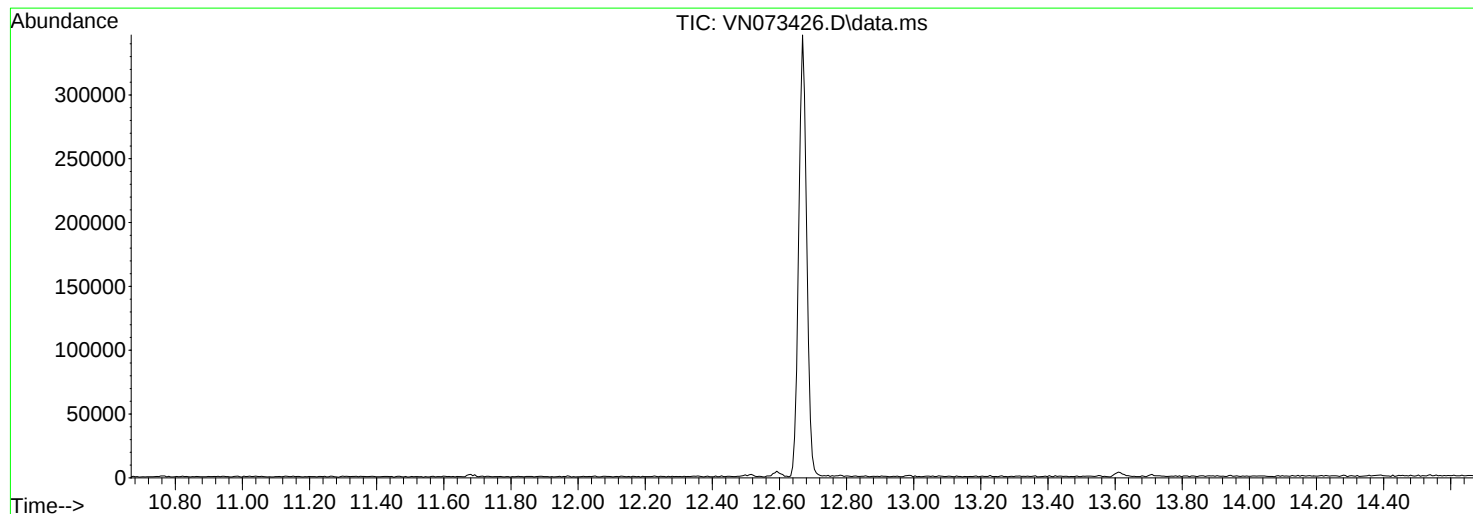

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	12882	PASS
75	95	30	60	53.6	34304	PASS
95	95	100	100	100.0	64003	PASS
96	95	5	9	6.6	4235	PASS
173	174	0.00	2	1.6	737	PASS
174	95	50	100	71.7	45901	PASS
175	174	5	9	7.6	3474	PASS
176	174	95	101	97.4	44720	PASS
177	176	5	9	6.3	2806	PASS