

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
 Data File : VN078484.D
 Acq On : 12 Jul 2023 17:33
 Operator : JC\MD
 Sample : 03585-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 50057

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Title : SW846 8260

Signal : TIC: VN078483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.518	90	96	103	rVB2	26586	45478	2.06%	0.313%
2	2.824	143	148	157	rVB3	26722	56462	2.55%	0.388%
3	3.247	216	220	228	rVB6	16665	36297	1.64%	0.249%
4	4.447	413	424	446	rBV	114205	360588	16.31%	2.478%
5	4.736	461	473	475	rBV3	14813	35958	1.63%	0.247%
6	5.812	641	656	668	rBV5	23590	83350	3.77%	0.573%
7	8.177	1047	1058	1062	rBV2	376093	881272	39.86%	6.056%
8	8.235	1062	1068	1082	rVB	575593	1309257	59.21%	8.997%
9	8.588	1115	1128	1139	rBV	349058	827892	37.44%	5.689%
10	9.112	1206	1217	1229	rBV	815445	1702162	76.99%	11.697%
11	10.576	1458	1466	1472	rBV	1163609	2211030	100.00%	15.194%
12	10.635	1472	1476	1485	rVV	155396	308150	13.94%	2.118%
13	11.200	1561	1572	1578	rBV6	10050	27187	1.23%	0.187%
14	11.870	1678	1686	1698	rBV	1113160	2041119	92.32%	14.027%
15	11.970	1698	1703	1709	rVB4	26204	45706	2.07%	0.314%
16	12.076	1715	1721	1730	rVB	46569	93573	4.23%	0.643%
17	12.406	1769	1777	1785	rBV3	68228	130714	5.91%	0.898%
18	12.853	1846	1853	1865	rBV	834041	1499880	67.84%	10.307%
19	13.135	1898	1901	1904	rVV5	17735	28326	1.28%	0.195%
20	13.176	1904	1908	1913	rVV5	25560	41924	1.90%	0.288%
21	13.488	1957	1961	1970	rVB2	27424	45010	2.04%	0.309%
22	13.735	1997	2003	2007	rBV3	20928	34261	1.55%	0.235%
23	13.800	2007	2014	2022	rVV	901005	1592861	72.04%	10.946%
24	13.876	2022	2027	2034	rVB2	24002	45731	2.07%	0.314%
25	14.006	2043	2049	2055	rBV8	14845	41529	1.88%	0.285%
26	14.059	2055	2058	2063	rVV3	17027	25834	1.17%	0.178%
27	14.111	2063	2067	2072	rVB7	19397	32949	1.49%	0.226%
28	14.335	2101	2105	2111	rVB3	16995	29207	1.32%	0.201%
29	14.964	2209	2212	2217	rVB7	17356	28794	1.30%	0.198%
30	15.041	2220	2225	2233	rBV6	40880	122214	5.53%	0.840%
31	15.123	2235	2239	2245	rVB3	36696	68093	3.08%	0.468%
32	15.217	2251	2255	2260	rVB8	14048	24382	1.10%	0.168%
33	15.329	2268	2274	2281	rBV7	32817	76326	3.45%	0.525%
34	15.400	2281	2286	2289	rBV6	16321	28387	1.28%	0.195%
35	15.511	2300	2305	2313	rVB6	26727	53002	2.40%	0.364%
36	15.594	2315	2319	2323	rBV7	21110	42195	1.91%	0.290%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
Data File : VN078484.D
Acq On : 12 Jul 2023 17:33
Operator : JC\MD
Sample : 03585-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50057

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M

Title : SW846 8260

37	15.647	2323	2328	2334	rVB	28695	52719	2.38%	0.362%
38	15.776	2345	2350	2356	rBV7	18458	43032	1.95%	0.296%
39	15.841	2356	2361	2371	rVB6	49549	114364	5.17%	0.786%
40	15.953	2373	2380	2386	rBV10	21041	57640	2.61%	0.396%
41	16.323	2438	2443	2445	rBV5	18390	30467	1.38%	0.209%
42	16.500	2464	2473	2479	rBV5	31790	95185	4.31%	0.654%
43	16.617	2488	2493	2499	rVB4	25123	44625	2.02%	0.307%
44	16.723	2506	2511	2515	rVB5	30135	56638	2.56%	0.389%




Sum of corrected areas: 14551770

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
Data File : VN078484.D
Acq On : 12 Jul 2023 17:33
Operator : JC\MD
Sample : 03585-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

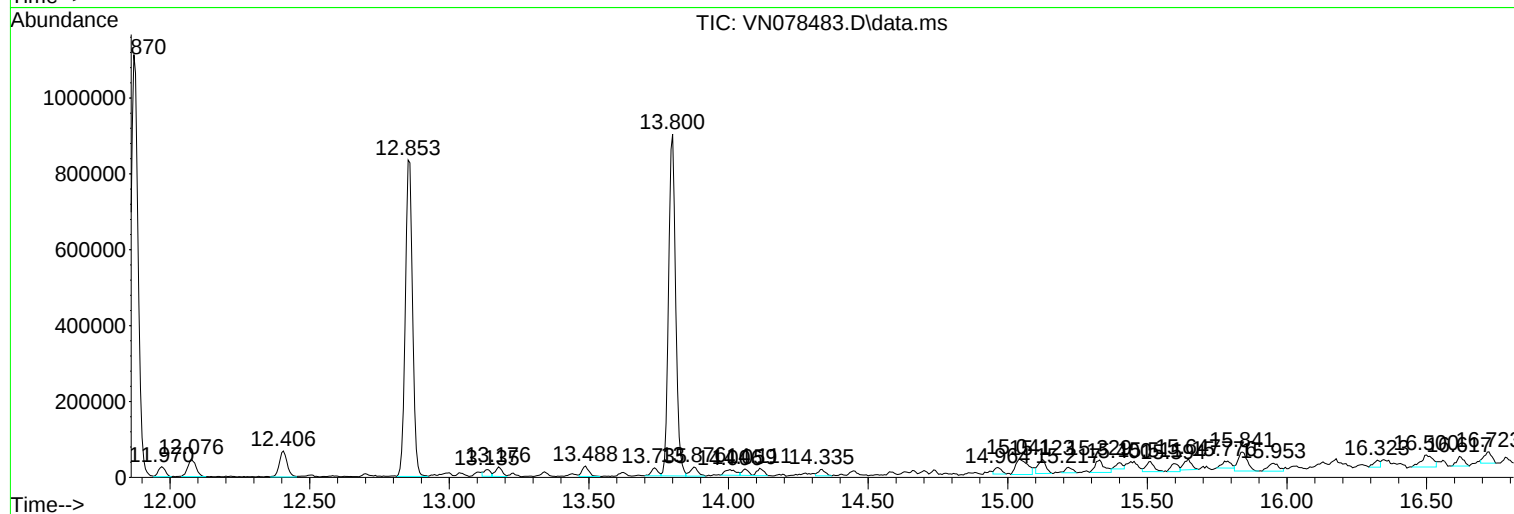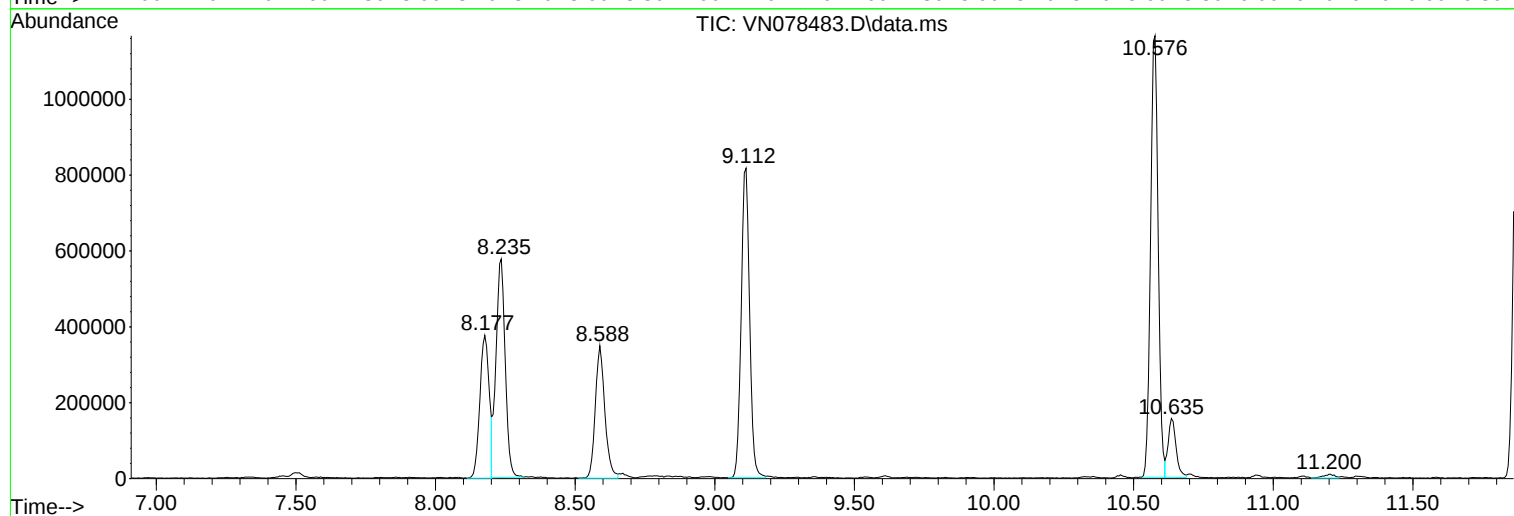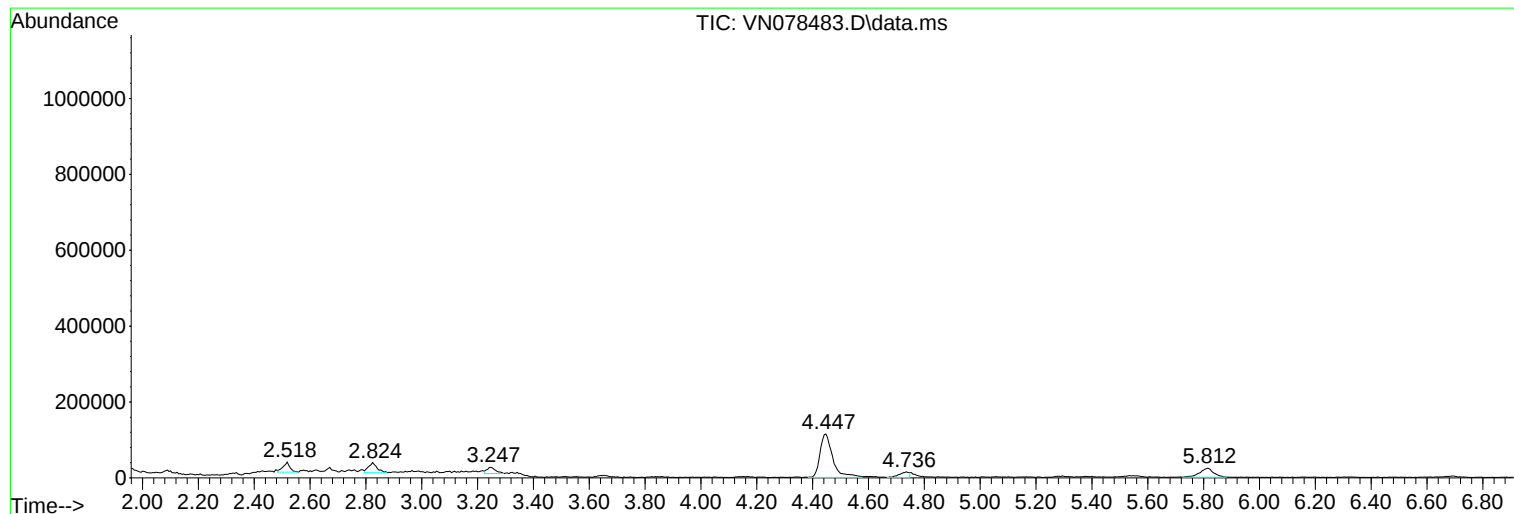

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
Data File : VN078484.D
Acq On : 12 Jul 2023 17:33
Operator : JC\MD
Sample : 03585-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
Data File : VN078484.D
Acq On : 12 Jul 2023 17:33
Operator : JC\MD
Sample : 03585-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
50057

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc