
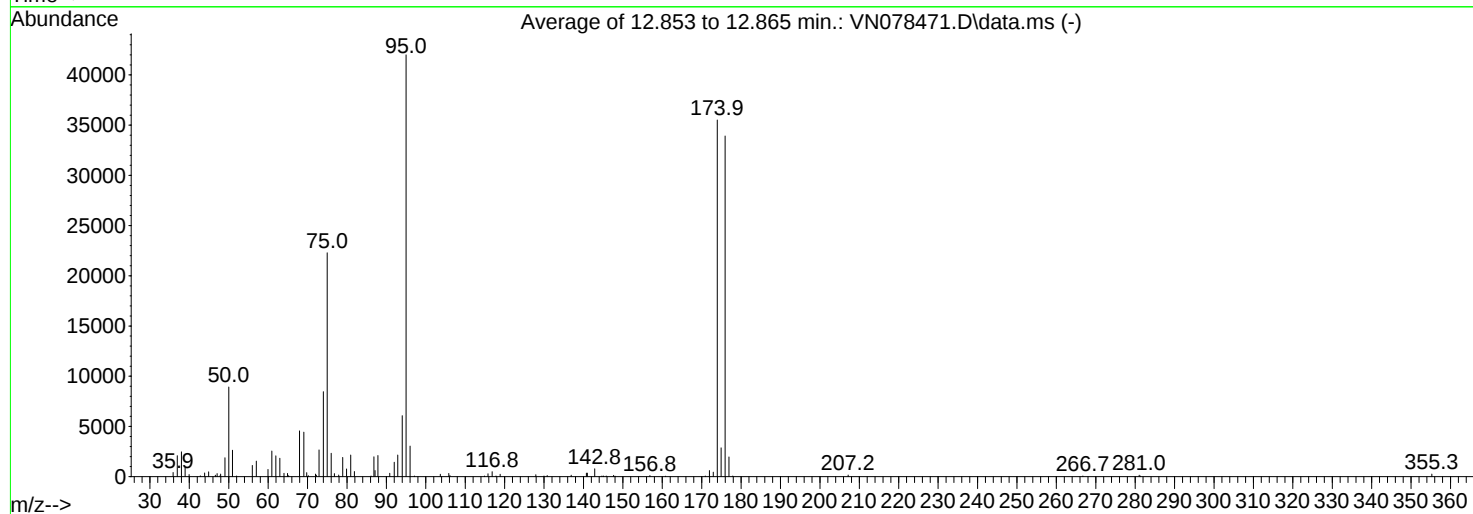


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071223\
Data File : VN078471.D
Acq On : 12 Jul 2023 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

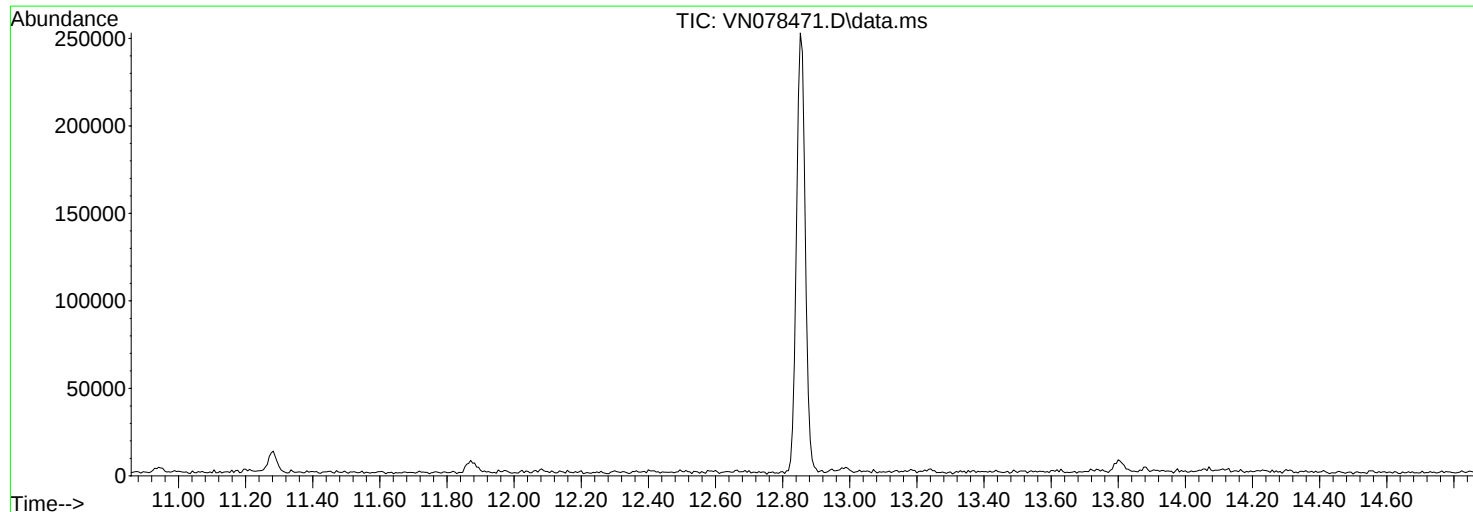

AutoFind: Scans 1853, 1854, 1855; Background Corrected with Scan 1845

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	8929	PASS
75	95	30	60	53.1	22288	PASS
95	95	100	100	100.0	42003	PASS
96	95	5	9	7.2	3039	PASS
173	174	0.00	2	1.2	440	PASS
174	95	50	100	84.6	35520	PASS
175	174	5	9	8.1	2865	PASS
176	174	95	101	95.5	33923	PASS
177	176	5	9	5.8	1968	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	419	47.95	261	64.00	340	75.00	2228
36.95	2083	49.05	1875	64.90	325	76.00	232
38.00	2476	50.00	8929	65.20	101	76.80	30
38.95	874	50.95	2623	67.95	4562	77.90	16
39.95	211	52.00	63	69.05	4428	78.90	1912
42.80	78	56.00	1116	69.80	404	79.90	758
43.90	374	57.00	1551	70.20	100	80.95	2149
44.90	486	59.95	711	72.00	256	81.90	511
46.60	137	60.95	2547	72.20	140	86.10	73
47.05	307	61.95	2064	72.90	2655	86.85	1982
47.80	84	62.95	1832	74.00	8456	87.10	610

Average of 12.853 to 12.865 min.: VN078471.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.85	2109	114.90	68	142.85	786	173.95	35520
90.85	343	115.80	288	144.70	61	174.95	2865
92.00	1443	116.85	495	145.10	62	175.95	33923
92.90	2144	117.80	68	145.80	72	176.90	1968
94.00	6074	118.85	237	147.65	125	177.90	65
95.00	42003	127.90	190	148.00	56	207.15	161
96.00	3039	130.00	72	156.85	106	266.70	58
97.10	59	130.80	109	160.80	51	281.00	143
103.70	233	136.90	140	170.90	63	281.30	65
105.85	327	140.75	358	171.95	607	355.25	253
106.10	108	141.00	354	172.95	440		

Instrument :

MSVOA_N

ClientSampleId :

BFB