
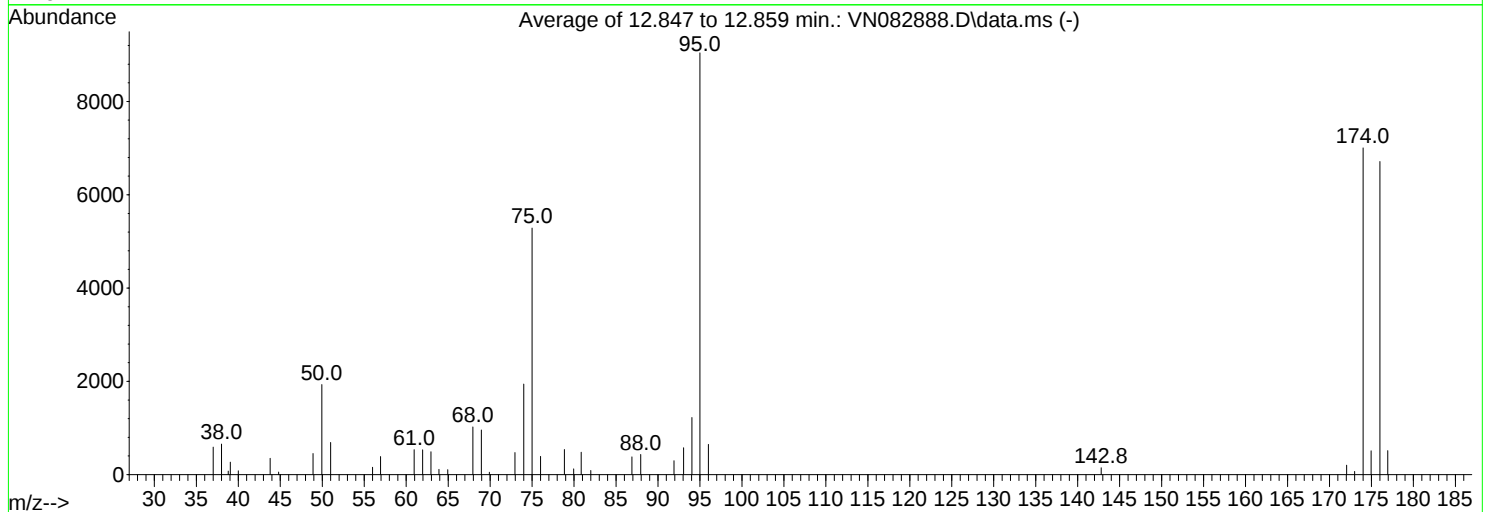


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071224\
Data File : VN082888.D
Acq On : 12 Jul 2024 10:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

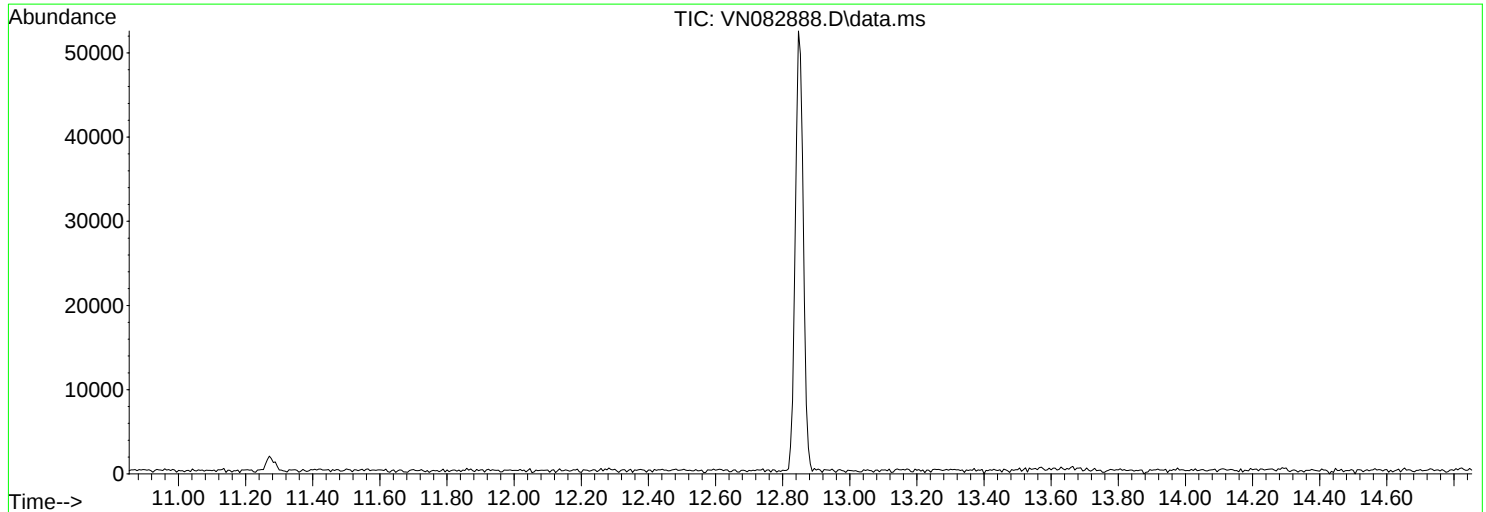

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	1931	PASS
75	95	30	60	58.5	5287	PASS
95	95	100	100	100.0	9043	PASS
96	95	5	9	7.2	649	PASS
173	174	0.00	2	1.0	69	PASS
174	95	50	100	77.5	7005	PASS
175	174	5	9	7.3	510	PASS
176	174	95	101	95.8	6714	PASS
177	176	5	9	7.7	515	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.00	590	56.95	387	75.00	5287	95.00	904
38.00	656	60.95	535	76.00	391	96.00	64
38.80	76	61.95	533	78.85	539	142.80	14
39.05	266	62.95	492	79.95	122	172.05	20
40.00	83	63.90	114	80.85	479	173.00	69
43.80	351	64.95	106	82.00	88	174.00	7005
44.80	56	67.95	1023	86.90	382	174.95	510
48.90	453	68.95	956	87.95	433	176.00	6714
49.95	1931	69.90	51	91.90	299	176.95	515
51.00	690	72.95	472	93.05	577		
56.00	158	74.00	1940	94.05	1226		

Instrument :

MSVOA_N

ClientSampleId :

BFB