


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071318\  
Data File : VN049812.D  
Acq On : 13 Jul 2018 22:12  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N071218W.M  
Title : SW846 8260  
Last Update : Thu Jul 12 15:51:38 2018

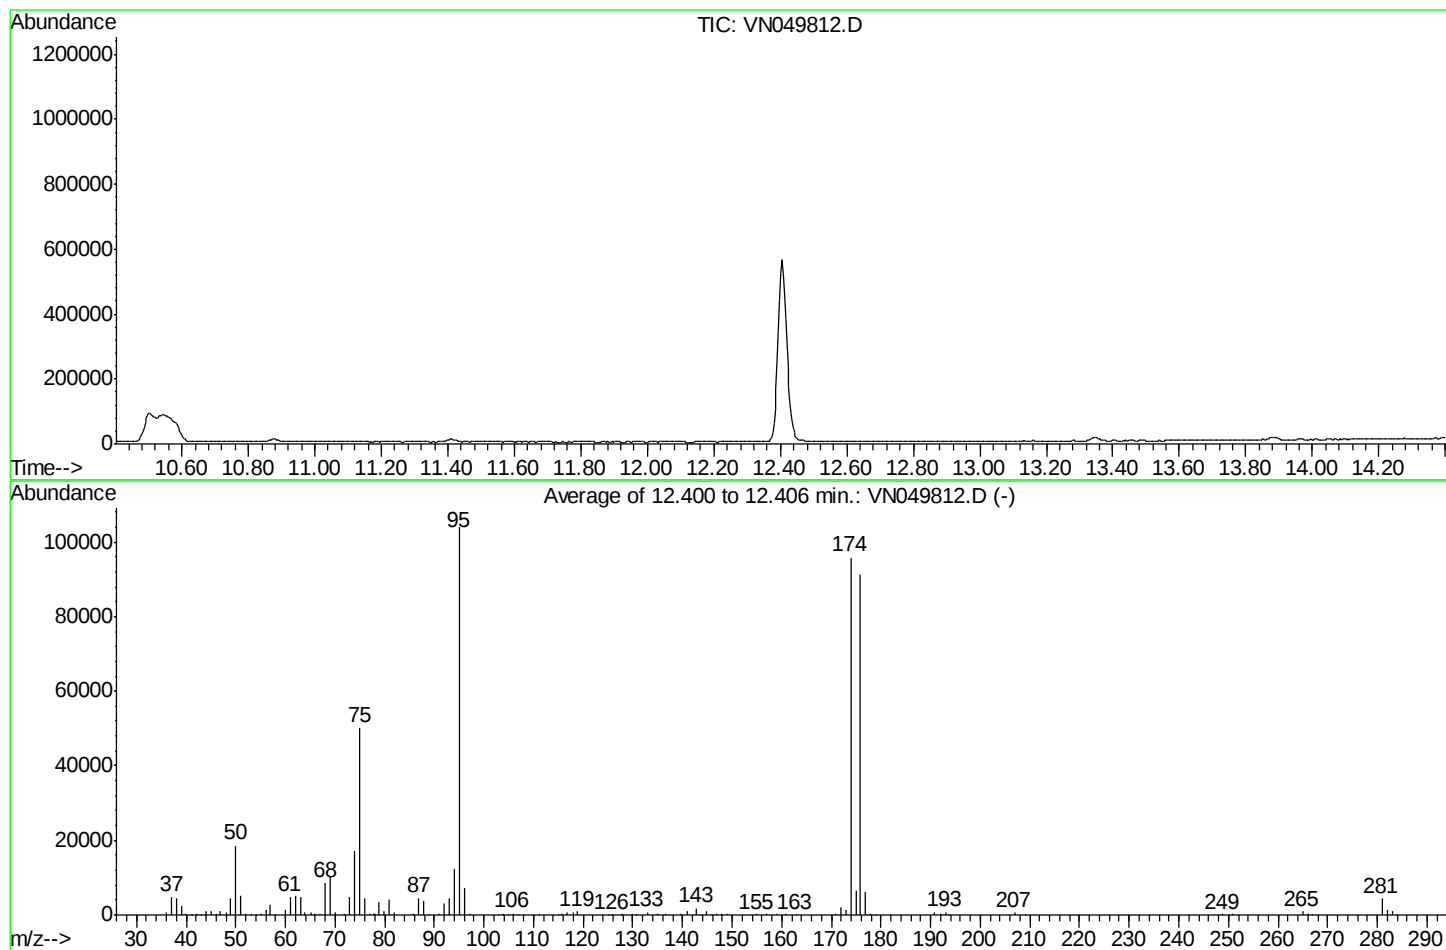

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.9      | 18592   | PASS             |
| 75          | 95           | 30           | 60           | 48.3      | 50144   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 103920  | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 7284    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.6       | 1505    | PASS             |
| 174         | 95           | 50           | 100          | 92.2      | 95802   | PASS             |
| 175         | 174          | 5            | 9            | 6.8       | 6543    | PASS             |
| 176         | 174          | 95           | 101          | 95.1      | 91136   | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 6328    | PASS             |