


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071319\
 Data File : VN056677.D
 Acq On : 12 Jul 2019 8:14
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N071319W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jul 12 23:58:13 2019

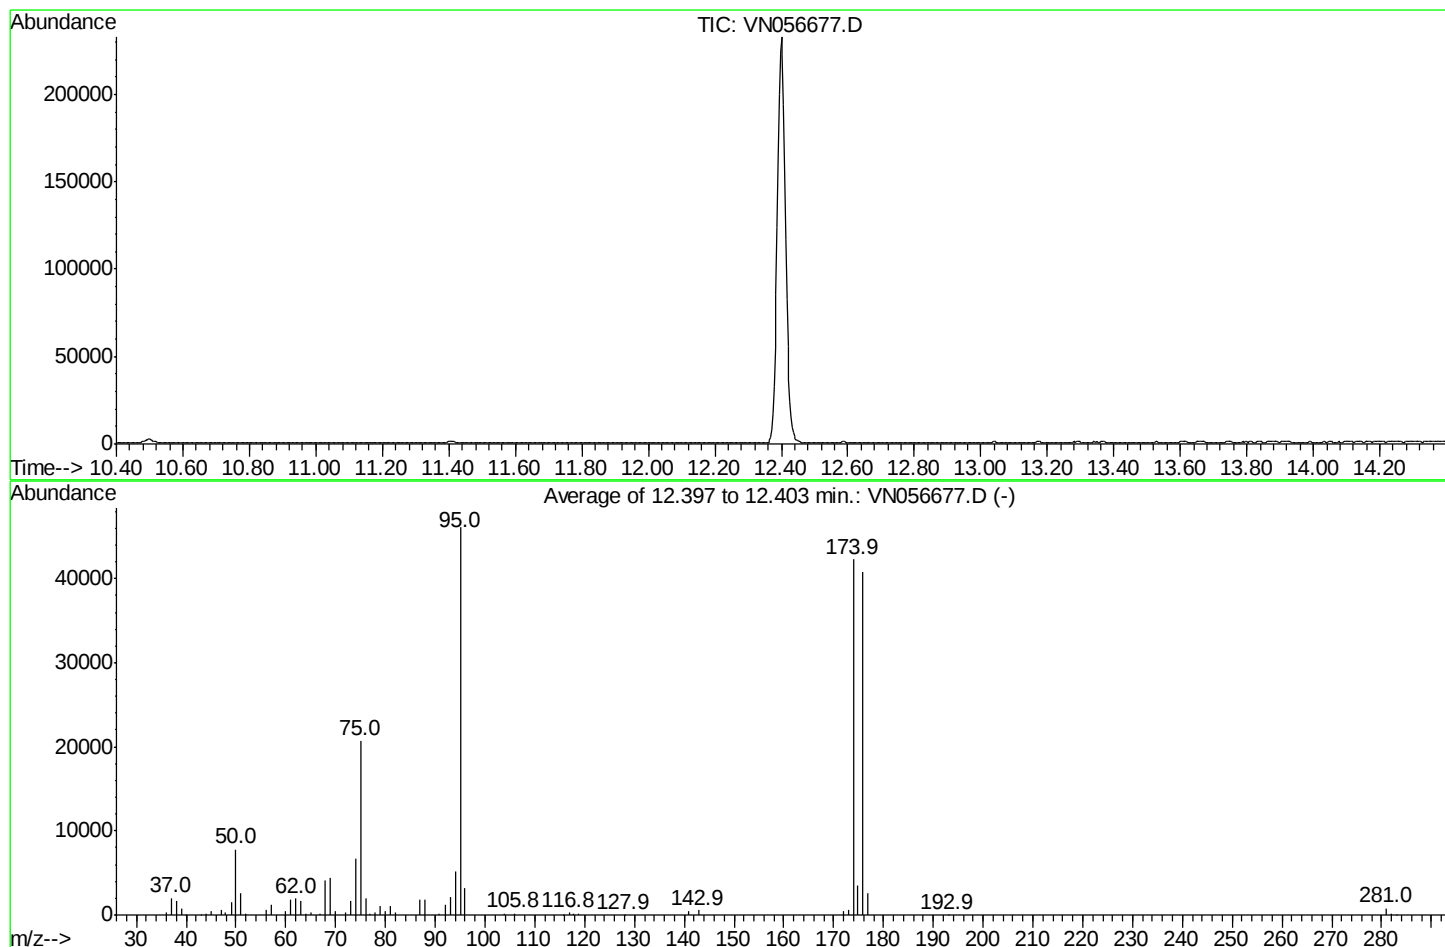

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	7823	PASS
75	95	30	60	45.1	20781	PASS
95	95	100	100	100.0	46096	PASS
96	95	5	9	6.9	3165	PASS
173	174	0.00	2	1.4	588	PASS
174	95	50	100	91.7	42288	PASS
175	174	5	9	8.1	3435	PASS
176	174	95	101	96.3	40741	PASS
177	176	5	9	6.3	2551	PASS