


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071320\
 Data File : VN062506.D
 Acq On : 13 Jul 2020 8:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N071320W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Jul 14 00:52:57 2020

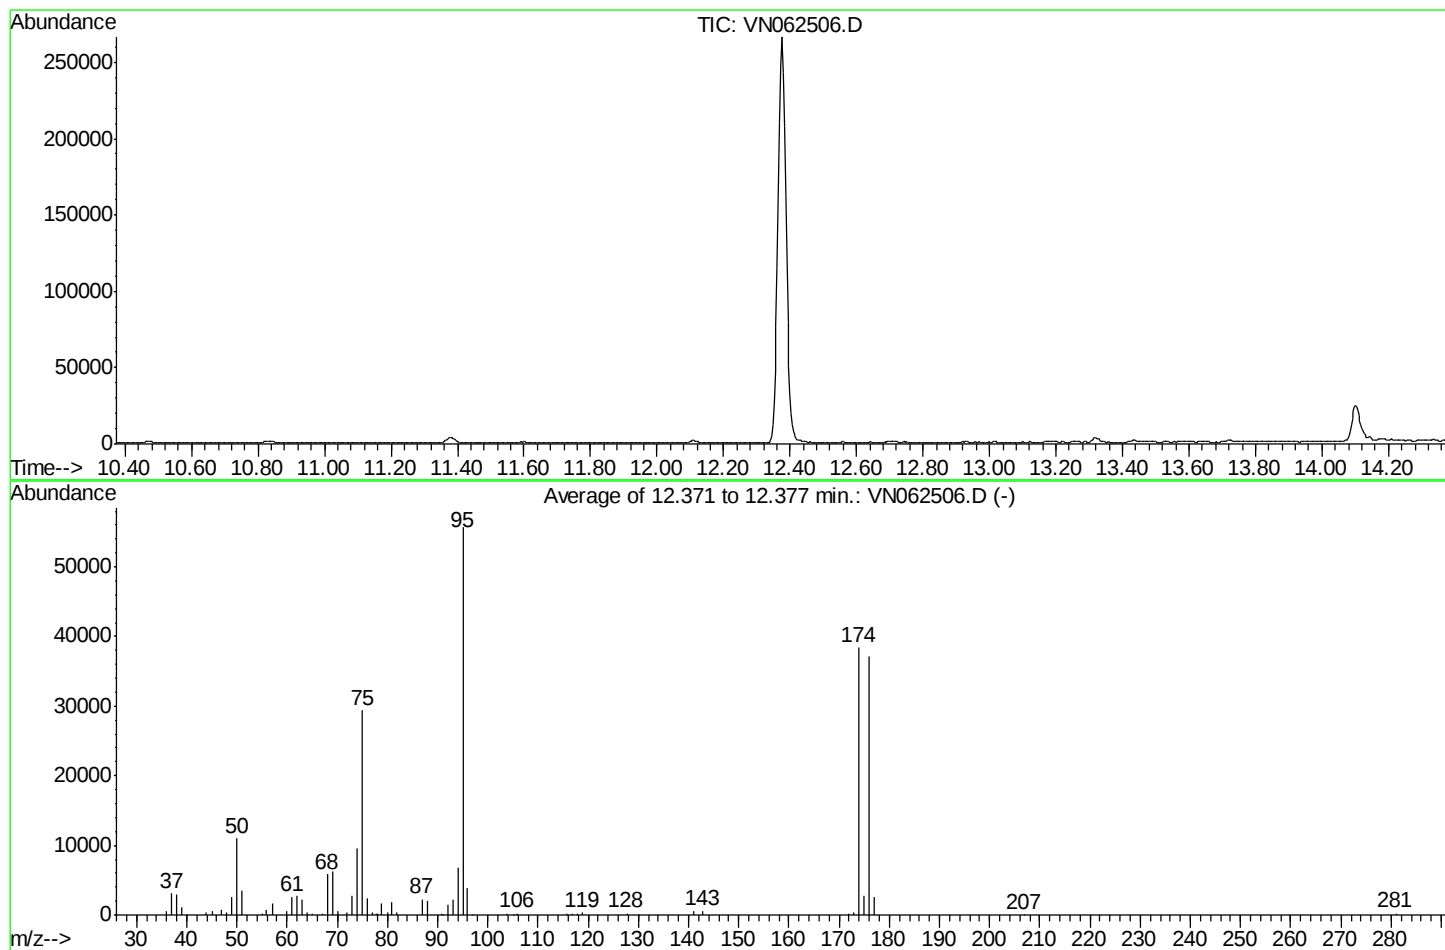

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	11031	PASS
75	95	30	60	52.7	29328	PASS
95	95	100	100	100.0	55677	PASS
96	95	5	9	6.8	3809	PASS
173	174	0.00	2	0.7	287	PASS
174	95	50	100	68.9	38370	PASS
175	174	5	9	7.2	2774	PASS
176	174	95	101	96.6	37058	PASS
177	176	5	9	6.7	2489	PASS