

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071321\
 Data File : VN067715.D
 Acq On : 13 Jul 2021 14:00
 Operator : JC/MD
 Sample : M2992-01DL 100X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Jul 13 22:16:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	346051	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	638539	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	592624	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	227996	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	266534	50.964	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.920%			
35) Dibromofluoromethane	8.024	113	192806	49.977	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 99.960%			
50) Toluene-d8	10.443	98	813911	50.403	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 100.800%			
62) 4-Bromofluorobenzene	12.733	95	266448	46.709	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 93.420%			
Target Compounds						
					Qvalue	
5) Bromomethane	2.823	94	78	Below Cal	#	4
6) Chloroethane	2.974	64	50	Below Cal		90
7) Trichlorofluoromethane	3.271	101	25	Below Cal	#	18
11) Tert butyl alcohol	5.393	59	365	0.486	ug/l #	71
13) Acrolein	4.049	56	233	Below Cal	#	41
16) Acetone	4.299	43	9878	6.003	ug/l	93
18) Methyl Acetate	4.851	43	1036	0.224	ug/l #	70
20) Methylene Chloride	5.079	84	1133	Below Cal	#	72
25) 2-Butanone	7.343	43	353539	129.377	ug/l	96
29) Tetrahydrofuran	7.699	42	636	0.354	ug/l #	80
31) Cyclohexane	8.083	56	9813	1.338	ug/l #	22
36) 1,1-Dichloropropene	8.086	75	30303	5.109	ug/l #	53
37) Ethyl Acetate	7.343	43	353539	61.516	ug/l #	69
38) Carbon Tetrachloride	8.088	117	39156	6.693	ug/l #	16
40) Benzene	8.458	78	8502	0.479	ug/l #	88
41) Methacrylonitrile	7.689	41	899	0.304	ug/l #	34
43) Isopropyl Acetate	8.686	43	2323	0.230	ug/l #	58
52) Toluene	10.507	92	43562	3.746	ug/l	97
53) t-1,3-Dichloropropene	10.505	75	415	1.798	ug/l #	1
59) 2-Hexanone	11.087	43	1695	0.391	ug/l #	48
67) Ethyl Benzene	11.846	91	9829	0.444	ug/l	90
68) m/p-Xylenes	11.956	106	11365	1.356	ug/l	91
69) o-Xylene	12.283	106	4186	0.508	ug/l	94
70) Styrene	12.299	104	5957	0.452	ug/l	89
76) 1,2,3-Trichloropropane	12.733	75	153185	32.900	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.733	75	153185	106.073	ug/l #	6
84) 1,2,4-Trimethylbenzene	13.399	105	38125	2.610	ug/l #	34
85) sec-Butylbenzene	13.399	105	38125	2.167	ug/l #	59
93) 1,2,4-Trichlorobenzene	15.260	180	877	2.893	ug/l #	14
95) Naphthalene	15.512	128	16523	4.403	ug/l #	91
96) 1,2,3-Trichlorobenzene	15.700	180	981	2.888	ug/l #	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jul 13 22:16:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




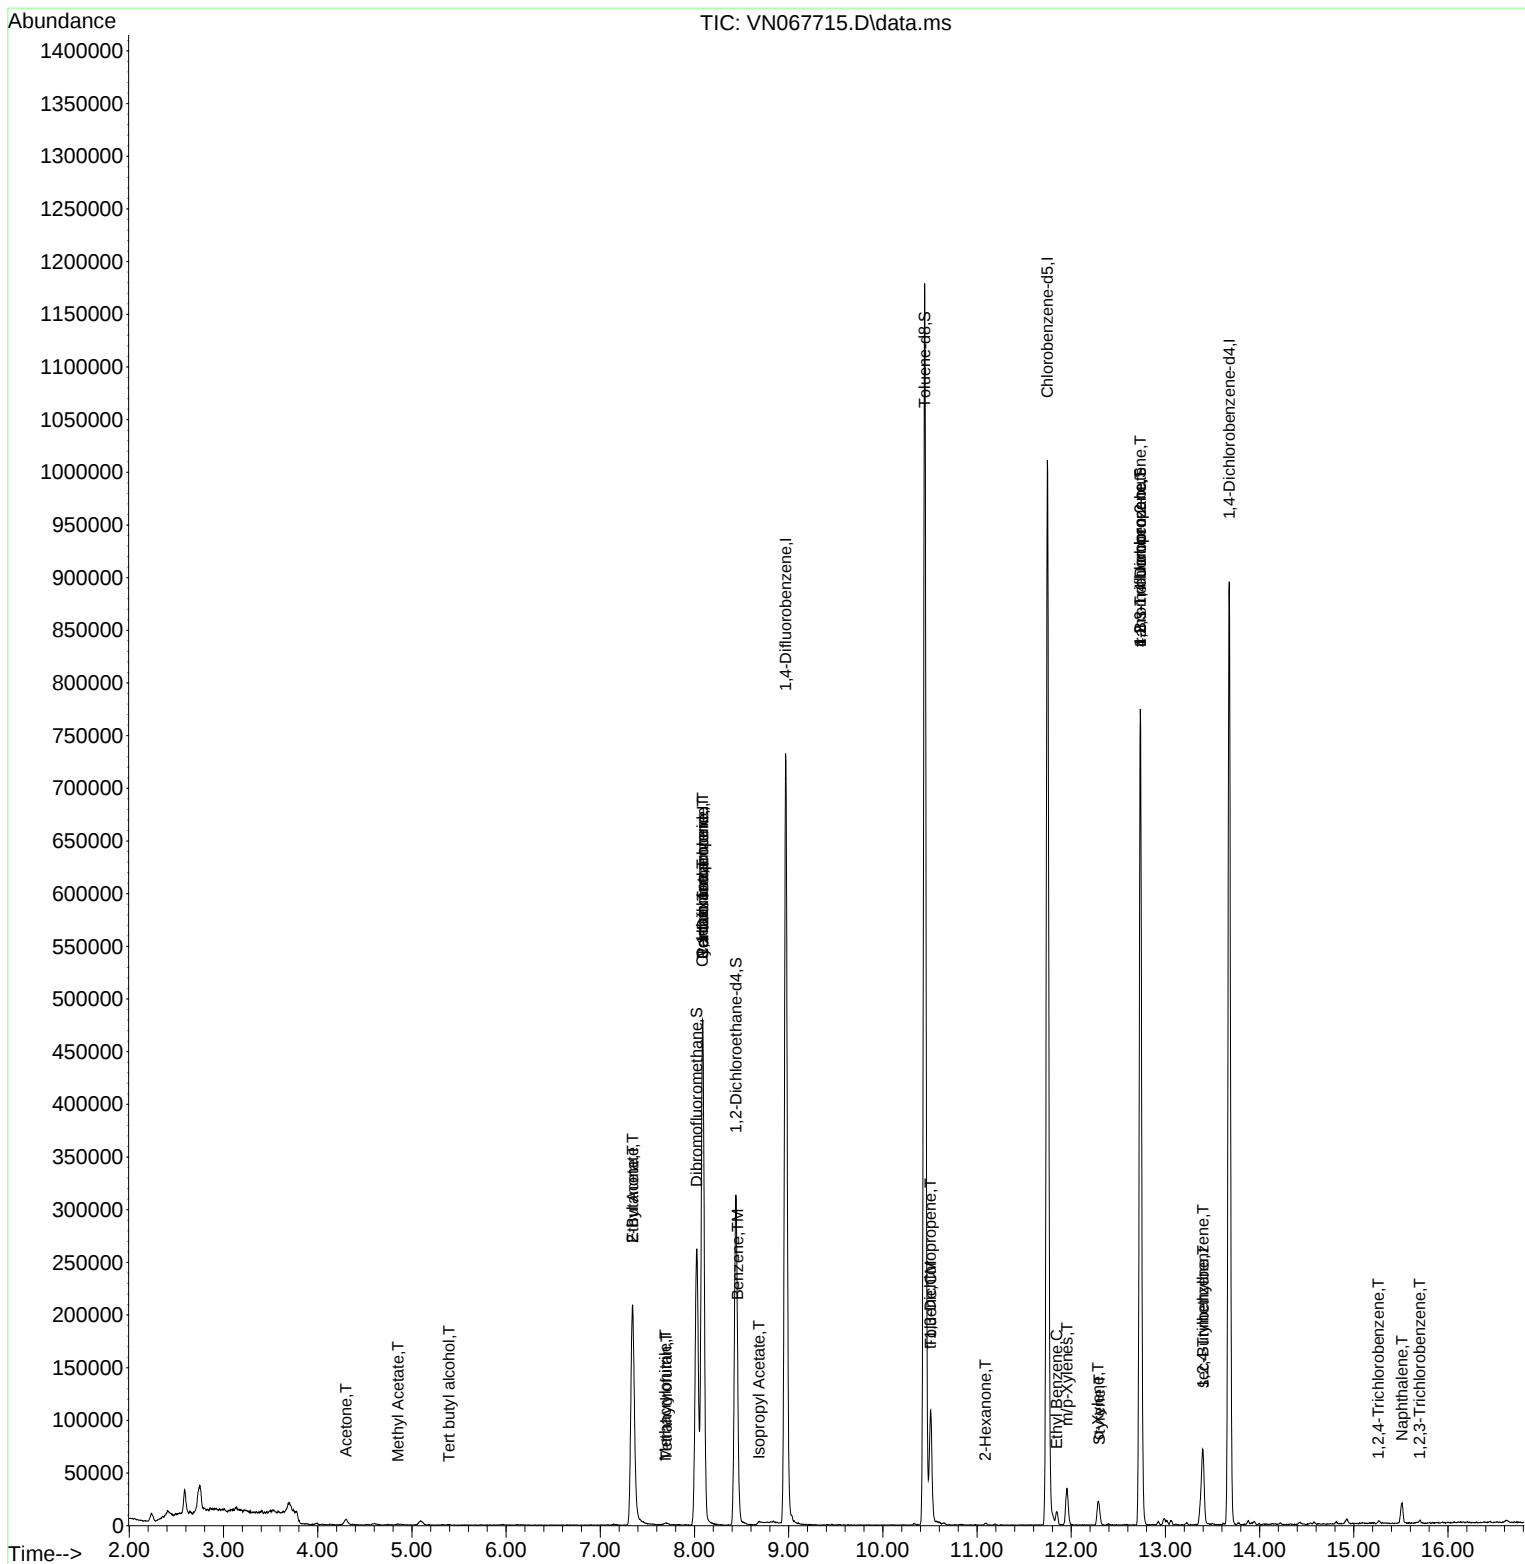




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 346051
Ion Ratio Lower Upper
168 100
99 63.8 62.9 94.3

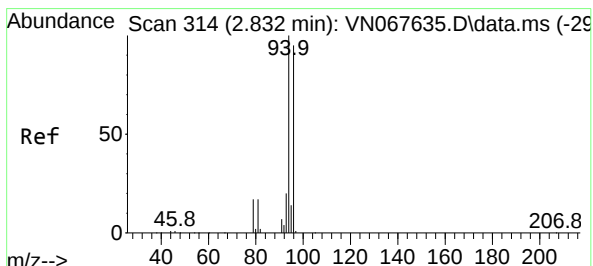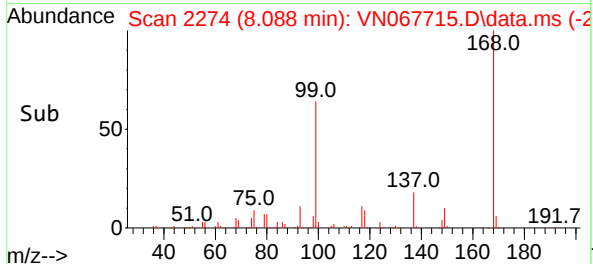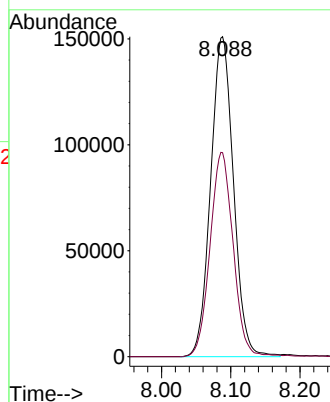

#5
Bromomethane
Concen: Below Cal
RT: 2.823 min Scan# 311
Delta R.T. -0.009 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 94 Resp: 78
Ion Ratio Lower Upper
94 100
96 0.0 73.7 110.5#


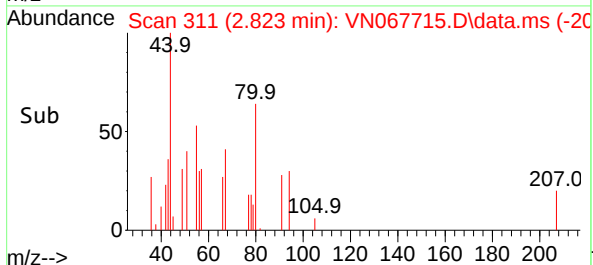

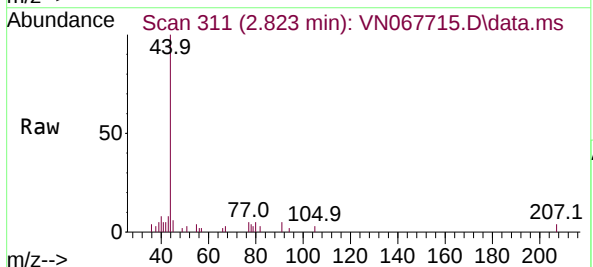


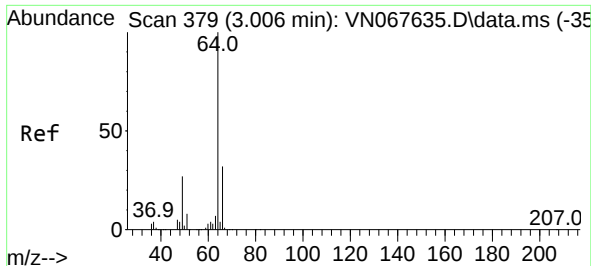

#6
Chloroethane
Concen: Below Cal
RT: 2.974 min Scan# 367
Delta R.T. -0.032 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 50
Ion Ratio Lower Upper
64 100
66 36.3 24.7 37.1

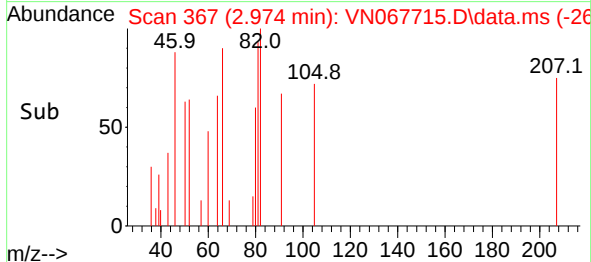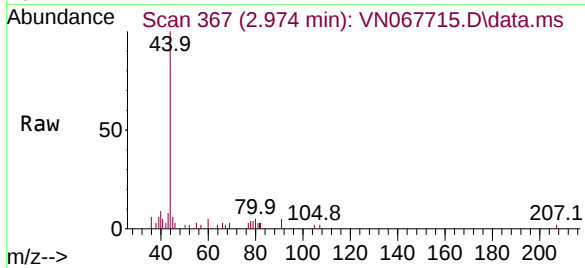

#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.271 min Scan# 478
Delta R.T. -0.094 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 101 Resp: 25
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#

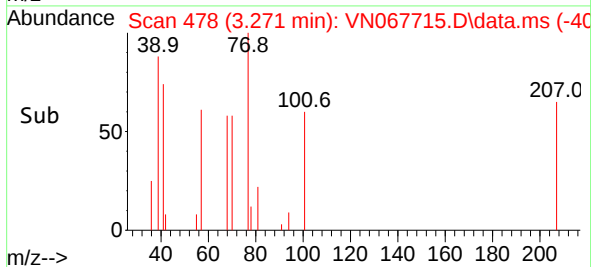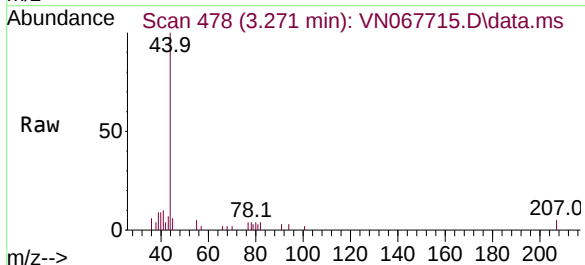




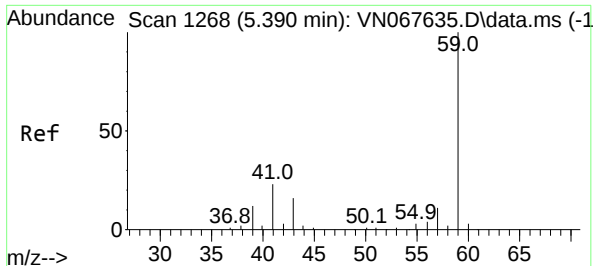


#11

Tert butyl alcohol
Concen: 0.486 ug/l
RT: 5.393 min Scan# 1269
Delta R.T. 0.003 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 365
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

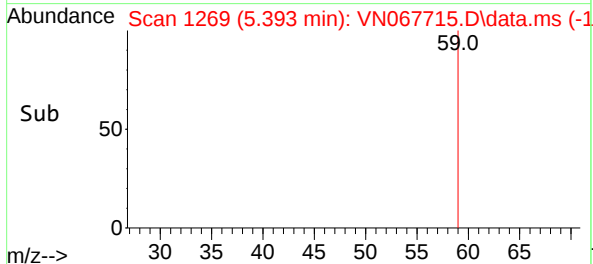


#13

Acrolein
Concen: Below Cal
RT: 4.049 min Scan# 768
Delta R.T. 0.010 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 56 Resp: 233
Ion Ratio Lower Upper
56 100
55 121.0 57.4 86.0#


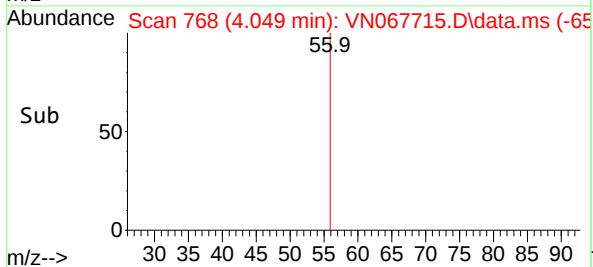

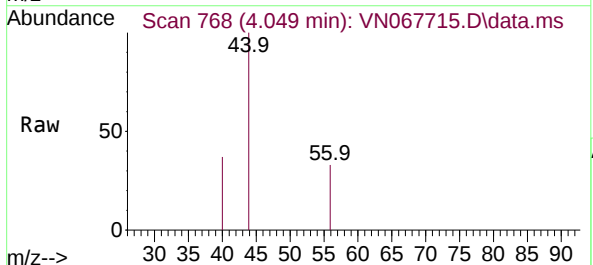


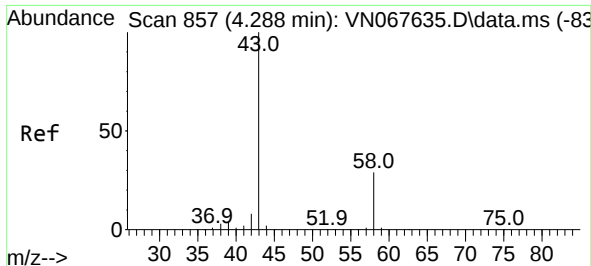

#16
Acetone
Concen: 6.003 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.011 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 9878
Ion Ratio Lower Upper
43 100
58 30.3 21.2 31.8

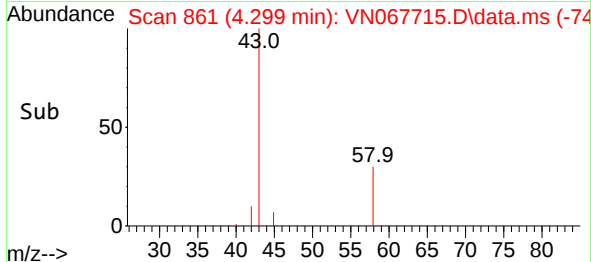

#18
Methyl Acetate
Concen: 0.224 ug/l
RT: 4.851 min Scan# 1067
Delta R.T. -0.006 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00


Tgt Ion: 43 Resp: 1036
Ion Ratio Lower Upper
43 100
74 7.3 17.4 26.0#

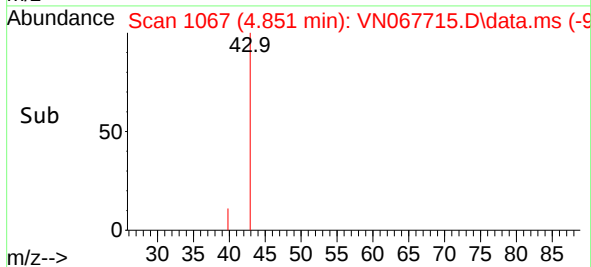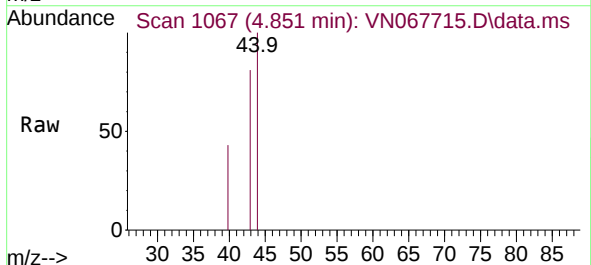



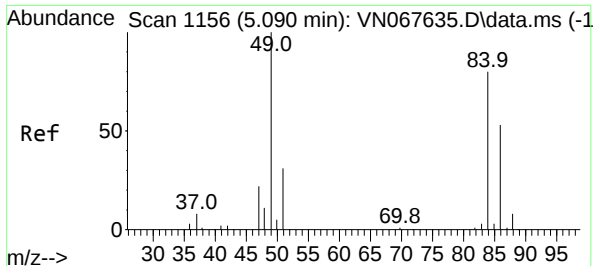


#20
Methylene Chloride
Concen: Below Cal
RT: 5.079 min Scan# 1152
Delta R.T. -0.011 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:	84	Resp:	1133
Ion	Ratio	Lower	Upper
84	100		
49	94.3	110.9	166.3#
51	35.7	32.6	49.0
86	46.5	51.6	77.4#

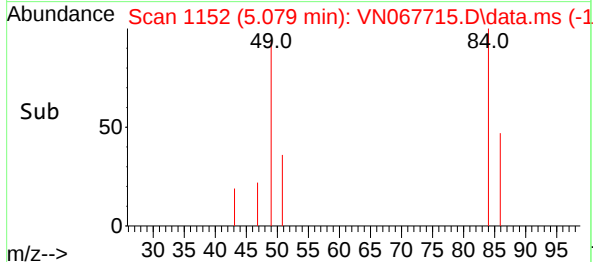

#25
2-Butanone
Concen: 129.377 ug/l
RT: 7.343 min Scan# 1996
Delta R.T. 0.006 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion:	43	Resp:	353539
Ion	Ratio	Lower	Upper
43	100		
72	26.4	19.7	29.5

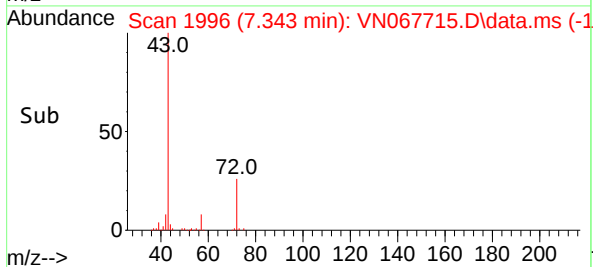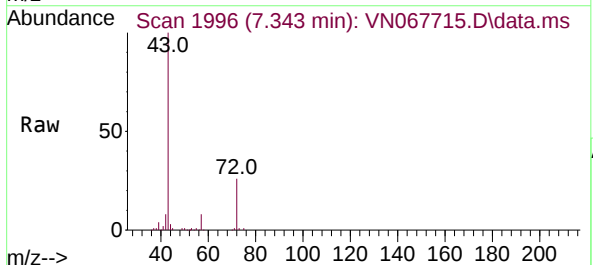

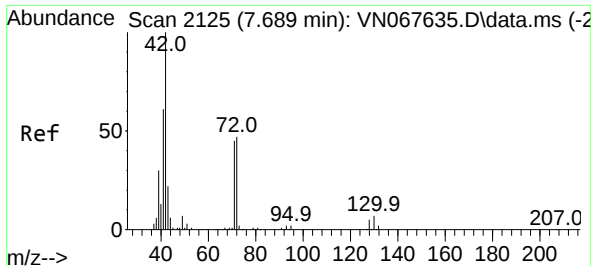

#29

Tetrahydrofuran

Concen: 0.354 ug/l


RT: 7.699 min Scan# 2129

Delta R.T. 0.010 min




Lab File: VN067715.D

Acq: 13 Jul 2021 14:00

Instrument :
MSVOA_N
ClientSampled :



Tgt Ion:	42	Resp:	636
Ion	Ratio	Lower	Upper
42	100		
72	29.1	32.8	49.2#
71	25.9	31.2	46.8#

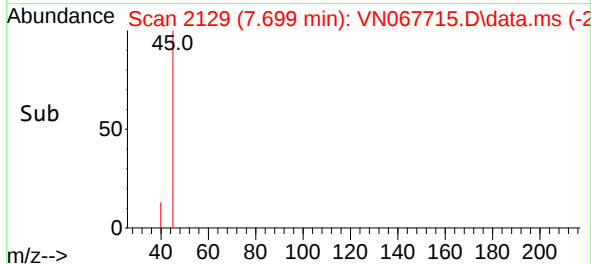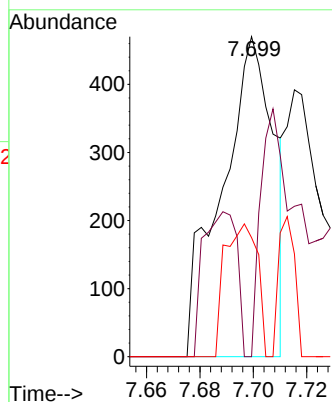

#31

Cyclohexane

Concen: 1.338 ug/l




RT: 8.083 min Scan# 2272


Delta R.T. -0.011 min

Lab File: VN067715.D

Acq: 13 Jul 2021 14:00

Tgt Ion:	56	Resp:	9813
Ion	Ratio	Lower	Upper
56	100		
69	144.8	27.3	40.9#
84	107.1	64.9	97.3#


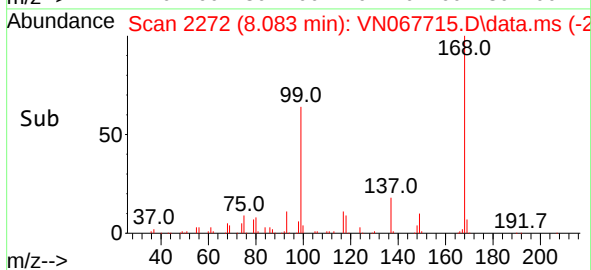

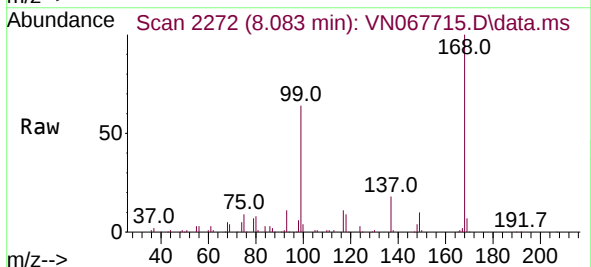




#33
 1,2-Dichloroethane-d4
 Concen: 50.964 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN067715.D
 Acq: 13 Jul 2021 14:00




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 65 Resp: 266534
 Ion Ratio Lower Upper
 65 100
 67 50.0 0.0 98.6

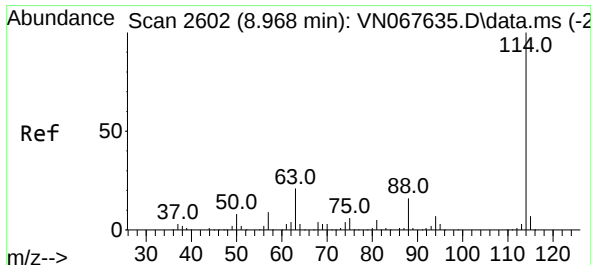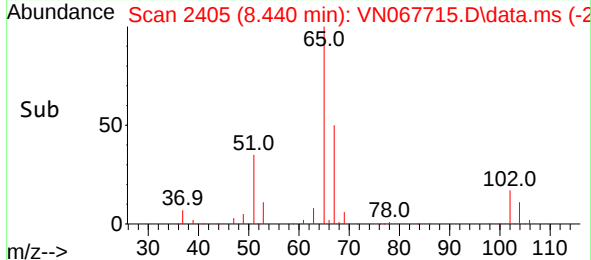

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.968 min Scan# 2602
 Delta R.T. -0.000 min
 Lab File: VN067715.D
 Acq: 13 Jul 2021 14:00

Tgt Ion: 114 Resp: 638539
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 49.0
 88 15.0 0.0 36.6

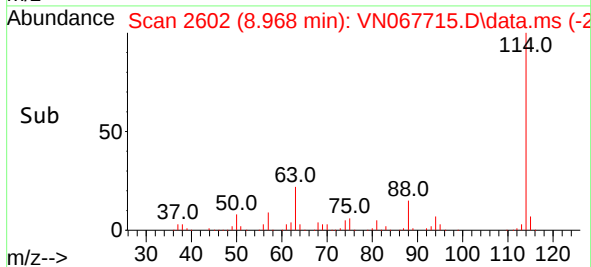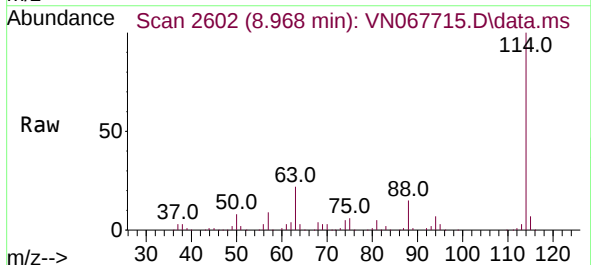

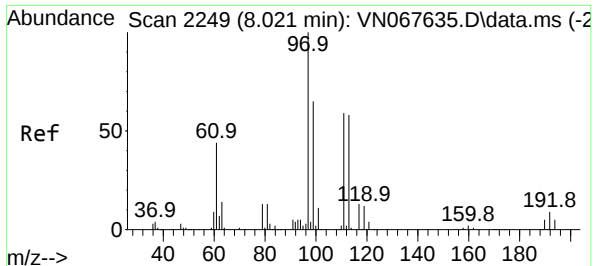

#35

Dibromofluoromethane

Concen: 49.977 ug/l

RT: 8.024 min Scan# 2250

Delta R.T. 0.003 min

Lab File: VN067715.D

Acq: 13 Jul 2021 14:00





Tgt Ion:113 Resp: 192806

Ion Ratio Lower Upper

113 100

111 103.2 83.8 125.8

192 16.1 13.4 20.0

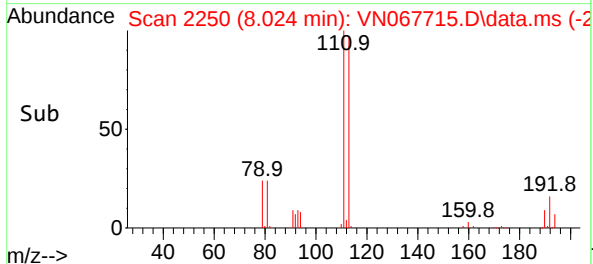

#36

1,1-Dichloropropene

Concen: 5.109 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.136 min

Lab File: VN067715.D

Acq: 13 Jul 2021 14:00




Tgt Ion: 75 Resp: 30303


Ion Ratio Lower Upper

75 100

110 10.6 15.7 47.0#

77 0.0 24.6 37.0#

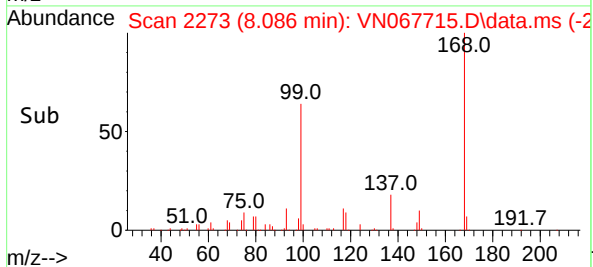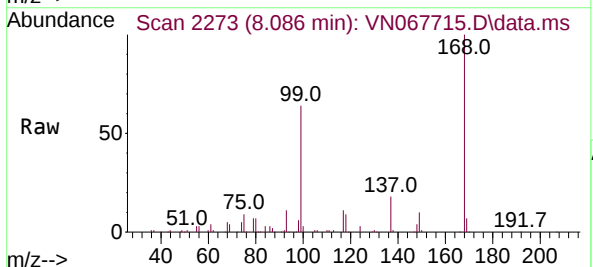

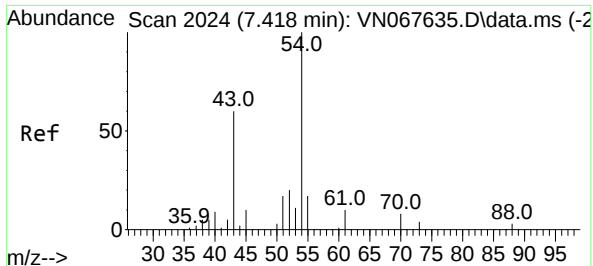

#37

Ethyl Acetate

Concen: 61.516 ug/l

RT: 7.343 min Scan# 1996





Delta R.T. -0.075 min

Lab File: VN067715.D

Acq: 13 Jul 2021 14:00

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:	43	Resp:	353539
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.1	8.1	12.1#

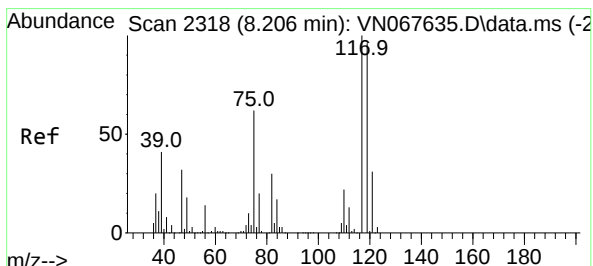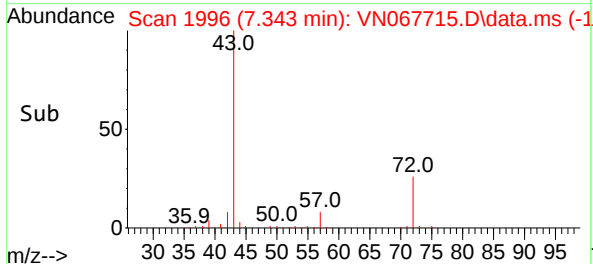

#38

Carbon Tetrachloride

Concen: 6.693 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.118 min

Lab File: VN067715.D

Acq: 13 Jul 2021 14:00

Tgt Ion:	117	Resp:	39156
Ion	Ratio	Lower	Upper
117	100		
119	4.1	75.4	113.2#
121	0.0	23.5	35.3#


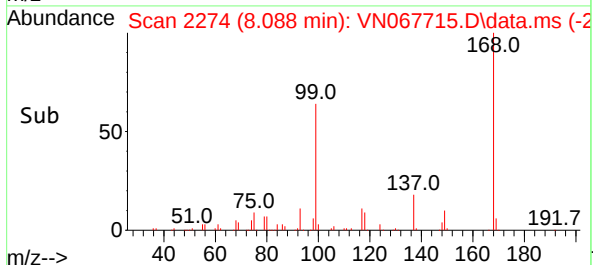
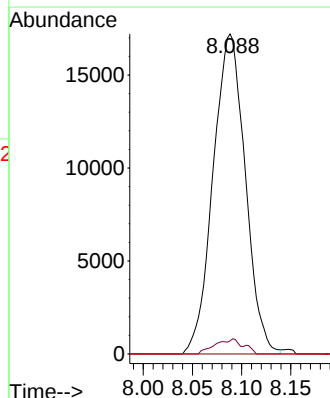
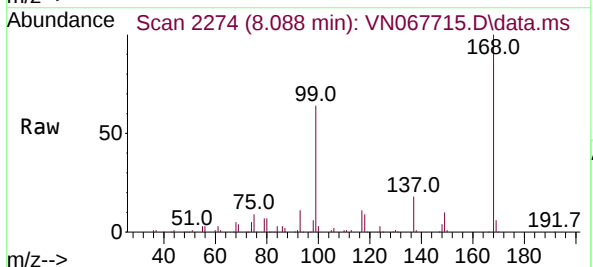




#40
Benzene
Concen: 0.479 ug/l
RT: 8.458 min Scan# 2412
Delta R.T. -0.003 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 78 Resp: 8502
Ion Ratio Lower Upper
78 100
77 17.8 18.9 28.3#

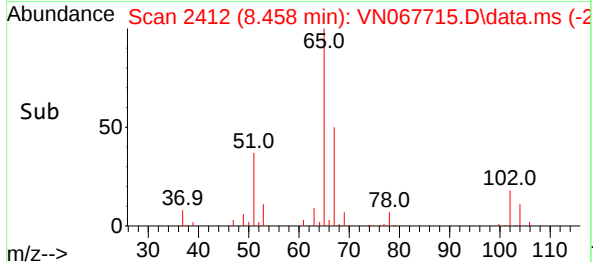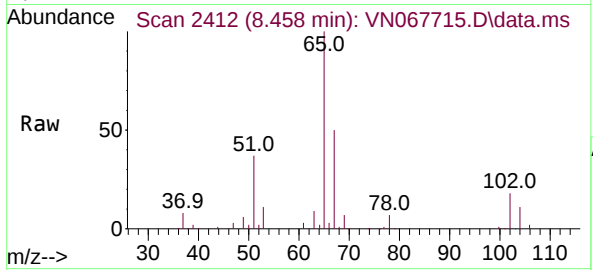

#41
Methacrylonitrile
Concen: 0.304 ug/l
RT: 7.689 min Scan# 2125
Delta R.T. 0.049 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 41 Resp: 899
Ion Ratio Lower Upper
41 100
39 24.7 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#



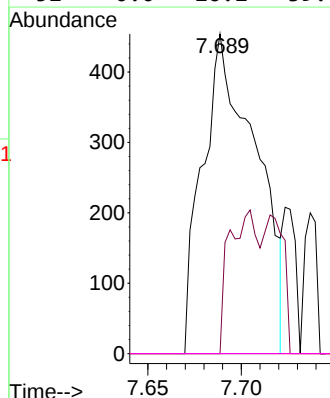
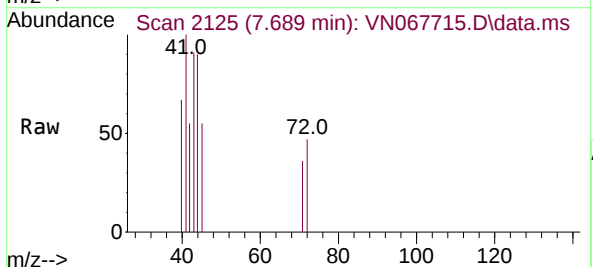




#43
Isopropyl Acetate
Concen: 0.230 ug/l
RT: 8.686 min Scan# 2497
Delta R.T. 0.123 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2323
Ion Ratio Lower Upper
43 100
61 0.0 19.0 28.4#
87 0.0 9.5 14.3#

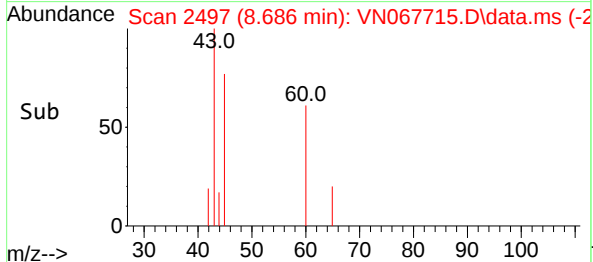

#50
Toluene-d8
Concen: 50.403 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 98 Resp: 813911
Ion Ratio Lower Upper
98 100
100 62.7 51.7 77.5


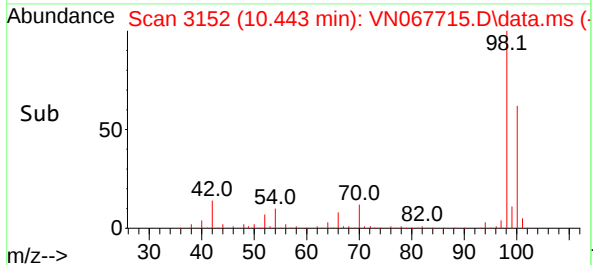

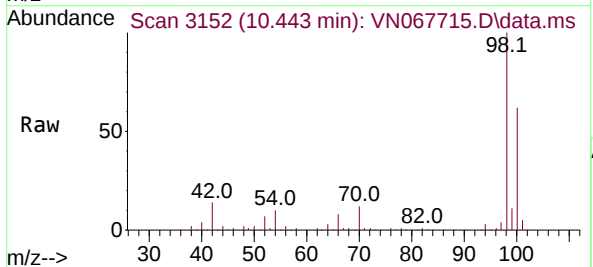




#52
Toluene
Concen: 3.746 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 92 Resp: 43562
Ion Ratio Lower Upper
92 100
91 178.7 139.6 209.4

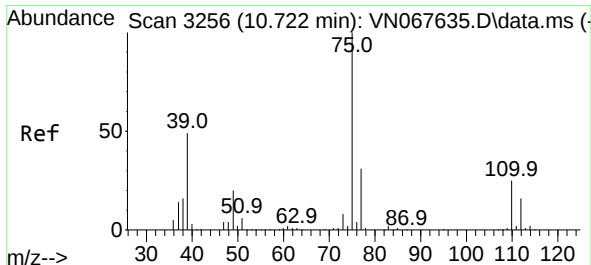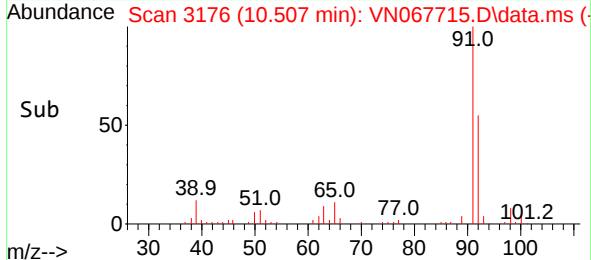

#53
t-1,3-Dichloropropene
Concen: 1.798 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.217 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 75 Resp: 415
Ion Ratio Lower Upper
75 100
77 143.3 25.1 37.7#


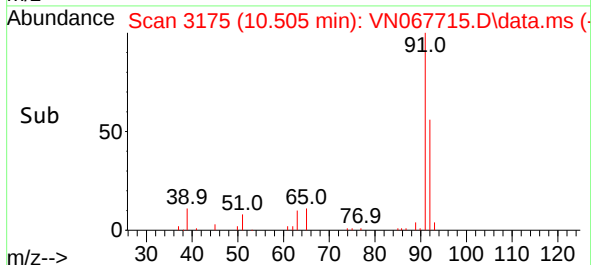
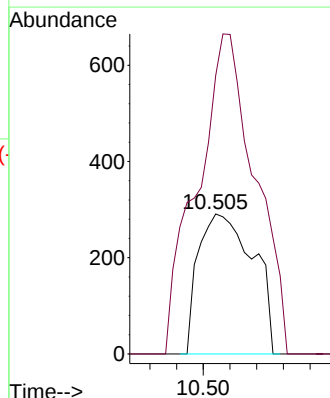
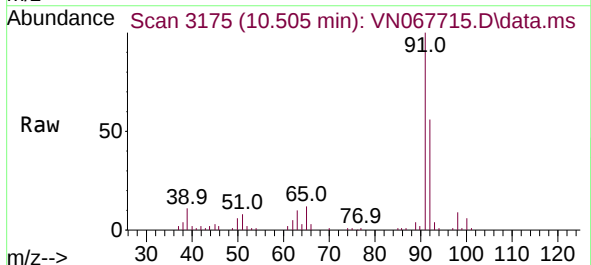




#59
2-Hexanone
Concen: 0.391 ug/l
RT: 11.087 min Scan# 3392
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1695
Ion Ratio Lower Upper
43 100
58 13.7 24.7 74.1#

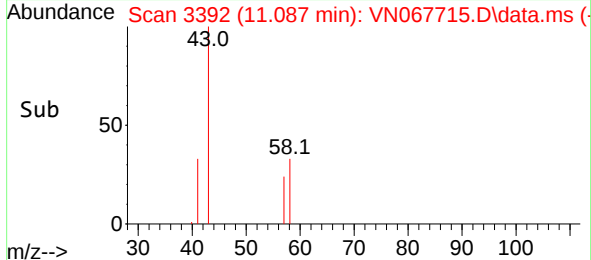

#62
4-Bromofluorobenzene
Concen: 46.709 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 95 Resp: 266448
Ion Ratio Lower Upper
95 100
174 71.8 0.0 122.0
176 69.1 0.0 117.6


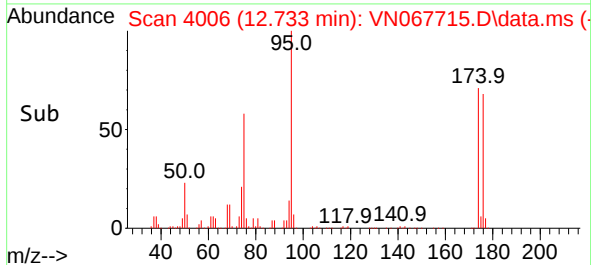

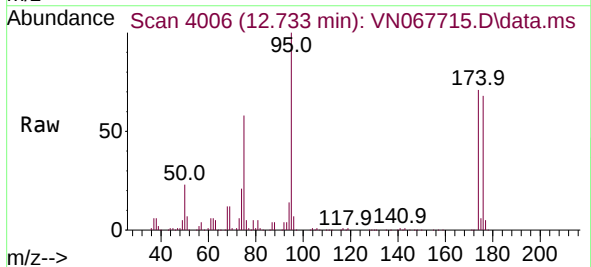




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 592624
Ion Ratio Lower Upper
117 100
82 58.1 53.1 79.7
119 32.7 25.5 38.3

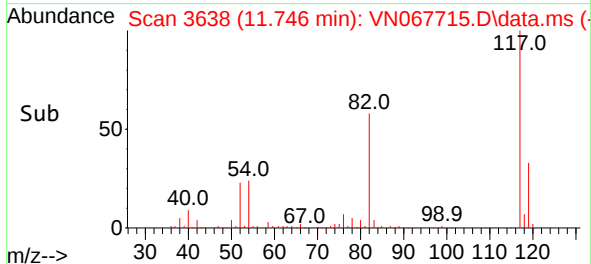

#67
Ethyl Benzene
Concen: 0.444 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 91 Resp: 9829
Ion Ratio Lower Upper
91 100
106 34.5 23.4 35.0


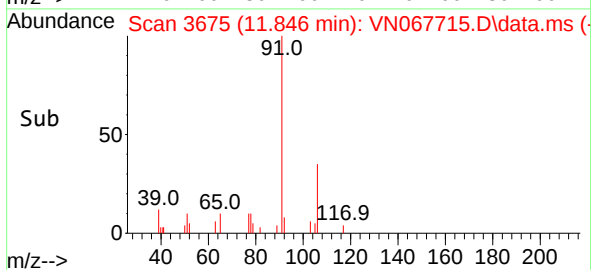

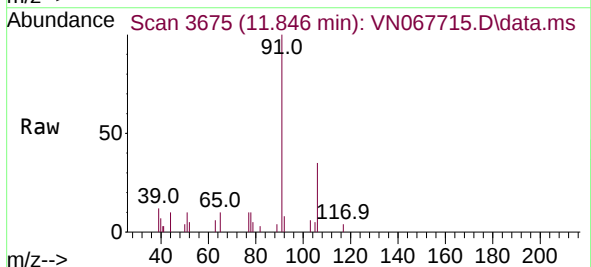




#68
m/p-Xylenes
Concen: 1.356 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:106 Resp: 11365
Ion Ratio Lower Upper
106 100
91 210.8 180.6 270.8

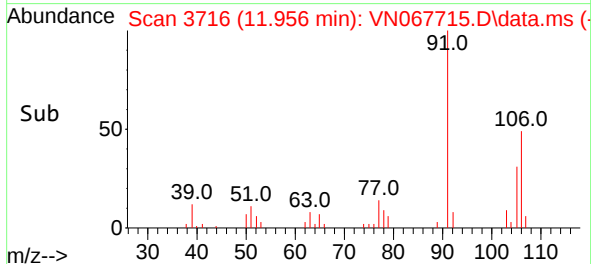

#69
o-Xylene
Concen: 0.508 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion:106 Resp: 4186
Ion Ratio Lower Upper
106 100
91 227.0 118.3 354.9


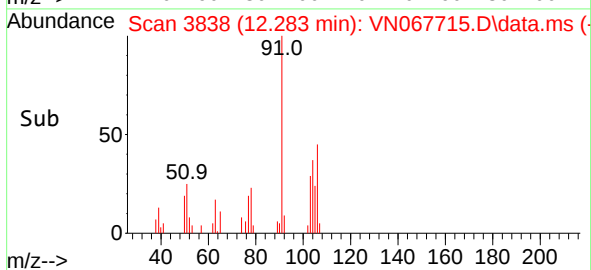

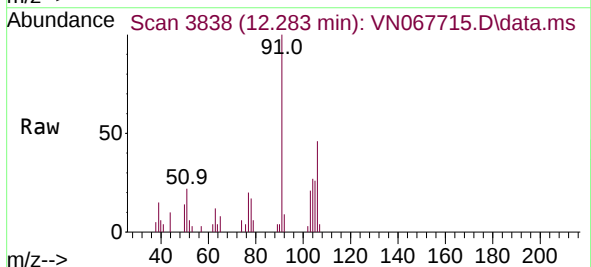




#70
Styrene
Concen: 0.452 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 5957
Ion Ratio Lower Upper
104 100
78 50.3 48.2 72.2
103 62.2 44.5 66.7

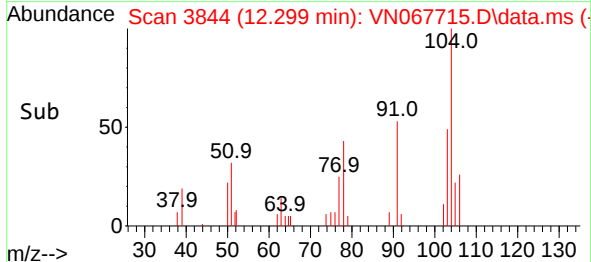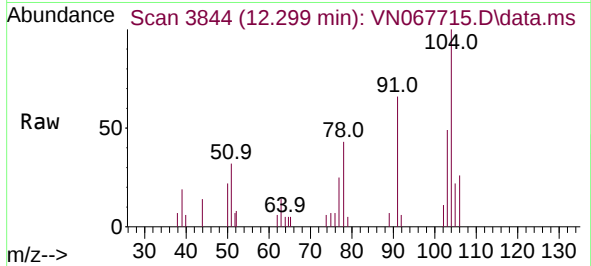

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion:152 Resp: 227996
Ion Ratio Lower Upper
152 100
115 63.4 36.1 108.5
150 160.0 0.0 351.8


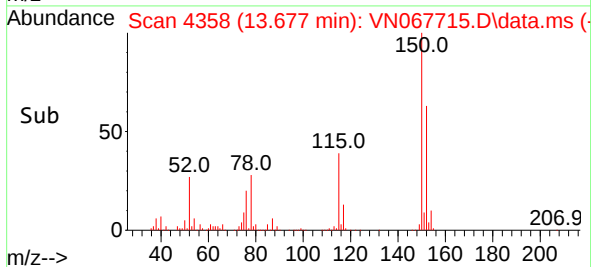

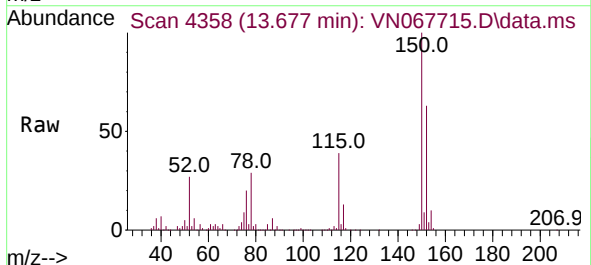


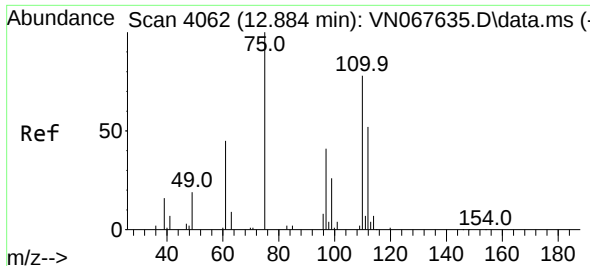

#76
1,2,3-Trichloropropane
Concen: 32.900 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 153185
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#

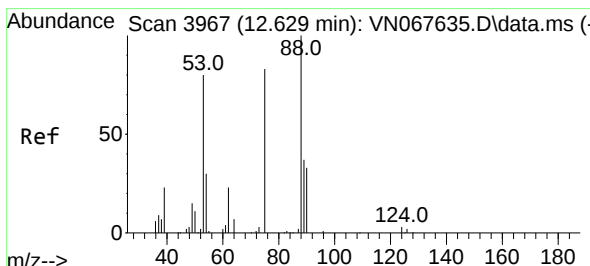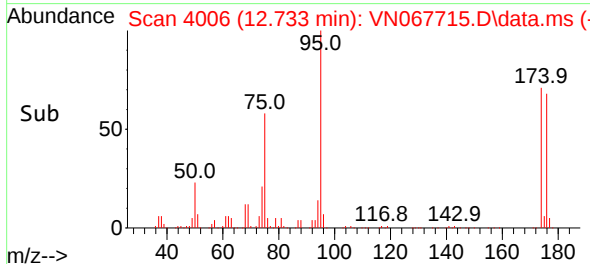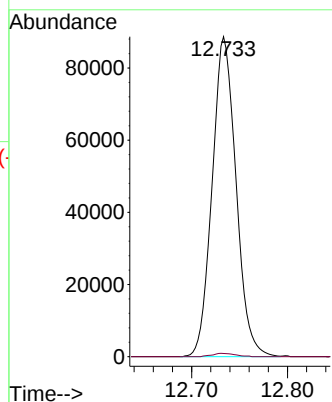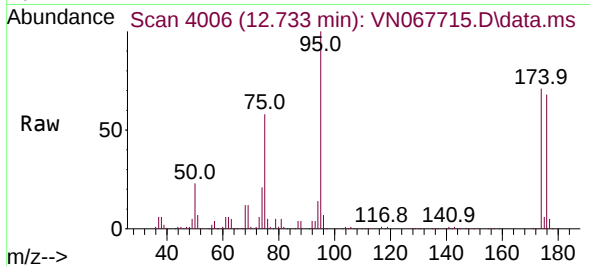

#81
trans-1,4-Dichloro-2-butene
Concen: 106.073 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

Tgt Ion: 75 Resp: 153185
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

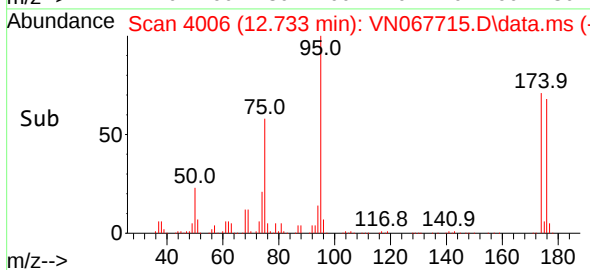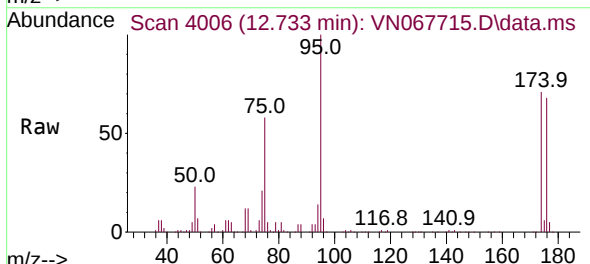



#84

1,2,4-Trimethylbenzene

Concen: 2.610 ug/l

RT: 13.399 min Scan# 4254

Delta R.T. 0.027 min

Lab File: VN067715.D





Acq: 13 Jul 2021 14:00

Tgt Ion:105 Resp: 38125

Ion Ratio Lower Upper

105 100

120 0.0 20.6 61.8#

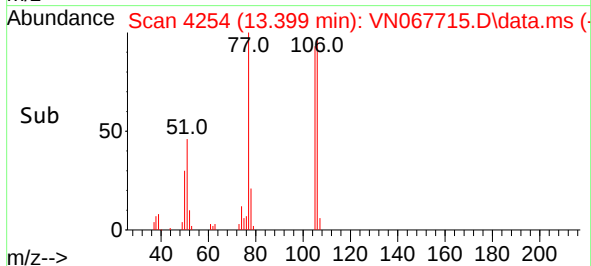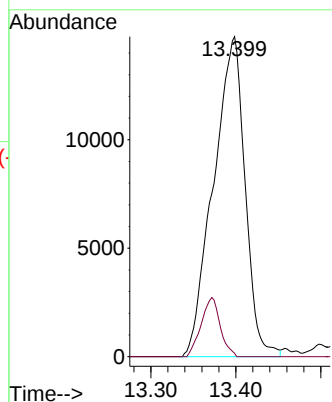

#85

sec-Butylbenzene

Concen: 2.167 ug/l

RT: 13.399 min Scan# 4254

Delta R.T. -0.104 min

Lab File: VN067715.D




Acq: 13 Jul 2021 14:00


Tgt Ion:105 Resp: 38125

Ion Ratio Lower Upper

105 100


134 0.0 9.0 27.1#

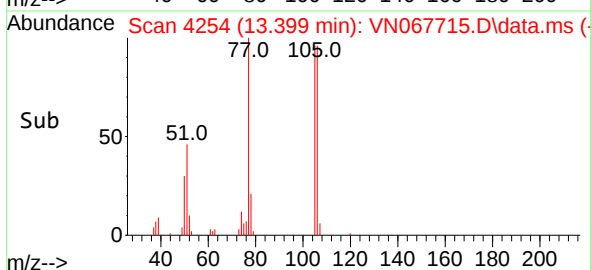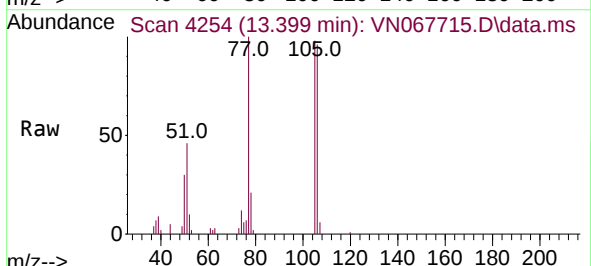



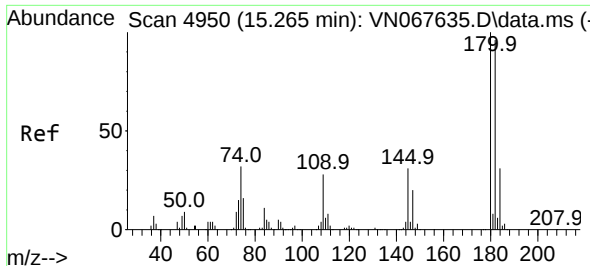


#93
1,2,4-Trichlorobenzene
Concen: 2.893 ug/l
RT: 15.260 min Scan# 4948
Delta R.T. -0.005 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00


Instrument :
MSVOA_N
ClientSampleId :

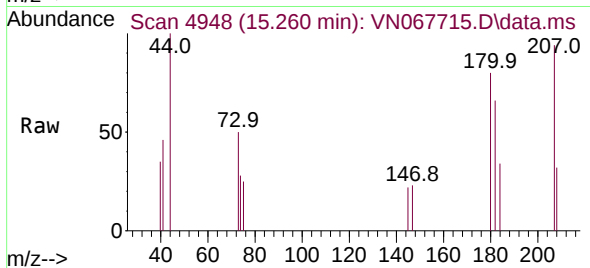



Tgt Ion:180 Resp: 877
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.5#
145 3.0 17.2 51.6#

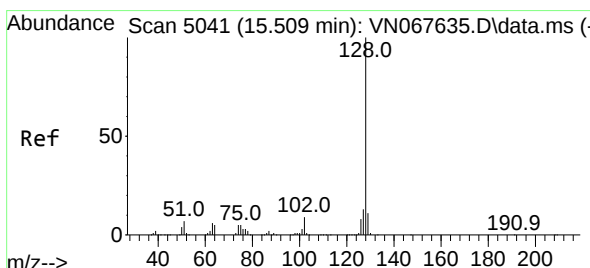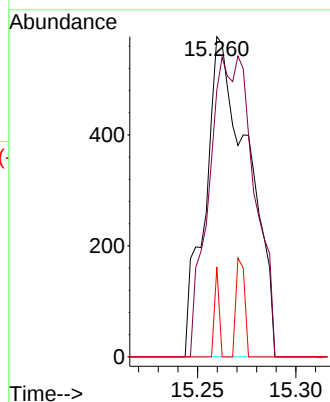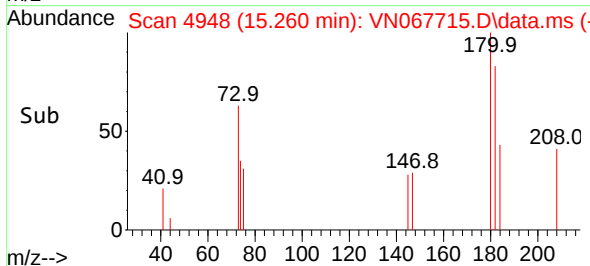


#95
Naphthalene
Concen: 4.403 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.003 min
Lab File: VN067715.D
Acq: 13 Jul 2021 14:00

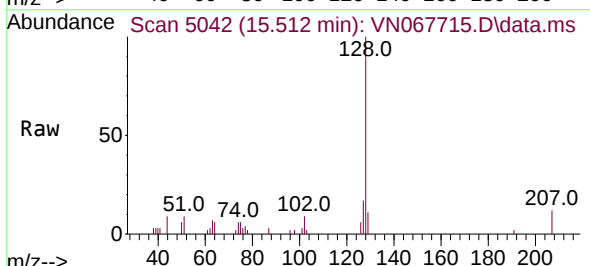


Tgt Ion:128 Resp: 16523
Ion Ratio Lower Upper
128 100
127 14.4 10.6 15.8
129 4.6 8.6 12.8#

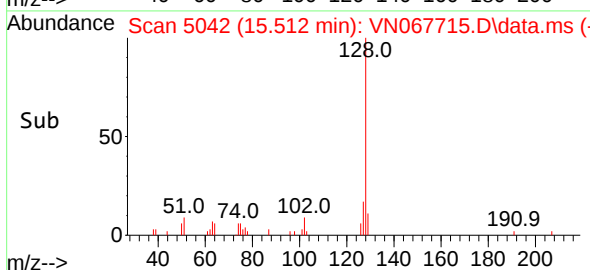

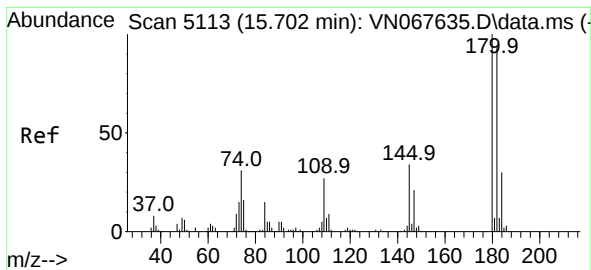

#96
 1,2,3-Trichlorobenzene
 Concen: 2.888 ug/l
 RT: 15.700 min Scan# 5112
 Delta R.T. -0.002 min
 Lab File: VN067715.D
 Acq: 13 Jul 2021 14:00

Instrument :
 MSVOA_N
 ClientSampleId :

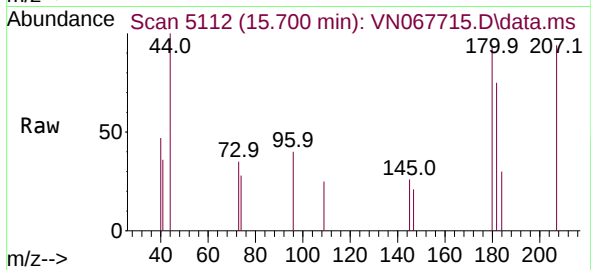

Tgt Ion:180 Resp: 981
 Ion Ratio Lower Upper
 180 100
 182 105.8 47.8 143.3
 145 11.7 18.2 54.6#

