

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071321\
 Data File : VN067710.D
 Acq On : 13 Jul 2021 11:37
 Operator : JC/MD
 Sample : VN0713WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0713WBL01

Quant Time: Jul 13 22:15:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	341111	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	636479	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	582128	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	203702	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	265309	51.46	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	102.92%
35) Dibromofluoromethane	8.021	113	191853	49.89	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.78%
50) Toluene-d8	10.443	98	808473	50.23	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.46%
62) 4-Bromofluorobenzene	12.733	95	252496	44.41	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.82%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071321\
Data File : VN067710.D
Acq On : 13 Jul 2021 11:37
Operator : JC/MD
Sample : VN0713WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0713WBL01

Quant Time: Jul 13 22:15:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




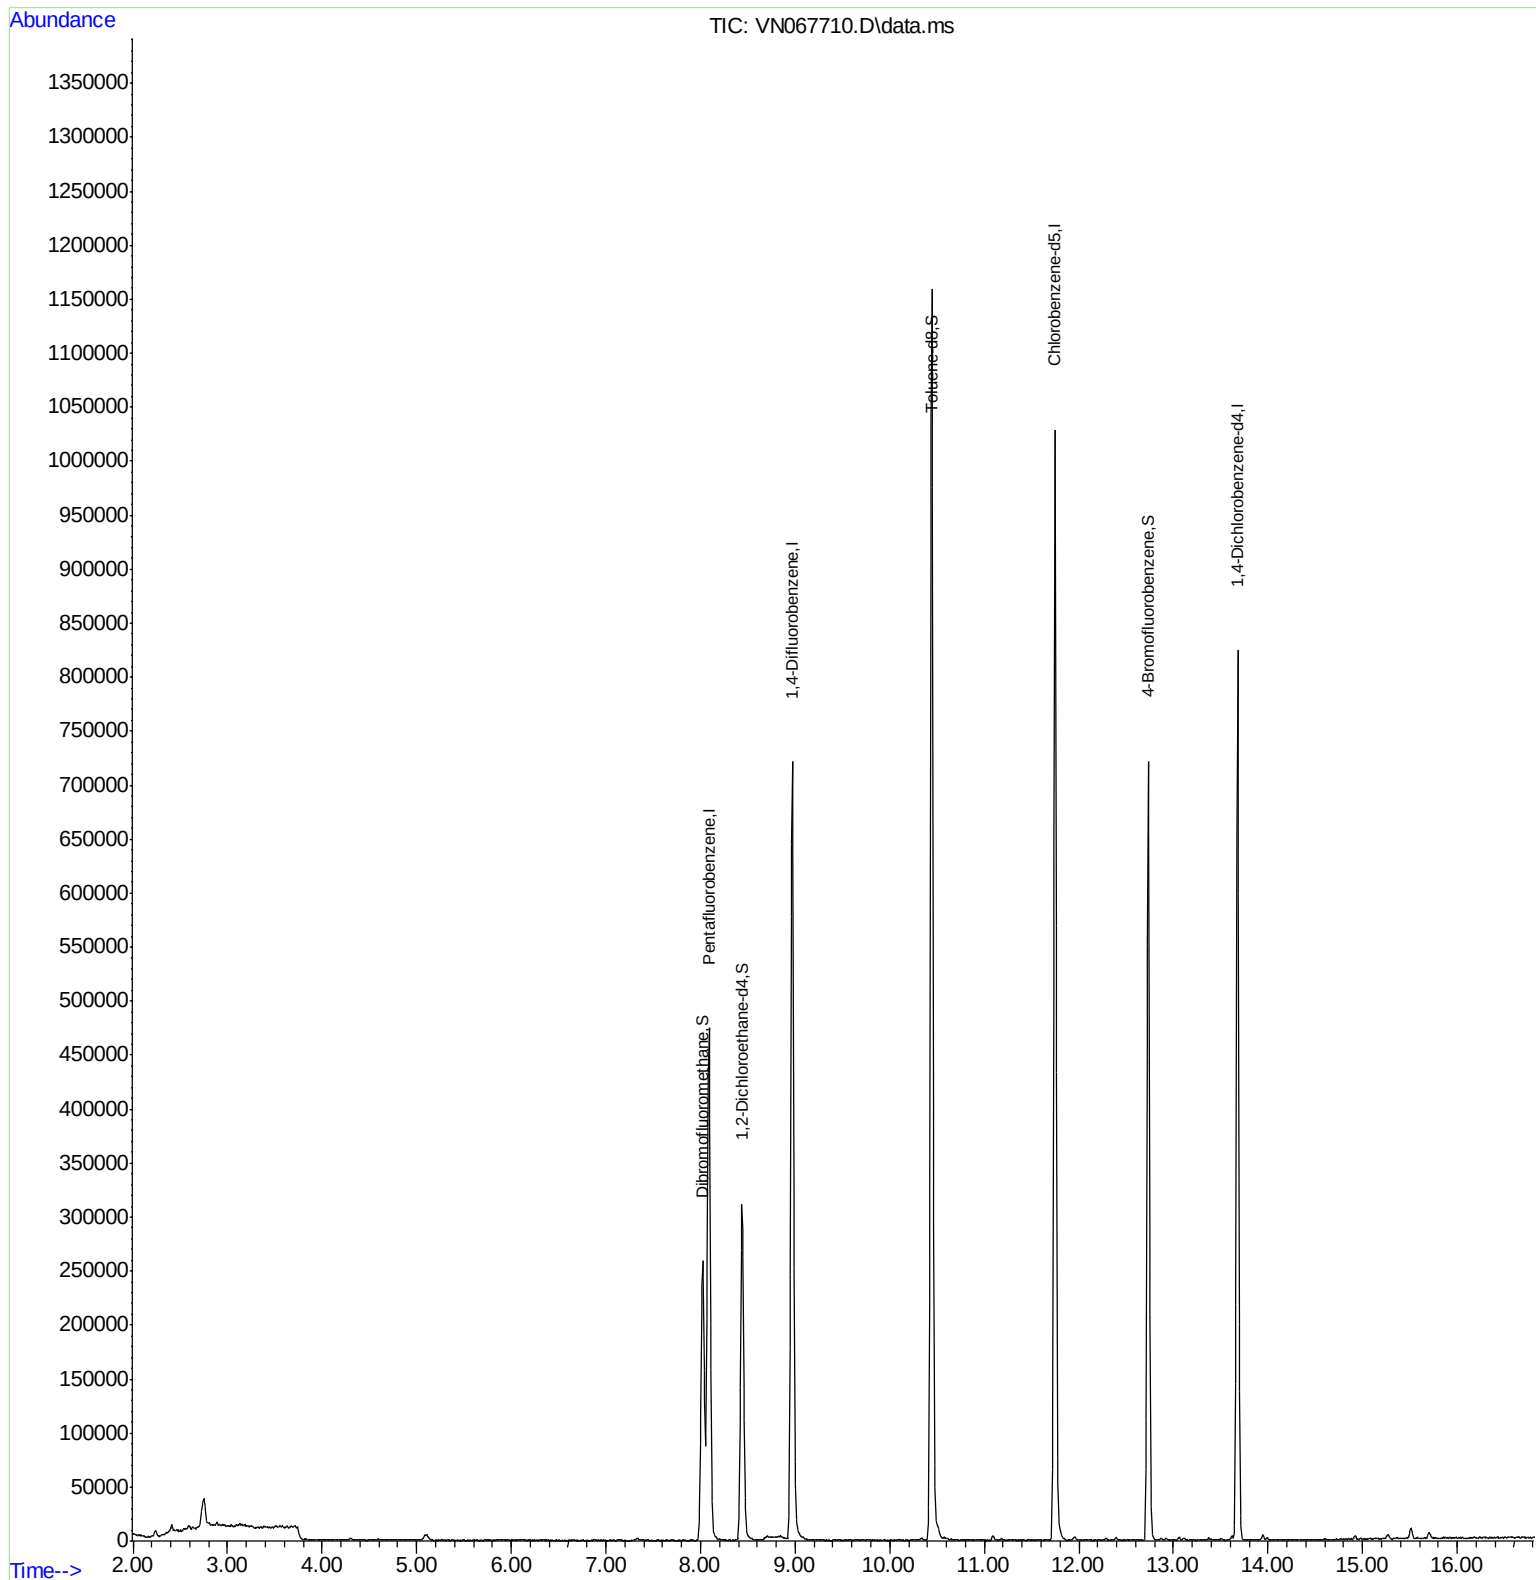


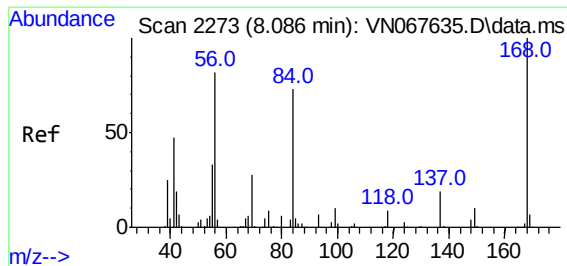

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0713WBL01


Tgt Ion:168 Resp: 341111
Ion Ratio Lower Upper
168 100
99 64.4 62.9 94.3

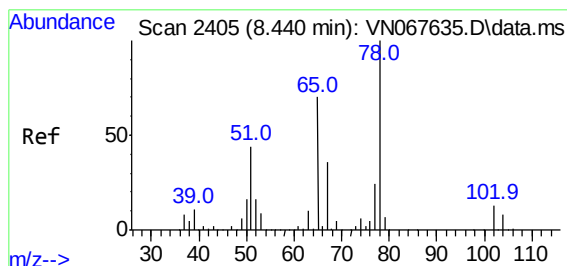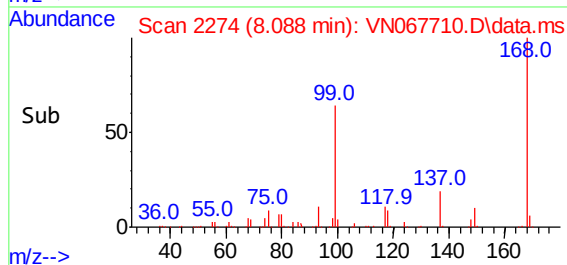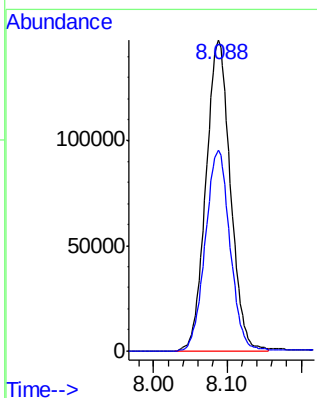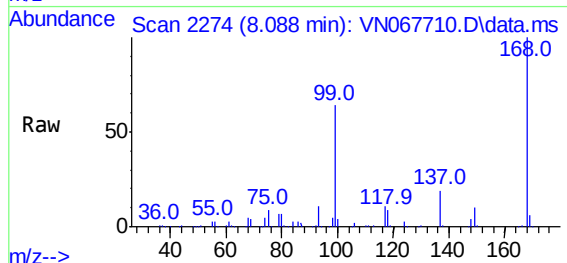

#33
1,2-Dichloroethane-d4
Concen: 51.46 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37

Tgt Ion: 65 Resp: 265309
Ion Ratio Lower Upper
65 100
67 50.4 0.0 98.6


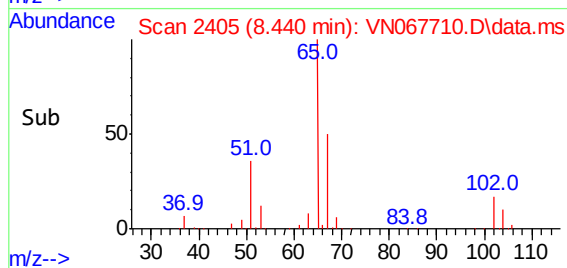
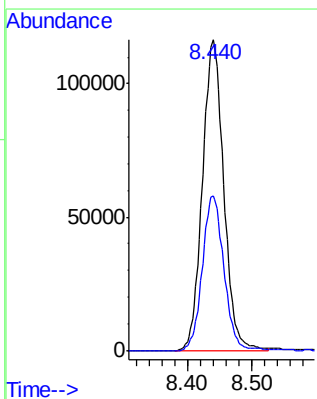
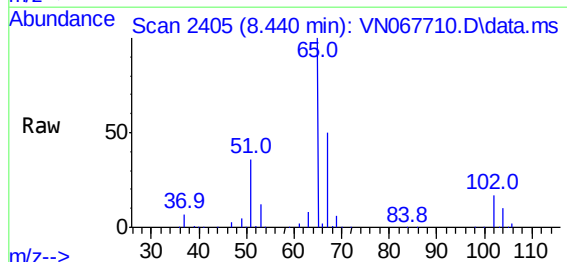


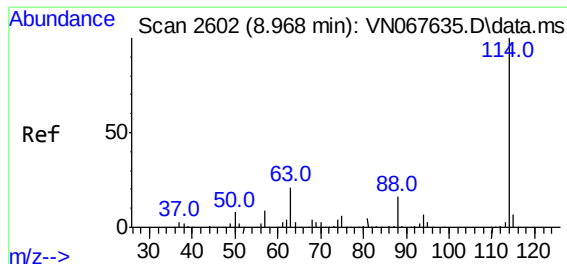

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0713WBL01


Tgt Ion:114 Resp: 636479
Ion Ratio Lower Upper
114 100
63 22.1 0.0 49.0
88 15.5 0.0 36.6

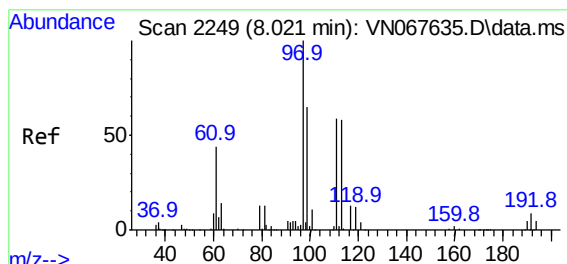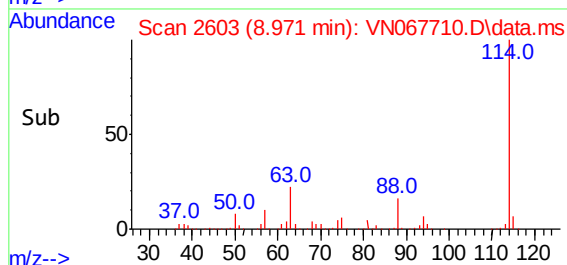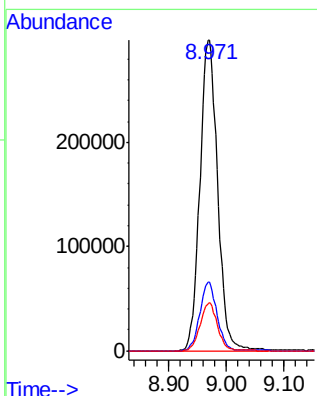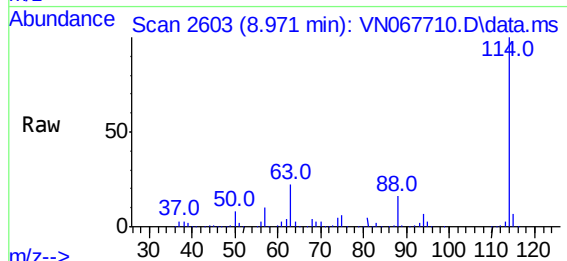

#35
Dibromofluoromethane
Concen: 49.89 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37

Tgt Ion:113 Resp: 191853
Ion Ratio Lower Upper
113 100
111 103.0 83.8 125.8
192 15.6 13.4 20.0


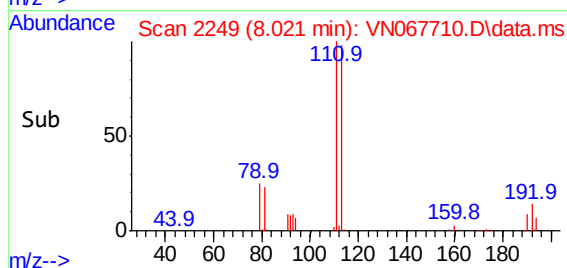
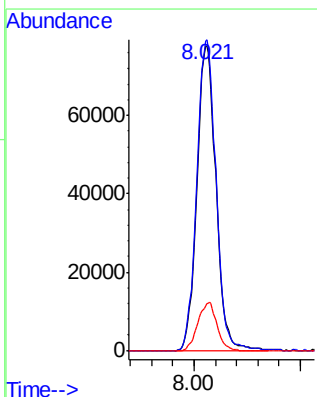
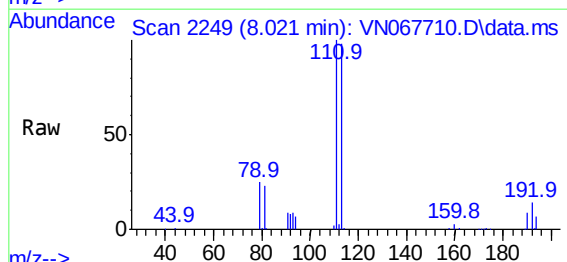


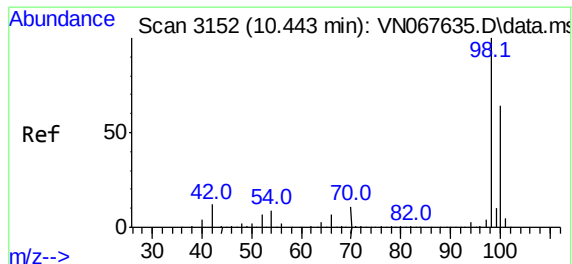

#50
Toluene-d8
Concen: 50.23 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37




Instrument :
MSVOA_N
ClientSampleId :
VN0713WBL01


Tgt Ion: 98 Resp: 808473
Ion Ratio Lower Upper
98 100
100 63.2 51.7 77.5

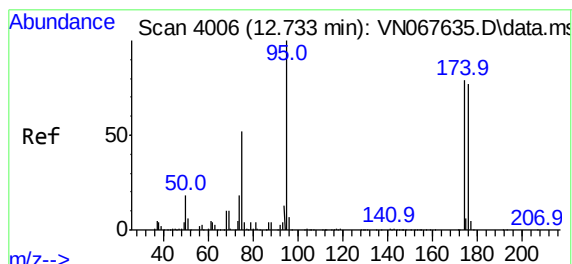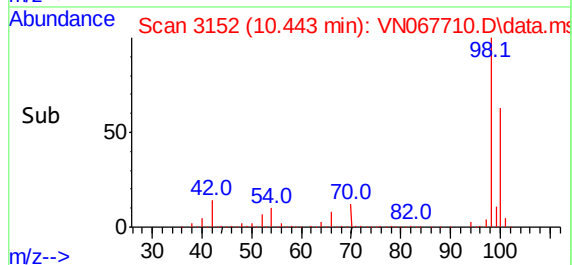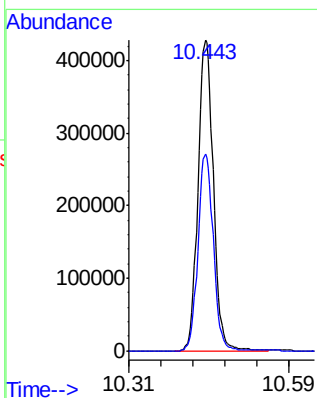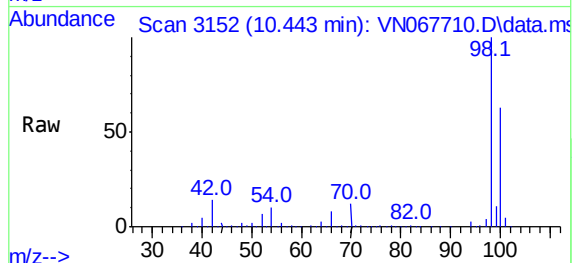

#62
4-Bromofluorobenzene
Concen: 44.41 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37

Tgt Ion: 95 Resp: 252496
Ion Ratio Lower Upper
95 100
174 71.2 0.0 122.0
176 67.7 0.0 117.6


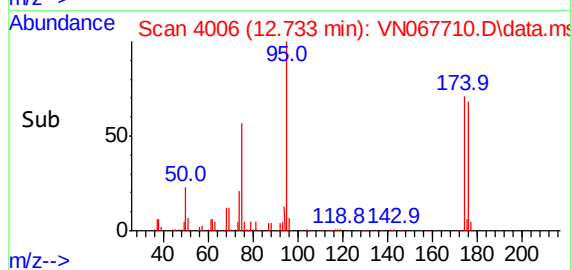
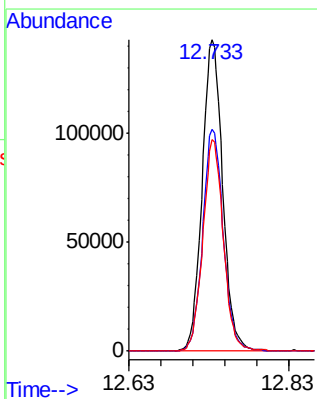
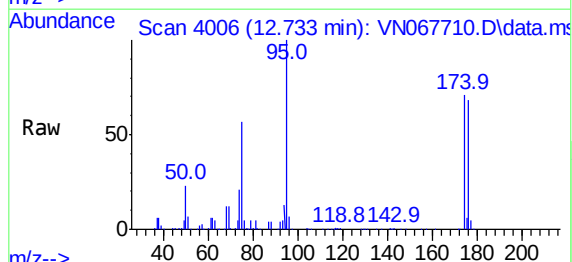


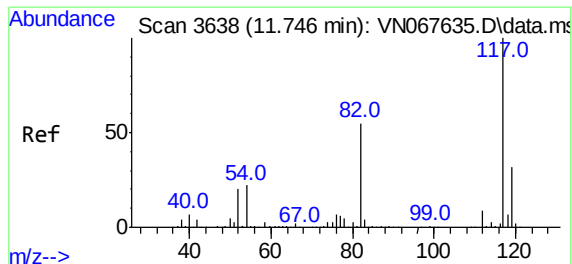

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37

Instrument :
MSVOA_N
ClientSampleId :
VN0713WBL01

Tgt Ion:117 Resp: 582128
Ion Ratio Lower Upper
117 100
82 57.5 53.1 79.7
119 31.8 25.5 38.3

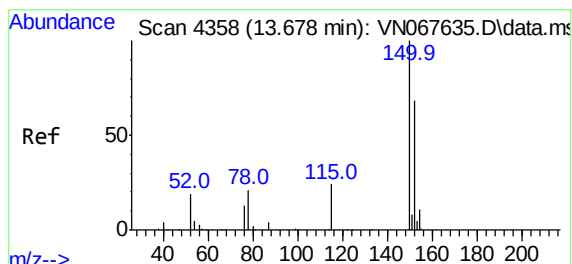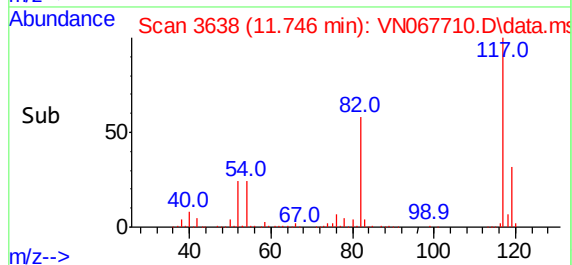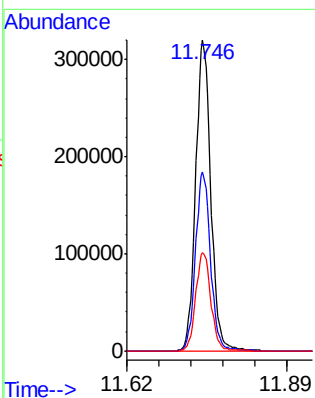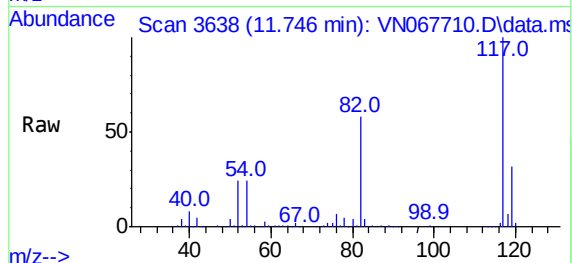

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN067710.D
Acq: 13 Jul 2021 11:37

Tgt Ion:152 Resp: 203702
Ion Ratio Lower Upper
152 100
115 62.9 36.1 108.5
150 160.2 0.0 351.8

