
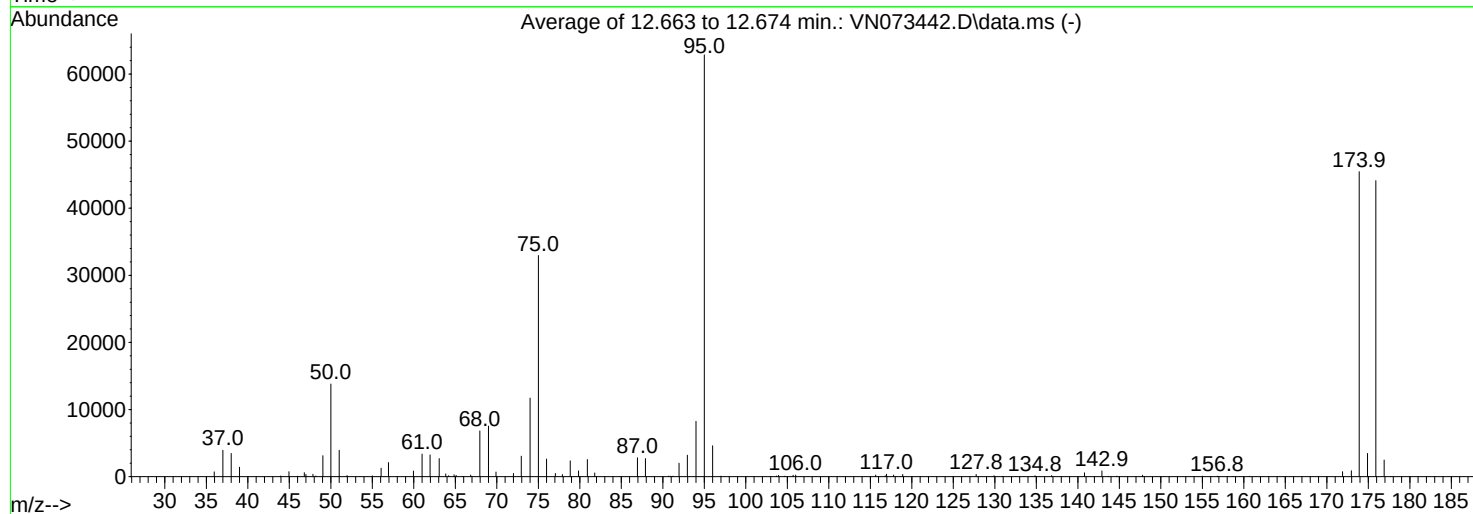


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN071322\  
 Data File : VN073442.D  
 Acq On : 13 Jul 2022 10:41  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N062822W.M  
 Title : SW846 8260  
 Last Update : Wed Jun 29 01:54:03 2022

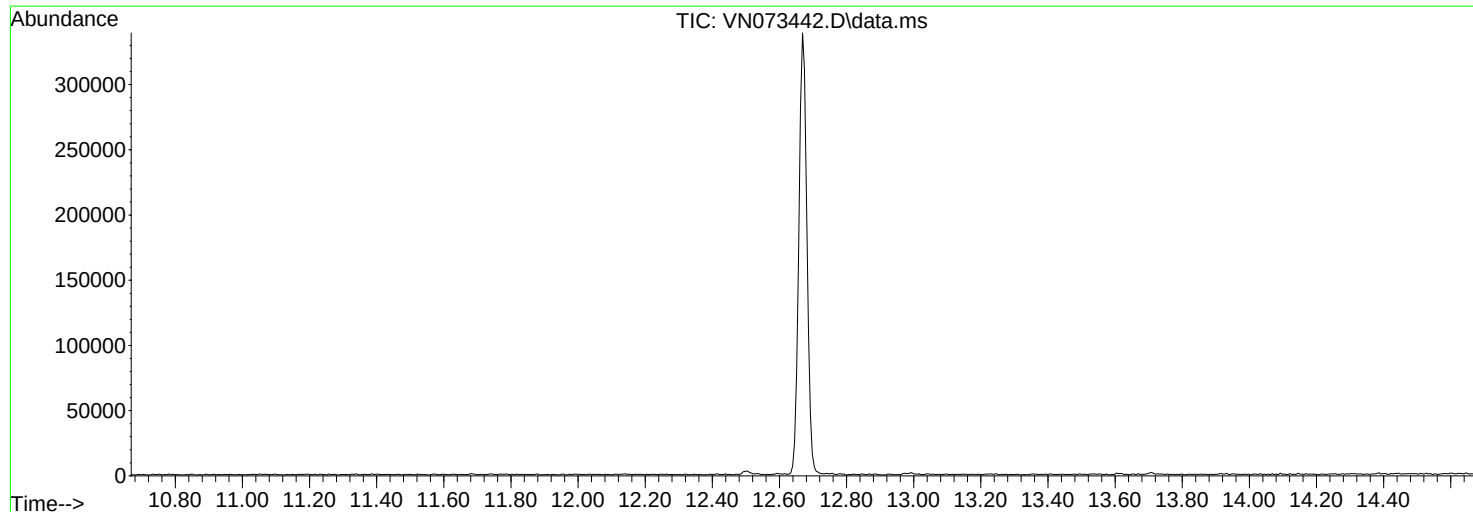

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 22.0         | 13804      | PASS                |
| 75             | 95              | 30              | 60              | 52.4         | 32949      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 62859      | PASS                |
| 96             | 95              | 5               | 9               | 7.3          | 4607       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.9          | 872        | PASS                |
| 174            | 95              | 50              | 100             | 72.3         | 45451      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 3457       | PASS                |
| 176            | 174             | 95              | 101             | 97.1         | 44123      | PASS                |
| 177            | 176             | 5               | 9               | 5.7          | 2494       | PASS                |