

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN071323\  
Data File : VN078493.D  
Acq On : 13 Jul 2023 12:57  
Operator : JC\MD  
Sample : 03606-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TB-01-071223

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N071023W.M

Title : SW846 8260

Signal : TIC: VN078493.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.830       | 141           | 149         | 154          | rVB4     | 24772          | 56114         | 2.47%           | 0.458%        |
| 2         | 4.742       | 462           | 474         | 479          | rBV5     | 7349           | 23133         | 1.02%           | 0.189%        |
| 3         | 7.441       | 927           | 933         | 935          | rBV2     | 14424          | 24001         | 1.05%           | 0.196%        |
| 4         | 8.177       | 1048          | 1058        | 1062         | rBV      | 392772         | 919218        | 40.39%          | 7.502%        |
| 5         | 8.236       | 1062          | 1068        | 1079         | rVB      | 574665         | 1319476       | 57.98%          | 10.769%       |
| 6         | 8.588       | 1118          | 1128        | 1141         | rBV      | 348801         | 784451        | 34.47%          | 6.402%        |
| 7         | 9.112       | 1206          | 1217        | 1233         | rBV      | 836060         | 1758385       | 77.26%          | 14.351%       |
| 8         | 10.577      | 1457          | 1466        | 1478         | rBV      | 1190914        | 2275896       | 100.00%         | 18.574%       |
| 9         | 11.871      | 1675          | 1686        | 1698         | rBV      | 1162972        | 2091392       | 91.89%          | 17.069%       |
| 10        | 12.859      | 1846          | 1854        | 1862         | rBV      | 872426         | 1521532       | 66.85%          | 12.418%       |
| 11        | 13.800      | 2006          | 2014        | 2023         | rVB      | 855541         | 1479306       | 65.00%          | 12.073%       |


Sum of corrected areas: 12252904

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN071323\  
Data File : VN078493.D  
Acq On : 13 Jul 2023 12:57  
Operator : JC\MD  
Sample : 03606-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TB-01-071223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N071023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

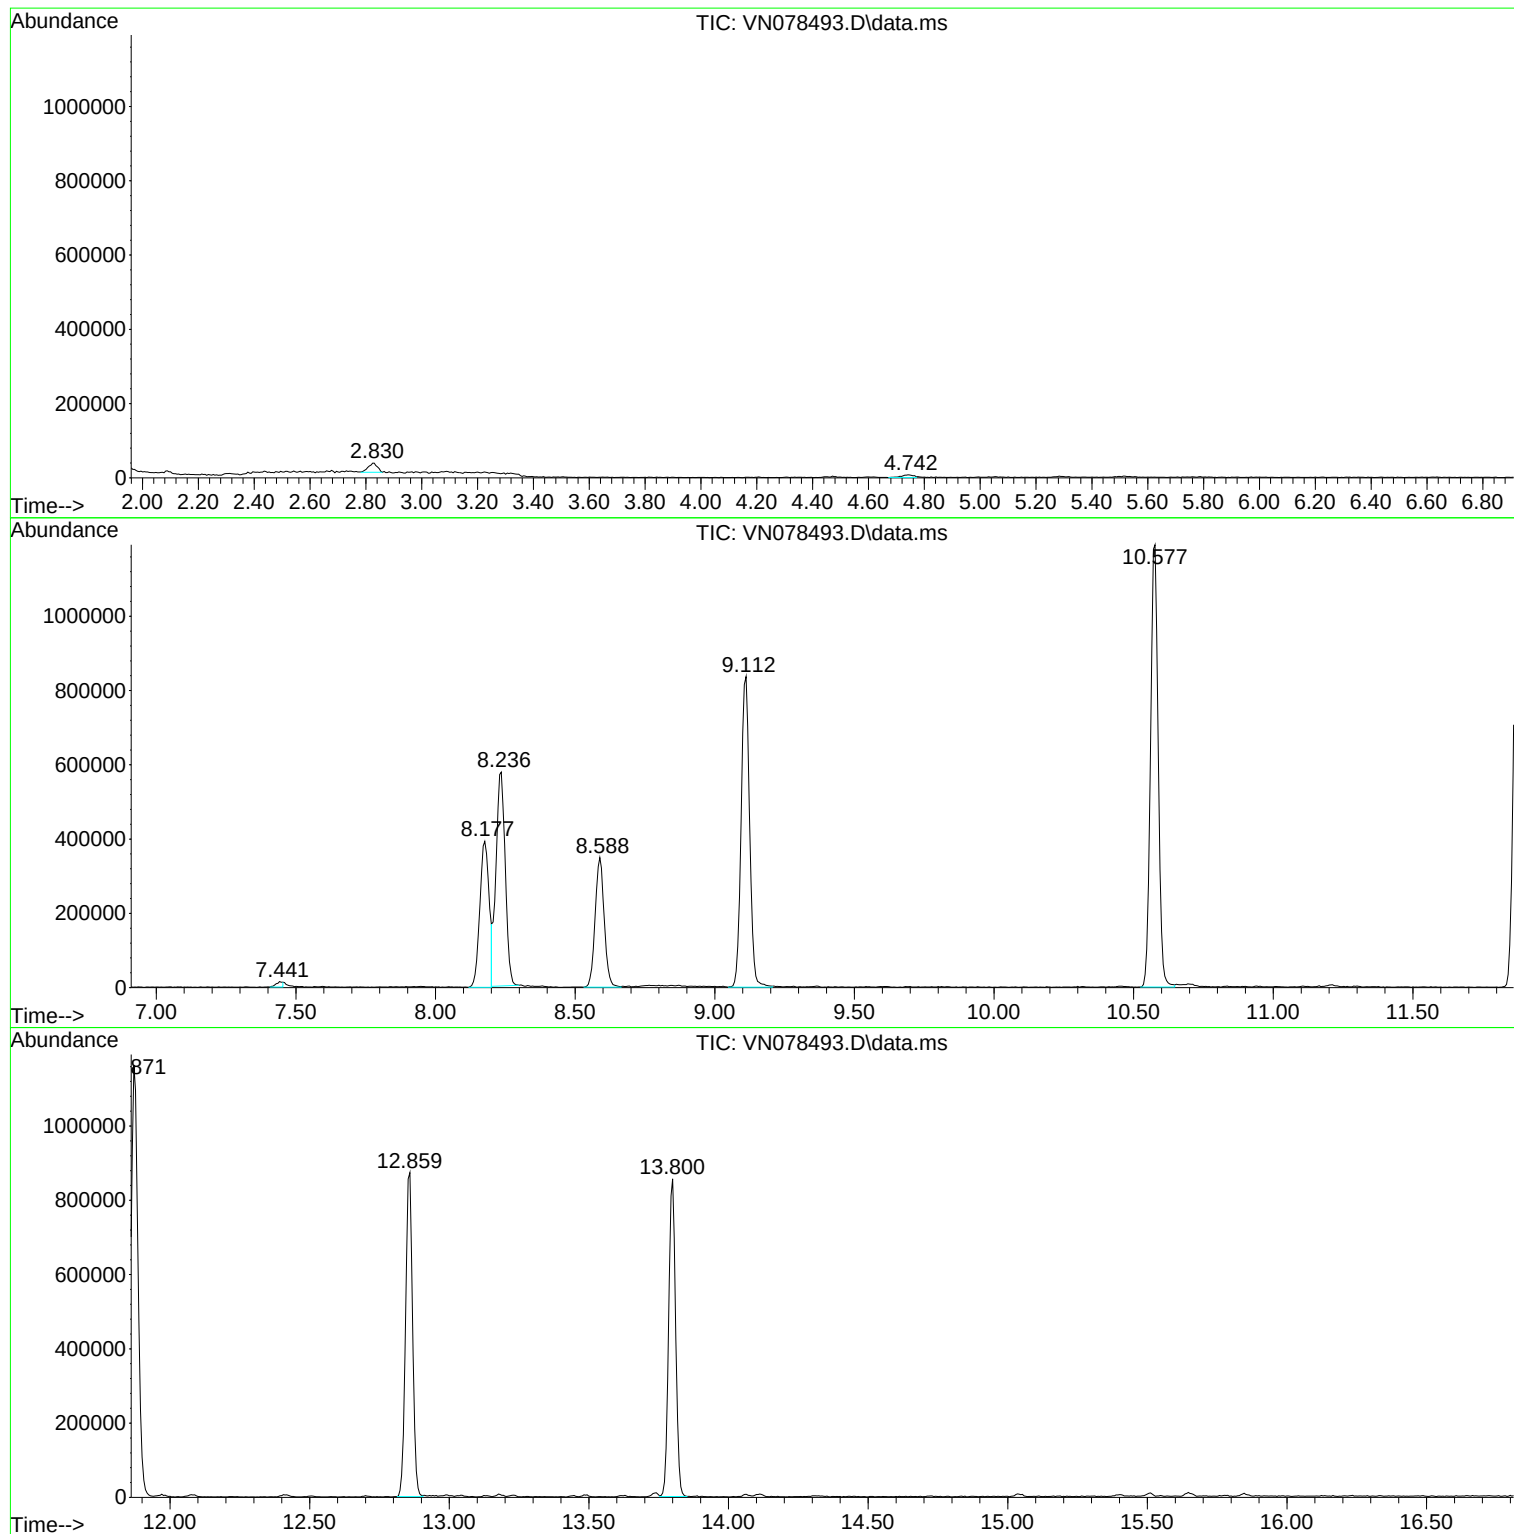

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN071323\  
Data File : VN078493.D  
Acq On : 13 Jul 2023 12:57  
Operator : JC\MD  
Sample : 03606-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TB-01-071223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N071023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN071323\  
Data File : VN078493.D  
Acq On : 13 Jul 2023 12:57  
Operator : JC\MD  
Sample : 03606-01  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TB-01-071223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N071023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |