
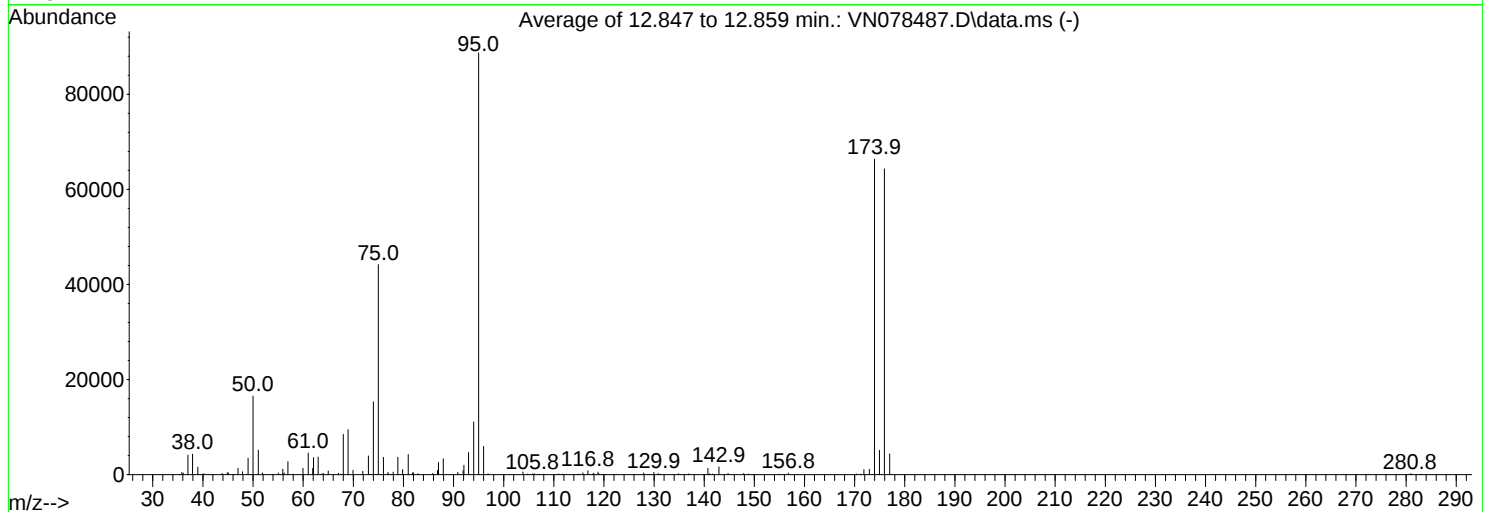


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071323\
Data File : VN078487.D
Acq On : 13 Jul 2023 09:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

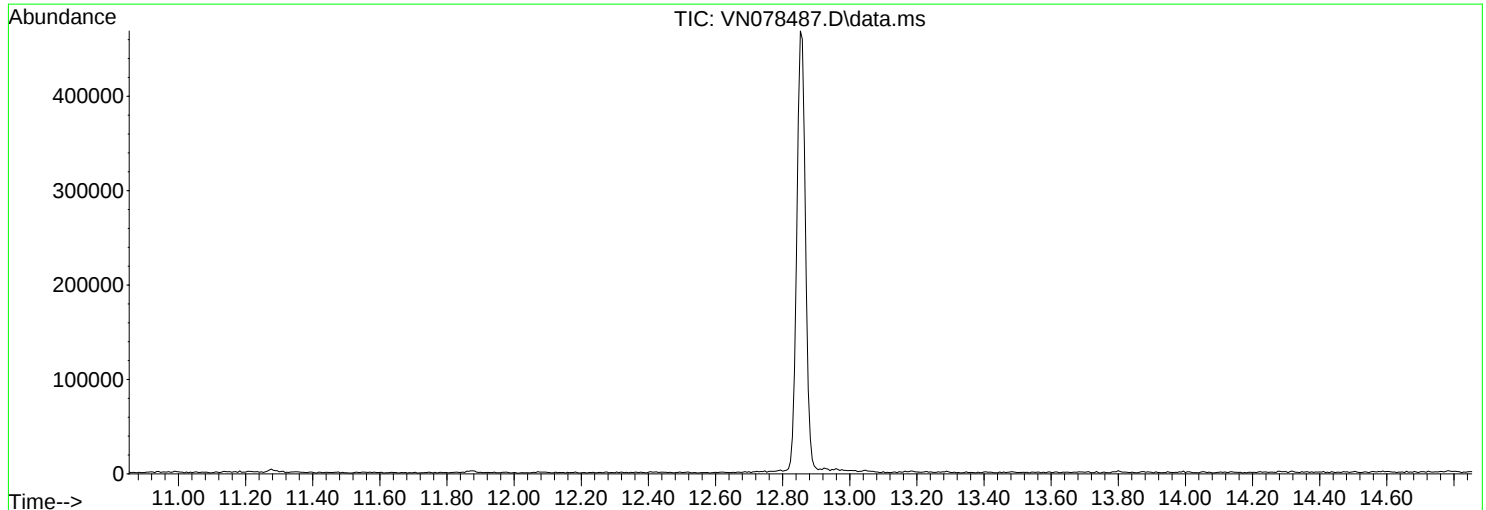

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	16515	PASS
75	95	30	60	49.8	44195	PASS
95	95	100	100	100.0	88723	PASS
96	95	5	9	6.7	5954	PASS
173	174	0.00	2	1.7	1124	PASS
174	95	50	100	74.8	66387	PASS
175	174	5	9	7.7	5104	PASS
176	174	95	101	96.9	64320	PASS
177	176	5	9	6.8	4380	PASS

Average of 12.847 to 12.859 min.: VN078487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.30	63	45.10	381	56.20	380	67.05	261
35.80	460	46.20	67	56.95	2726	68.00	849
36.10	328	47.00	1347	58.00	89	68.95	947
37.00	4099	47.90	604	59.95	1366	69.95	92
37.95	4323	49.00	3456	61.00	4560	71.90	705
39.00	1593	50.00	16515	61.90	1327	73.00	3934
39.85	15	51.05	5147	62.05	3557	74.00	15304
40.00	154	51.90	349	63.00	3696	75.00	44195
40.20	191	53.80	53	63.80	172	76.00	3625
43.85	283	55.05	335	64.05	253	76.80	104
44.85	405	55.95	1162	65.00	779	76.95	470

Average of 12.847 to 12.859 min.: VN078487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.60	80	87.95	3321	105.75	181	117.95	312
77.95	556	90.85	470	106.10	214	118.80	555
78.90	3683	91.90	829	107.00	57	119.00	164
79.85	1073	92.05	1978	107.90	109	119.60	73
80.95	4256	93.00	4634	111.00	120	127.90	345
81.80	353	94.00	11069	111.70	104	129.10	66
81.95	482	95.00	88723	114.70	65	129.95	468
82.90	202	96.00	5954	115.00	107	130.80	212
85.85	241	96.90	157	115.80	367	131.20	112
86.80	866	103.85	578	116.80	799	134.90	211
87.00	2549	104.80	151	117.70	102	136.80	69

Average of 12.847 to 12.859 min.: VN078487.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
136.95	182	170.40	142	283.10	79		
140.75	1314	171.20	110				
141.10	208	171.85	1052				
141.70	120	172.95	1124				
142.95	1621	173.95	66387				
144.75	281	174.95	5104				
147.90	270	175.95	64320				
148.85	151	177.00	4380				
149.90	71	280.80	180				
154.90	111	281.05	145				
156.80	307	282.90	53				