


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071420\
Data File : VN062519.D
Acq On : 14 Jul 2020 9:01
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N071320W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Jul 14 00:52:57 2020

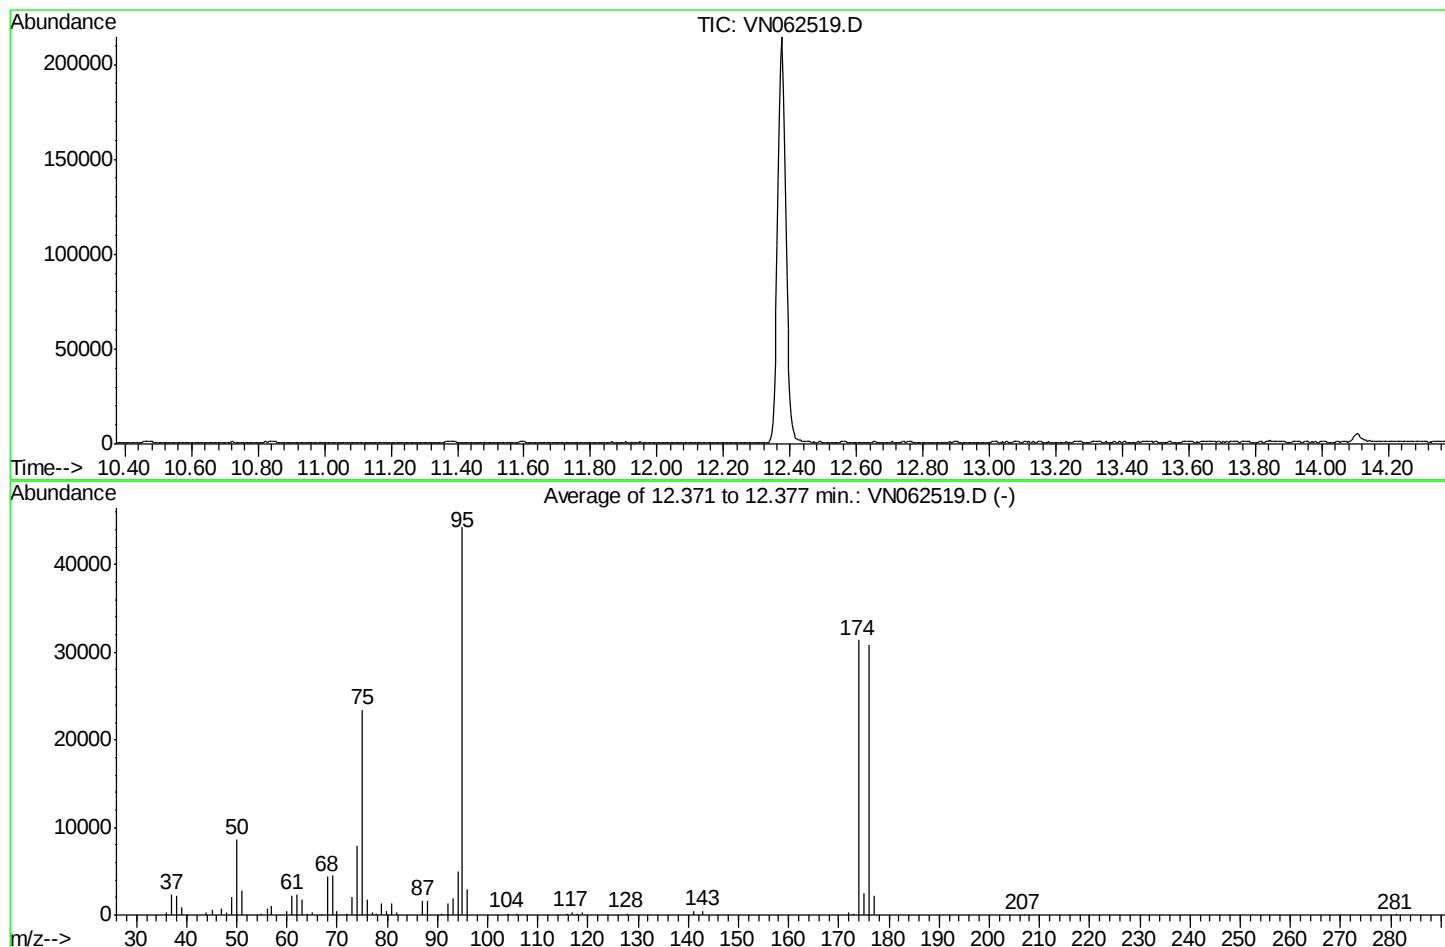

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	8569	PASS
75	95	30	60	52.9	23432	PASS
95	95	100	100	100.0	44269	PASS
96	95	5	9	6.7	2969	PASS
173	174	0.00	2	0.5	171	PASS
174	95	50	100	70.9	31389	PASS
175	174	5	9	7.8	2463	PASS
176	174	95	101	98.2	30810	PASS
177	176	5	9	7.2	2209	PASS