

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071421\
 Data File : VN067736.D
 Acq On : 14 Jul 2021 11:46
 Operator : JC/MD
 Sample : VN0714MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0714MBL01

Quant Time: Jul 14 17:49:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	340093	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	622886	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	574032	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	196268	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	260930	50.766	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	101.540%
35) Dibromofluoromethane	8.024	113	186083	49.446	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.900%
50) Toluene-d8	10.443	98	791657	50.256	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.520%
62) 4-Bromofluorobenzene	12.734	95	248875	44.725	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	89.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071421\
Data File : VN067736.D
Acq On : 14 Jul 2021 11:46
Operator : JC/MD
Sample : VN0714MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0714MBL01

Quant Time: Jul 14 17:49:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




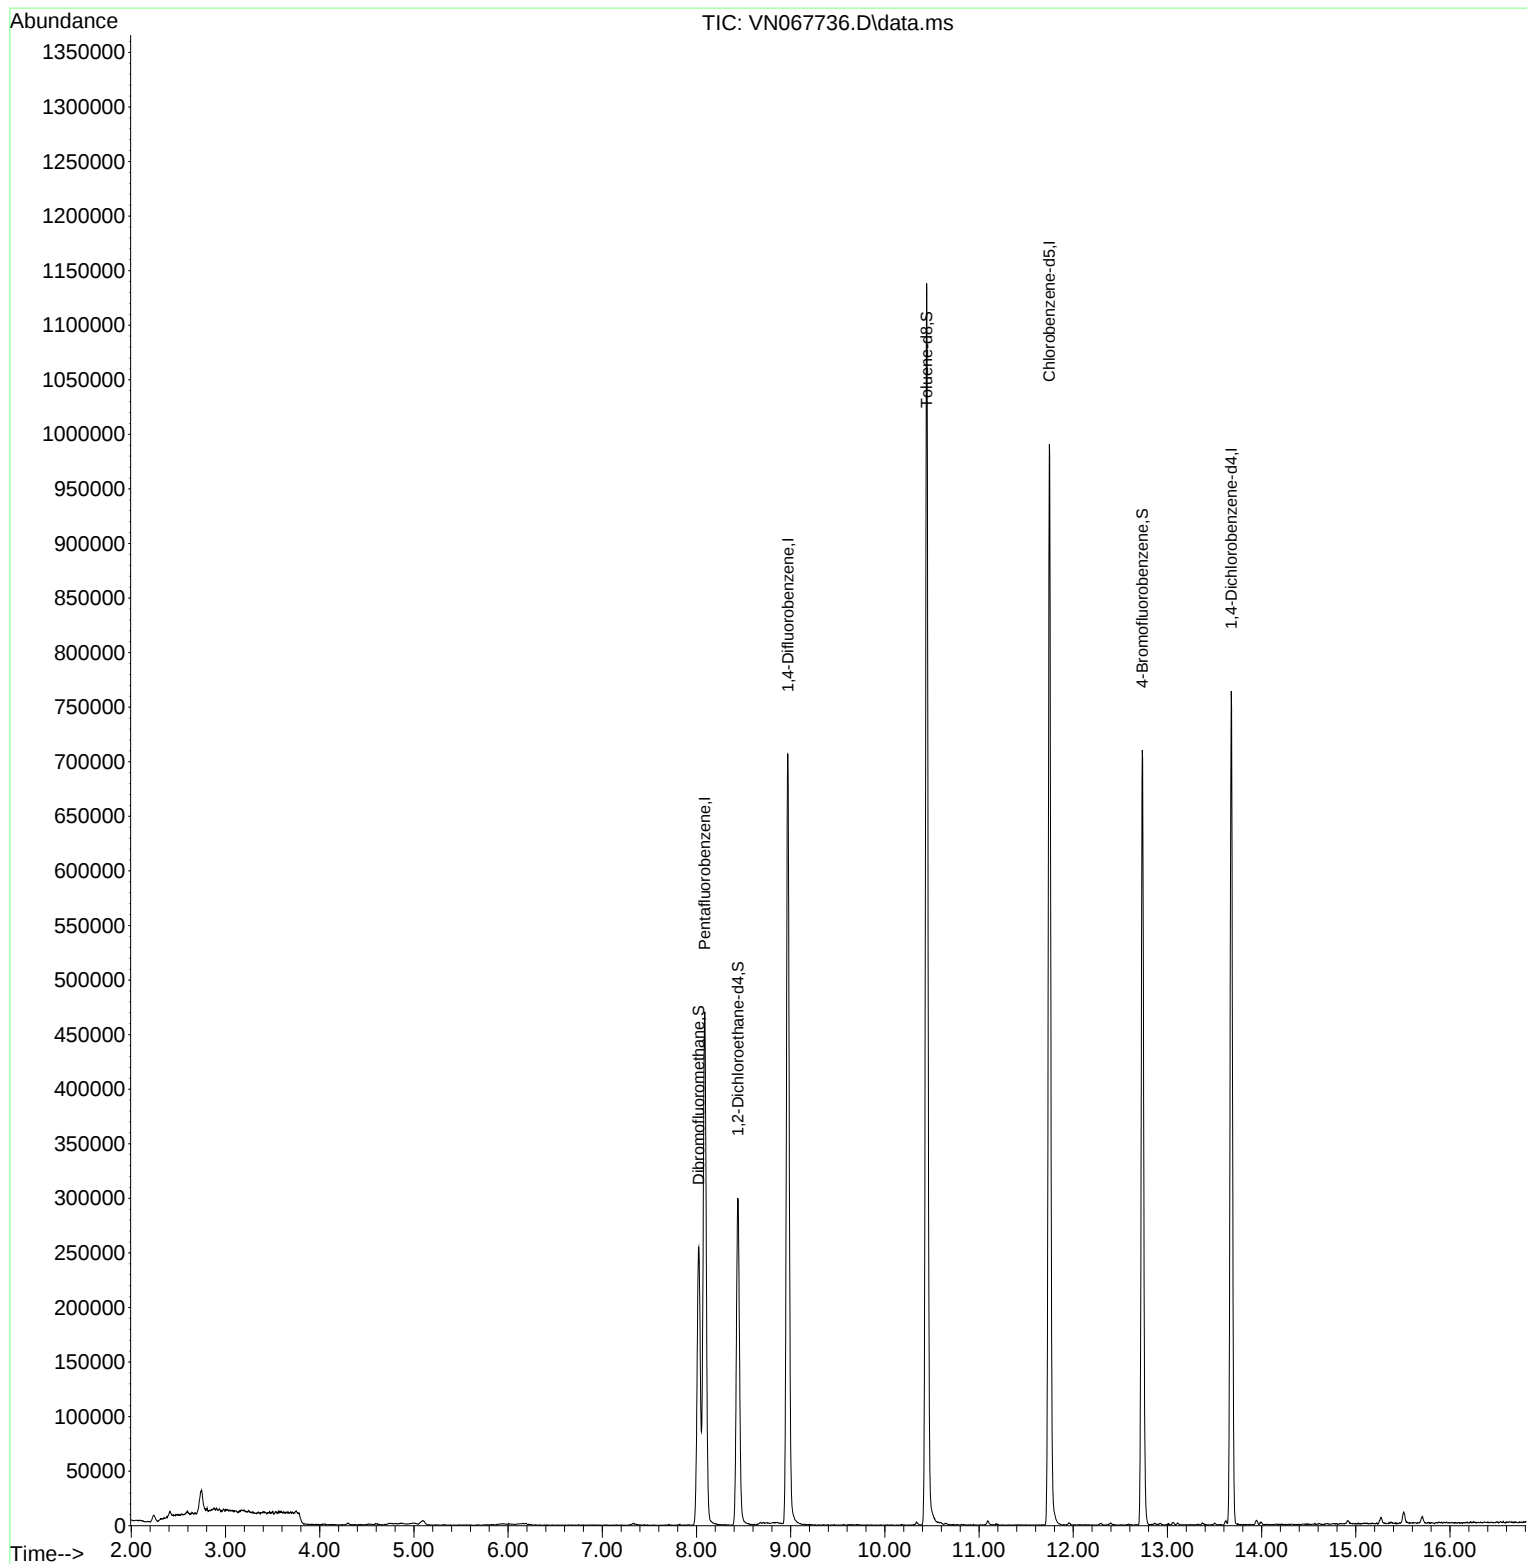


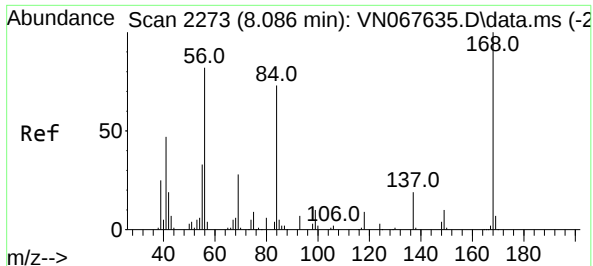

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46




Instrument :
MSVOA_N
ClientSampleId :
VN0714MBL01


Tgt Ion:168 Resp: 340093
Ion Ratio Lower Upper
168 100
99 63.5 62.9 94.3

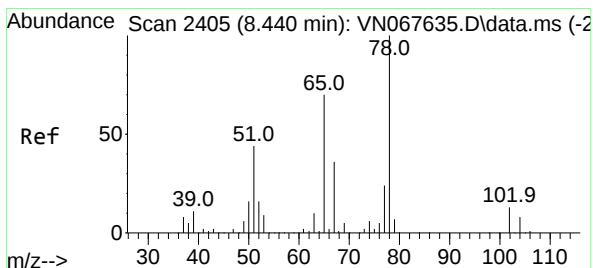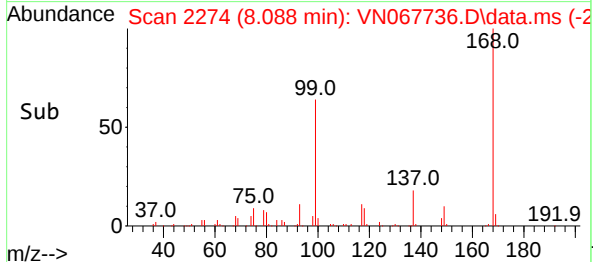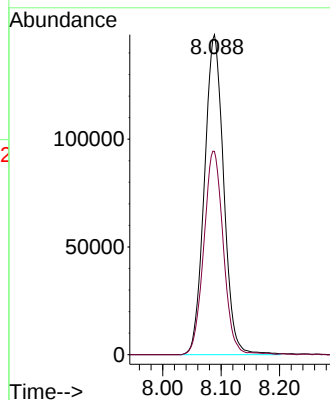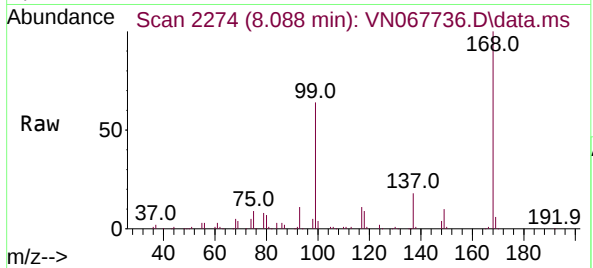

#33
1,2-Dichloroethane-d4
Concen: 50.766 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46

Tgt Ion: 65 Resp: 260930
Ion Ratio Lower Upper
65 100
67 49.4 0.0 98.6


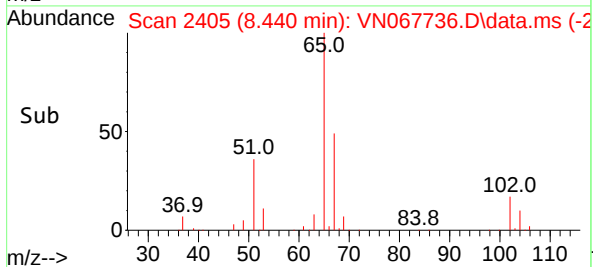
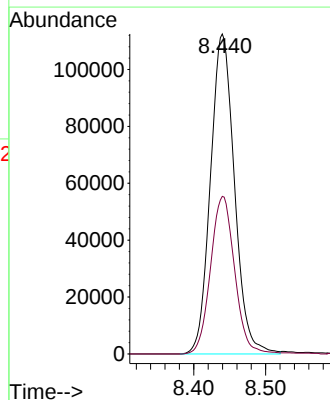
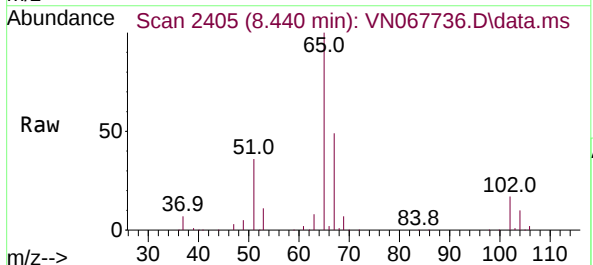


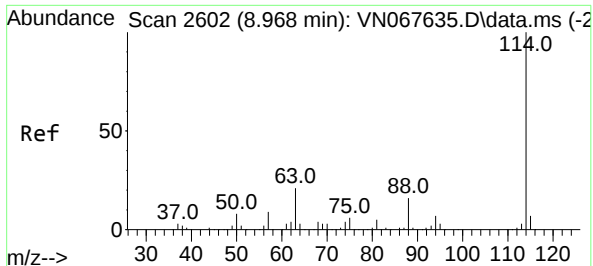

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46




Instrument :
MSVOA_N
ClientSampleId :
VN0714MBL01


Tgt Ion:114 Resp: 622886
Ion Ratio Lower Upper
114 100
63 20.9 0.0 49.0
88 15.5 0.0 36.6

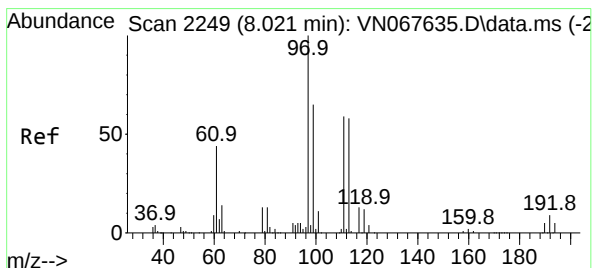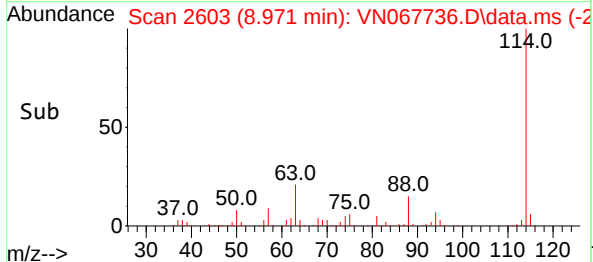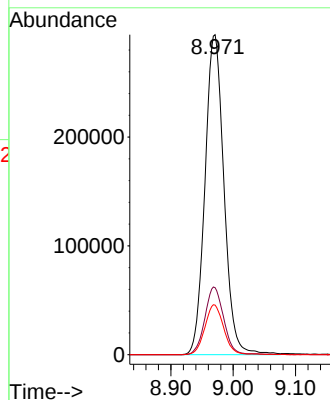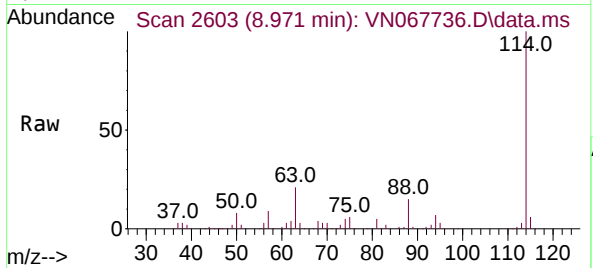

#35
Dibromofluoromethane
Concen: 49.446 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46

Tgt Ion:113 Resp: 186083
Ion Ratio Lower Upper
113 100
111 103.6 83.8 125.8
192 16.2 13.4 20.0


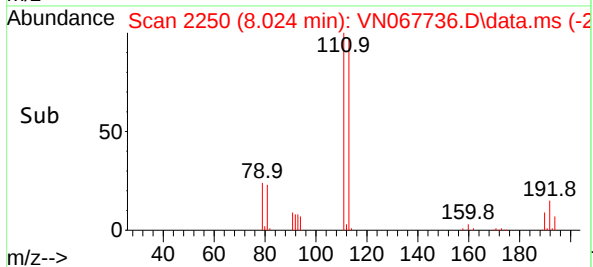
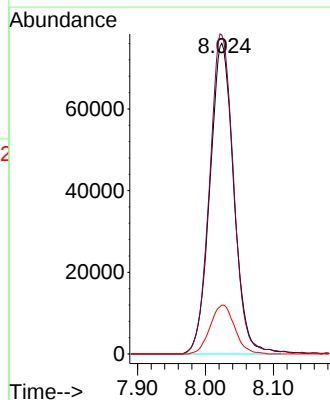
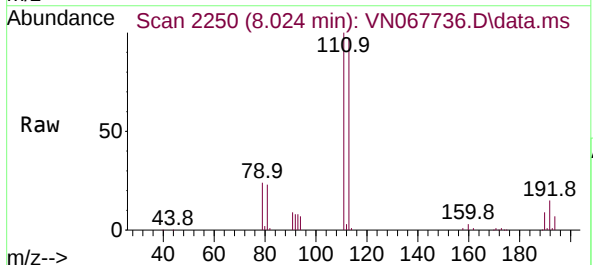


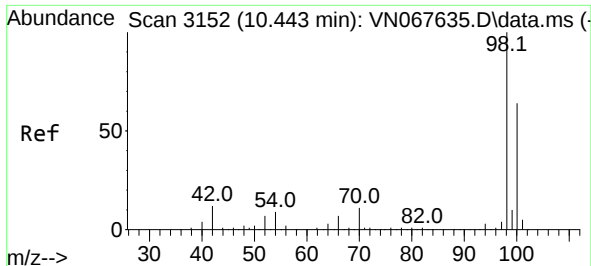

#50
Toluene-d8
Concen: 50.256 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46




Instrument :
MSVOA_N
ClientSampleId :
VN0714MBL01


Tgt Ion: 98 Resp: 791657
Ion Ratio Lower Upper
98 100
100 63.3 51.7 77.5

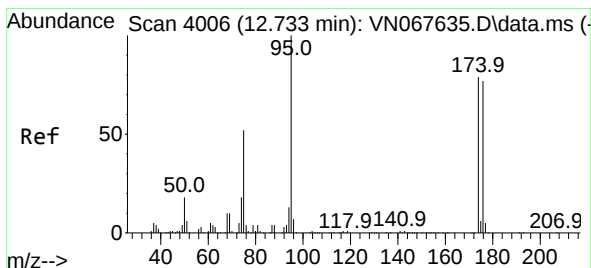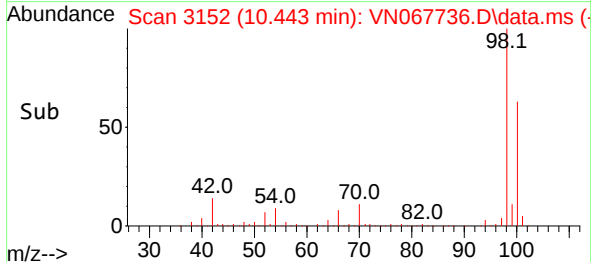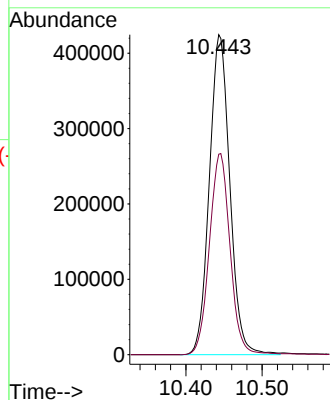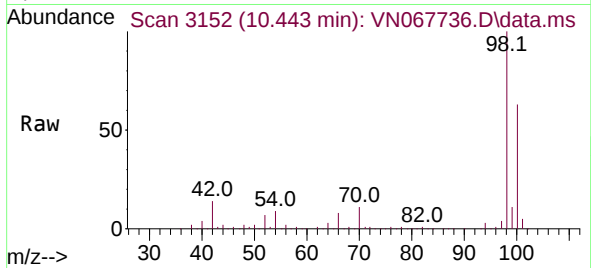

#62
4-Bromofluorobenzene
Concen: 44.725 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46

Tgt Ion: 95 Resp: 248875
Ion Ratio Lower Upper
95 100
174 71.9 0.0 122.0
176 67.9 0.0 117.6


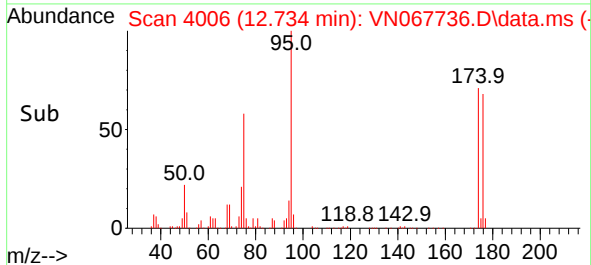
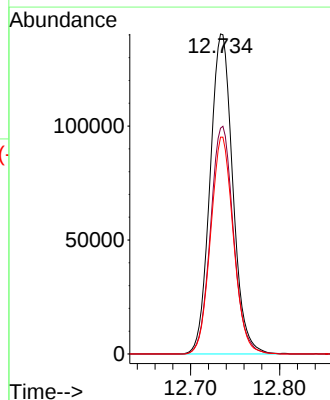
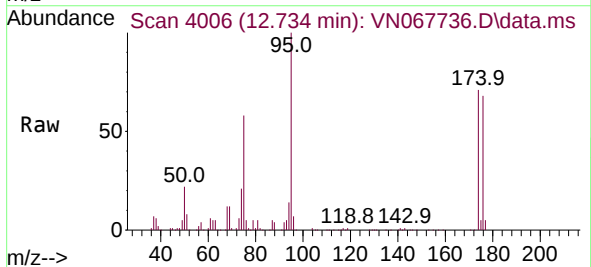


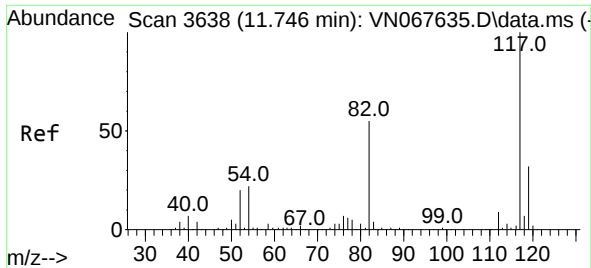

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46

Instrument :
MSVOA_N
ClientSampleId :
VN0714MBL01

Tgt Ion:117 Resp: 574032
Ion Ratio Lower Upper
117 100
82 58.1 53.1 79.7
119 31.6 25.5 38.3

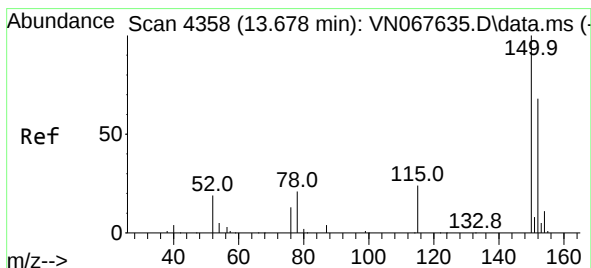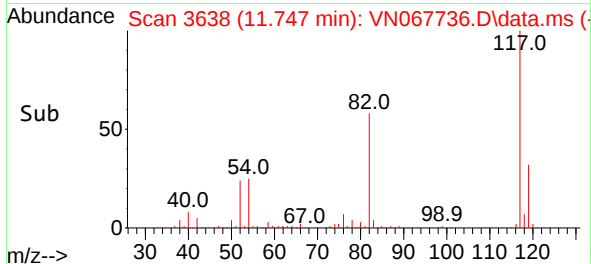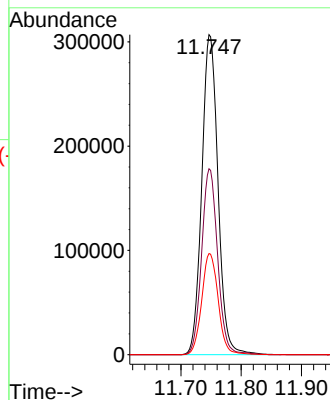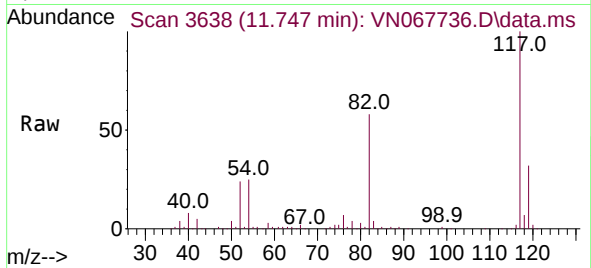

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067736.D
Acq: 14 Jul 2021 11:46

Tgt Ion:152 Resp: 196268
Ion Ratio Lower Upper
152 100
115 62.8 36.1 108.5
150 157.5 0.0 351.8

